

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 05:01
 Operator : AR\AJ
 Sample : PB137673BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 07:27:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.585	7866507	19268508	19.514	18.684
28)	SA Decachlor...	10.432	11.510	9359423	18409999	22.681	20.462
Target Compounds							
8)	B Heptachlo...	0.000	8.052	0	6190088	N.D.	5.569 #
13)	MA Dieldrin	7.797	0.000	356529	0	0.784	N.D. #
14)	MA Endrin	8.102f	8.980	1049795	1105306	2.437	1.247 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 05:01
Operator : AR\AJ
Sample : PB137673BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 07:27:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

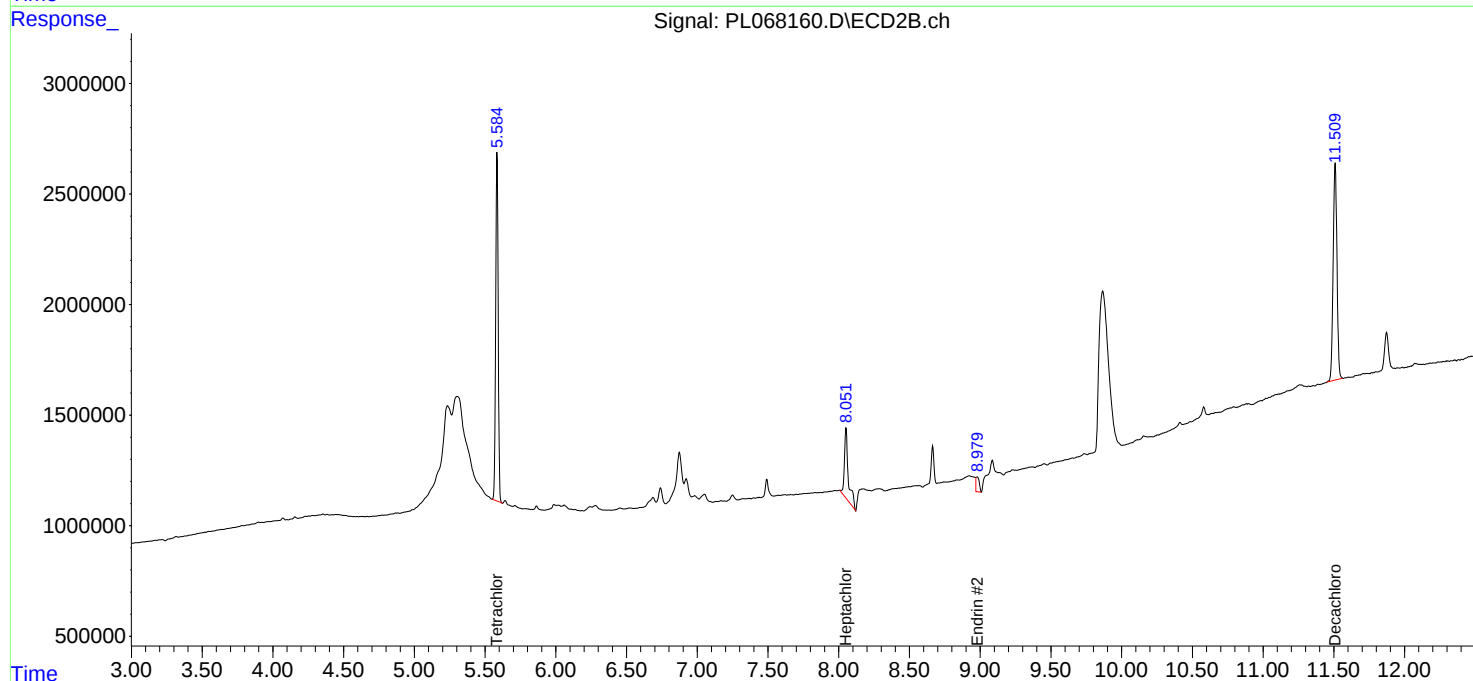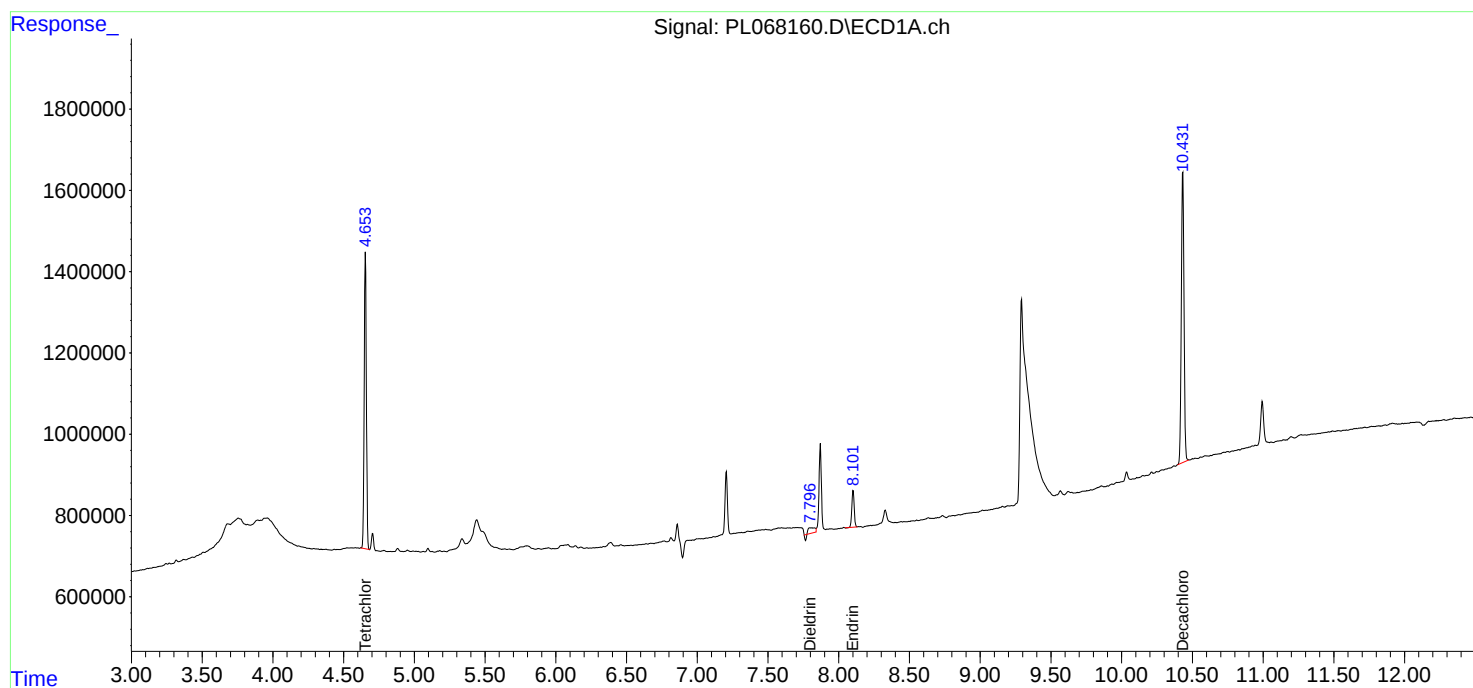

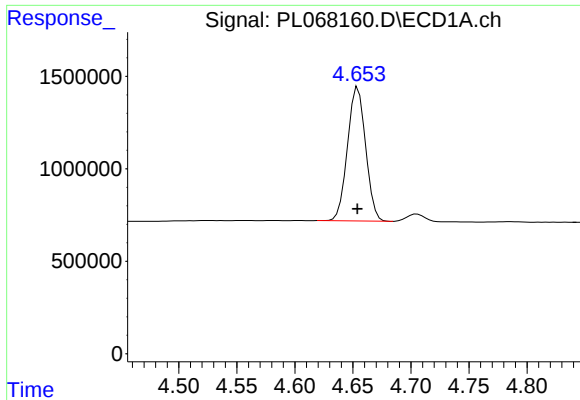


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 7866507
Conc: 19.51 ng/ml

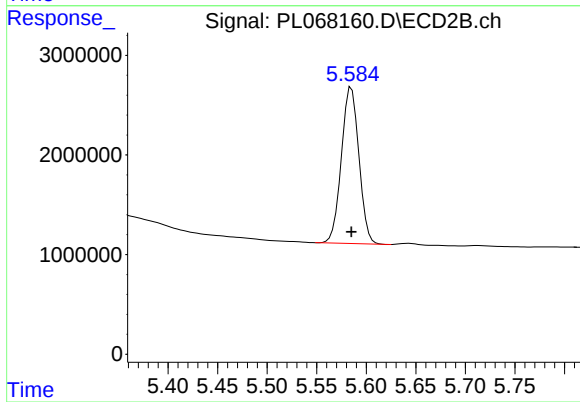


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 19268508
Conc: 18.68 ng/ml

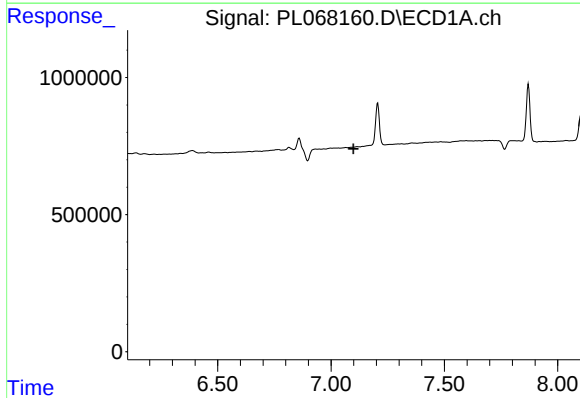


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.100 min
Response: 0
Conc: N.D.

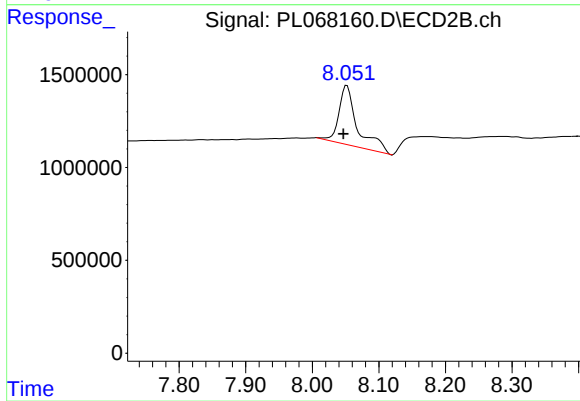


#8 Heptachlor epoxide

R.T.: 8.052 min
Delta R.T.: 0.005 min
Response: 6190088
Conc: 5.57 ng/ml

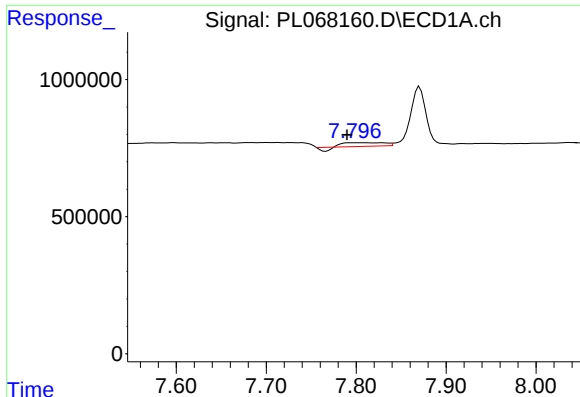


#13 Dieldrin

R.T.: 7.797 min
Delta R.T.: 0.007 min
Response: 356529
Conc: 0.78 ng/ml

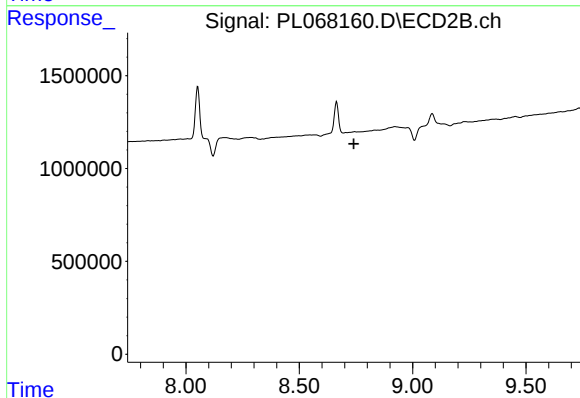


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.741 min
Response: 0
Conc: N.D.

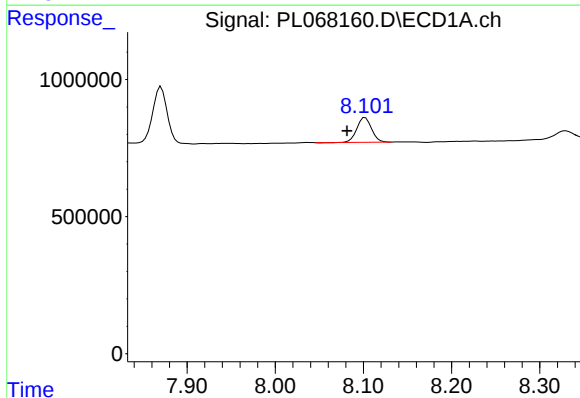


#14 Endrin

R.T.: 8.102 min
Delta R.T.: 0.021 min
Response: 1049795
Conc: 2.44 ng/ml

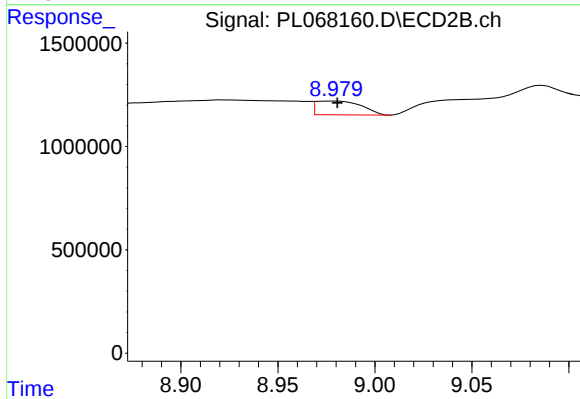


#14 Endrin

R.T.: 8.980 min
Delta R.T.: 0.000 min
Response: 1105306
Conc: 1.25 ng/ml

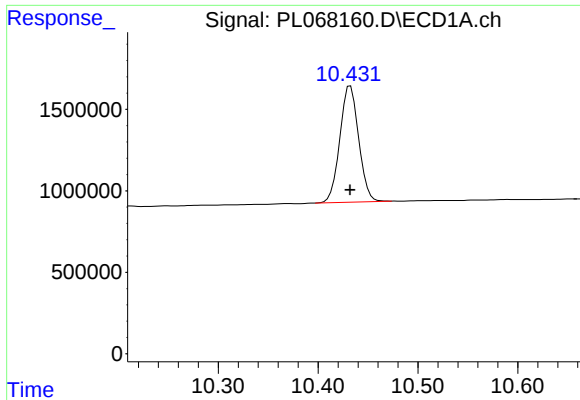

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 9359423
Conc: 22.68 ng/ml

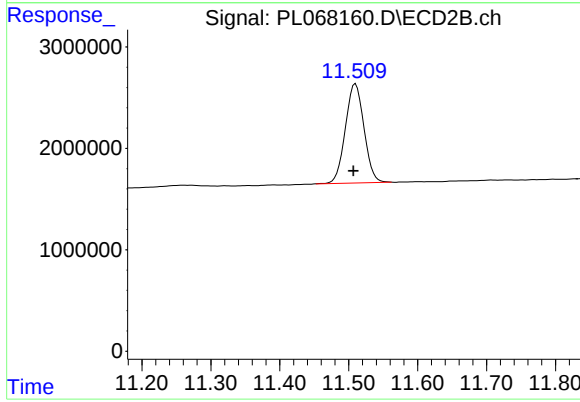

#28 Decachlorobiphenyl

R.T.: 11.510 min
Delta R.T.: 0.003 min
Response: 18409999
Conc: 20.46 ng/ml