

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 05:35
 Operator : AR\AJ
 Sample : M3023-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 07:28:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.586	4319069	9462818	10.714	9.176
28)	SA Decachlor...	10.432	11.510	4735772	9631017	11.476	10.705
Target Compounds							
10)	B gamma-Chl...	0.000	8.315	0	360654	N.D.	0.324 #
11)	B alpha-Chl...	0.000	8.399	0	718661	N.D.	0.645 #
12)	B 4,4'-DDE	0.000	8.579	0	521079	N.D.	0.513 #
13)	MA Dieldrin	0.000	8.761f	0	153320	N.D.	0.147 #
16)	A 4,4'-DDD	0.000	9.121	0	586188	N.D.	0.684 #
25)	Chlordane-3	0.000	8.315	0	360654	N.D.	2.234 #
26)	Chlordane-4	0.000	8.399	0	718661	N.D.	3.642 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 05:35
Operator : AR\AJ
Sample : M3023-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 07:28:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

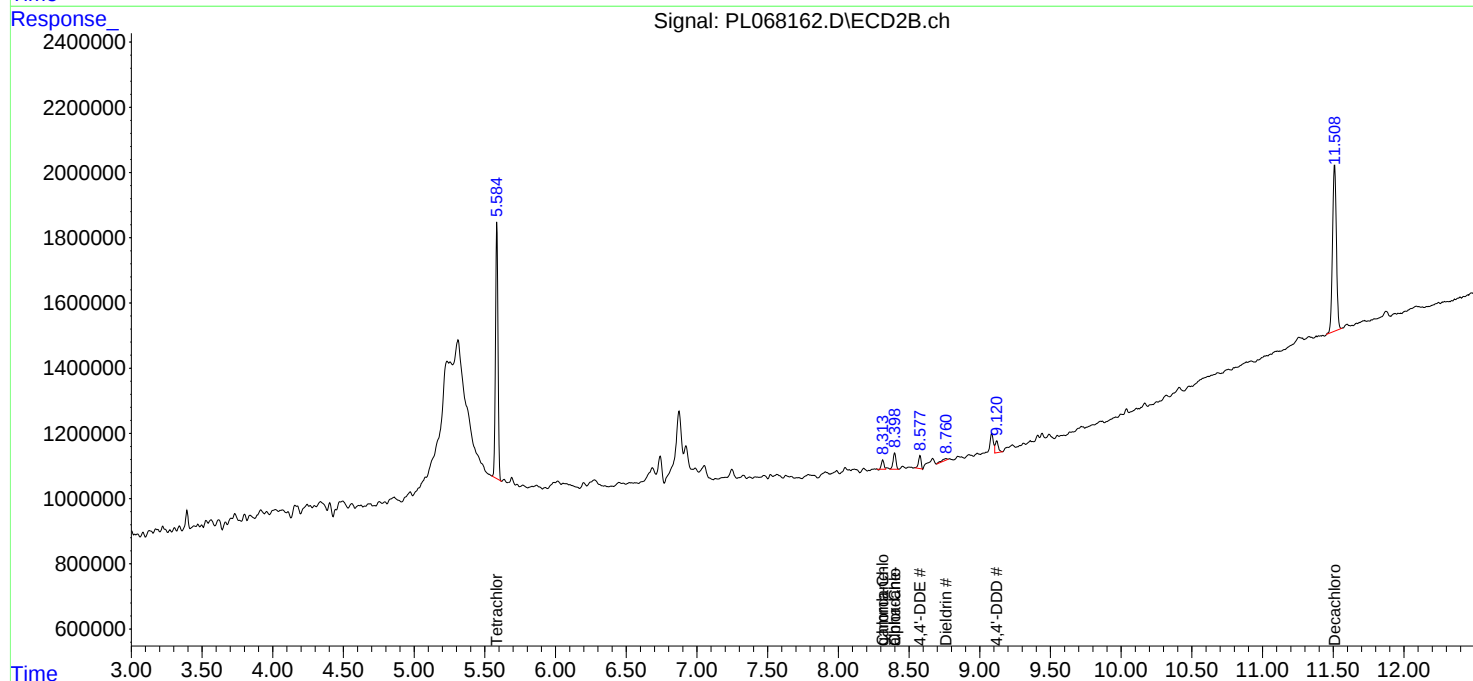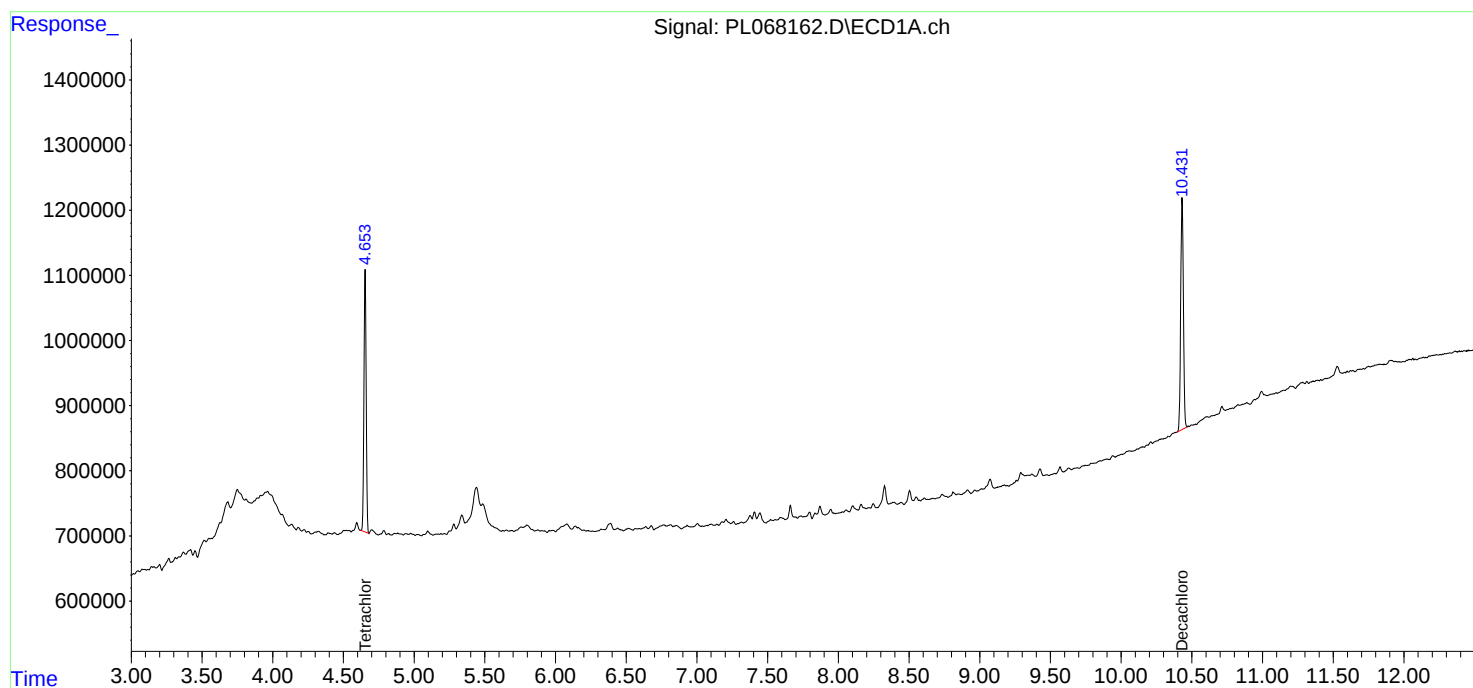

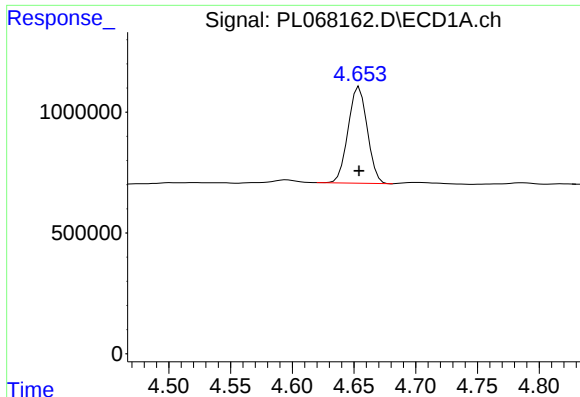


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 4319069
Conc: 10.71 ng/ml

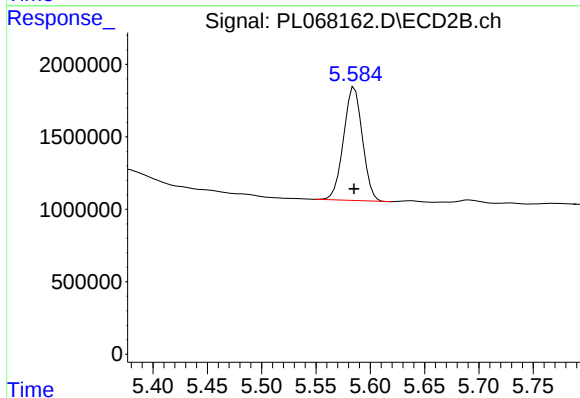


#1 Tetrachloro-m-xylene

R.T.: 5.586 min
Delta R.T.: 0.000 min
Response: 9462818
Conc: 9.18 ng/ml

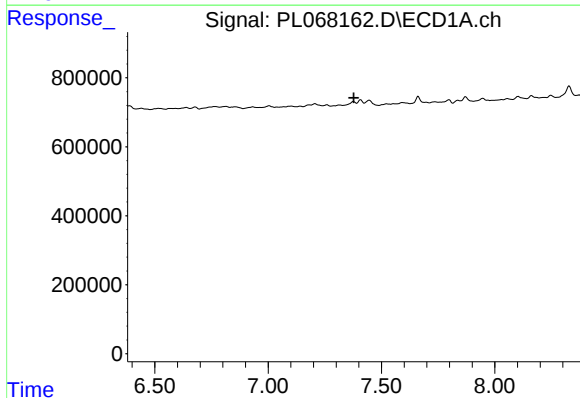


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.377 min
Response: 0
Conc: N.D.

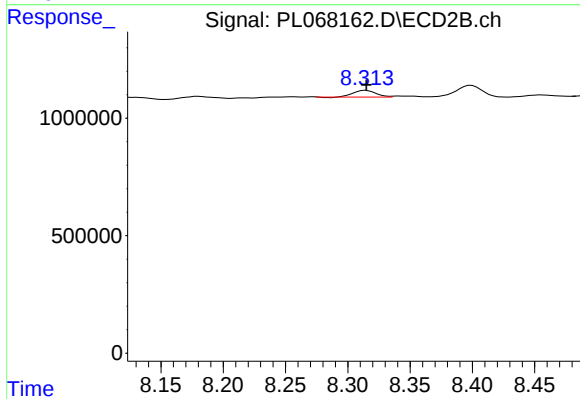


#10 gamma-Chlordane

R.T.: 8.315 min
Delta R.T.: 0.000 min
Response: 360654
Conc: 0.32 ng/ml

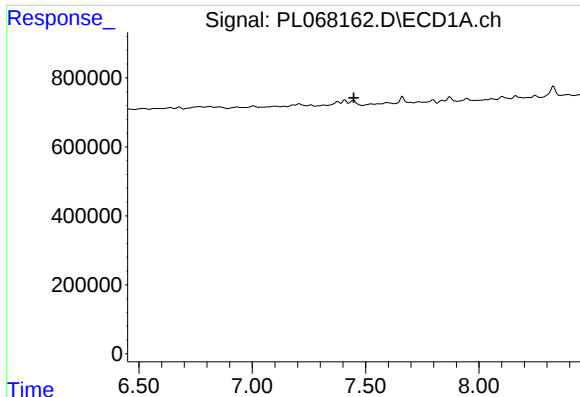


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.448 min
Response: 0
Conc: N.D.

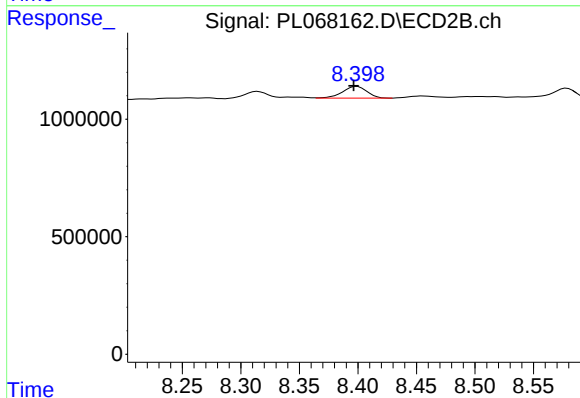


#11 alpha-Chlordane

R.T.: 8.399 min
Delta R.T.: 0.003 min
Response: 718661
Conc: 0.64 ng/ml

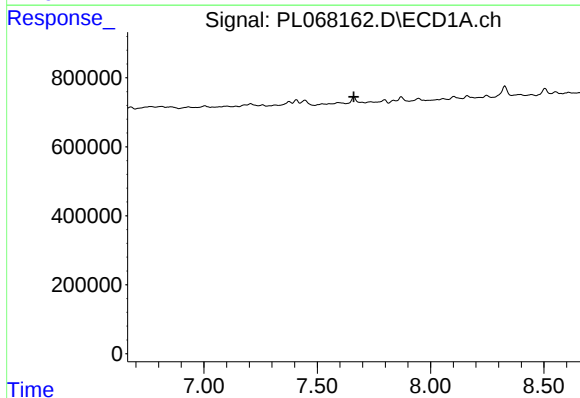


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 7.661 min
Response: 0
Conc: N.D.

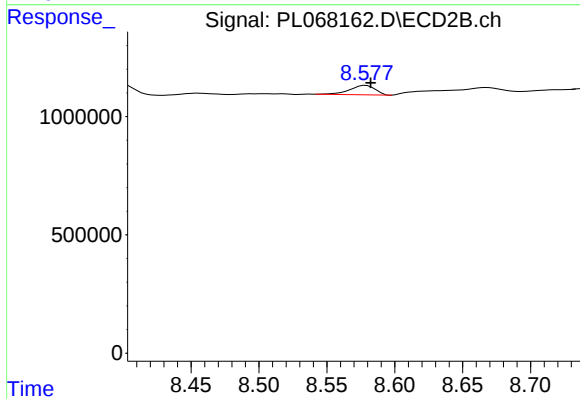


#12 4,4'-DDE

R.T.: 8.579 min
Delta R.T.: -0.004 min
Response: 521079
Conc: 0.51 ng/ml

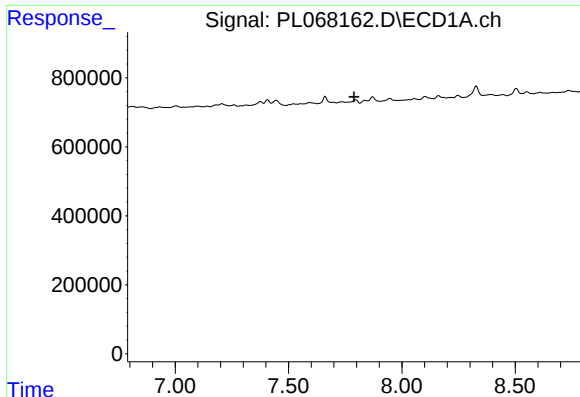


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 7.790 min
Response: 0
Conc: N.D.

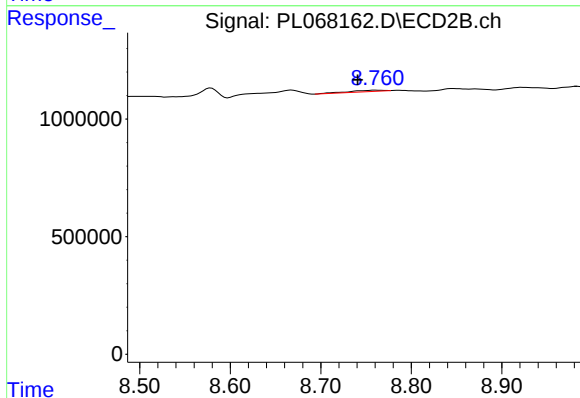


#13 Dieldrin

R.T.: 8.761 min
Delta R.T.: 0.020 min
Response: 153320
Conc: 0.15 ng/ml

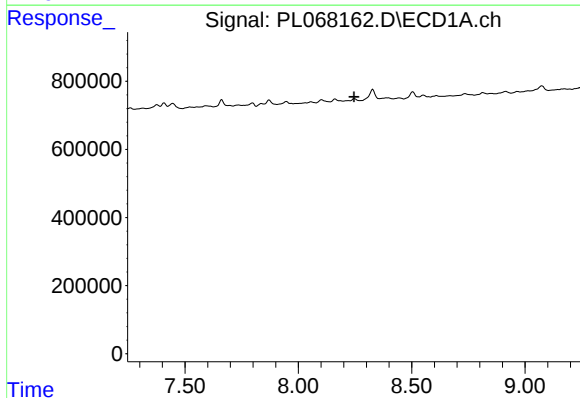


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.246 min
Response: 0
Conc: N.D.

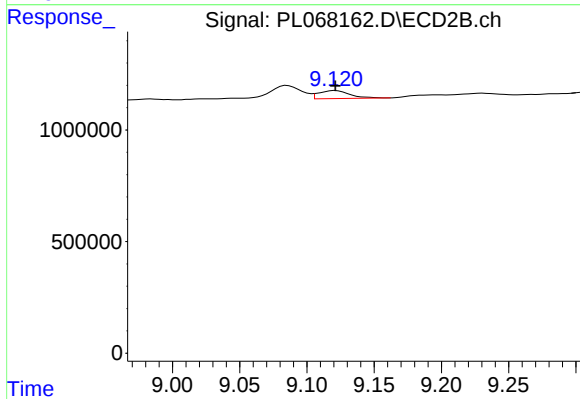


#16 4,4'-DDD

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 586188
Conc: 0.68 ng/ml

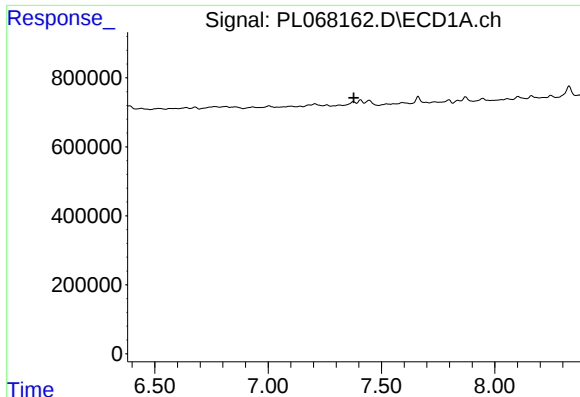


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.378 min
Response: 0
Conc: N.D.

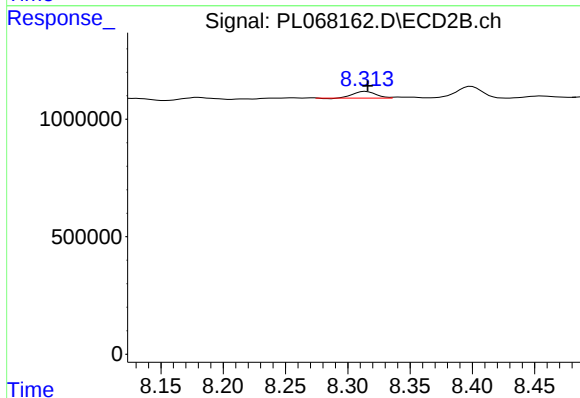


#25 Chlordane-3

R.T.: 8.315 min
Delta R.T.: -0.001 min
Response: 360654
Conc: 2.23 ng/ml

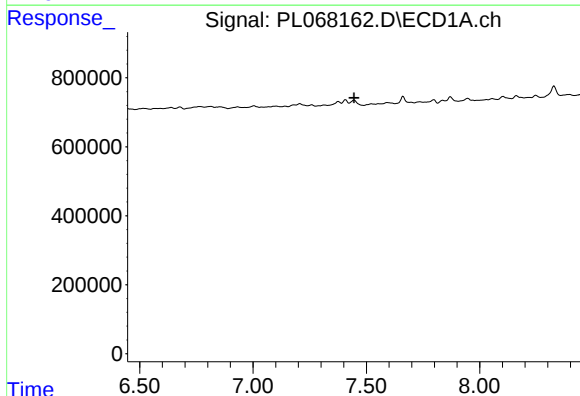


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.446 min
Response: 0
Conc: N.D.

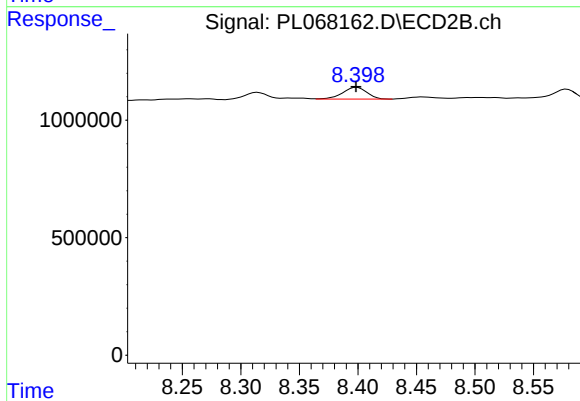


#26 Chlordane-4

R.T.: 8.399 min
Delta R.T.: 0.000 min
Response: 718661
Conc: 3.64 ng/ml

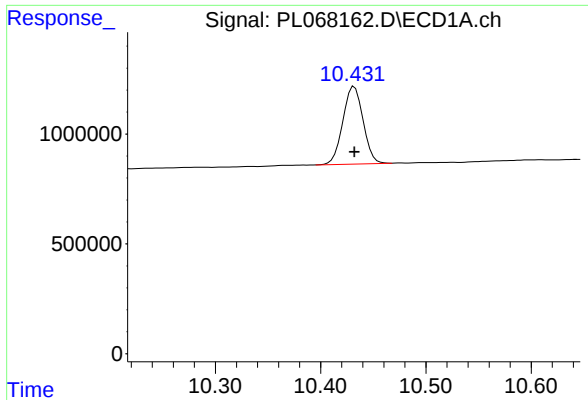

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 4735772
Conc: 11.48 ng/ml

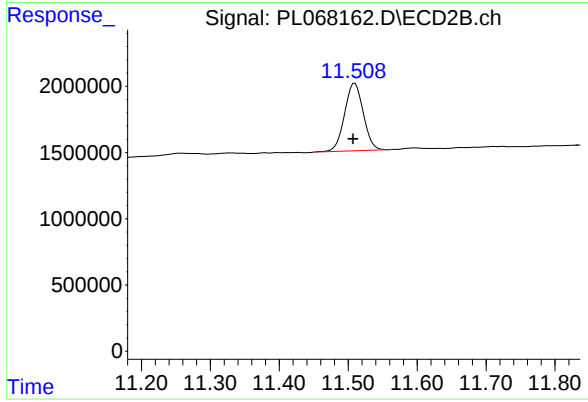

#28 Decachlorobiphenyl

R.T.: 11.510 min
Delta R.T.: 0.003 min
Response: 9631017
Conc: 10.70 ng/ml