

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2021 19:54
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 03:48:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 03:47:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.585	40218538	84906779	74.708	75.553
28)	SA Decachlor...	10.433	11.509	32571507	68549780	78.051	73.116
Target Compounds							
23)	Chlordane-1	5.986	6.969	11094586	29064487	751.328	750.938
24)	Chlordane-2	6.676	7.560	14023825	33149985	739.937	737.640
25)	Chlordane-3	7.378	8.316	38459670	125.4E6	760.970	775.895
26)	Chlordane-4	7.447	8.399	39912666	151.0E6	748.368	765.928
27)	Chlordane-5	8.398	9.287	13228390	27997897	745.179	763.490



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2021 19:54
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 03:48:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 03:47:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

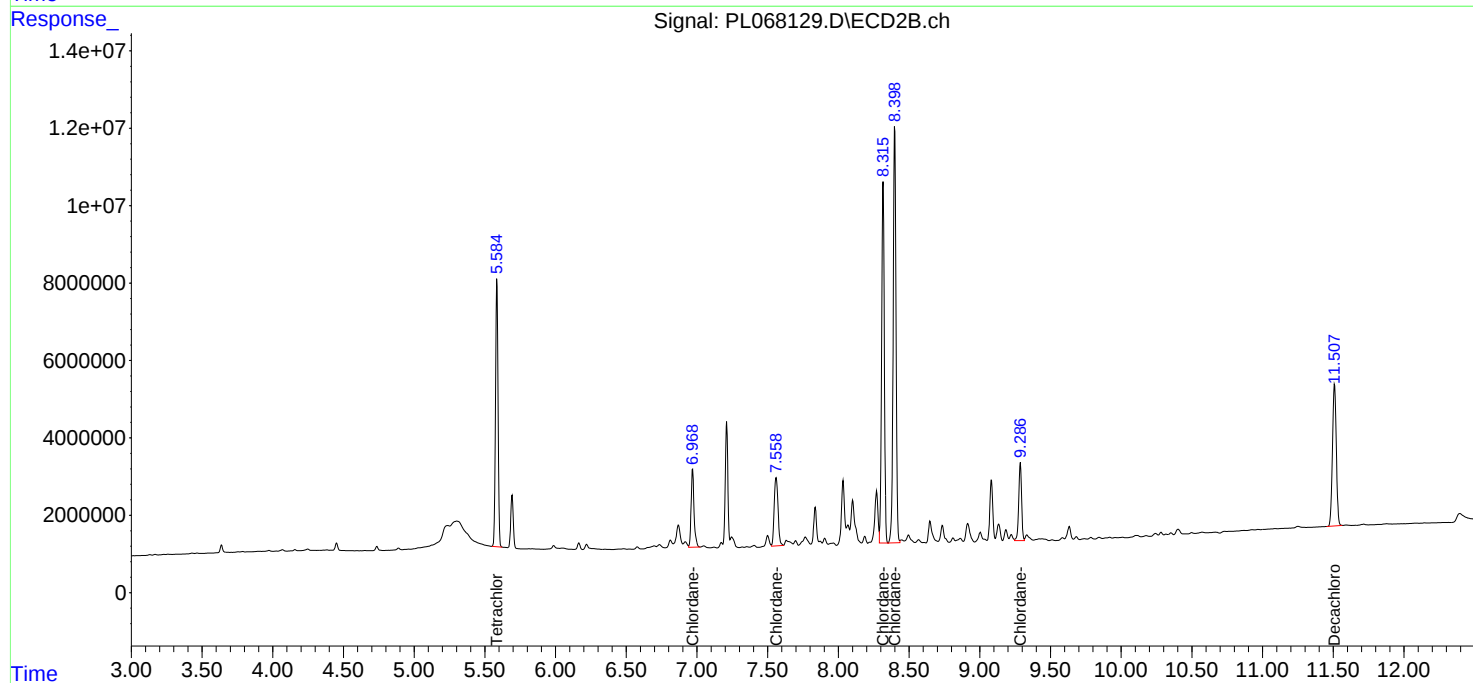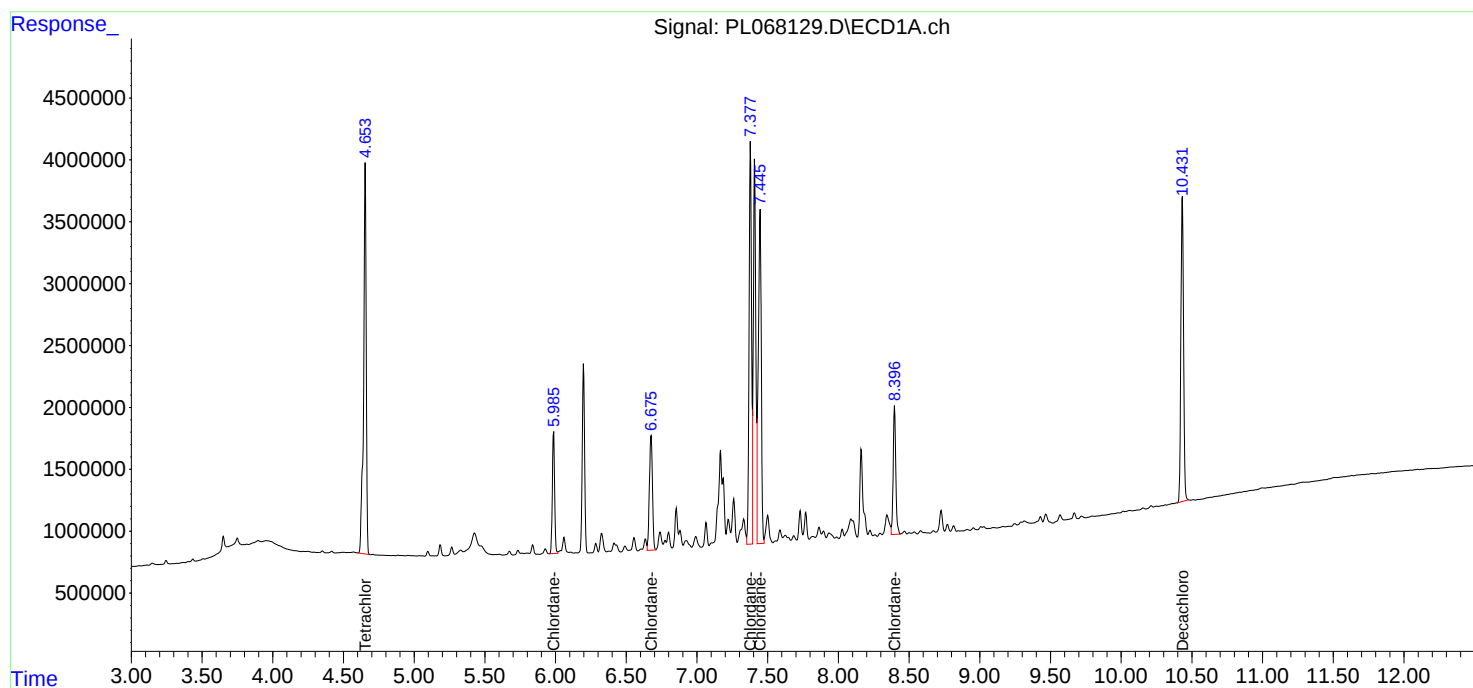


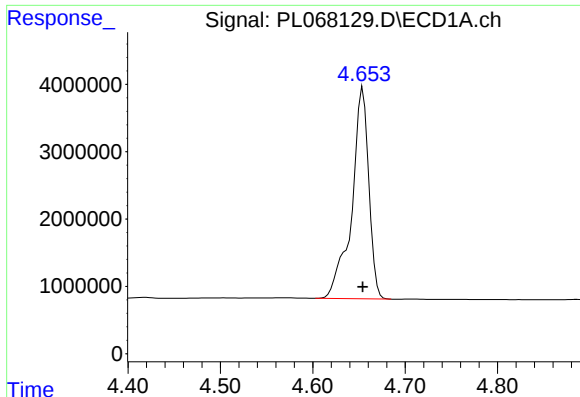

#1 Tetrachloro-m-xylene


R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 40218538
Conc: 74.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

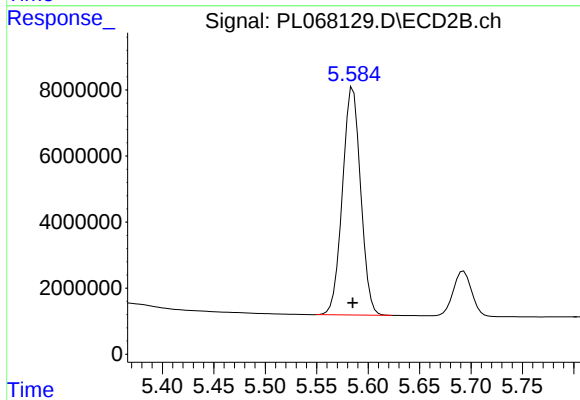


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 84906779
Conc: 75.55 ng/ml

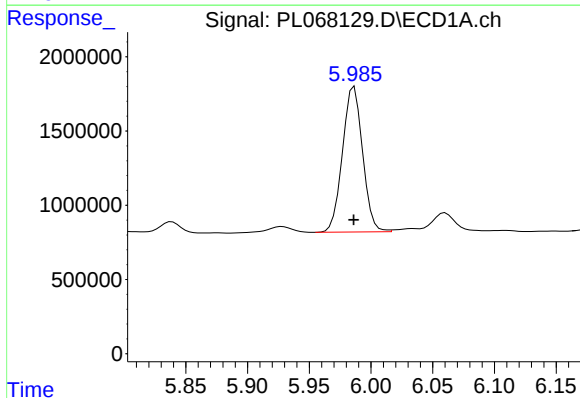


#23 Chlordane-1

R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 11094586
Conc: 751.33 ng/ml

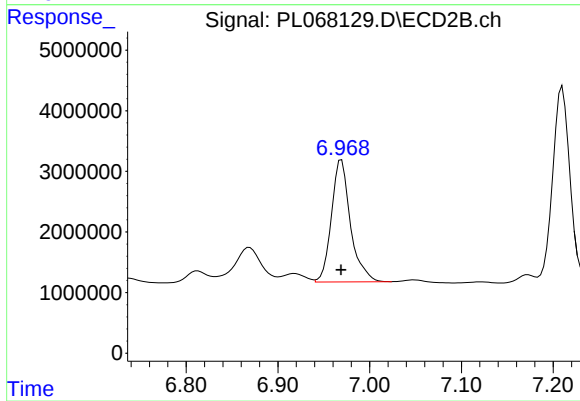

#23 Chlordane-1


R.T.: 6.969 min
Delta R.T.: 0.000 min
Response: 29064487
Conc: 750.94 ng/ml

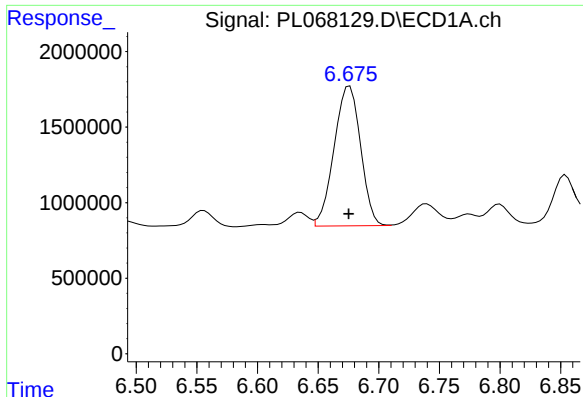

#24 Chlordane-2


R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 14023825
Conc: 739.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

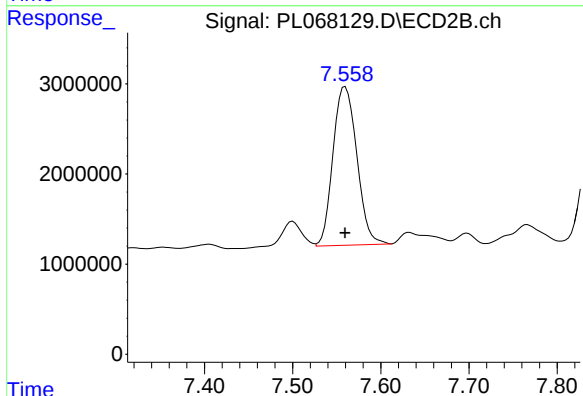


#24 Chlordane-2

R.T.: 7.560 min
Delta R.T.: 0.000 min
Response: 33149985
Conc: 737.64 ng/ml

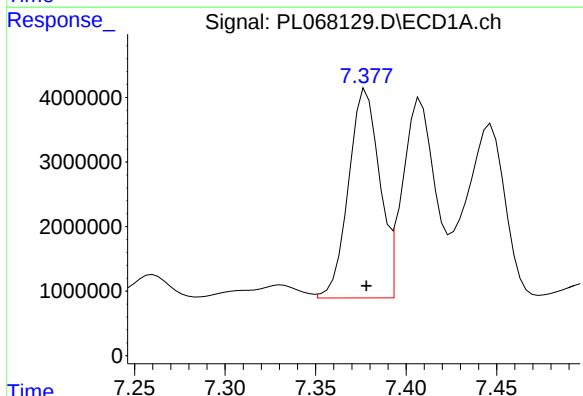


#25 Chlordane-3

R.T.: 7.378 min
Delta R.T.: 0.000 min
Response: 38459670
Conc: 760.97 ng/ml

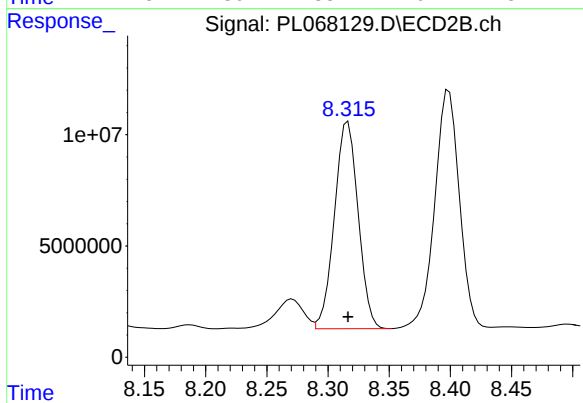

#25 Chlordane-3


R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 125435438
Conc: 775.90 ng/ml

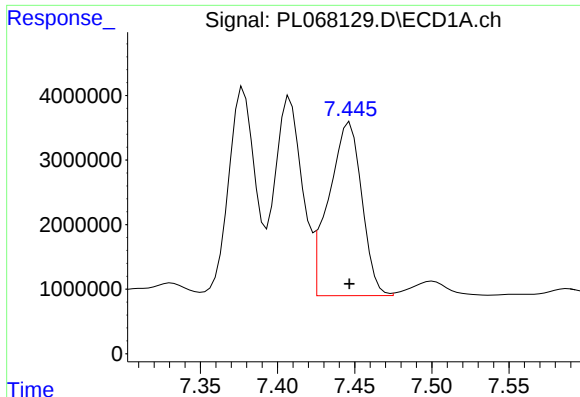

#26 Chlordane-4


R.T.: 7.447 min
Delta R.T.: 0.000 min
Response: 39912666
Conc: 748.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

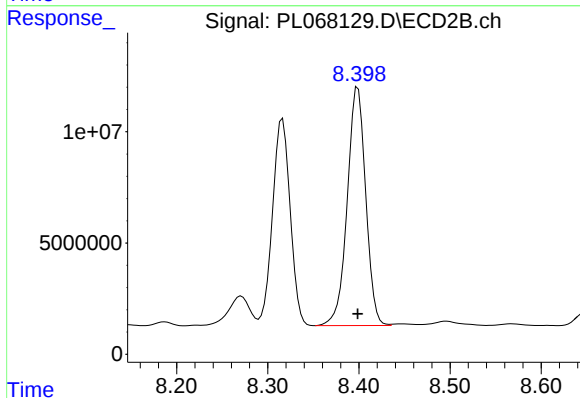


#26 Chlordane-4

R.T.: 8.399 min
Delta R.T.: 0.000 min
Response: 151045100
Conc: 765.93 ng/ml

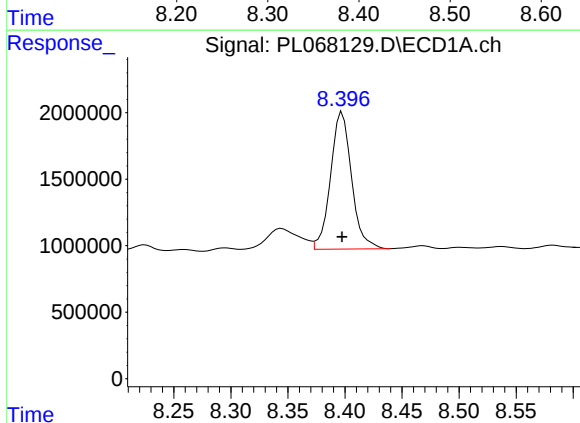


#27 Chlordane-5

R.T.: 8.398 min
Delta R.T.: 0.000 min
Response: 13228390
Conc: 745.18 ng/ml

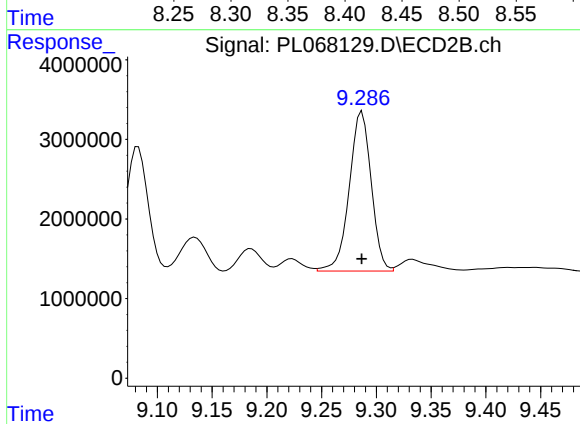

#27 Chlordane-5


R.T.: 9.287 min
Delta R.T.: 0.000 min
Response: 27997897
Conc: 763.49 ng/ml

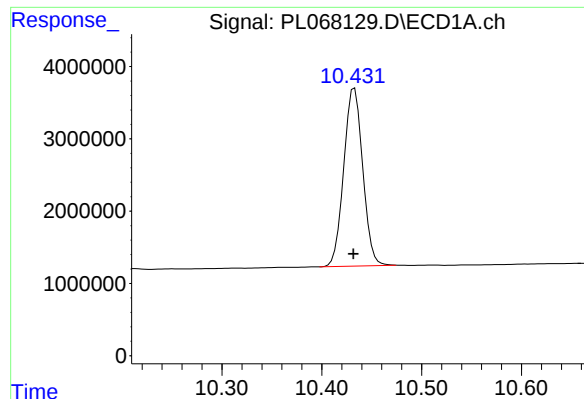

#28 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: 0.000 min
Response: 32571507
Conc: 78.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

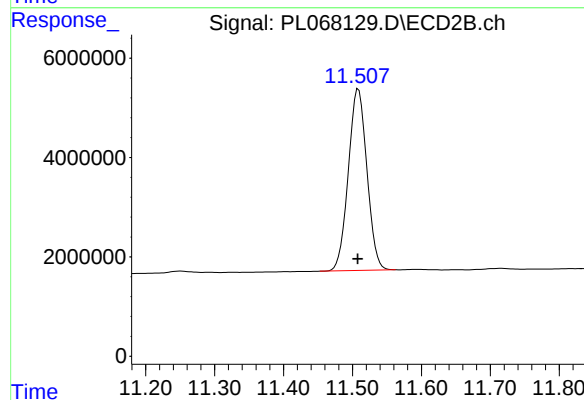

#28 Decachlorobiphenyl

R.T.: 11.509 min
Delta R.T.: 0.000 min
Response: 68549780
Conc: 73.12 ng/ml