

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2021 20:11
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 03:48:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 03:47:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.585	26917158	56190167	50.000	50.000
28)	SA Decachlor...	10.432	11.508	20865462	46877649	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.986	6.969	7383320	19352129	500.000	500.000
24)	Chlordane-2	6.675	7.559	9476367	22470294	500.000	500.000
25)	Chlordane-3	7.378	8.316	25270164	80832714	500.000	500.000
26)	Chlordane-4	7.447	8.399	26666483	98602721	500.000	500.000
27)	Chlordane-5	8.398	9.287	8875986	18335477	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2021 20:11
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 03:48:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 03:47:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

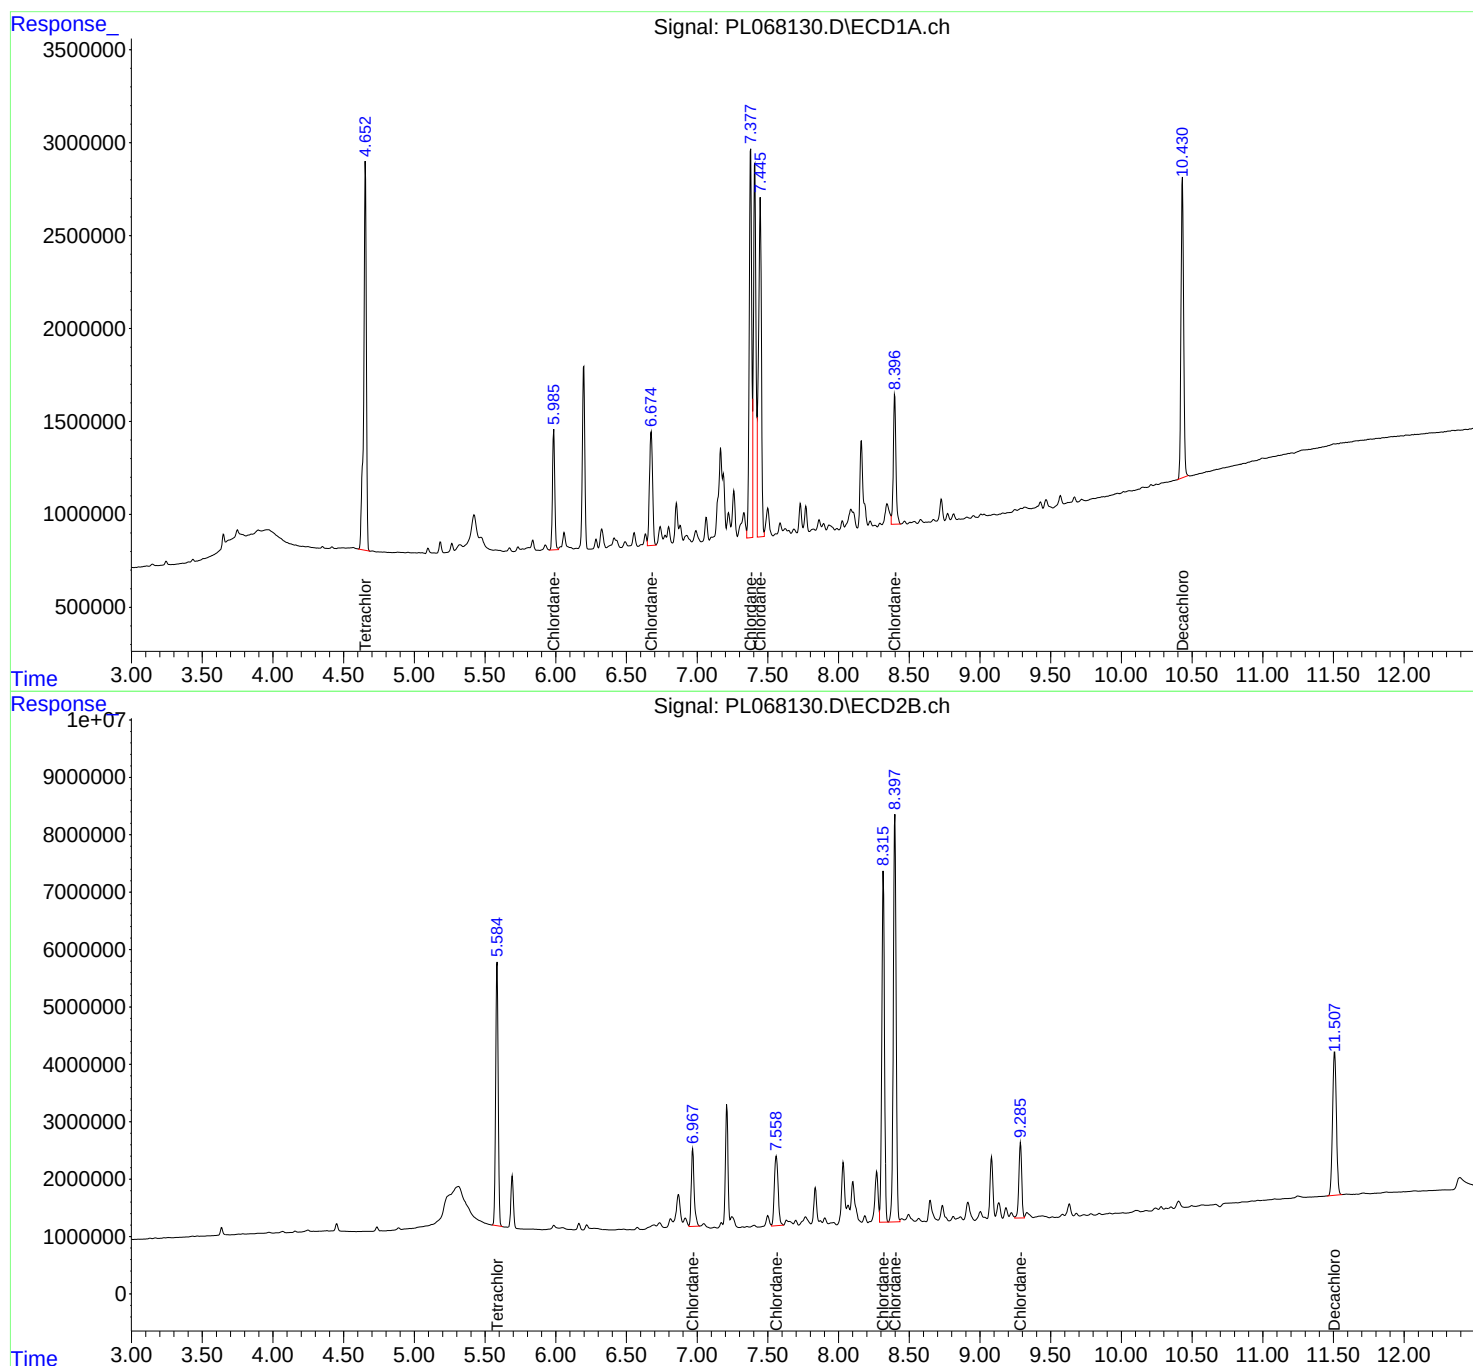


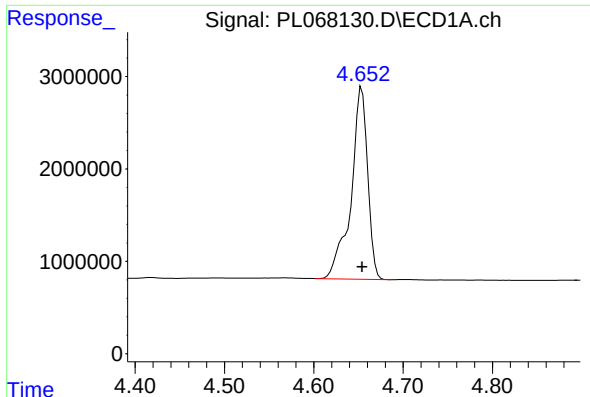

#1 Tetrachloro-m-xylene


R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 26917158
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

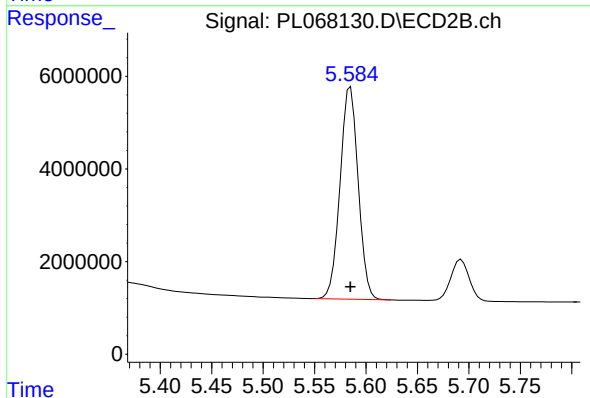


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 56190167
Conc: 50.00 ng/ml

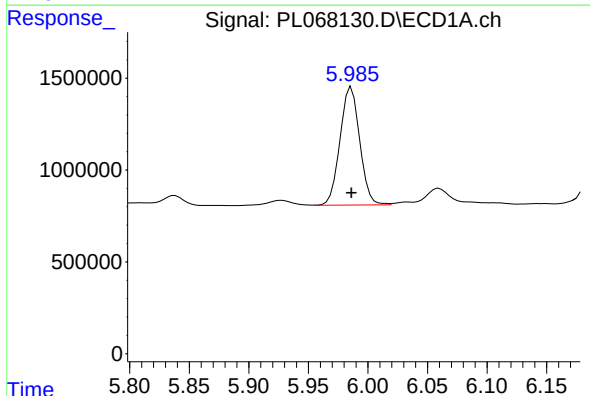


#23 Chlordane-1

R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 7383320
Conc: 500.00 ng/ml

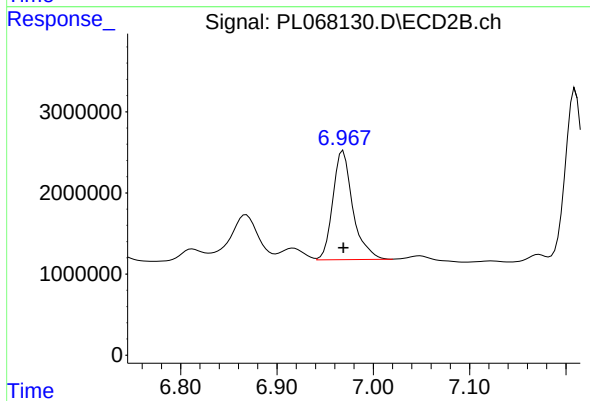

#23 Chlordane-1


R.T.: 6.969 min
Delta R.T.: 0.000 min
Response: 19352129
Conc: 500.00 ng/ml

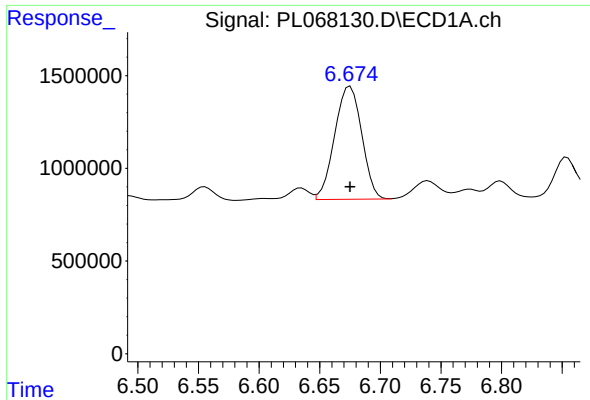

#24 Chlordane-2


R.T.: 6.675 min
Delta R.T.: 0.000 min
Response: 9476367
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

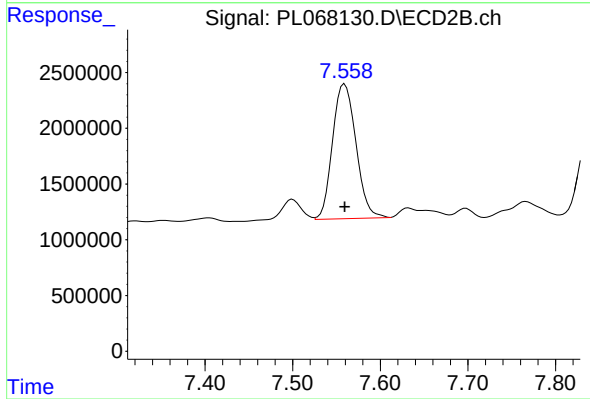


#24 Chlordane-2

R.T.: 7.559 min
Delta R.T.: 0.000 min
Response: 22470294
Conc: 500.00 ng/ml

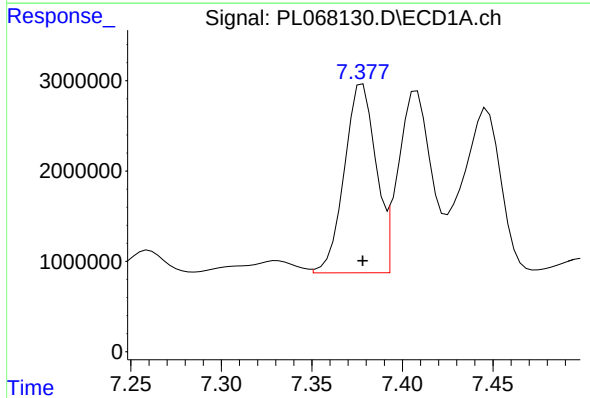


#25 Chlordane-3

R.T.: 7.378 min
Delta R.T.: 0.000 min
Response: 25270164
Conc: 500.00 ng/ml

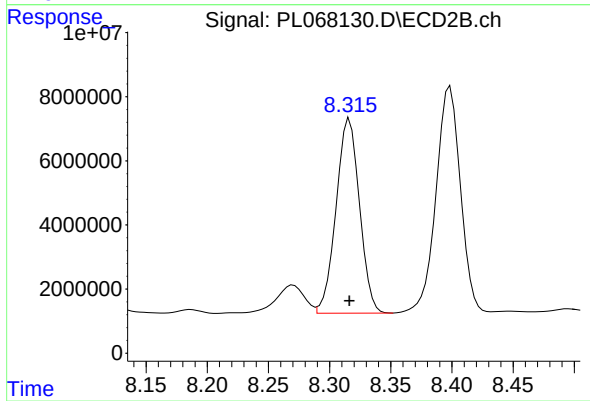

#25 Chlordane-3


R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 80832714
Conc: 500.00 ng/ml

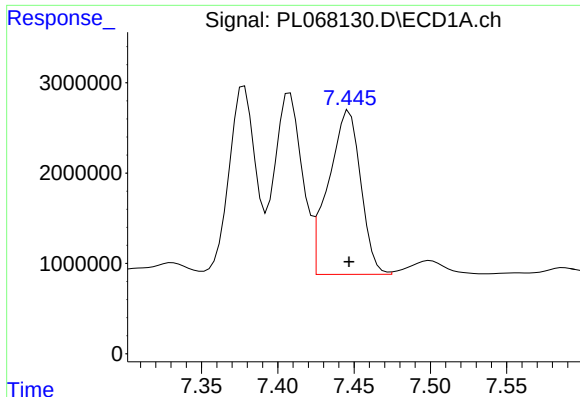

#26 Chlordane-4


R.T.: 7.447 min
Delta R.T.: 0.000 min
Response: 26666483
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

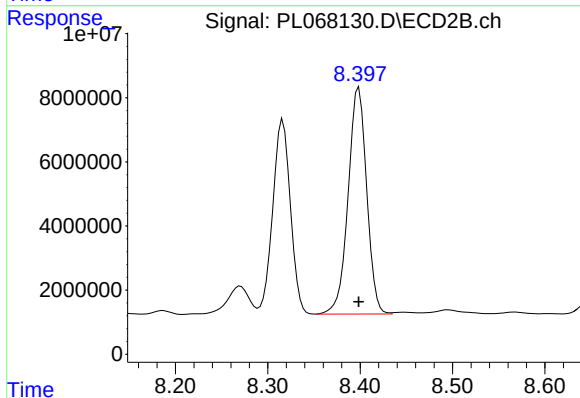


#26 Chlordane-4

R.T.: 8.399 min
Delta R.T.: 0.000 min
Response: 98602721
Conc: 500.00 ng/ml

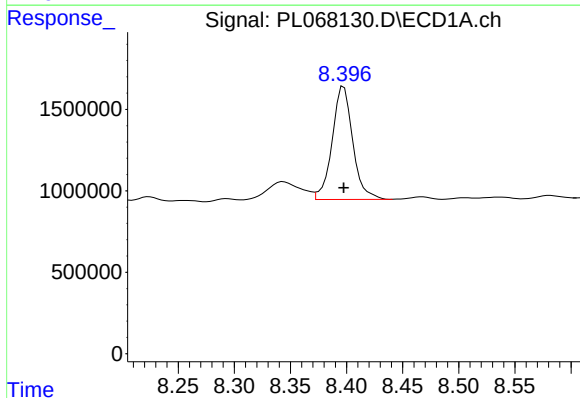


#27 Chlordane-5

R.T.: 8.398 min
Delta R.T.: 0.000 min
Response: 8875986
Conc: 500.00 ng/ml

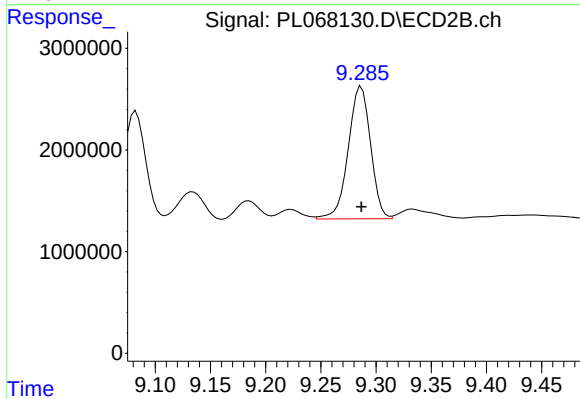

#27 Chlordane-5


R.T.: 9.287 min
Delta R.T.: 0.000 min
Response: 18335477
Conc: 500.00 ng/ml

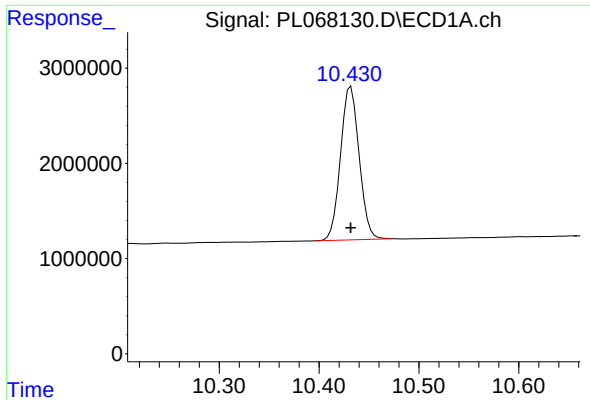

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 20865462
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

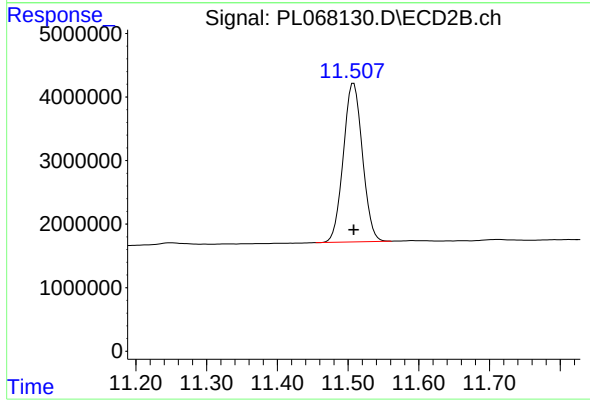

#28 Decachlorobiphenyl

R.T.: 11.508 min
Delta R.T.: 0.000 min
Response: 46877649
Conc: 50.00 ng/ml