

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2021 20:27
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 03:48:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 03:47:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.585	13430861	27705519	24.949	24.653
28)	SA Decachlor...	10.432	11.509	10495282	24002848	25.150	25.602
Target Compounds							
23)	Chlordane-1	5.987	6.969	3735399	9249969	252.962	238.991
24)	Chlordane-2	6.676	7.559	4981105	11477781	262.817	255.399
25)	Chlordane-3	7.378	8.316	12481424	38934157	246.960	240.832
26)	Chlordane-4	7.447	8.399	13033373	48000864	244.377	243.405
27)	Chlordane-5	8.398	9.287	4380345	9016492	246.753	245.876



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2021 20:27
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 03:48:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 03:47:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

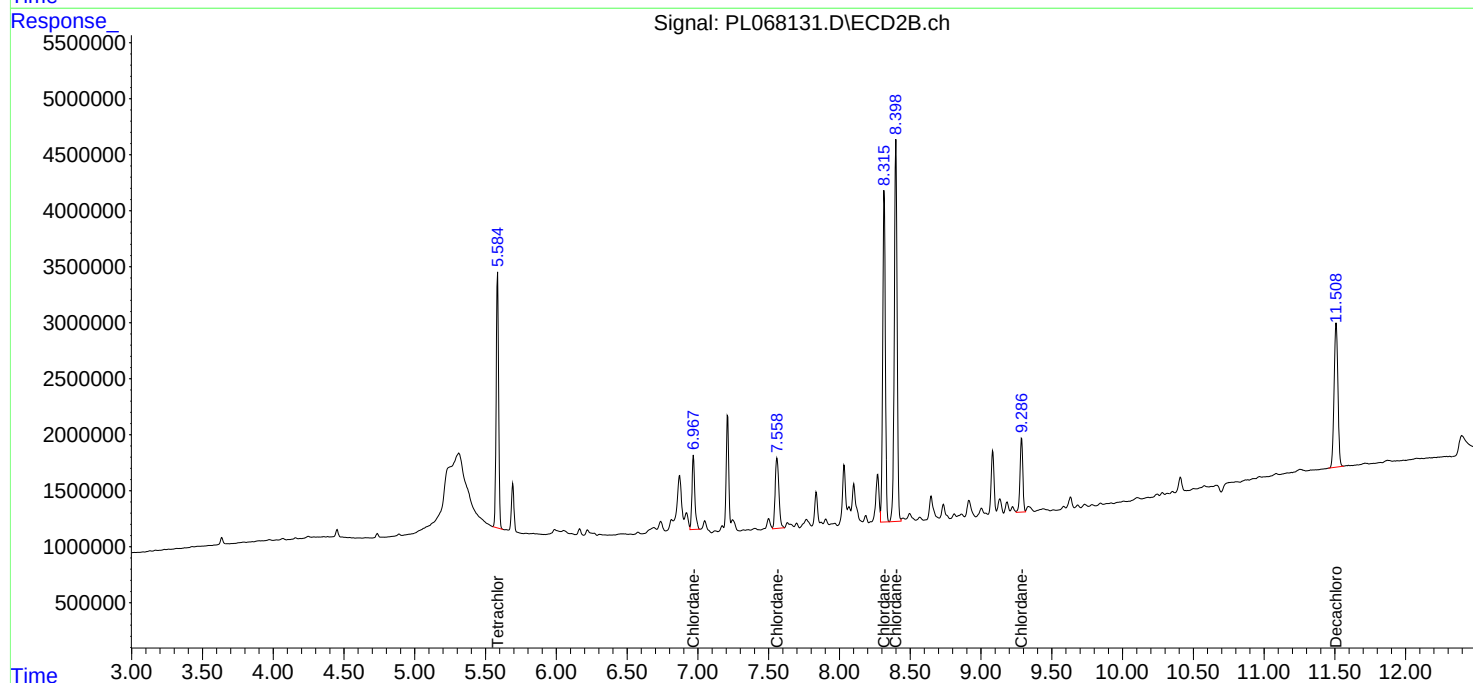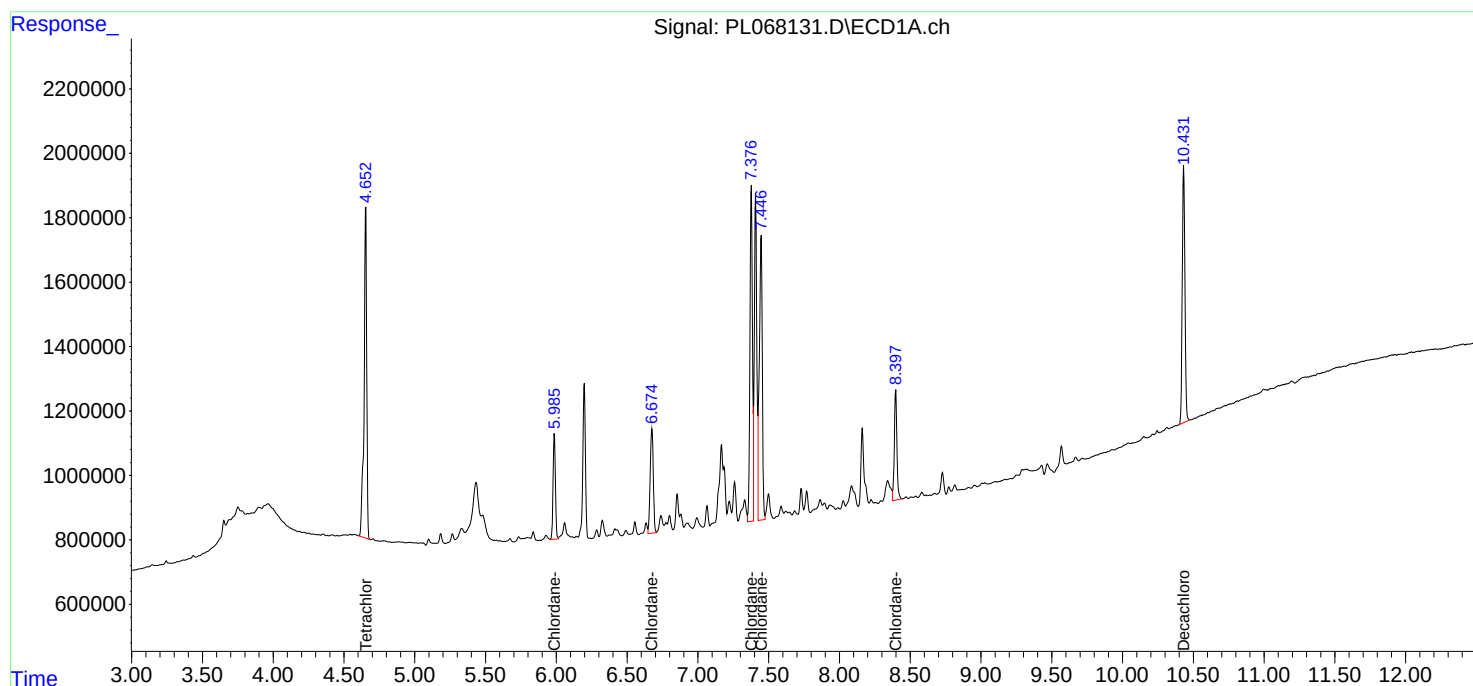


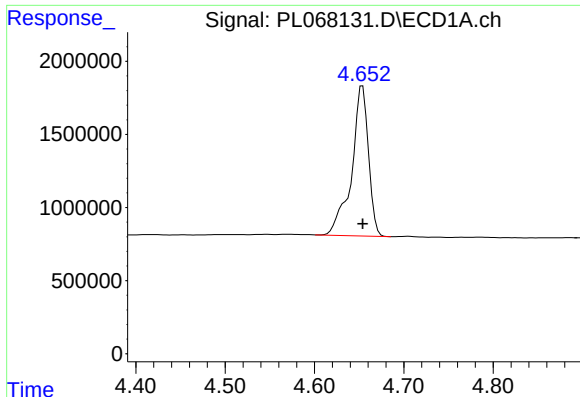

#1 Tetrachloro-m-xylene


R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 13430861
Conc: 24.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

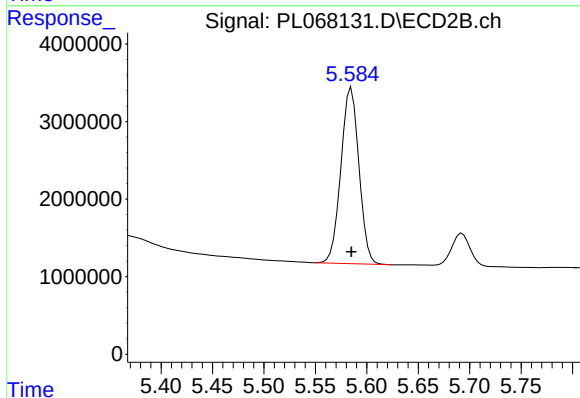


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 27705519
Conc: 24.65 ng/ml

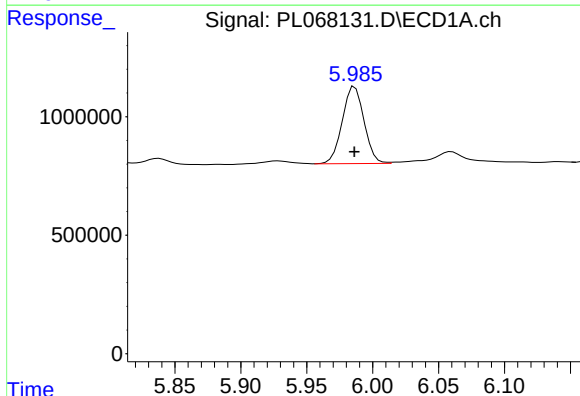


#23 Chlordane-1

R.T.: 5.987 min
Delta R.T.: 0.000 min
Response: 3735399
Conc: 252.96 ng/ml

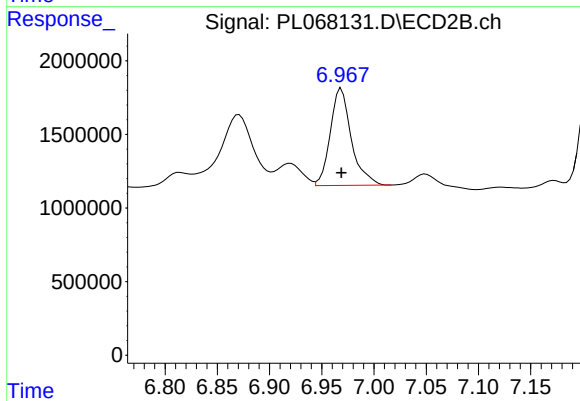

#23 Chlordane-1


R.T.: 6.969 min
Delta R.T.: 0.000 min
Response: 9249969
Conc: 238.99 ng/ml

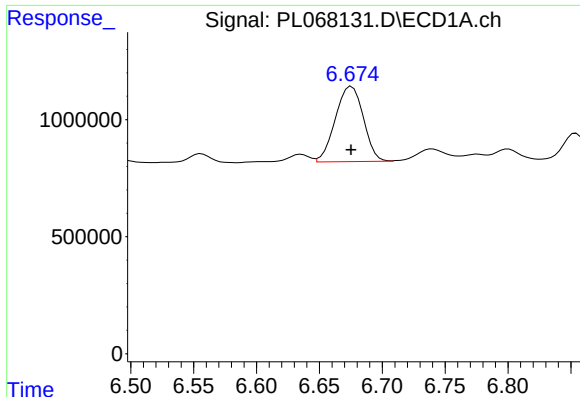

#24 Chlordane-2


R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 4981105
Conc: 262.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

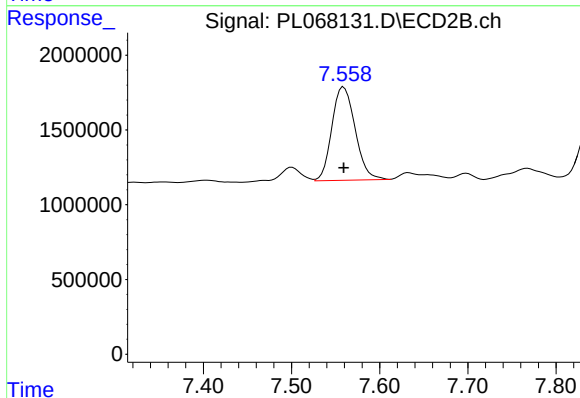


#24 Chlordane-2

R.T.: 7.559 min
Delta R.T.: 0.000 min
Response: 11477781
Conc: 255.40 ng/ml

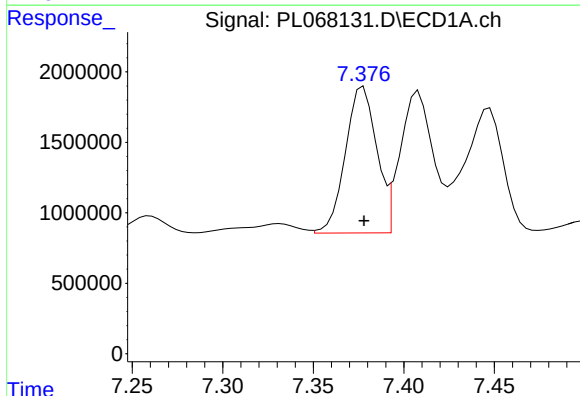


#25 Chlordane-3

R.T.: 7.378 min
Delta R.T.: 0.000 min
Response: 12481424
Conc: 246.96 ng/ml

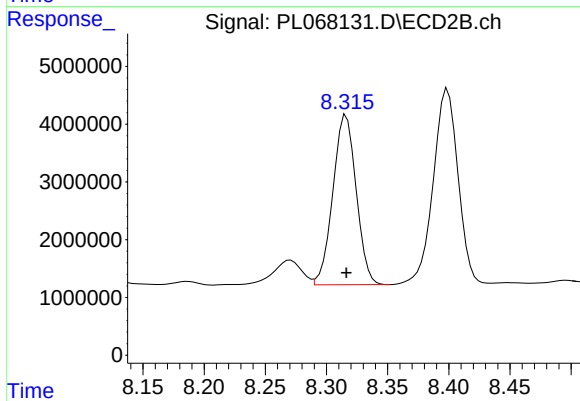

#25 Chlordane-3


R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 38934157
Conc: 240.83 ng/ml

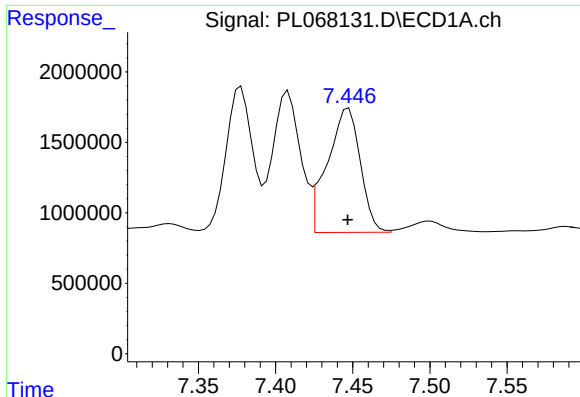

#26 Chlordane-4


R.T.: 7.447 min
Delta R.T.: 0.000 min
Response: 13033373
Conc: 244.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

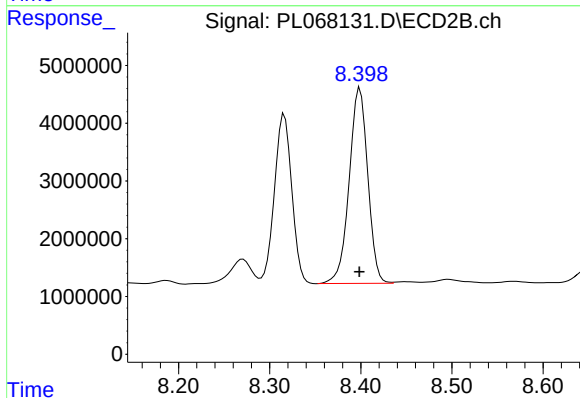


#26 Chlordane-4

R.T.: 8.399 min
Delta R.T.: 0.000 min
Response: 48000864
Conc: 243.41 ng/ml

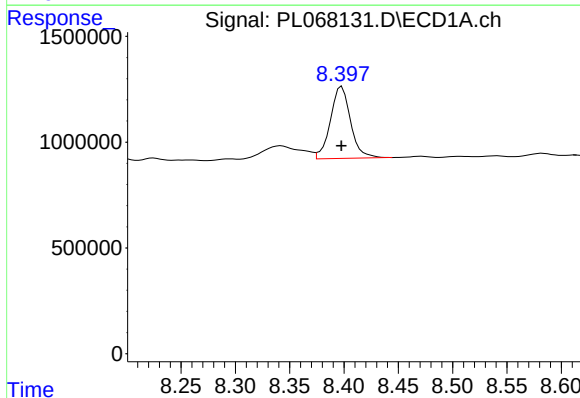


#27 Chlordane-5

R.T.: 8.398 min
Delta R.T.: 0.000 min
Response: 4380345
Conc: 246.75 ng/ml

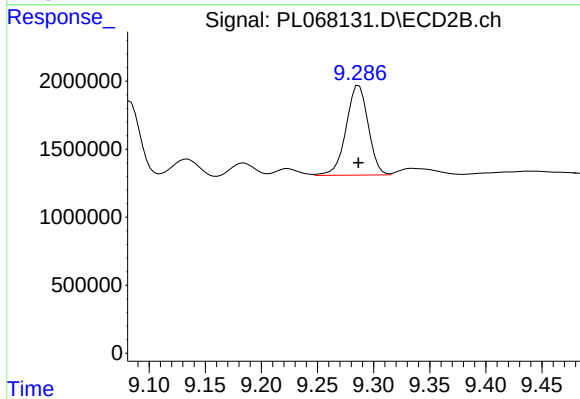

#27 Chlordane-5


R.T.: 9.287 min
Delta R.T.: 0.000 min
Response: 9016492
Conc: 245.88 ng/ml

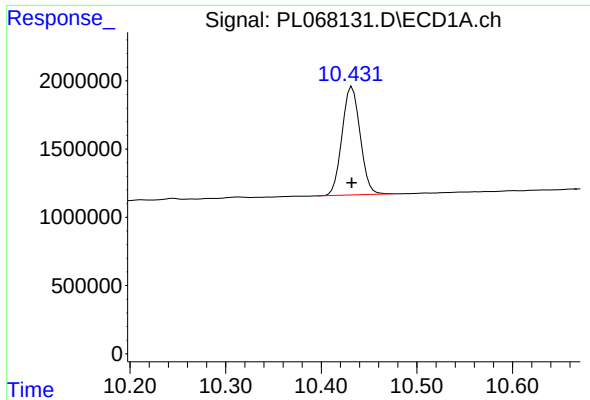

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 10495282
Conc: 25.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

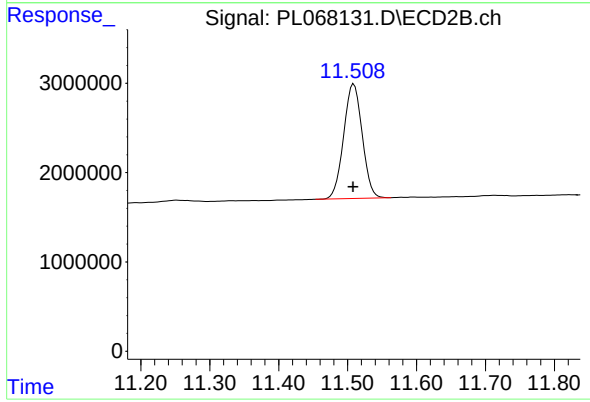

#28 Decachlorobiphenyl

R.T.: 11.509 min
Delta R.T.: 0.001 min
Response: 24002848
Conc: 25.60 ng/ml