

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 01:09
 Operator : AR\AJ
 Sample : M3012-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PS-TP1

Manual Integrations
 APPROVED

Ankita
 7/15/2021 12:06:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 04:49:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.653	5.585	8804278	20924421	21.841m	20.290
28)	SA Decachlor...	10.433	11.510	8762082	18864970	21.233	20.968

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 01:09
Operator : AR\AJ
Sample : M3012-02
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampled :
PS-TP1


Manual Integrations
APPROVED

Ankita
7/15/2021 12:06:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 04:49:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

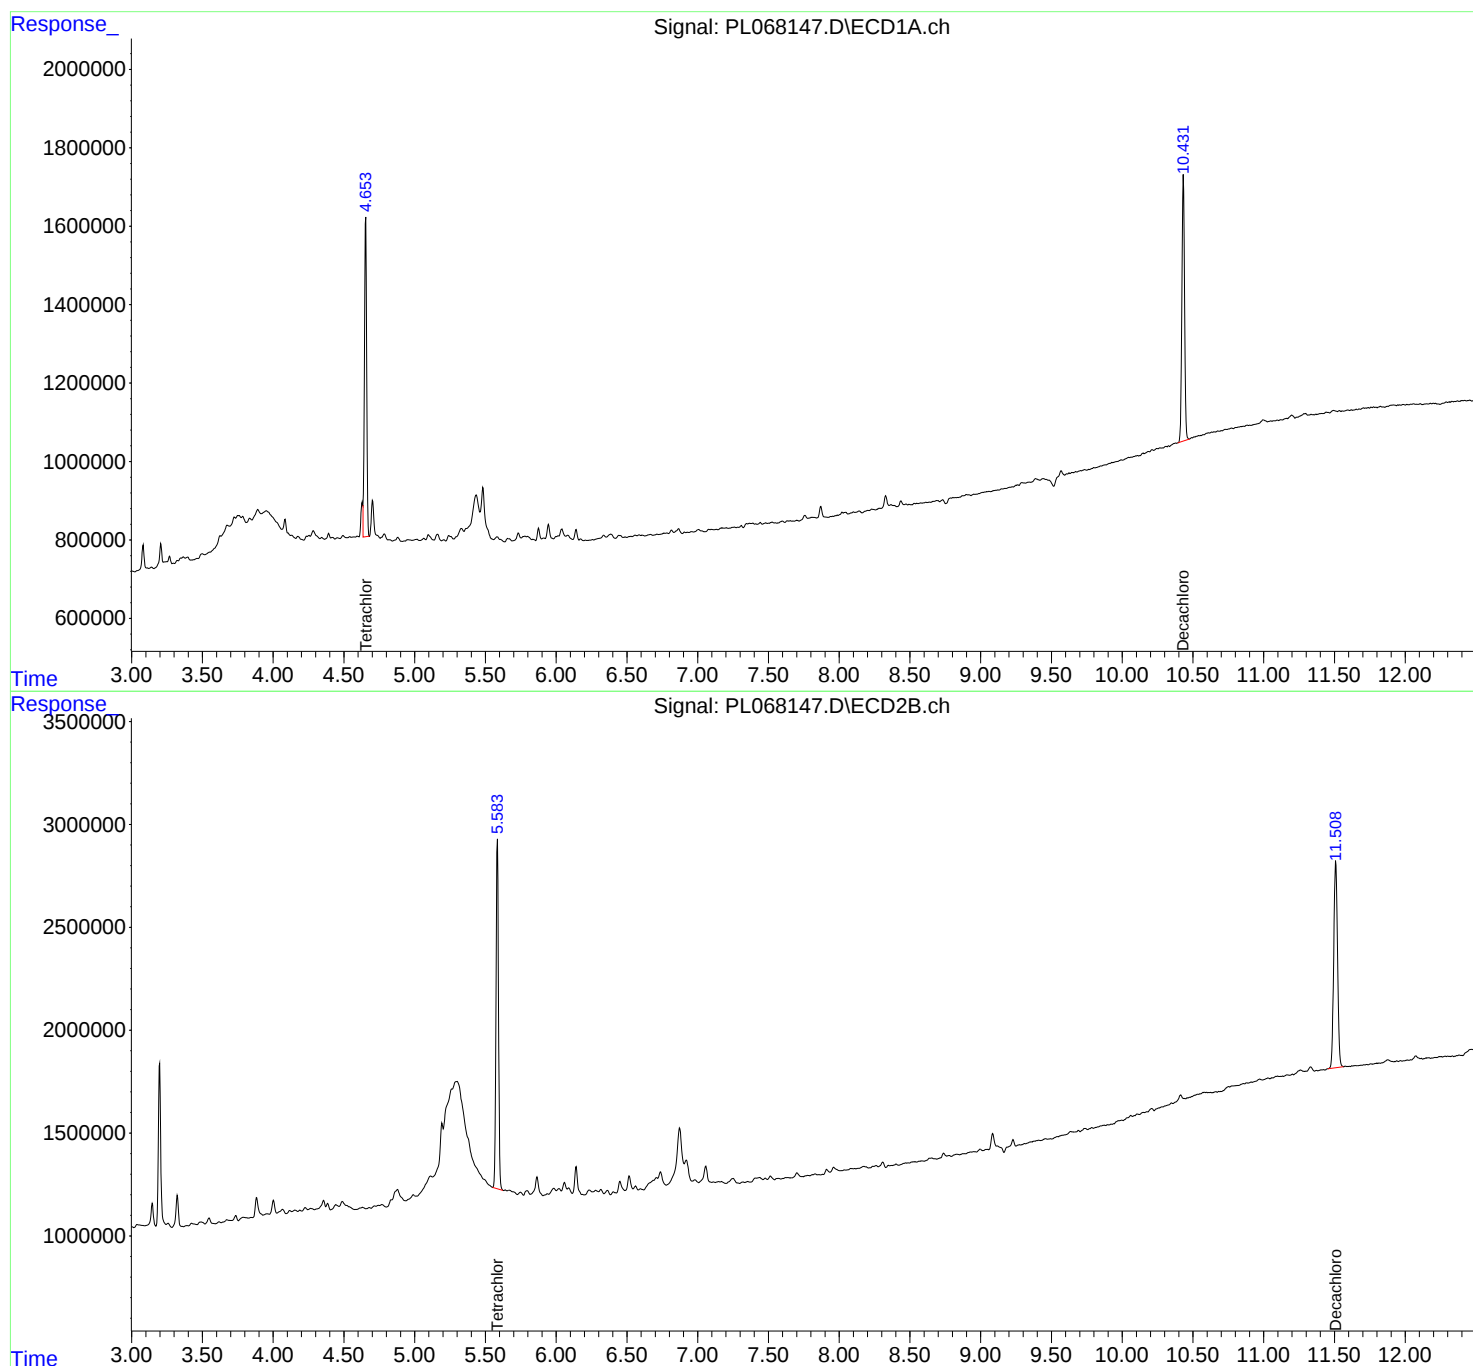

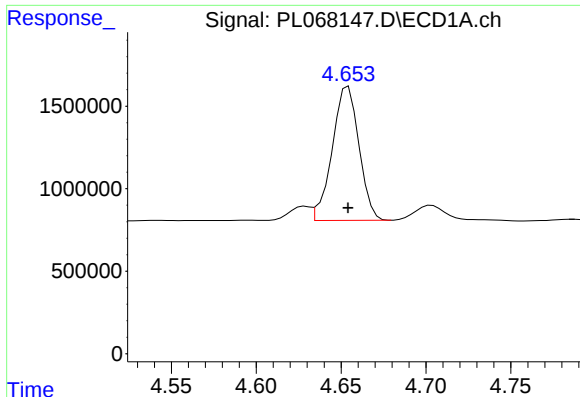


#1 Tetrachloro-m-xylene

R.T.: 4.653 min
Delta R.T.: -0.001 min
Response: 8804278
Conc: 21.84 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PS-TP1


Manual Integrations
APPROVED

Ankita
7/15/2021 12:06:21 PM

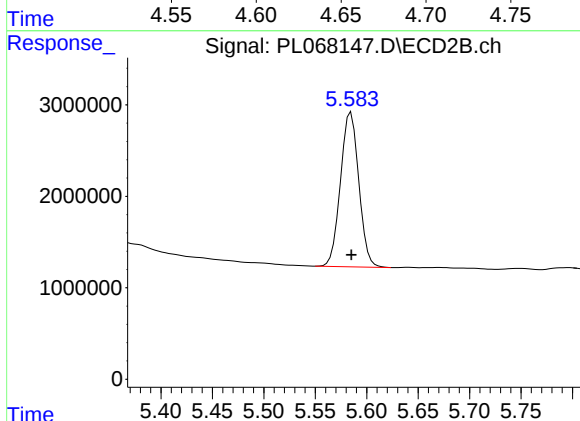


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 20924421
Conc: 20.29 ng/ml

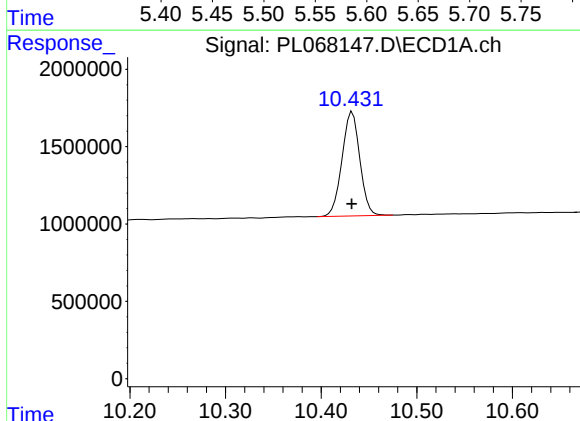

#28 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: 0.000 min
Response: 8762082
Conc: 21.23 ng/ml

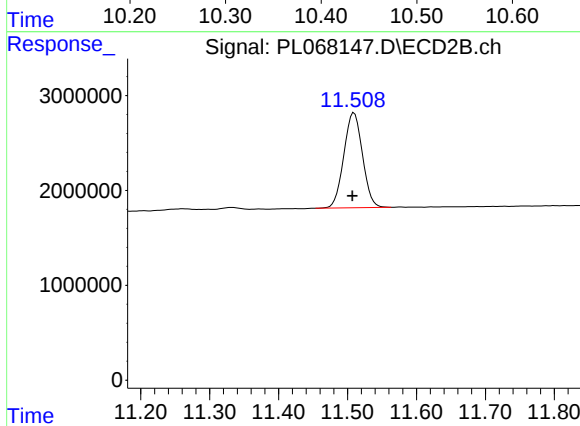

#28 Decachlorobiphenyl

R.T.: 11.510 min
Delta R.T.: 0.002 min
Response: 18864970
Conc: 20.97 ng/ml