

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 05:35
 Operator : AR\AJ
 Sample : M3023-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-071321

Manual Integrations
 APPROVED

Ankita
 7/15/2021 12:06:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 07:28:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.586	4319069	9462818	10.714	9.176
28)	SA Decachlor...	10.432	11.510	4735772	9631017	11.476	10.705
Target Compounds							
11)	B alpha-Chl...	7.444	8.399	287141	718661	0.600m	0.645
12)	B 4,4'-DDE	7.660	8.579	232954	521079	0.539m	0.513

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 05:35
Operator : AR\AJ
Sample : M3023-01
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-02-071321


Manual Integrations
APPROVED

Ankita
7/15/2021 12:06:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 07:28:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

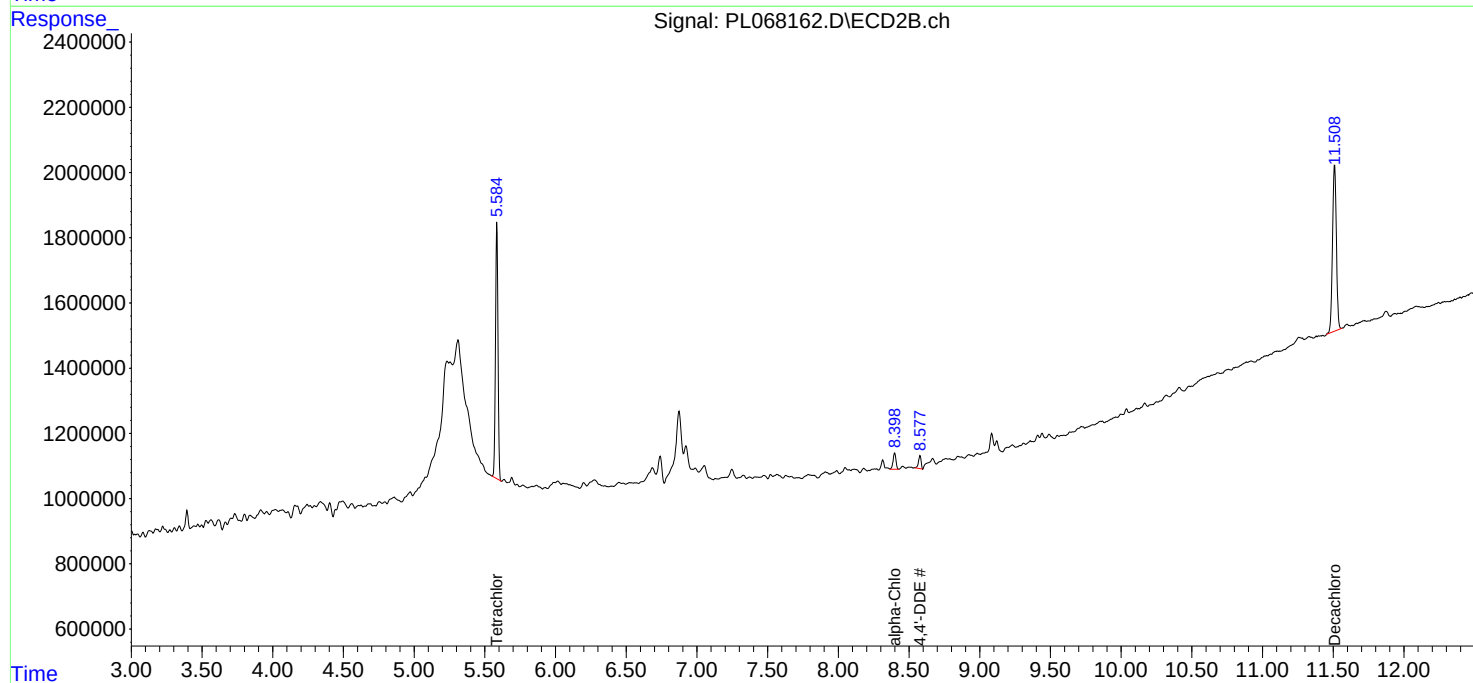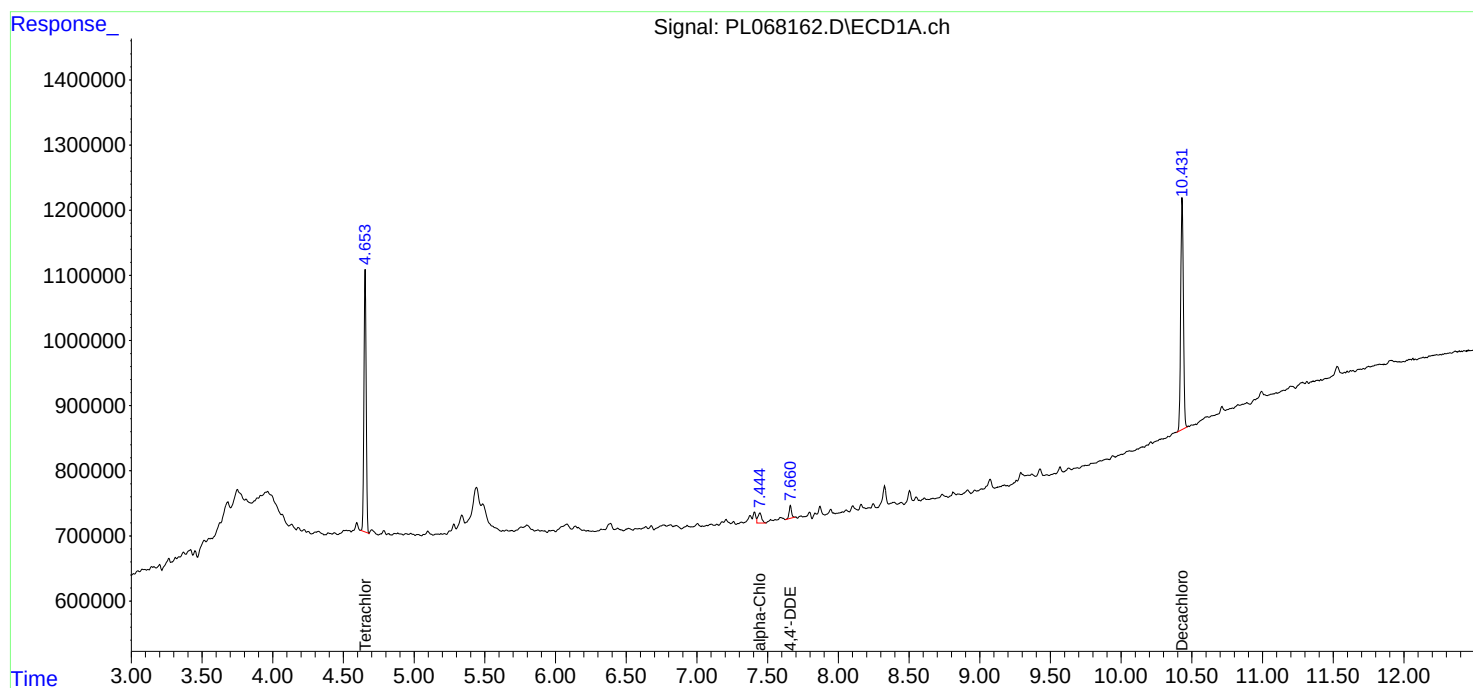

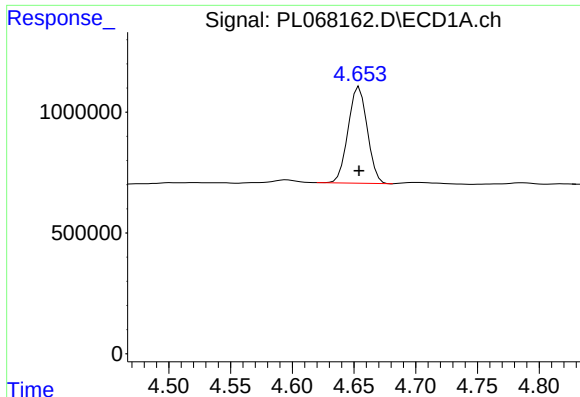


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 4319069
Conc: 10.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-071321


Manual Integrations
APPROVED

Ankita
7/15/2021 12:06:26 PM

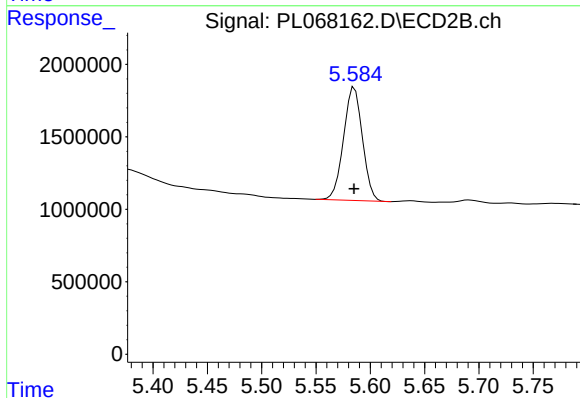


#1 Tetrachloro-m-xylene

R.T.: 5.586 min
Delta R.T.: 0.000 min
Response: 9462818
Conc: 9.18 ng/ml

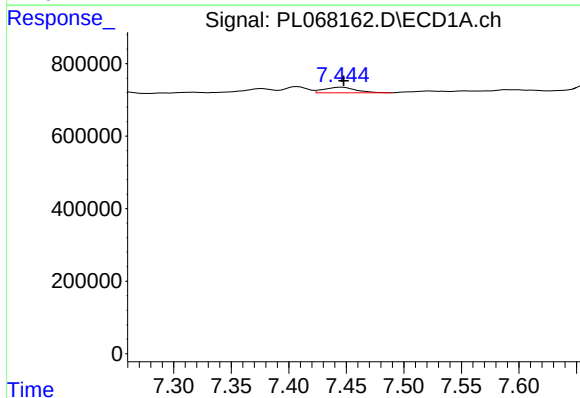


#11 alpha-Chlordane

R.T.: 7.444 min
Delta R.T.: -0.003 min
Response: 287141
Conc: 0.60 ng/ml m

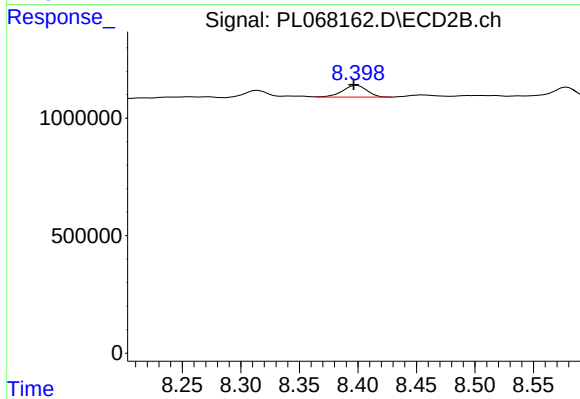

#11 alpha-Chlordane

R.T.: 8.399 min
Delta R.T.: 0.003 min
Response: 718661
Conc: 0.64 ng/ml

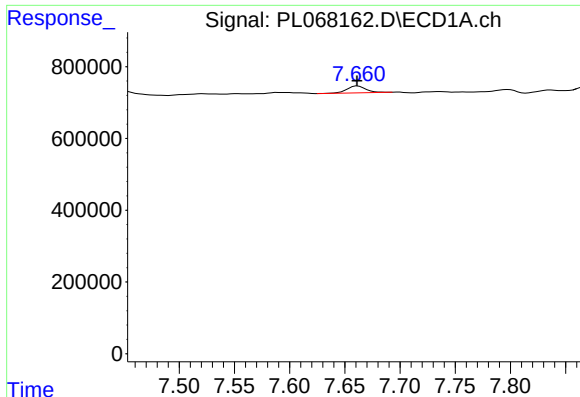


#12 4,4'-DDE

R.T.: 7.660 min
Delta R.T.: 0.000 min
Response: 232954
Conc: 0.54 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OR-02-071321


Manual Integrations
APPROVED

Ankita
7/15/2021 12:06:26 PM

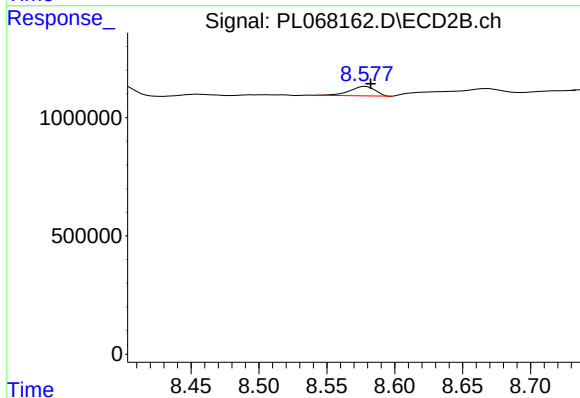


#12 4,4'-DDE

R.T.: 8.579 min
Delta R.T.: -0.004 min
Response: 521079
Conc: 0.51 ng/ml

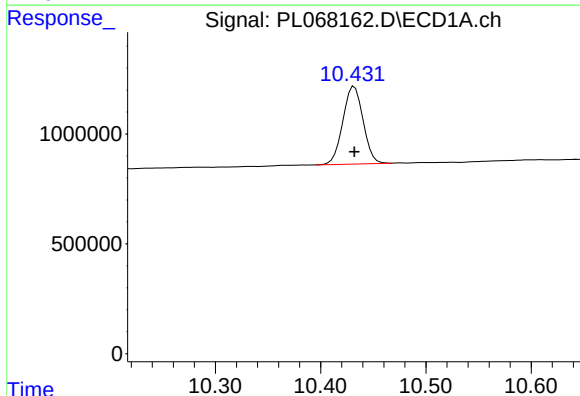

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 4735772
Conc: 11.48 ng/ml

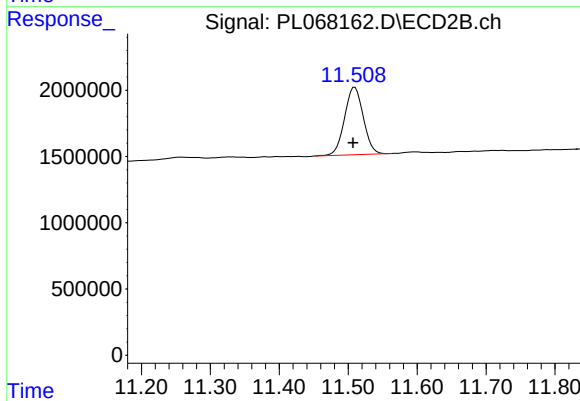

#28 Decachlorobiphenyl

R.T.: 11.510 min
Delta R.T.: 0.003 min
Response: 9631017
Conc: 10.70 ng/ml