

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071523\
 Data File : PL083929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 01:54
 Operator : AR\AJ
 Sample : TOXAPH401
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 03:05:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 03:04:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.688	96335367	49693248	38.908	39.688
27)	SA Decachlor...	9.021	7.870	112.0E6	109.6E6	74.351	78.457
Target Compounds							
22)	Toxaphene-1	6.187	5.257	65296992	25621647	3856.280	4050.486
23)	Toxaphene-2	7.010	5.618	213.3E6	29414900	4013.958	4138.969
24)	Toxaphene-3	7.101	6.663	153.2E6	160.9E6	4009.550	4137.958
25)	Toxaphene-4	7.200	6.979	87791323	102.8E6	3920.396	4163.950
26)	Toxaphene-5	7.888	7.113	103.0E6	62680376	3964.397	4178.905

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071523\
Data File : PL083929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 01:54
Operator : AR\AJ
Sample : TOXAPH401
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 03:05:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 03:04:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

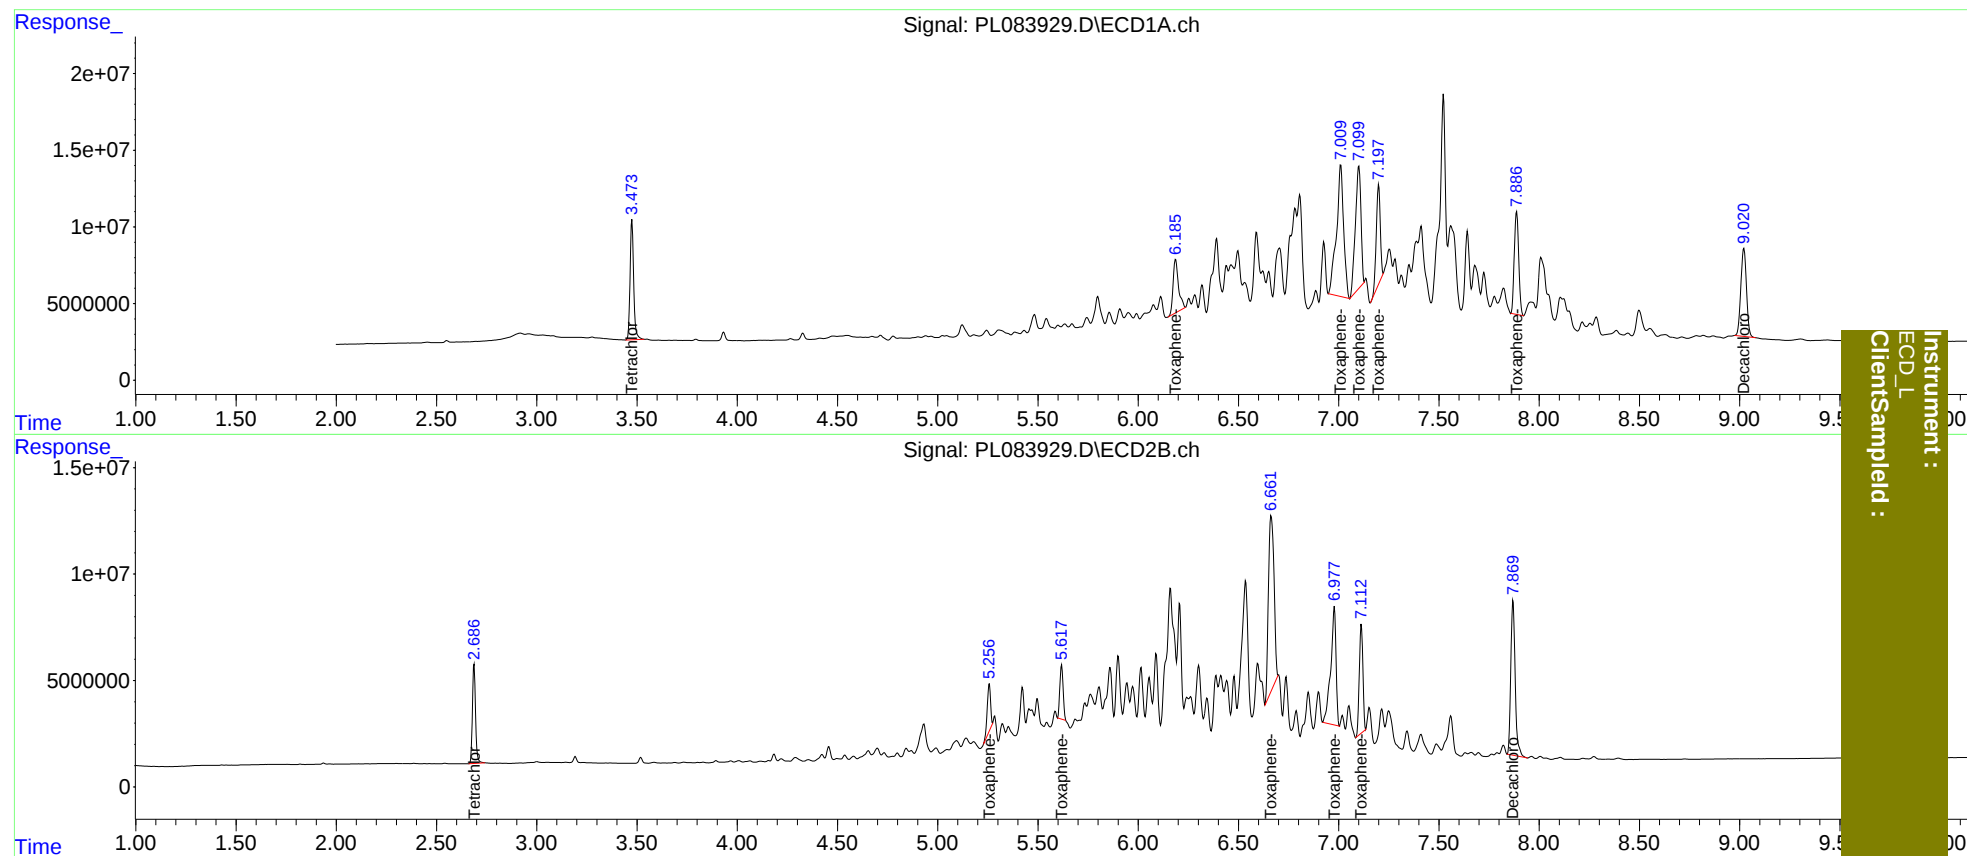

Instrument :
ECD_L
ClientSampled :
PL083929.D