

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071524\
 Data File : PL090516.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2024 10:46
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 11:52:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 15 11:49:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.790	197.9E6	202.9E6	99.970	102.914
28)	SA Decachlor...	9.064	7.936	119.4E6	138.7E6	98.570	99.405
Target Compounds							
23)	Chlordane-1	4.710	3.791	85124711	63031431	990.084	1023.463
24)	Chlordane-2	5.240	4.369	93152167	72977513	966.010	999.759
25)	Chlordane-3	5.950	4.999	315.2E6	218.6E6	1000.706	1033.547
26)	Chlordane-4	6.032	5.062	378.8E6	204.1E6	996.575	1029.197
27)	Chlordane-5	6.880	5.729	65556531	58354609	986.652	1009.115



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071524\
Data File : PL090516.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2024 10:46
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 11:52:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 11:49:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

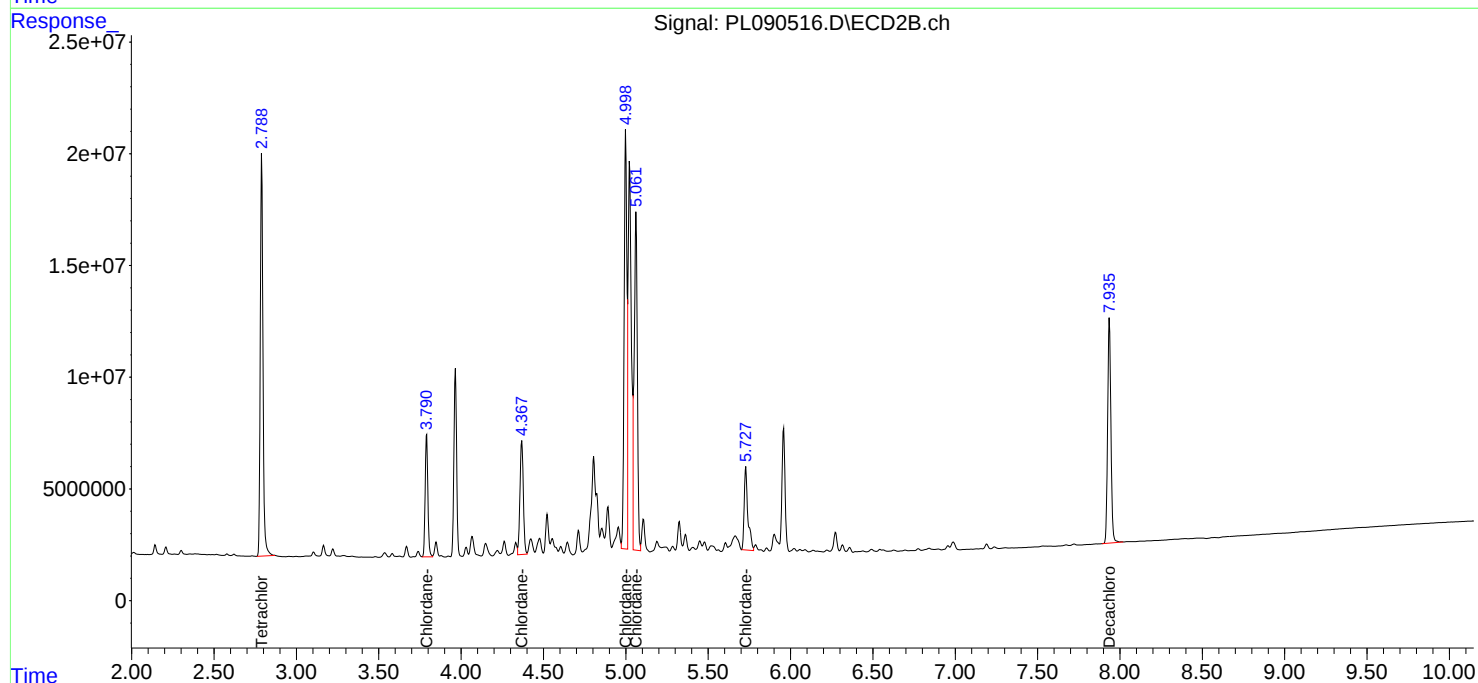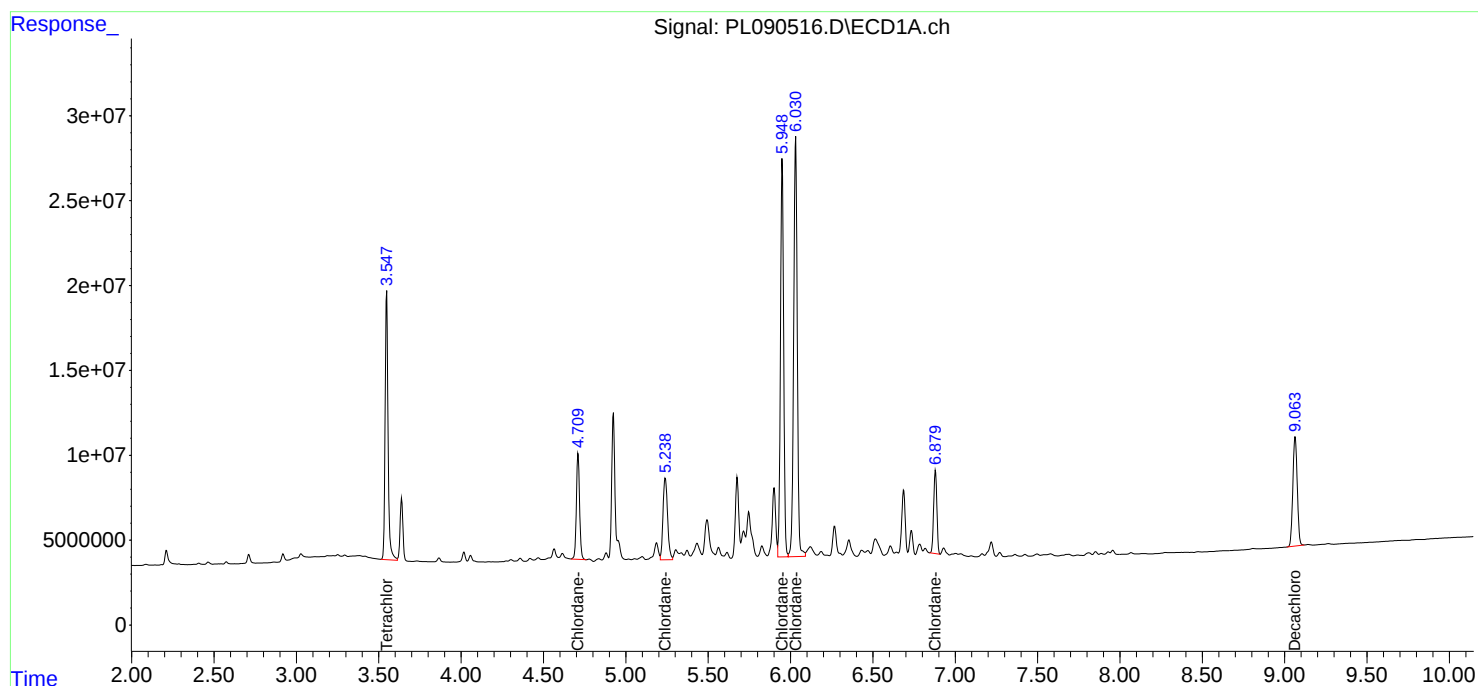


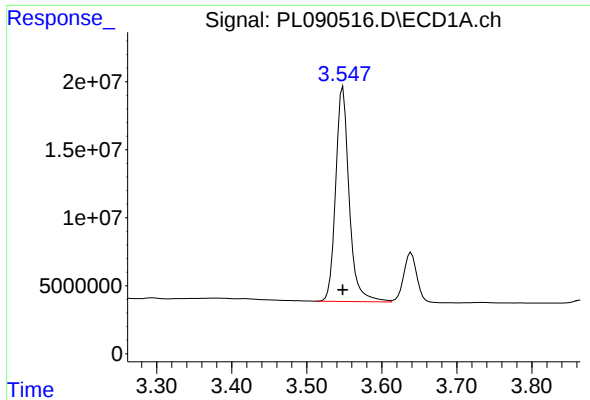

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 197889697
Conc: 99.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

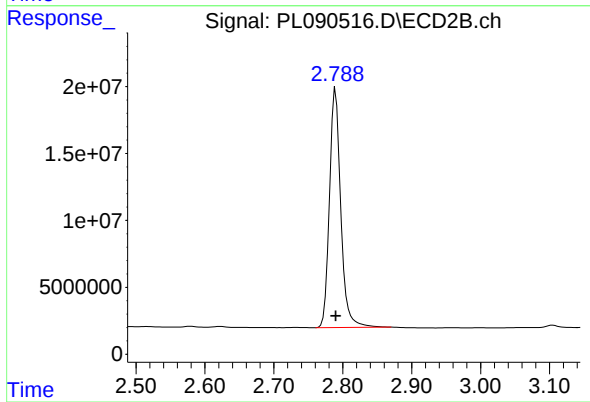


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.000 min
Response: 202918854
Conc: 102.91 ng/ml

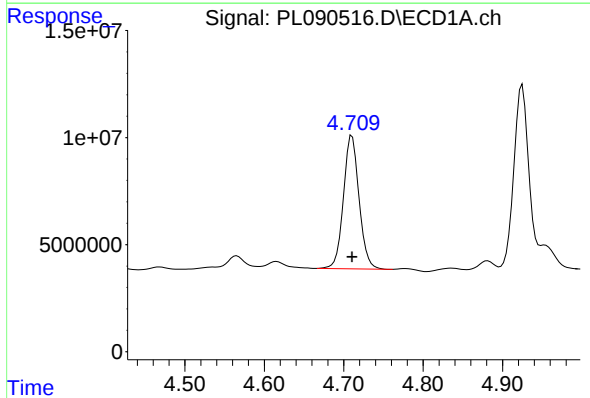


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 85124711
Conc: 990.08 ng/ml

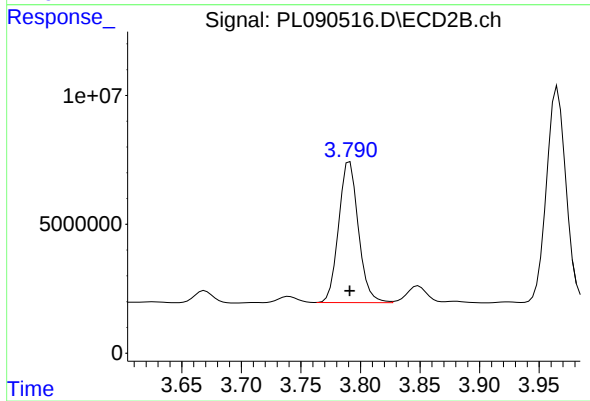

#23 Chlordane-1


R.T.: 3.791 min
Delta R.T.: 0.000 min
Response: 63031431
Conc: 1023.46 ng/ml

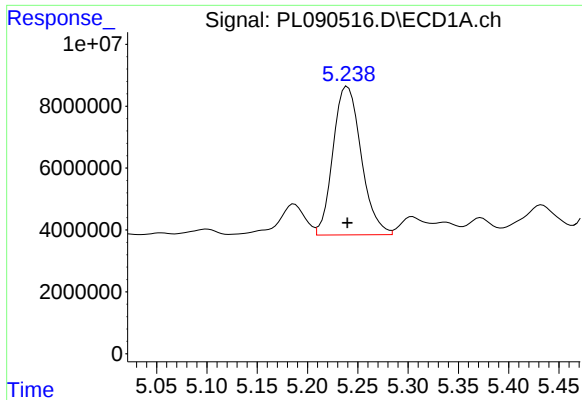

#24 Chlordane-2


R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 93152167
Conc: 966.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

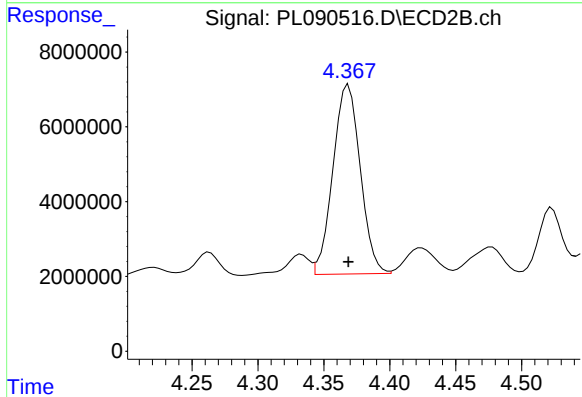


#24 Chlordane-2

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 72977513
Conc: 999.76 ng/ml

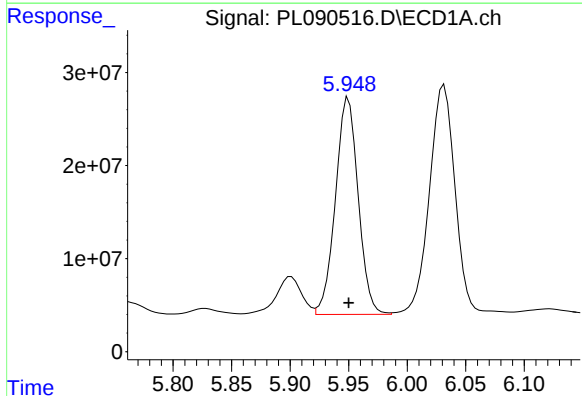


#25 Chlordane-3

R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 315212935
Conc: 1000.71 ng/ml

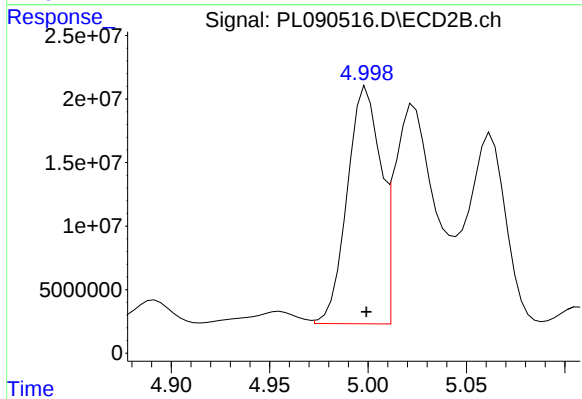

#25 Chlordane-3


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 218577468
Conc: 1033.55 ng/ml

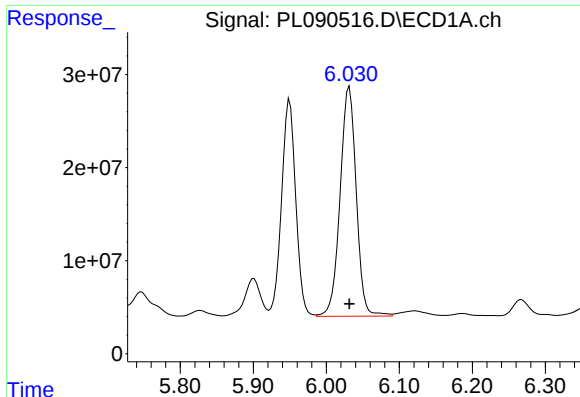

#26 Chlordane-4


R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 378824489
Conc: 996.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

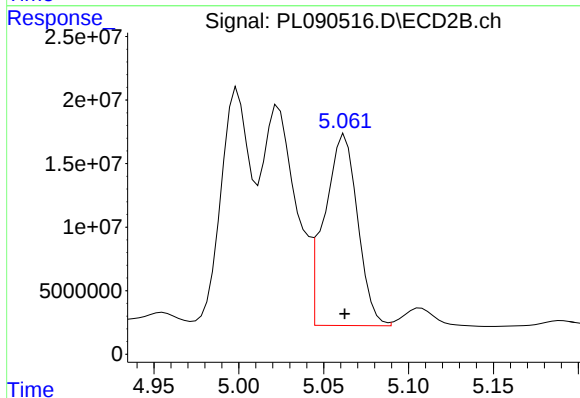


#26 Chlordane-4

R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 204148224
Conc: 1029.20 ng/ml

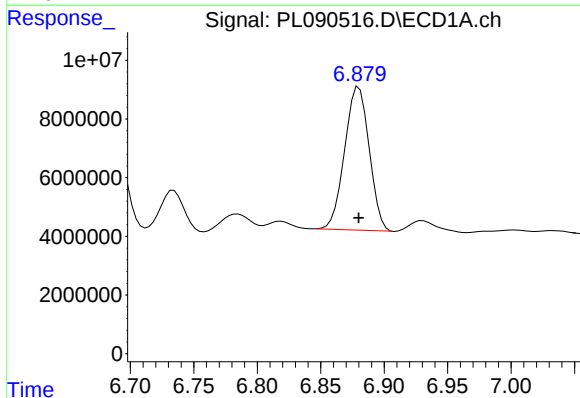


#27 Chlordane-5

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 65556531
Conc: 986.65 ng/ml

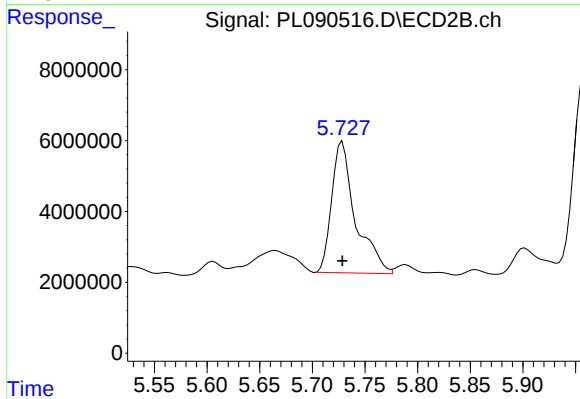

#27 Chlordane-5


R.T.: 5.729 min
Delta R.T.: 0.000 min
Response: 58354609
Conc: 1009.11 ng/ml

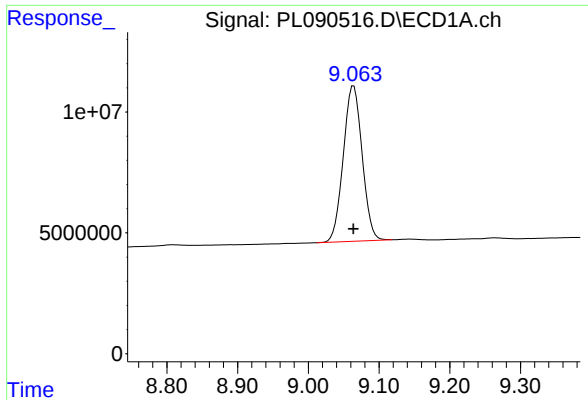

#28 Decachlorobiphenyl

R.T.: 9.064 min
Delta R.T.: 0.000 min
Response: 119373980
Conc: 98.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

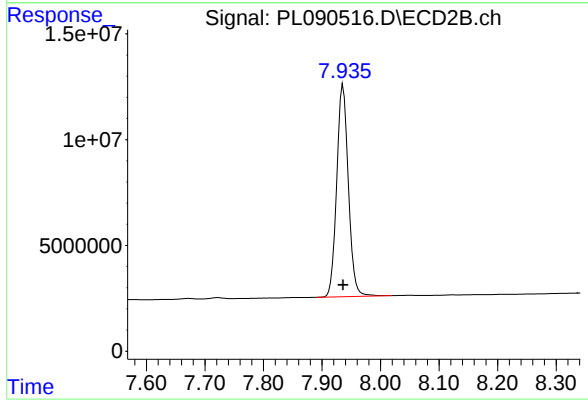

#28 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: 0.000 min
Response: 138686297
Conc: 99.41 ng/ml