

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071524\
 Data File : PL090517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2024 10:59
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 11:54:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 15 11:49:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.790	145.7E6	145.5E6	74.070	74.178
28)	SA Decachlor...	9.064	7.936	90062039	103.3E6	74.576	74.361
Target Compounds							
23)	Chlordane-1	4.710	3.791	63876171	45455030	745.280	742.004
24)	Chlordane-2	5.239	4.369	71342763	53831188	743.197	741.595
25)	Chlordane-3	5.950	4.999	233.4E6	157.1E6	743.852	745.331
26)	Chlordane-4	6.032	5.062	280.9E6	147.7E6	742.689	746.462
27)	Chlordane-5	6.880	5.729	49319586	42640826	744.835	741.539



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071524\
Data File : PL090517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2024 10:59
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 11:54:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 11:49:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

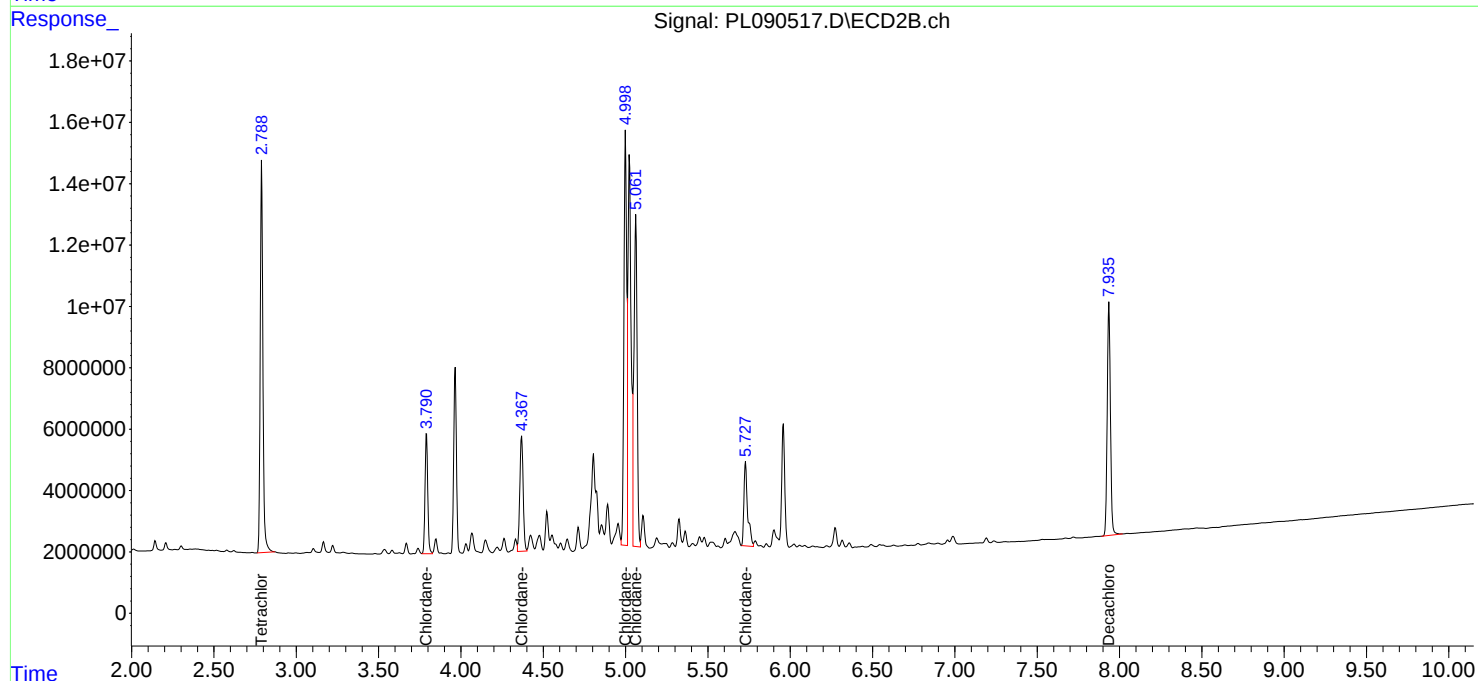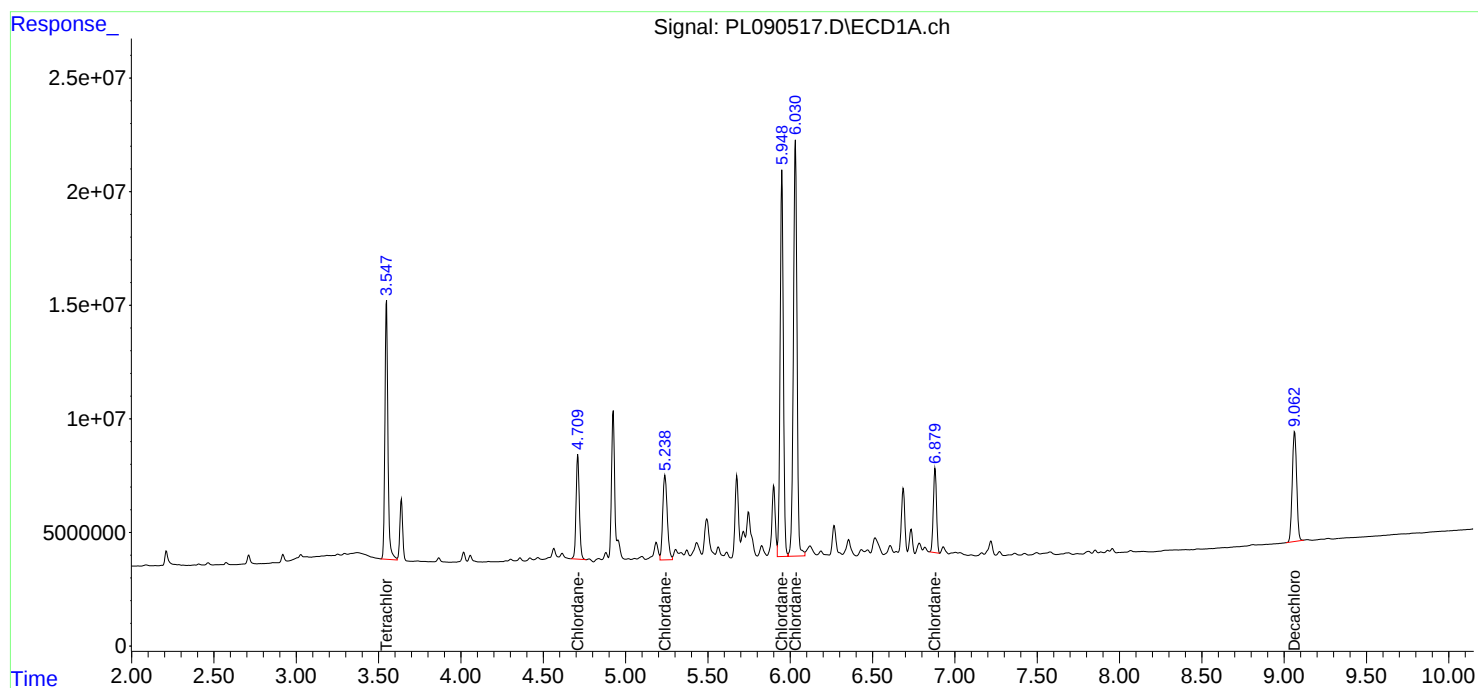


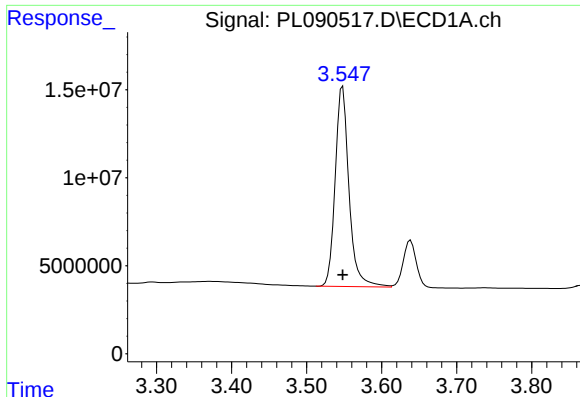

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 145718481
Conc: 74.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

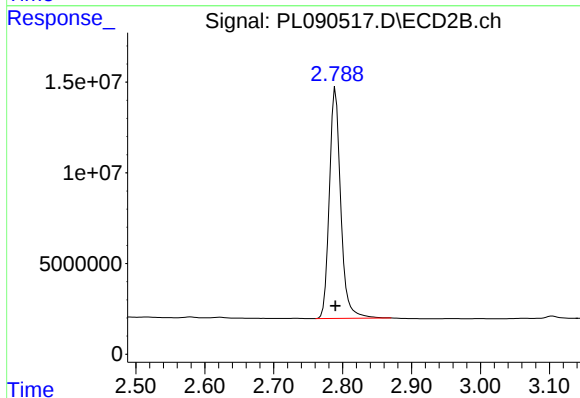


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.000 min
Response: 145462169
Conc: 74.18 ng/ml

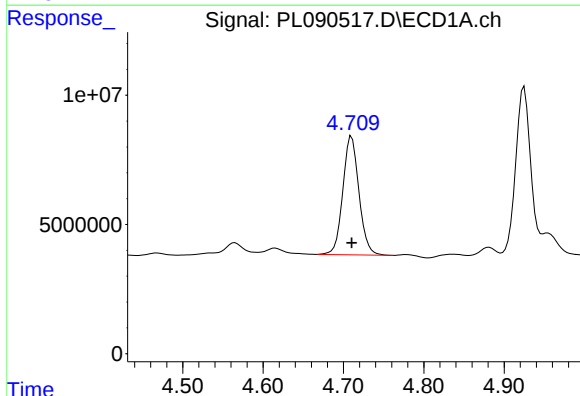


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 63876171
Conc: 745.28 ng/ml

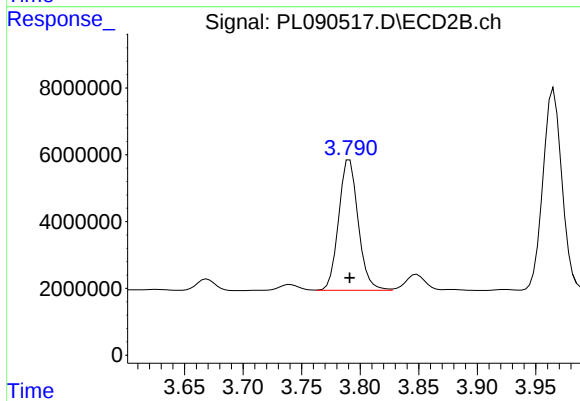

#23 Chlordane-1


R.T.: 3.791 min
Delta R.T.: 0.000 min
Response: 45455030
Conc: 742.00 ng/ml

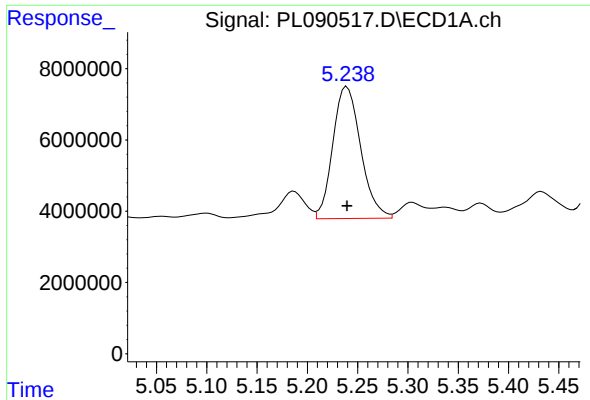

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 71342763
Conc: 743.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

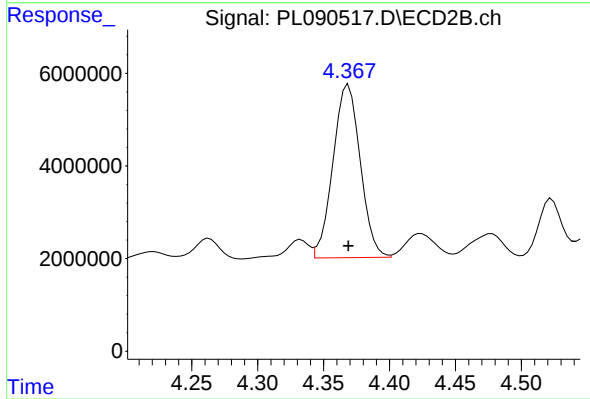


#24 Chlordane-2

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 53831188
Conc: 741.60 ng/ml

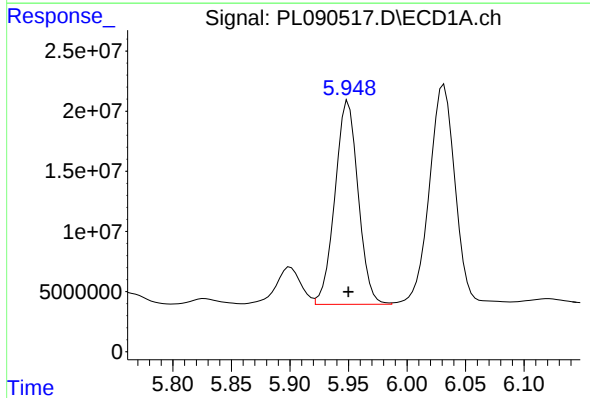


#25 Chlordane-3

R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 233350053
Conc: 743.85 ng/ml

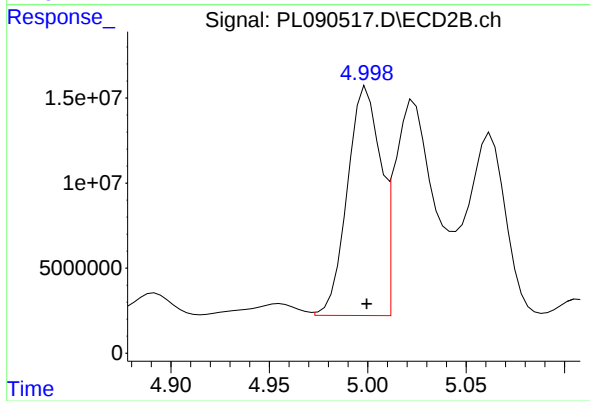

#25 Chlordane-3


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 157135477
Conc: 745.33 ng/ml

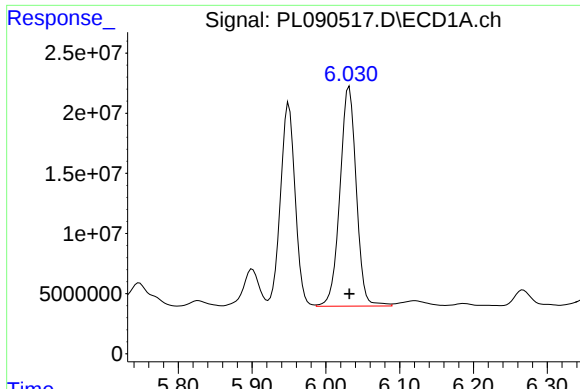

#26 Chlordane-4


R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 280946456
Conc: 742.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

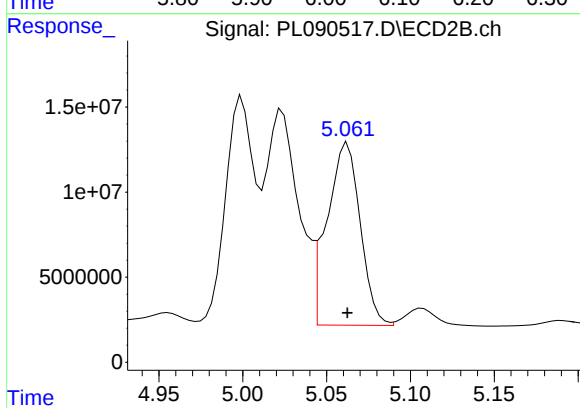


#26 Chlordane-4

R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 147717456
Conc: 746.46 ng/ml

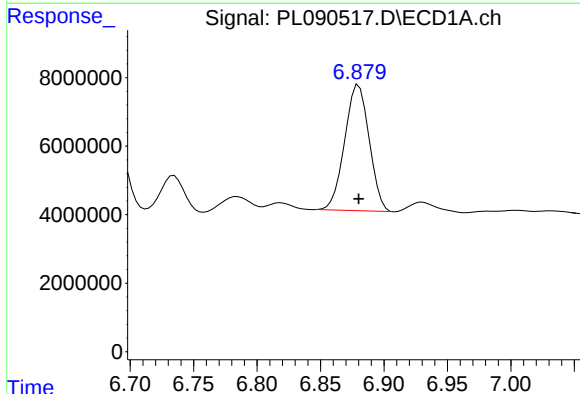


#27 Chlordane-5

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 49319586
Conc: 744.84 ng/ml

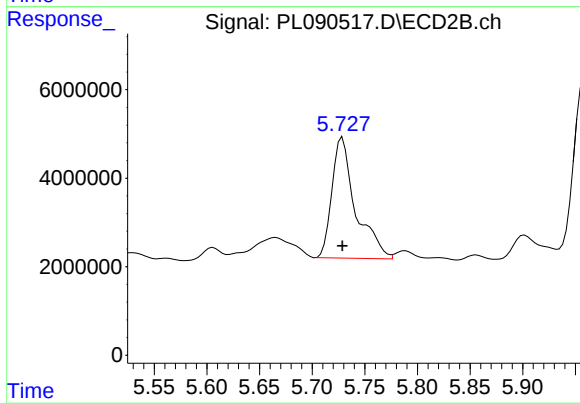

#27 Chlordane-5

R.T.: 5.729 min
Delta R.T.: 0.000 min
Response: 42640826
Conc: 741.54 ng/ml

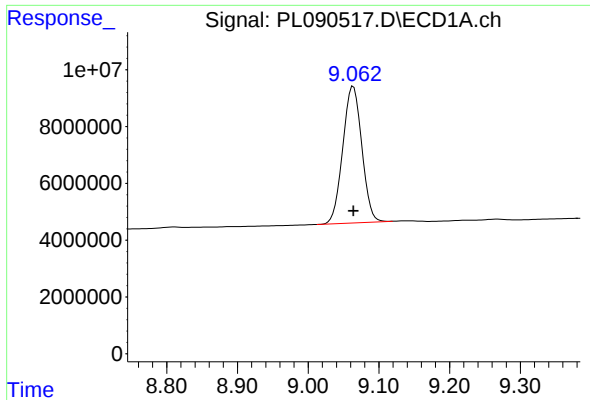

#28 Decachlorobiphenyl


R.T.: 9.064 min

Delta R.T.: 0.000 min

Response: 90062039

Conc: 74.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

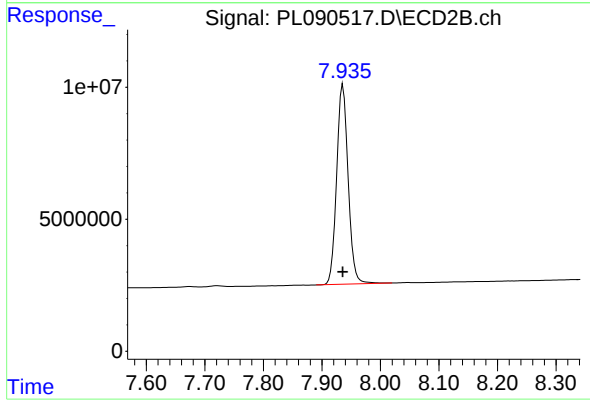

#28 Decachlorobiphenyl

R.T.: 7.936 min

Delta R.T.: 0.000 min

Response: 103305626

Conc: 74.36 ng/ml