

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071524\
 Data File : PL090519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2024 11:26
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 11:59:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 15 11:58:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.789	50348166	45939303	25.442	23.801
28)	SA Decachlor...	9.058	7.932	31946416	35618013	26.074	25.476
Target Compounds							
23)	Chlordane-1	4.708	3.790	22410984	14619470	258.514	241.387
24)	Chlordane-2	5.237	4.367	27288435	18317582	274.852	251.757
25)	Chlordane-3	5.946	4.998	80793045	48625850	255.616	235.196
26)	Chlordane-4	6.029	5.061	98194436	45993839	257.116	236.580
27)	Chlordane-5	6.877	5.726	17208251	14179513	257.340	247.431



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071524\
Data File : PL090519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2024 11:26
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 11:59:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 11:58:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

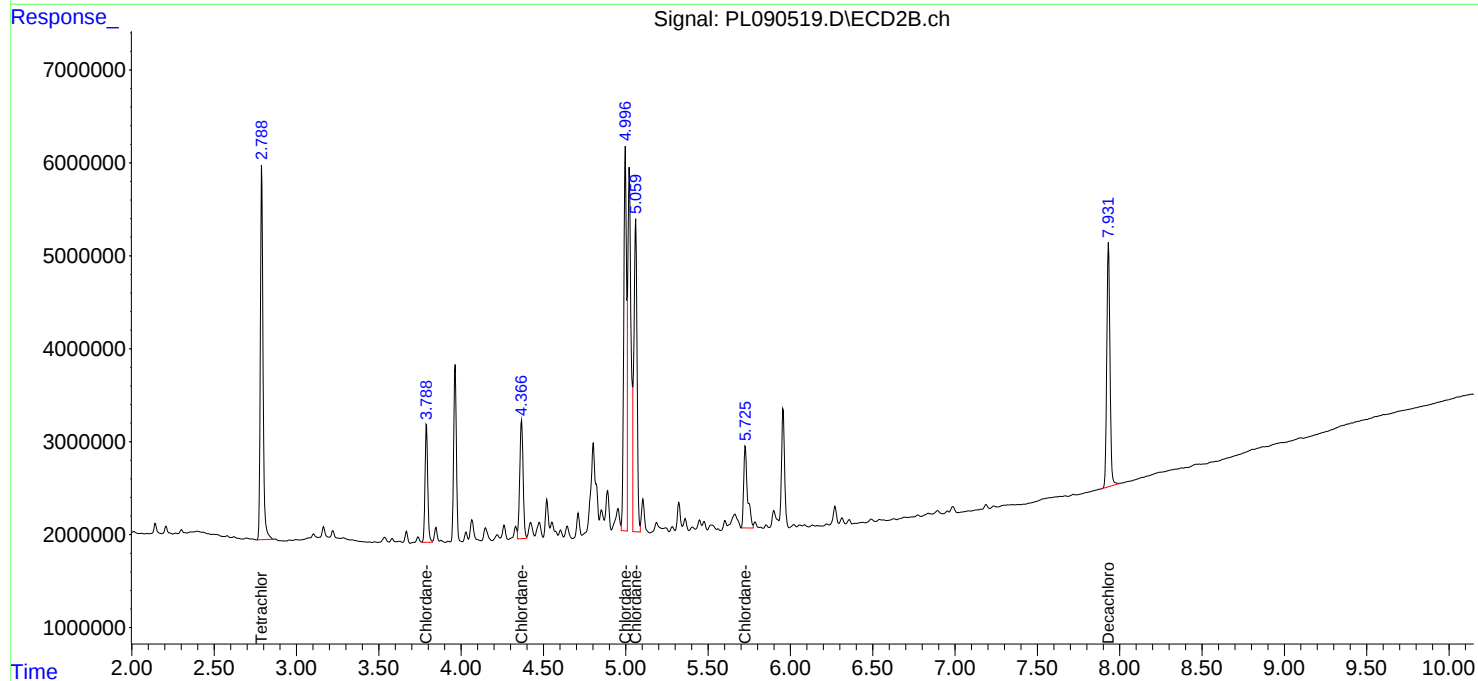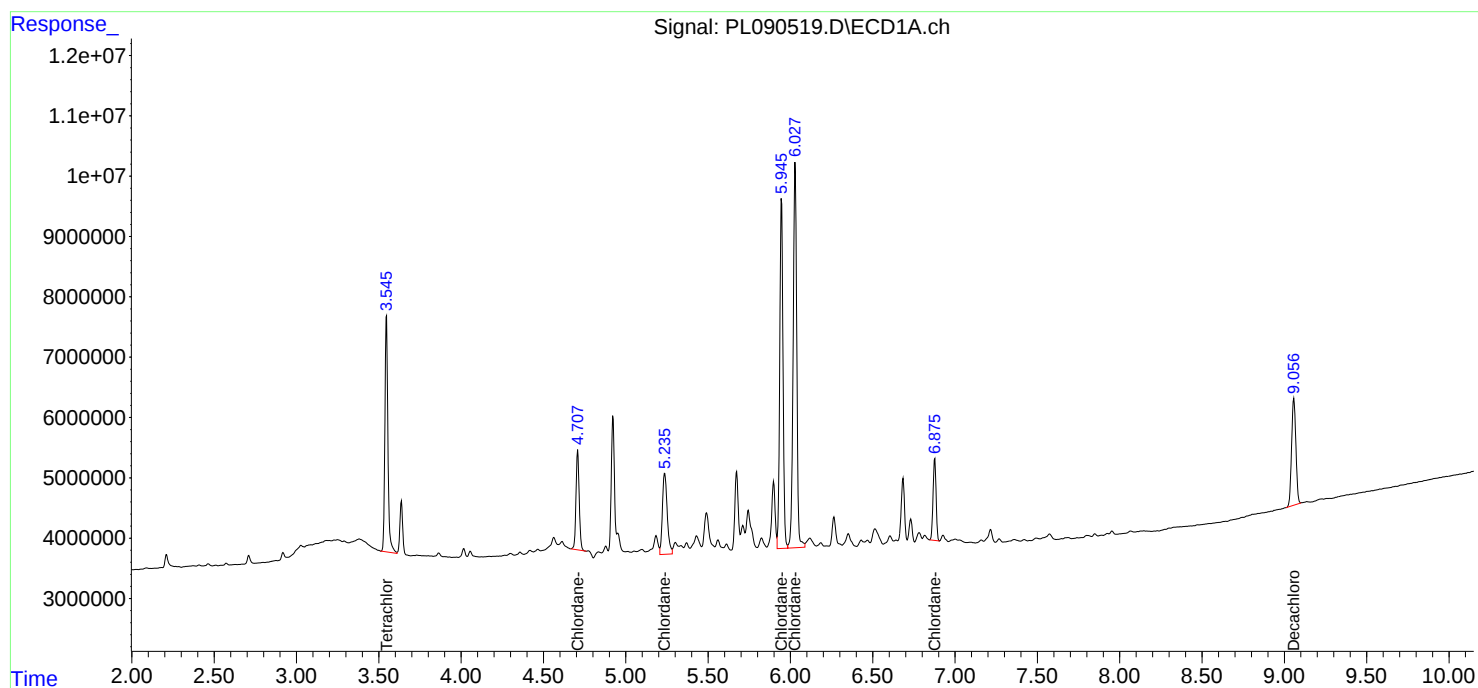


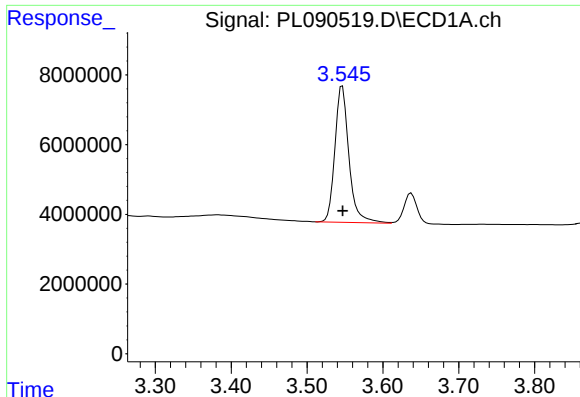

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 50348166
Conc: 25.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

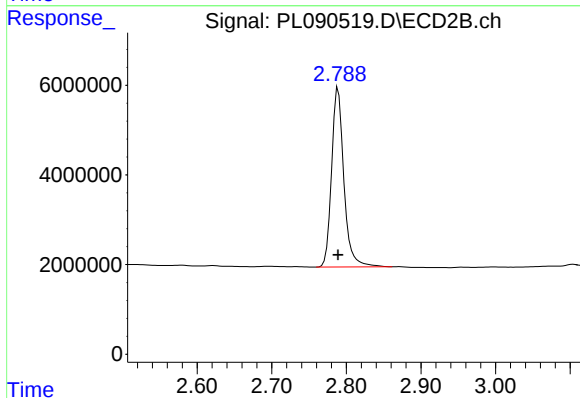


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.000 min
Response: 45939303
Conc: 23.80 ng/ml

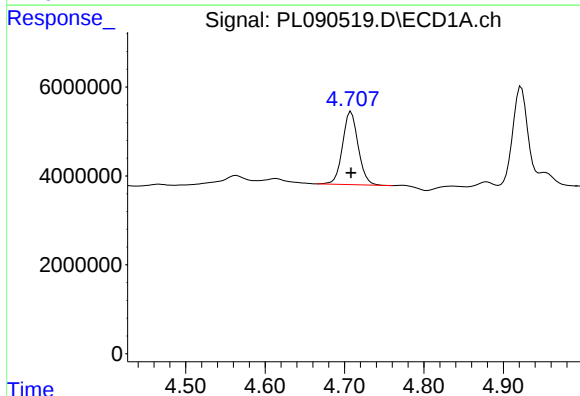


#23 Chlordane-1

R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 22410984
Conc: 258.51 ng/ml

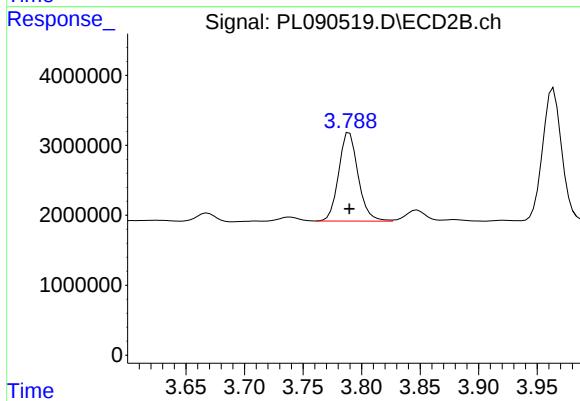

#23 Chlordane-1


R.T.: 3.790 min
Delta R.T.: 0.000 min
Response: 14619470
Conc: 241.39 ng/ml

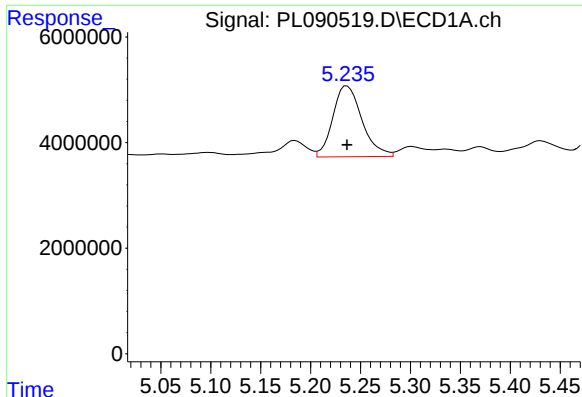

#24 Chlordane-2


R.T.: 5.237 min
Delta R.T.: 0.000 min
Response: 27288435
Conc: 274.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

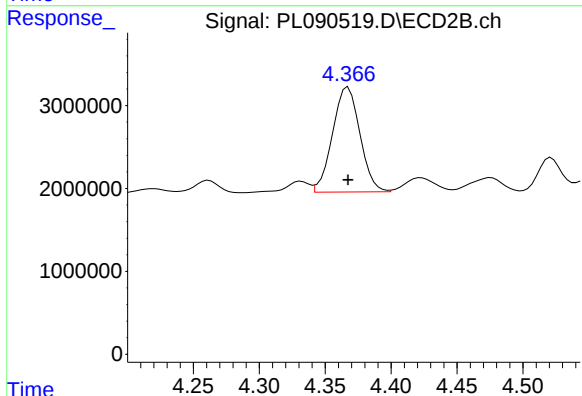


#24 Chlordane-2

R.T.: 4.367 min
Delta R.T.: 0.000 min
Response: 18317582
Conc: 251.76 ng/ml

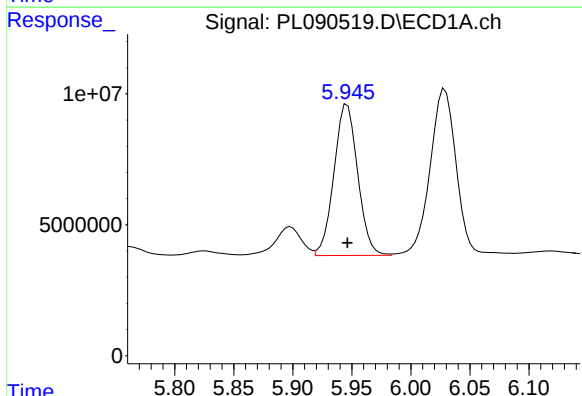


#25 Chlordane-3

R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 80793045
Conc: 255.62 ng/ml

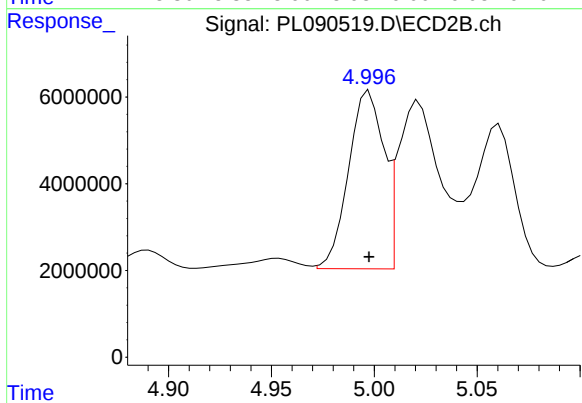

#25 Chlordane-3


R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 48625850
Conc: 235.20 ng/ml

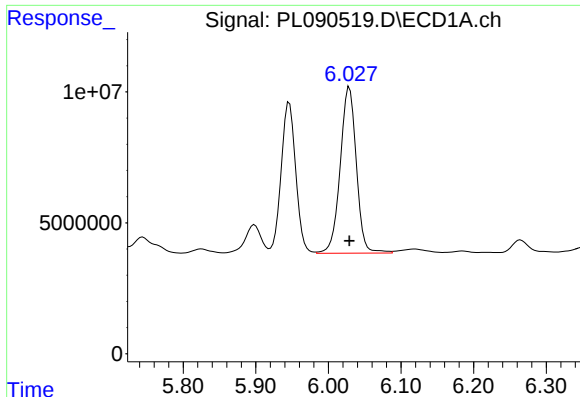

#26 Chlordane-4


R.T.: 6.029 min
Delta R.T.: 0.000 min
Response: 98194436
Conc: 257.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

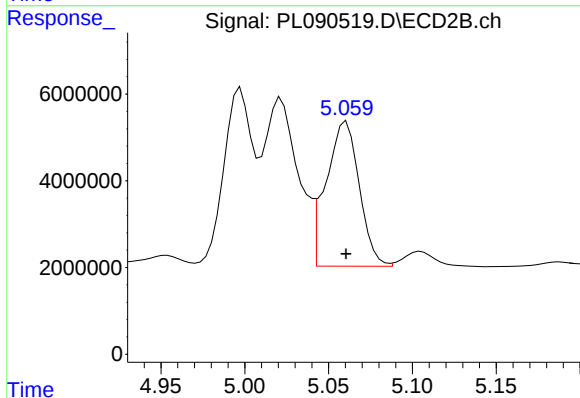


#26 Chlordane-4

R.T.: 5.061 min
Delta R.T.: 0.000 min
Response: 45993839
Conc: 236.58 ng/ml

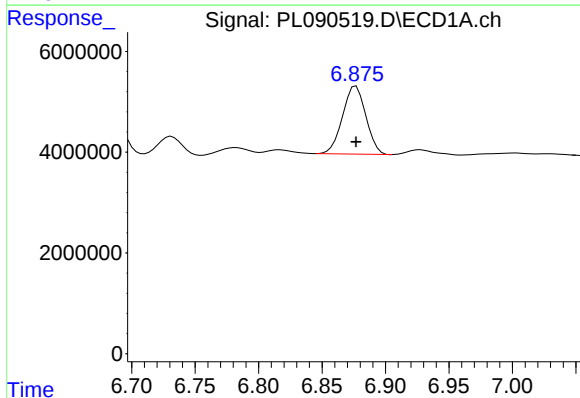


#27 Chlordane-5

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 17208251
Conc: 257.34 ng/ml

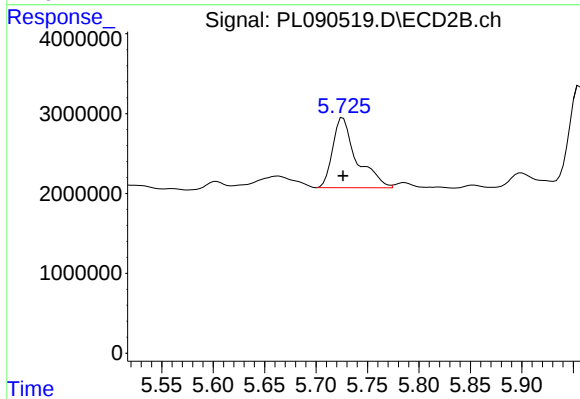

#27 Chlordane-5


R.T.: 5.726 min
Delta R.T.: 0.000 min
Response: 14179513
Conc: 247.43 ng/ml

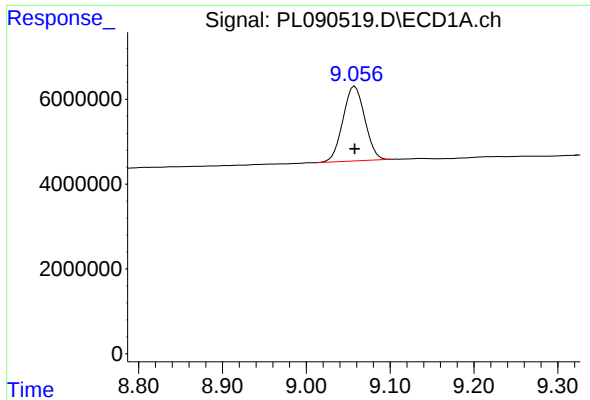

#28 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: 0.000 min
Response: 31946416
Conc: 26.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

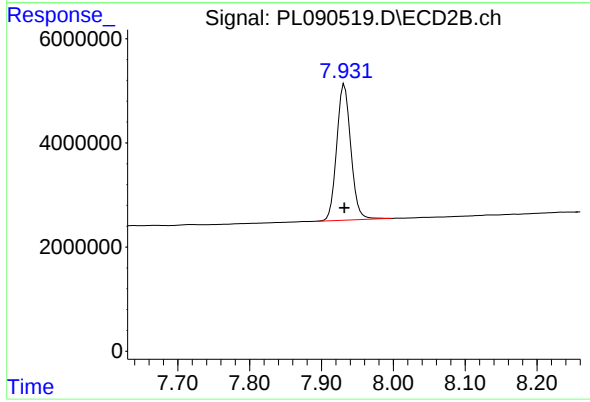

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 35618013
Conc: 25.48 ng/ml