

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071524\
 Data File : PL090518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2024 11:13
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 11:50:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 15 11:49:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.789	99004562	95713450	50.000	50.000
28)	SA Decachlor...	9.063	7.936	61418612	70172771	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.710	3.791	43414928	30070695	500.000	500.000
24)	Chlordane-2	5.240	4.369	49853691	36506368	500.000	500.000
25)	Chlordane-3	5.949	5.000	157.4E6	102.2E6	500.000	500.000
26)	Chlordane-4	6.031	5.062	190.7E6	96282739	500.000	500.000
27)	Chlordane-5	6.880	5.728	33665142	28650215	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071524\
Data File : PL090518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2024 11:13
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 11:50:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 11:49:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

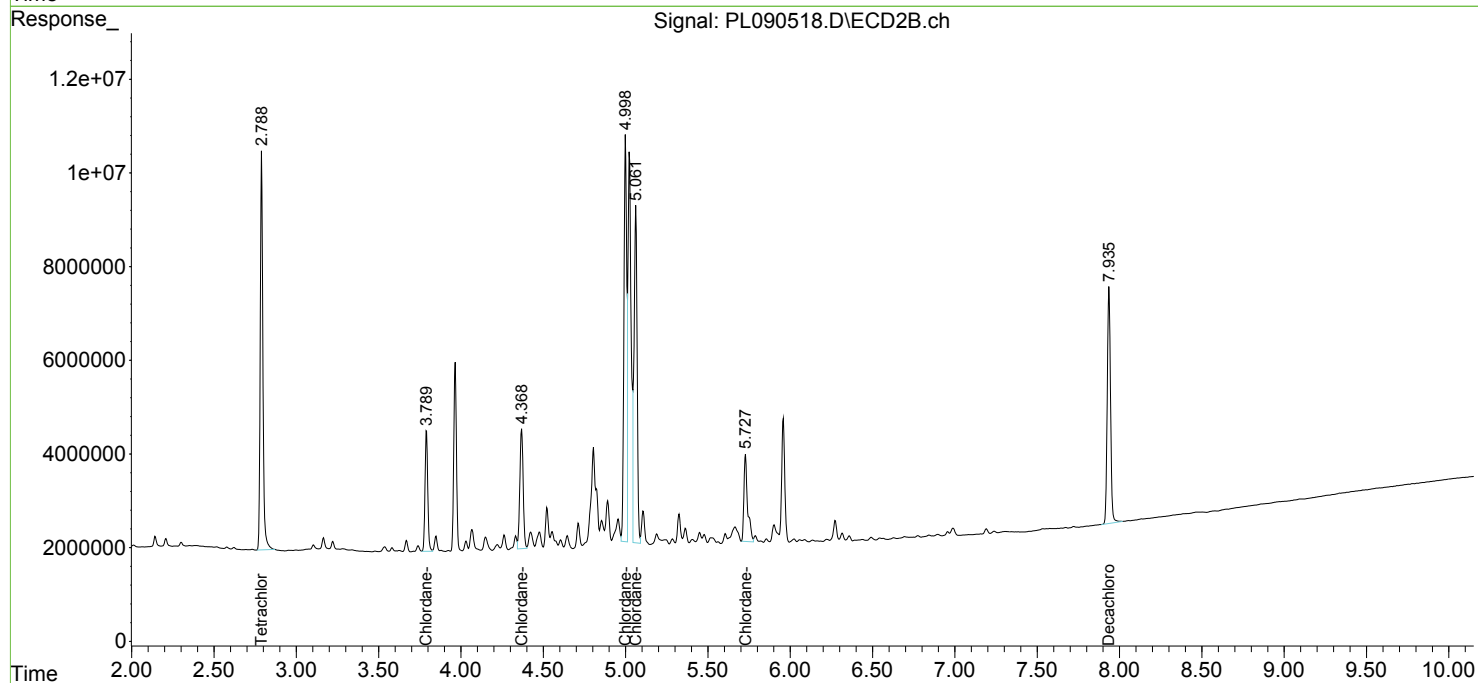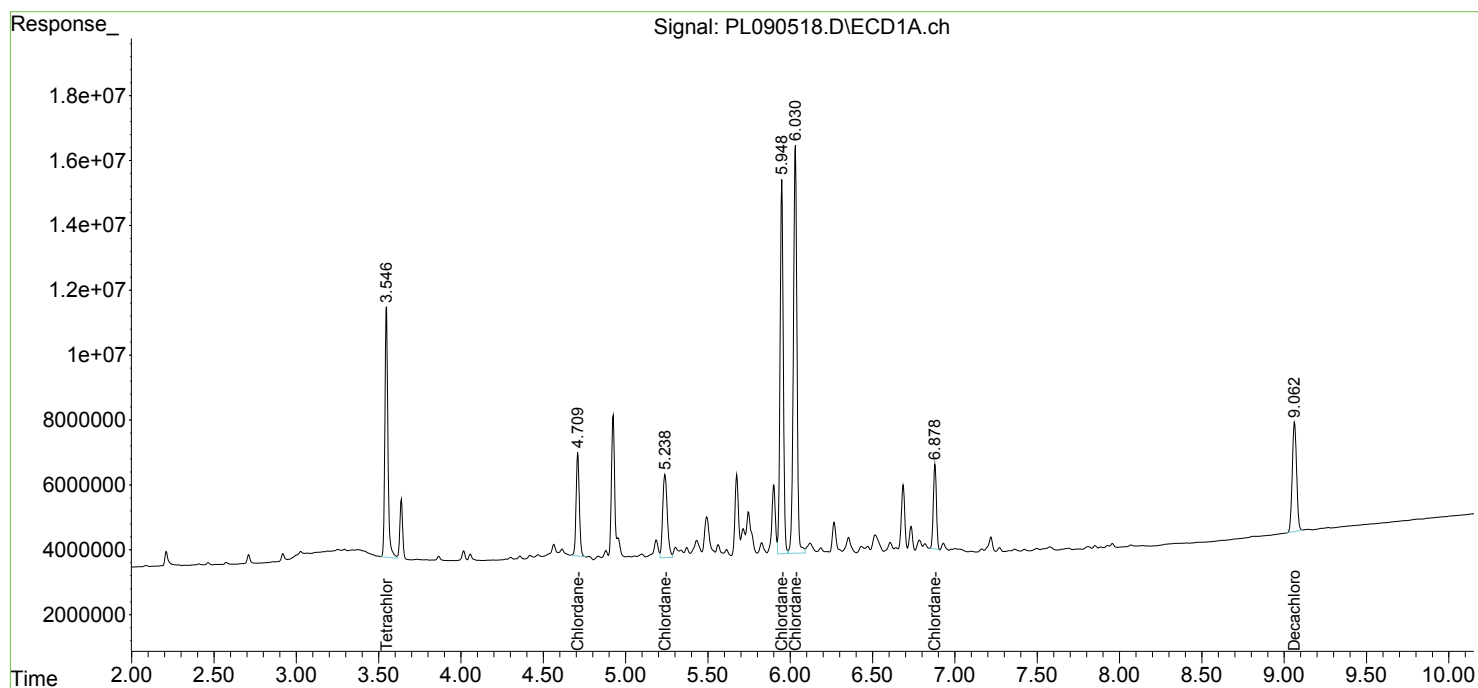


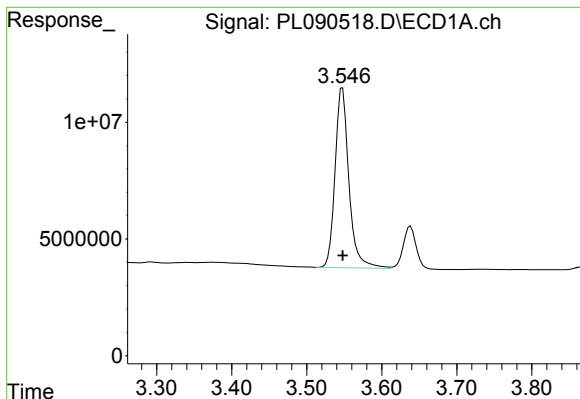

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 99004562
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

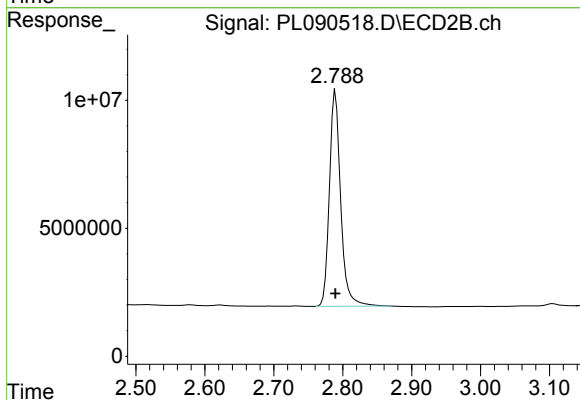


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.000 min
Response: 95713450
Conc: 50.00 ng/ml

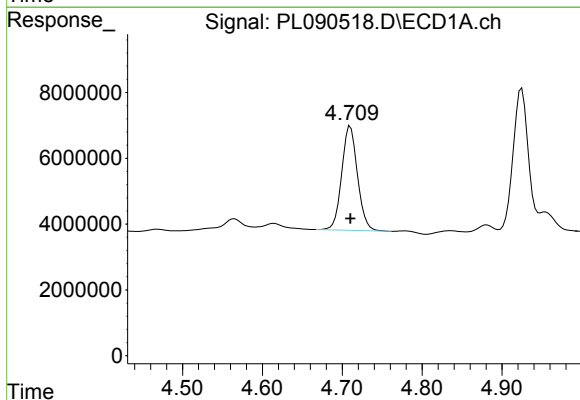


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 43414928
Conc: 500.00 ng/ml

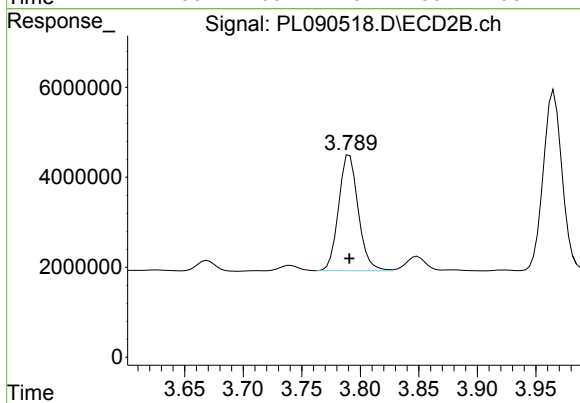

#23 Chlordane-1


R.T.: 3.791 min
Delta R.T.: 0.000 min
Response: 30070695
Conc: 500.00 ng/ml

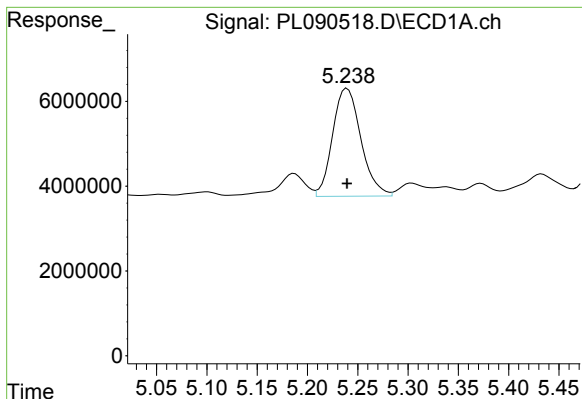

#24 Chlordane-2


R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 49853691
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

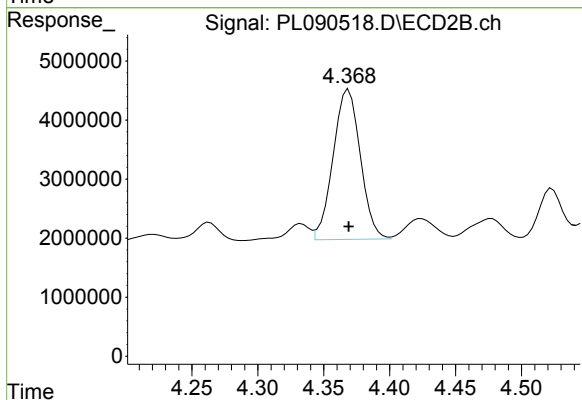


#24 Chlordane-2

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 36506368
Conc: 500.00 ng/ml

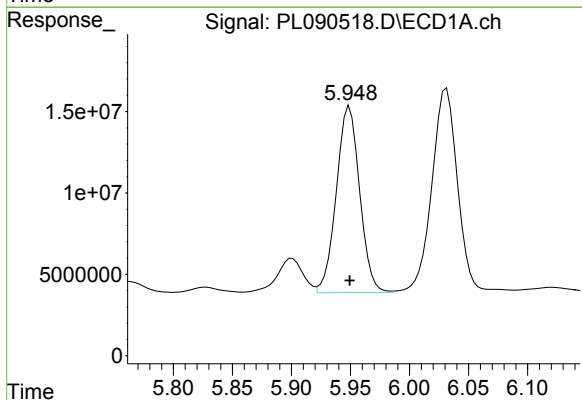


#25 Chlordane-3

R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 157384140
Conc: 500.00 ng/ml

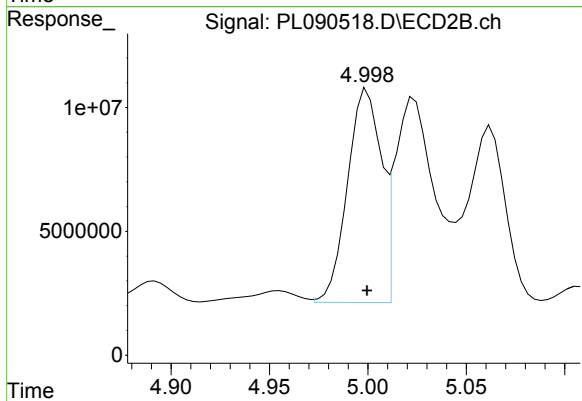

#25 Chlordane-3


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 102194125
Conc: 500.00 ng/ml

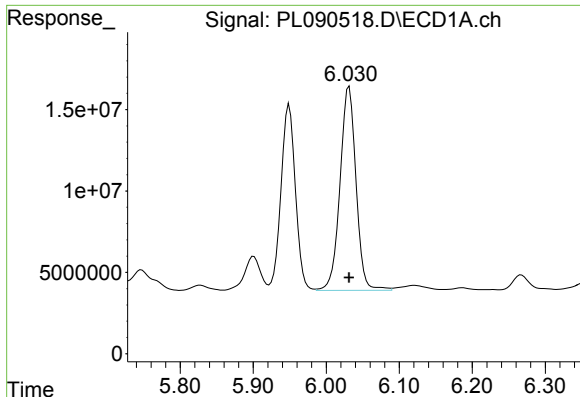

#26 Chlordane-4


R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 190714305
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

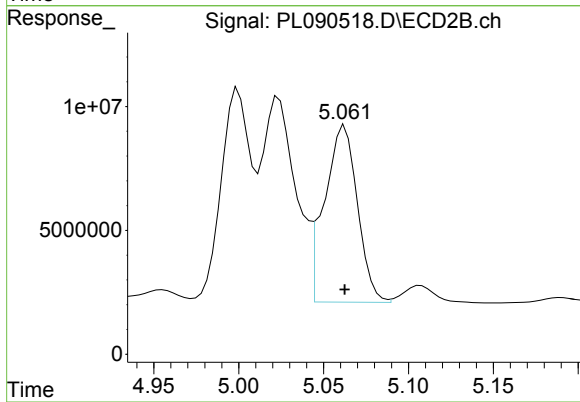


#26 Chlordane-4

R.T.: 5.062 min
Delta R.T.: 0.000 min
Response: 96282739
Conc: 500.00 ng/ml

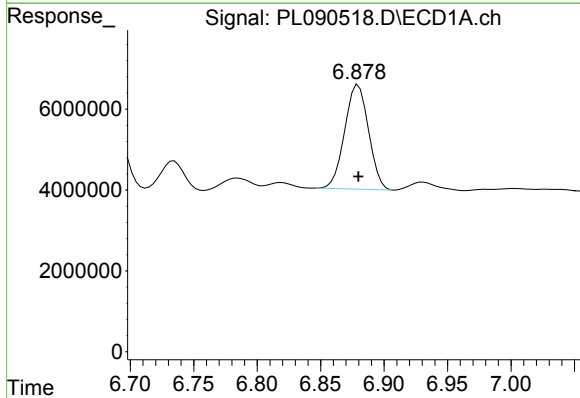


#27 Chlordane-5

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 33665142
Conc: 500.00 ng/ml

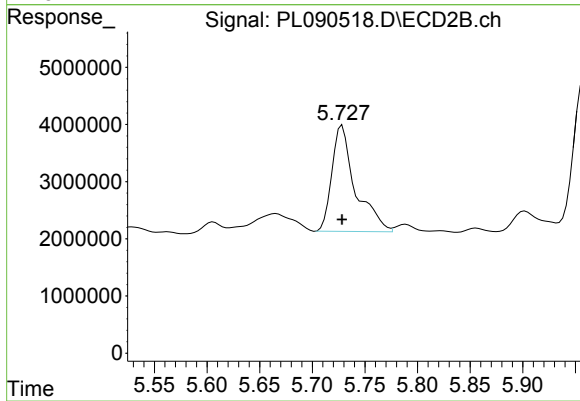

#27 Chlordane-5


R.T.: 5.728 min
Delta R.T.: 0.000 min
Response: 28650215
Conc: 500.00 ng/ml

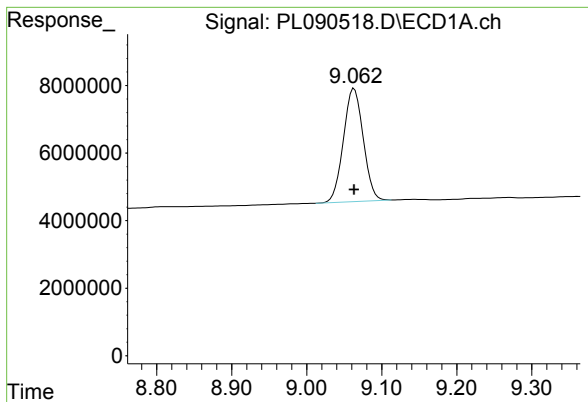

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: 0.000 min
Response: 61418612
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

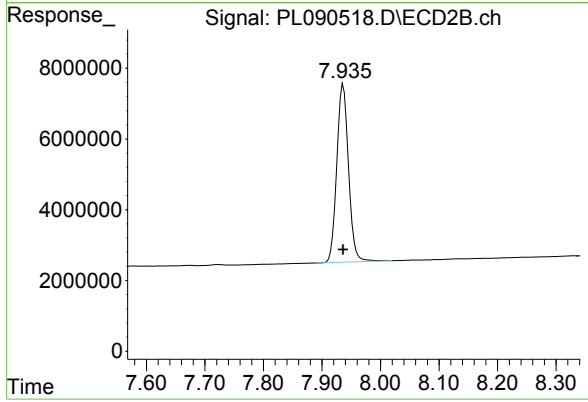

#28 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: 0.000 min
Response: 70172771
Conc: 50.00 ng/ml