

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071525\
 Data File : PL096367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2025 14:22
 Operator : AR\AJ
 Sample : Q2597-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-26899

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/16/2025
 Supervised By : mohammad ahmed 07/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:36:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.828	52388936	61324602	14.357m	10.626 #
28)	SA Decachlor...	9.031	7.993	55084177	79463081	19.582	15.936

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071525\
Data File : PL096367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2025 14:22
Operator : AR\AJ
Sample : Q2597-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT-26899


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/16/2025
Supervised By : mohammad ahmed 07/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:36:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

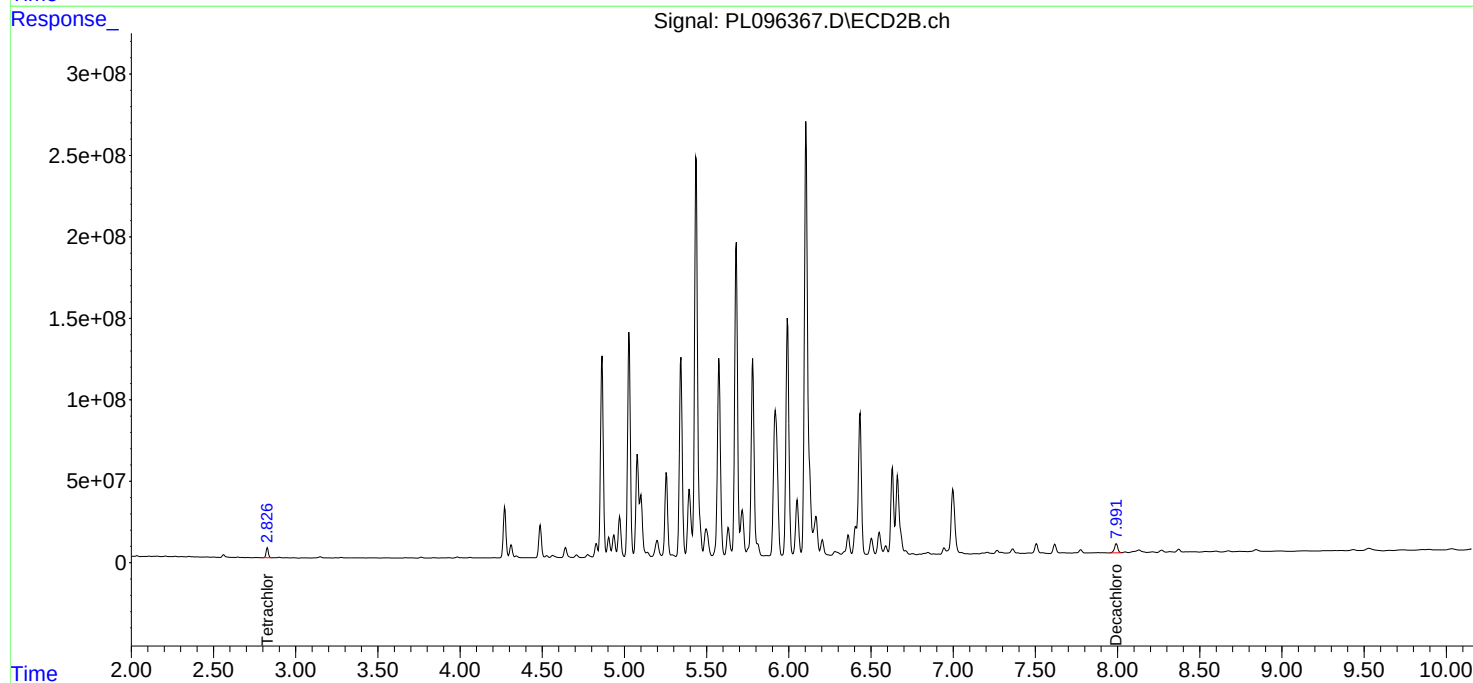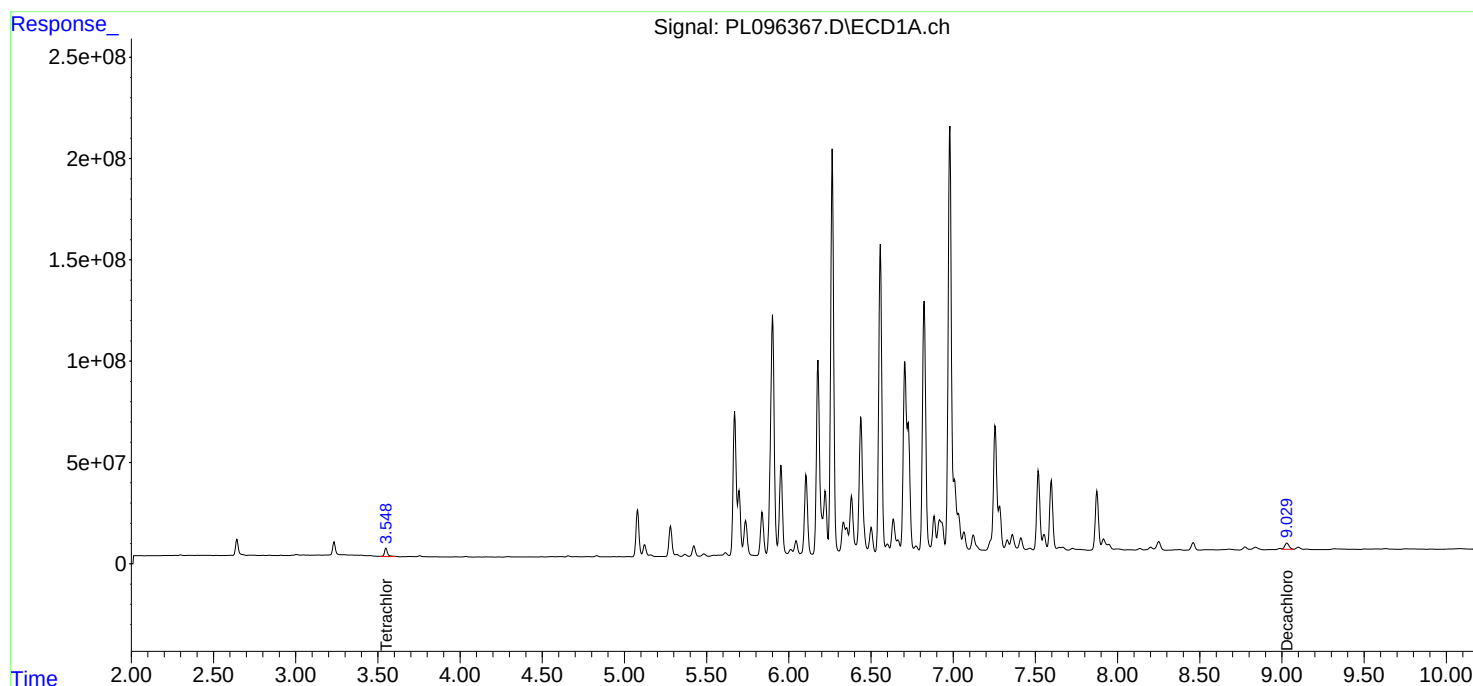

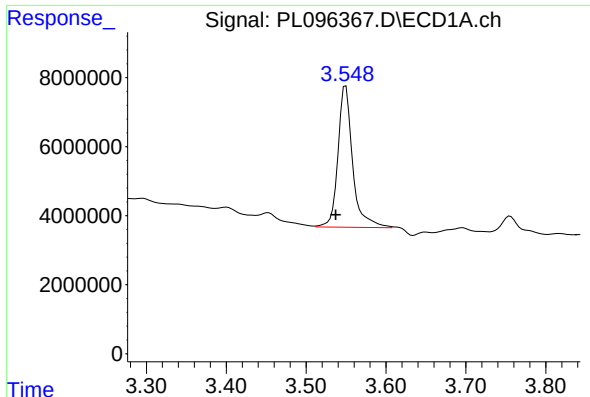


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: 0.011 min
Response: 52388936
Conc: 14.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26899


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/16/2025
Supervised By :mohammad ahmed 07/17/2025

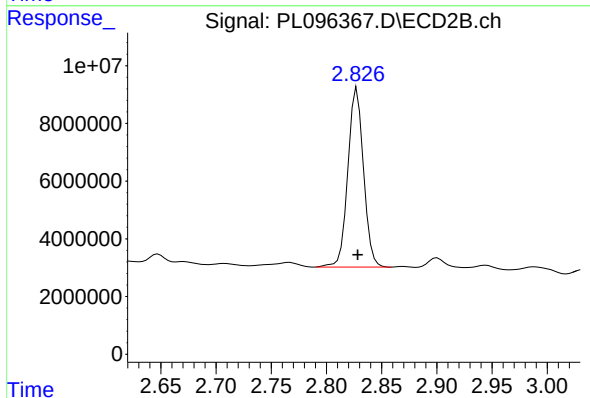


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 61324602
Conc: 10.63 ng/ml

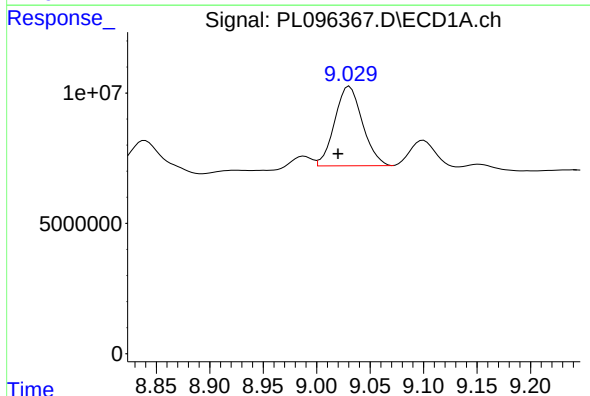

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: 0.011 min
Response: 55084177
Conc: 19.58 ng/ml

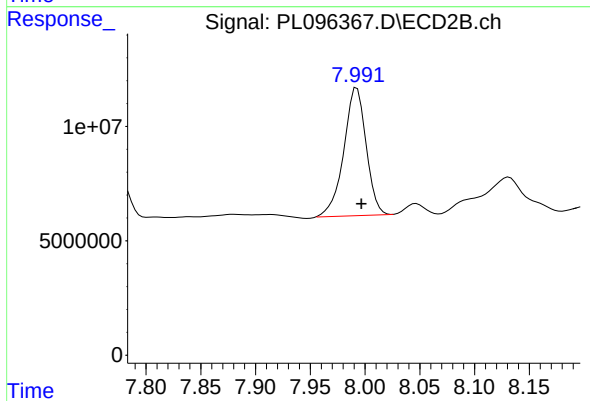

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.004 min
Response: 79463081
Conc: 15.94 ng/ml