

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071618\
 Data File : PL038117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2018 16:23
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:44:05 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.930	134.9E6	51316011	18.115	19.549
28)	SA Decachlor...	8.003	8.940	135.7E6	46669835	17.888	19.092
Target Compounds							
4)	MA Heptachlor	0.000	5.051f	0	1320090	N.D.	0.413 #
6)	B beta-BHC	4.245f	0.000	5167158	0	1.095	N.D. #
7)	B delta-BHC	0.000	4.960	0	2390192	N.D.	0.721 #
8)	B Heptachlo...	0.000	5.773	0	2972874	N.D.	1.046 #
12)	B 4,4'-DDE	0.000	6.299f	0	1761920	N.D.	0.659 #
15)	B Endosulfa...	6.036f	0.000	35336379	0	4.456	N.D. #
16)	A 4,4'-DDD	0.000	6.678f	0	11496941	N.D.	5.371 #
23)	Chlordane-1	0.000	4.960	0	2390192	N.D.	20.626 #
24)	Chlordane-2	0.000	5.309	0	3091406	N.D.	25.815 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071618\
Data File : PL038117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2018 16:23
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:44:05 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

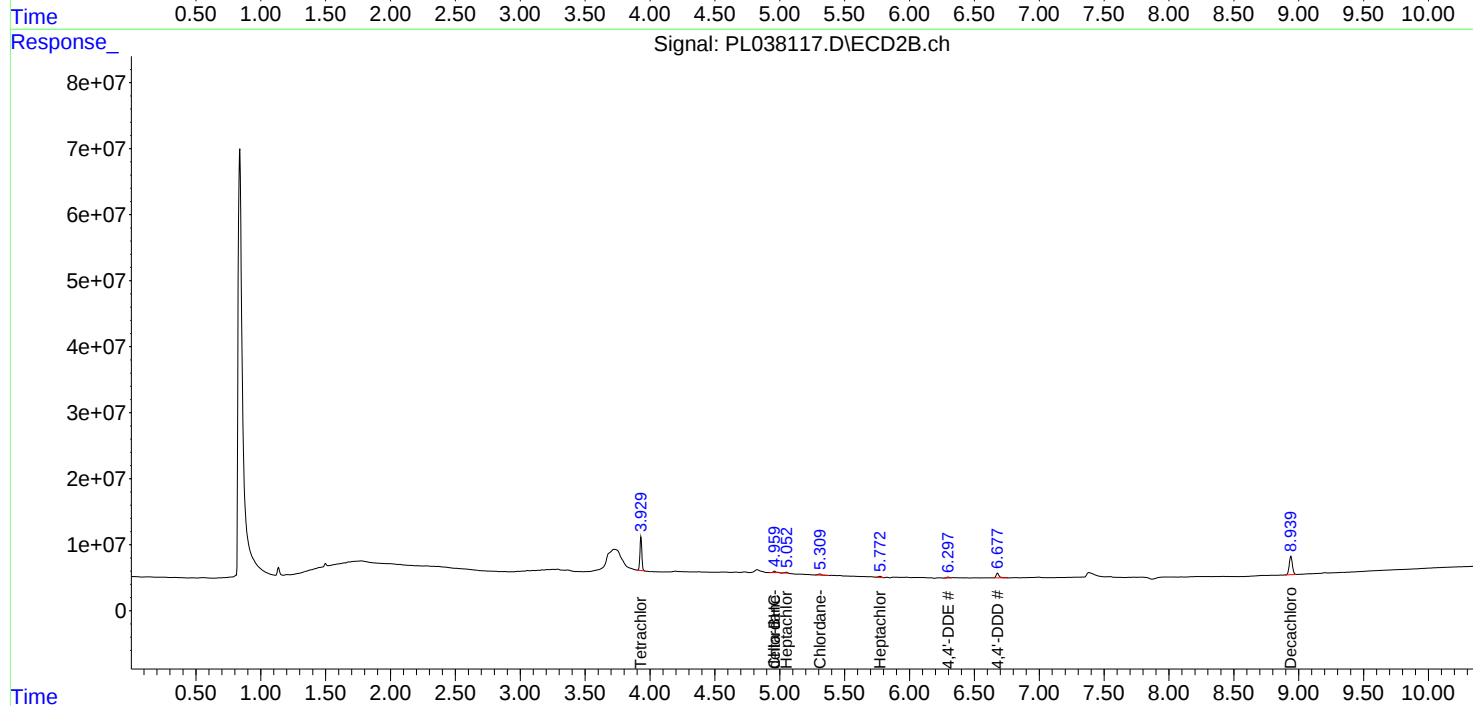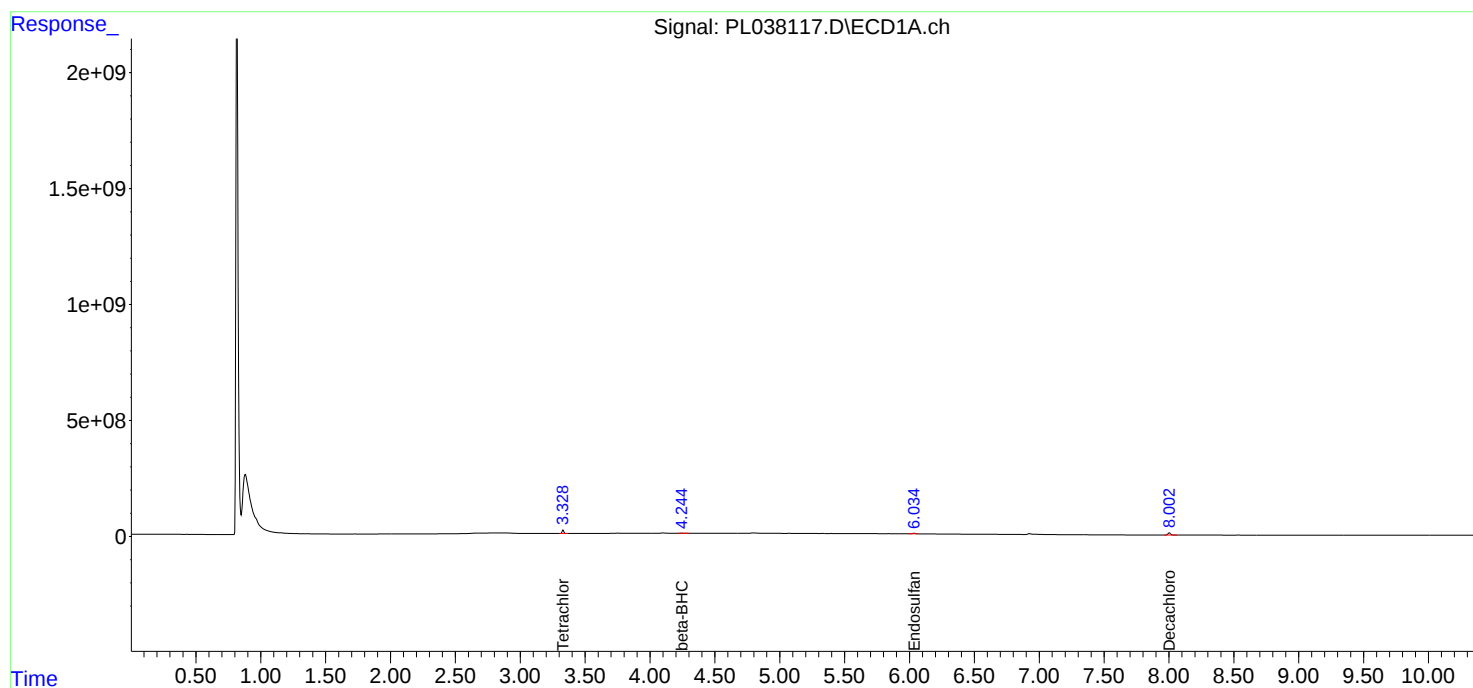


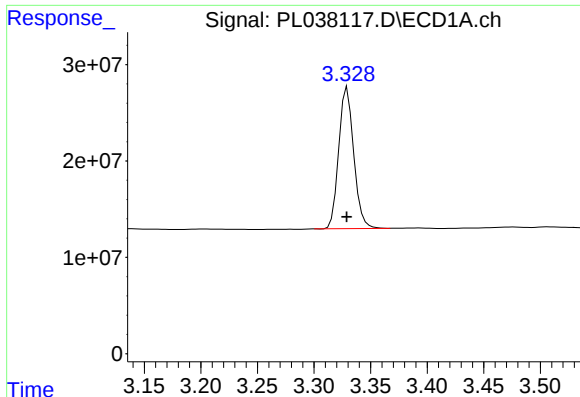

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 134890506
Conc: 18.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

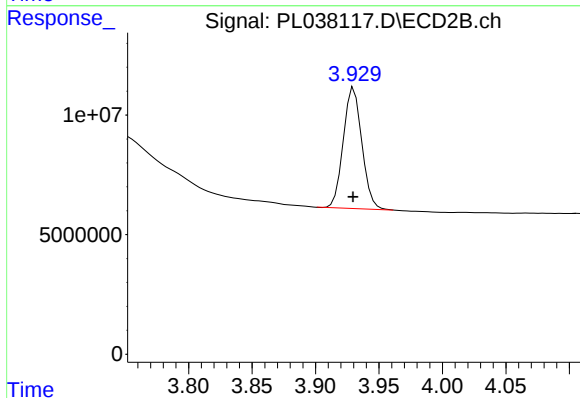


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 51316011
Conc: 19.55 ng/ml

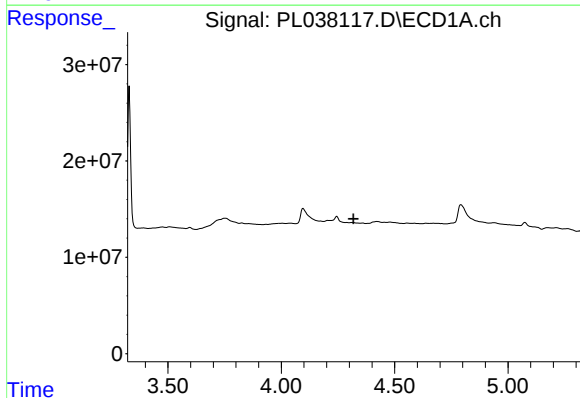


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

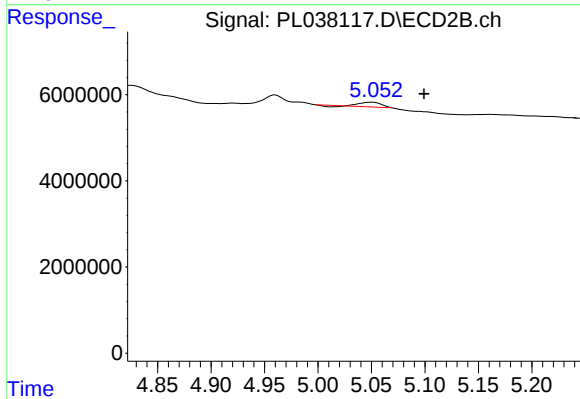

#4 Heptachlor


R.T.: 5.051 min
Delta R.T.: -0.048 min
Response: 1320090
Conc: 0.41 ng/ml

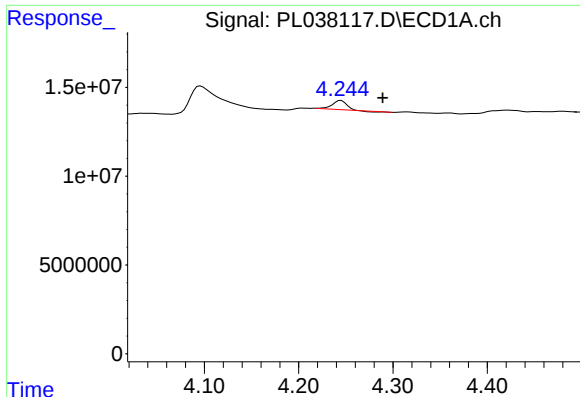

#6 beta-BHC


R.T.: 4.245 min
Delta R.T.: -0.044 min
Response: 5167158
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

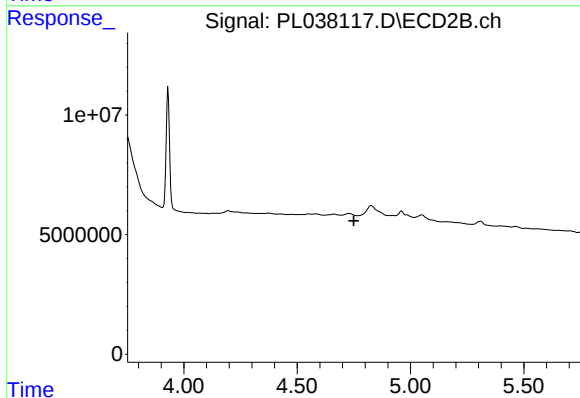


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

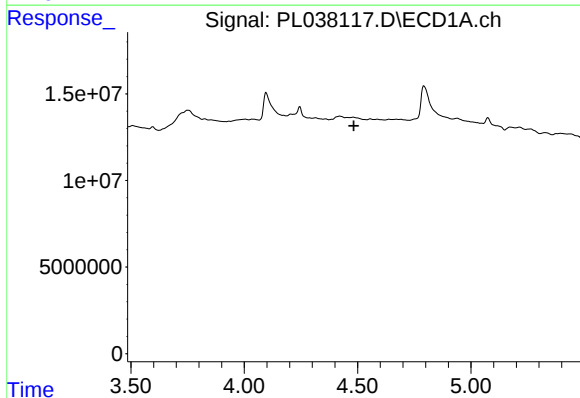


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

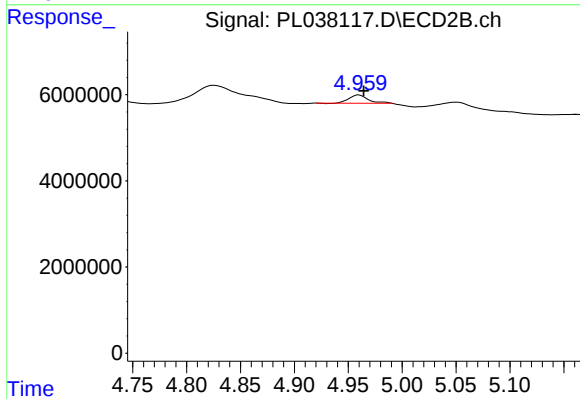

#7 delta-BHC


R.T.: 4.960 min
Delta R.T.: -0.004 min
Response: 2390192
Conc: 0.72 ng/ml

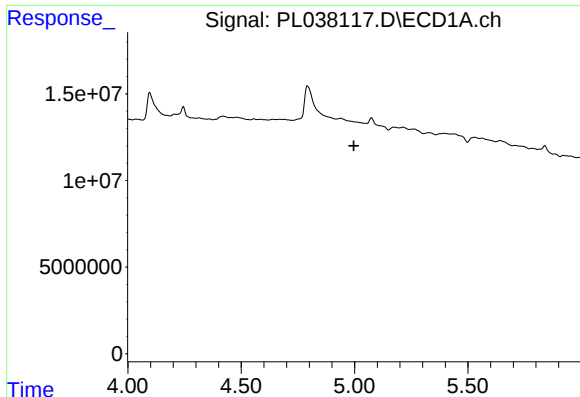

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

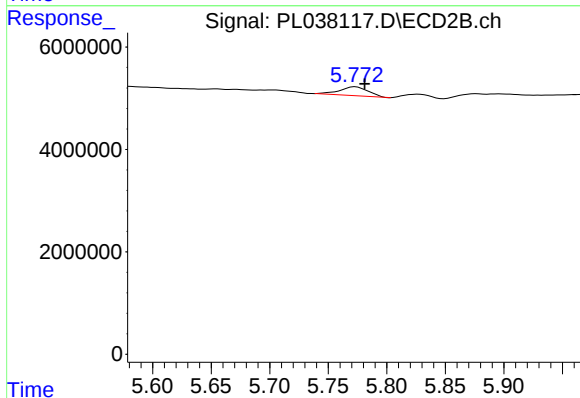


#8 Heptachlor epoxide

R.T.: 5.773 min
Delta R.T.: -0.008 min
Response: 2972874
Conc: 1.05 ng/ml

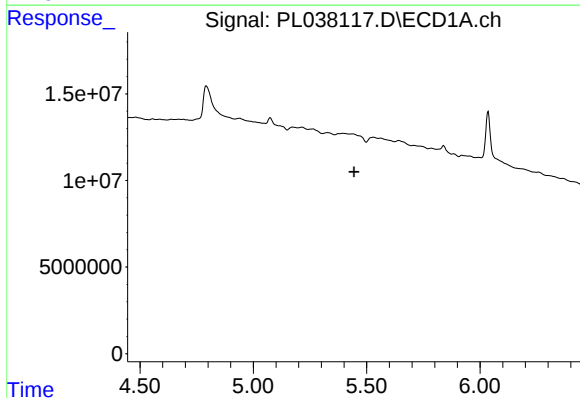


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.444 min
Response: 0
Conc: N.D.

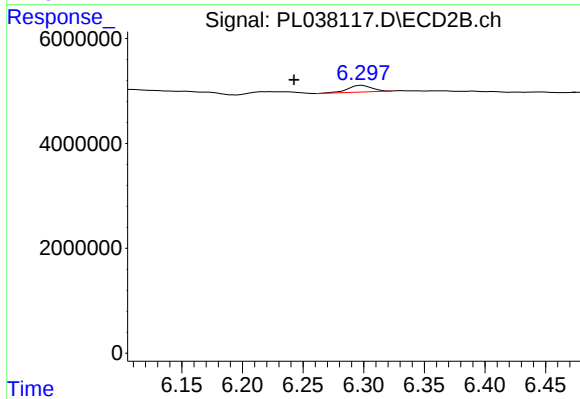

#12 4,4'-DDE


R.T.: 6.299 min
Delta R.T.: 0.056 min
Response: 1761920
Conc: 0.66 ng/ml

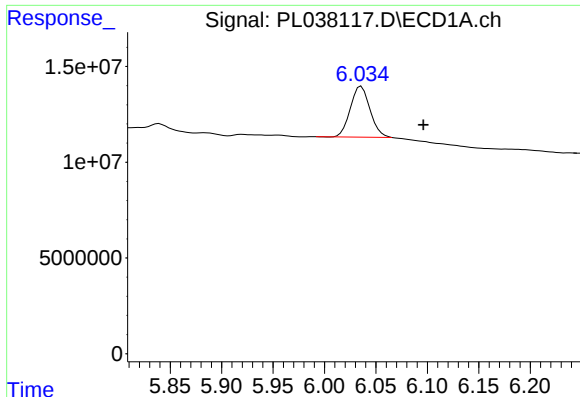

#15 Endosulfan II


R.T.: 6.036 min
Delta R.T.: -0.060 min
Response: 35336379
Conc: 4.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

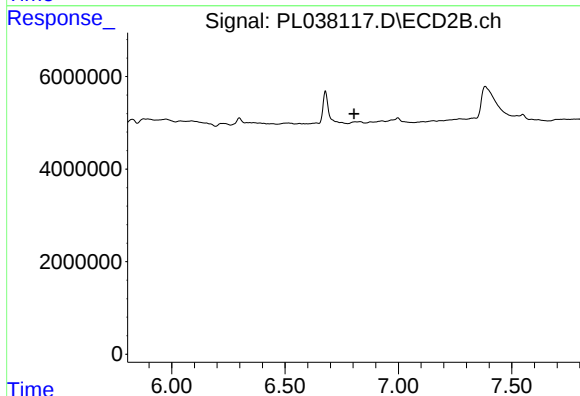


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

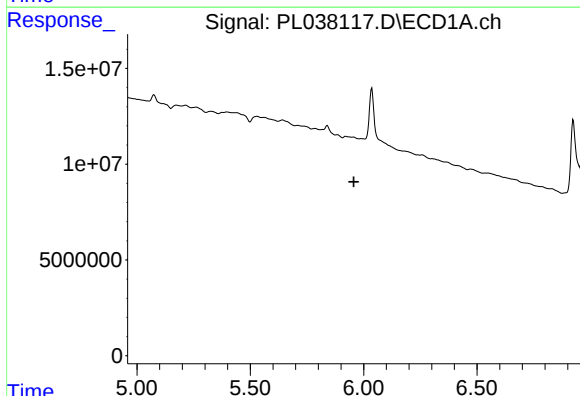


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

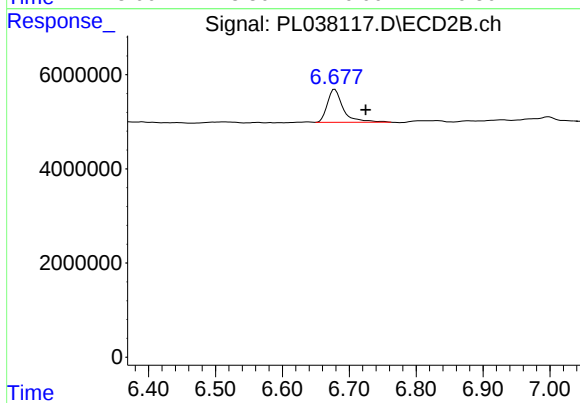

#16 4,4'-DDD


R.T.: 6.678 min
Delta R.T.: -0.046 min
Response: 11496941
Conc: 5.37 ng/ml

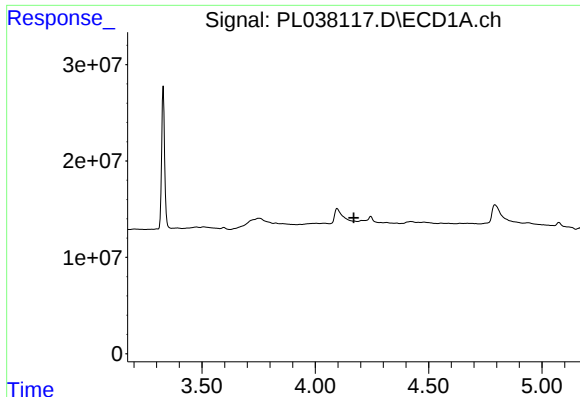

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

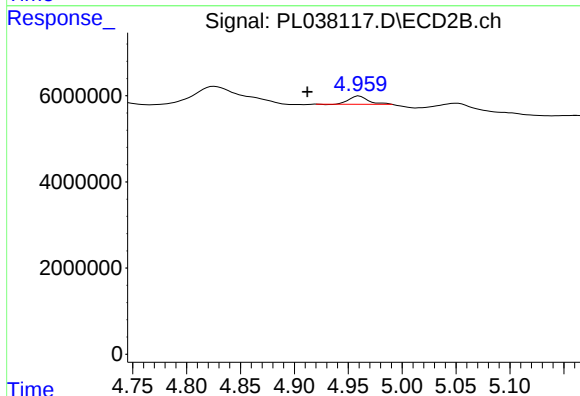


#23 Chlordane-1

R.T.: 4.960 min
Delta R.T.: 0.048 min
Response: 2390192
Conc: 20.63 ng/ml

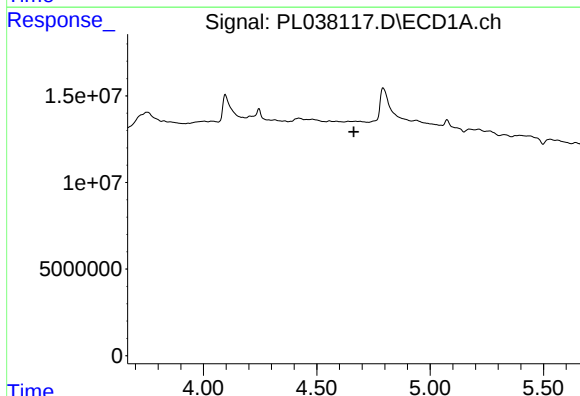


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.663 min
Response: 0
Conc: N.D.

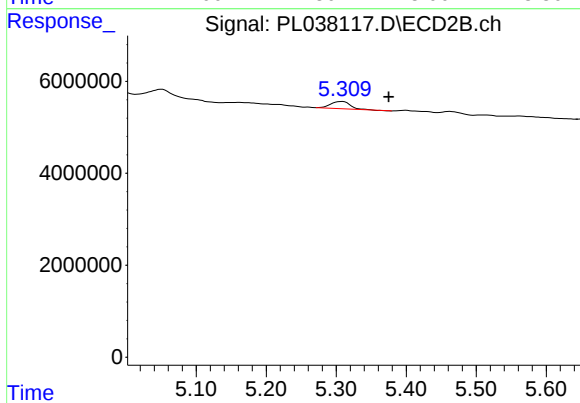

#24 Chlordane-2


R.T.: 5.309 min
Delta R.T.: -0.066 min
Response: 3091406
Conc: 25.82 ng/ml

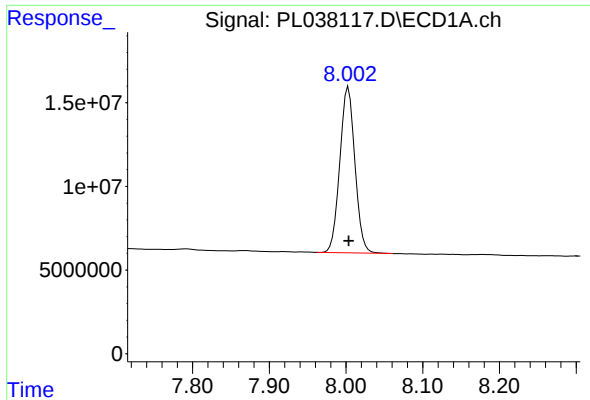

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 135699133
Conc: 17.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

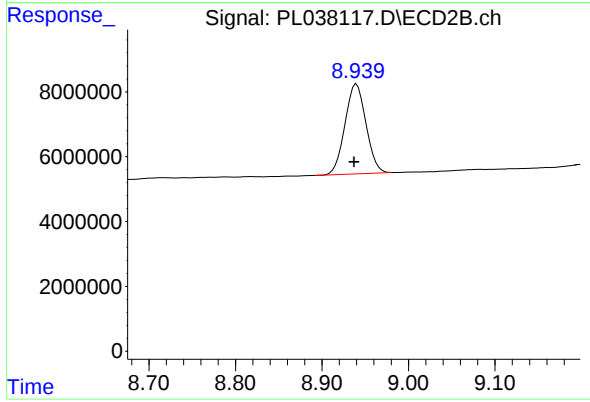

#28 Decachlorobiphenyl

R.T.: 8.940 min
Delta R.T.: 0.003 min
Response: 46669835
Conc: 19.09 ng/ml