

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071618\
 Data File : PL038120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2018 17:06
 Operator : AJ\SJ
 Sample : J3975-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:44:48 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.931	173.0E6	67858999	23.236	25.852
28)	SA Decachlor...	8.003	8.940	120.0E6	46374612	15.814	18.971
Target Compounds							
2)	A alpha-BHC	0.000	4.279f	0	4866275	N.D.	1.257 #
4)	MA Heptachlor	0.000	5.052f	0	2146596	N.D.	0.672 #
6)	B beta-BHC	4.246f	0.000	23032110	0	4.879	N.D. #
7)	B delta-BHC	0.000	4.959	0	5209937	N.D.	1.571 #
8)	B Heptachlo...	0.000	5.773	0	5712173	N.D.	2.010 #
15)	B Endosulfa...	6.036f	0.000	34617550	0	4.365	N.D. #
16)	A 4,4'-DDD	0.000	6.679f	0	13066259	N.D.	6.105 #
23)	Chlordane-1	0.000	4.959	0	5209937	N.D.	44.958 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071618\
Data File : PL038120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2018 17:06
Operator : AJ\SJ
Sample : J3975-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:44:48 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

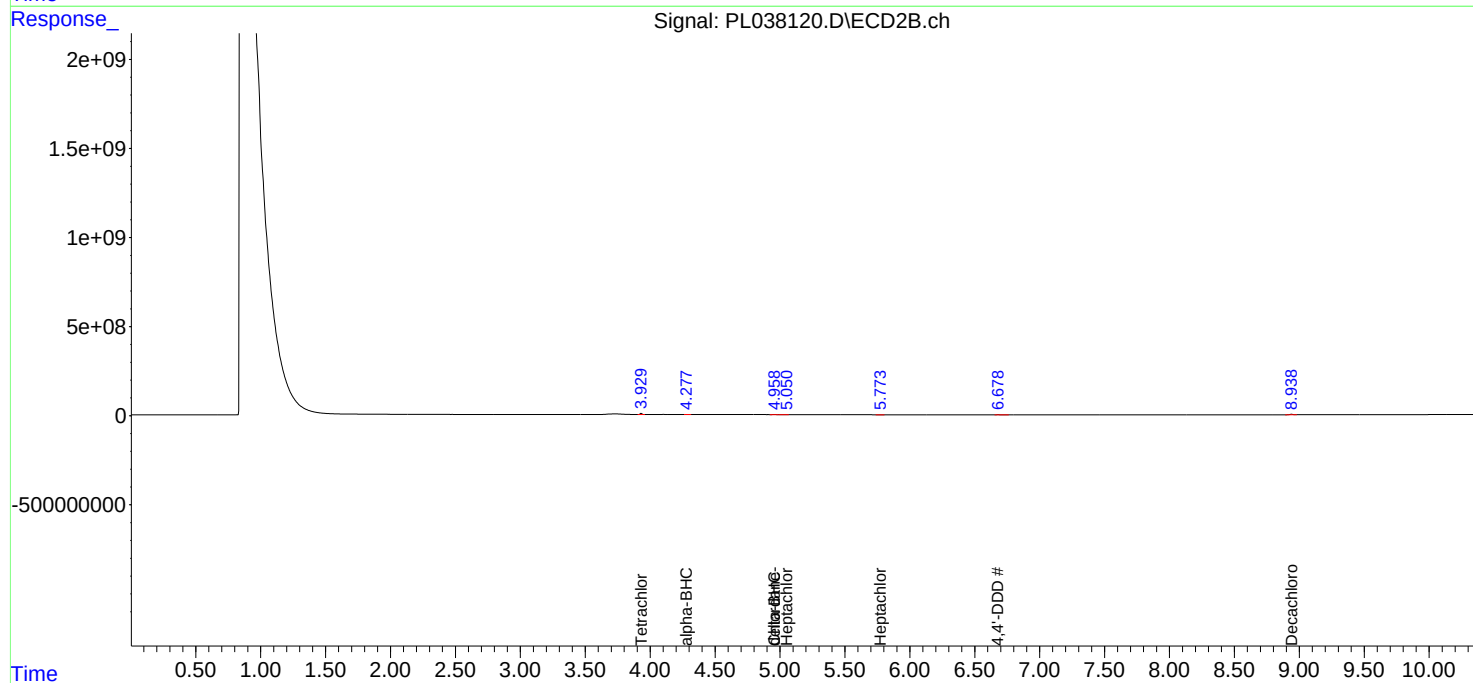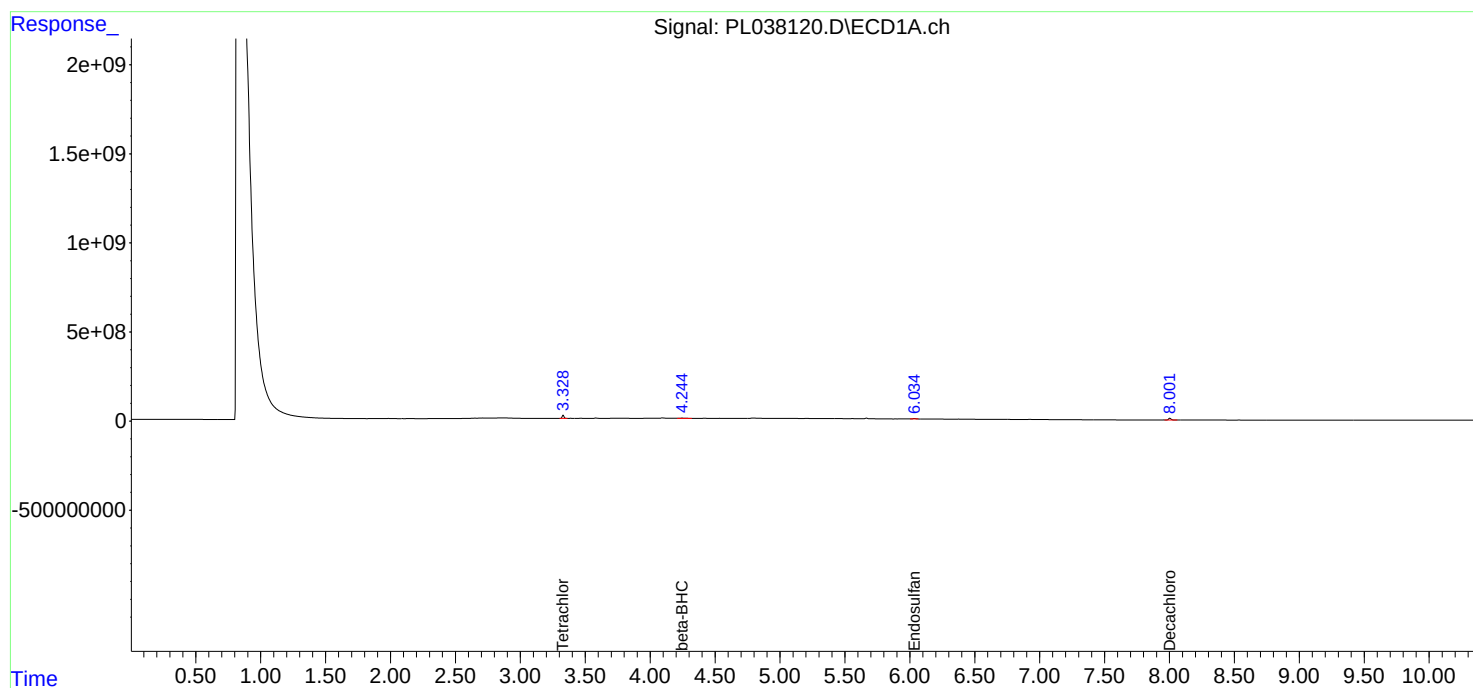


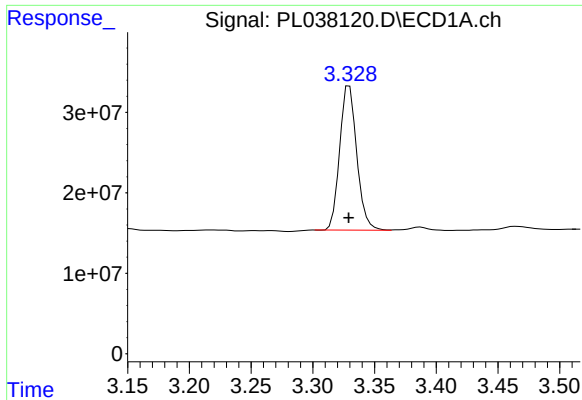

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 173021285
Conc: 23.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

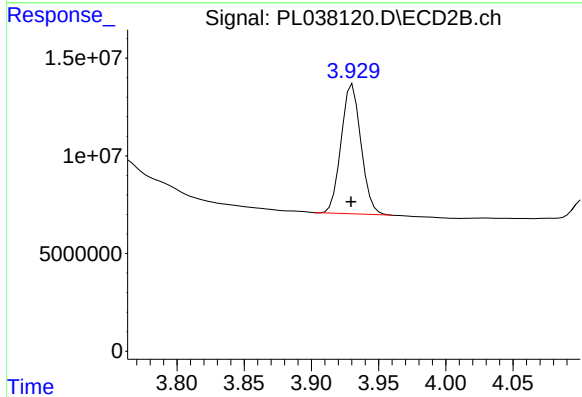


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 67858999
Conc: 25.85 ng/ml

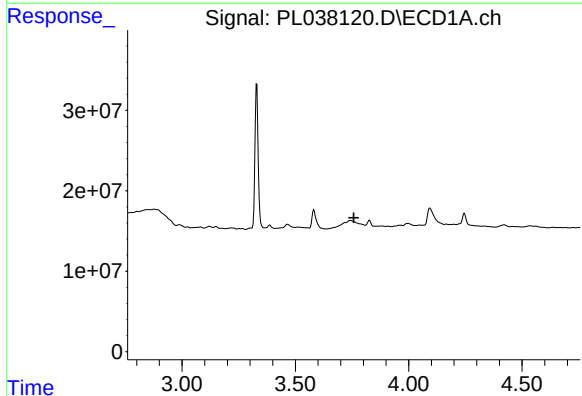


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

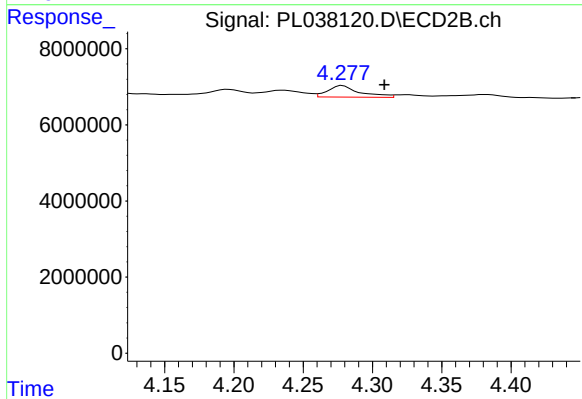

#2 alpha-BHC


R.T.: 4.279 min
Delta R.T.: -0.030 min
Response: 4866275
Conc: 1.26 ng/ml

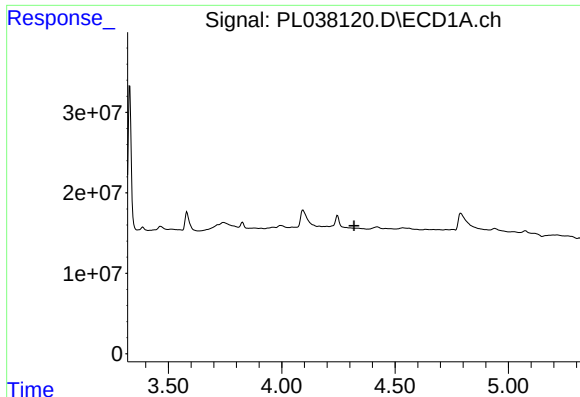

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

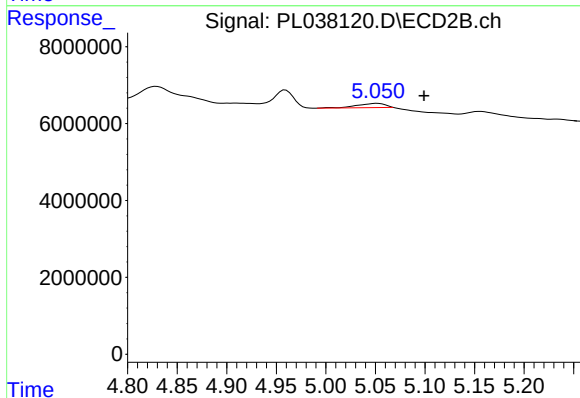


#4 Heptachlor

R.T.: 5.052 min
Delta R.T.: -0.047 min
Response: 2146596
Conc: 0.67 ng/ml

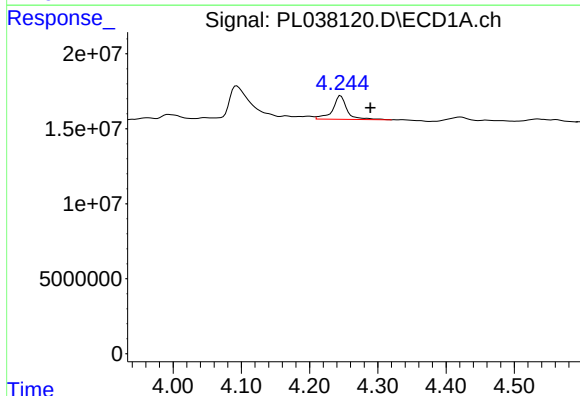


#6 beta-BHC

R.T.: 4.246 min
Delta R.T.: -0.044 min
Response: 23032110
Conc: 4.88 ng/ml

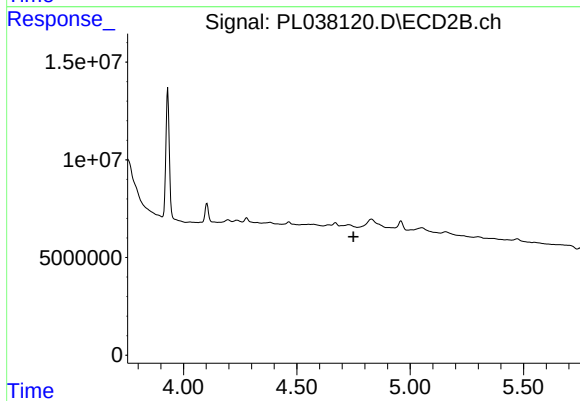

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.750 min
Response: 0
Conc: N.D.

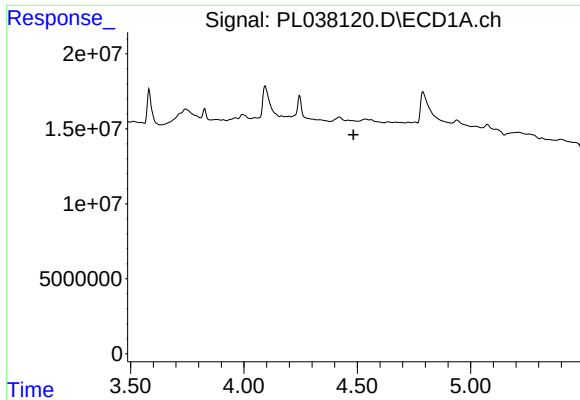

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

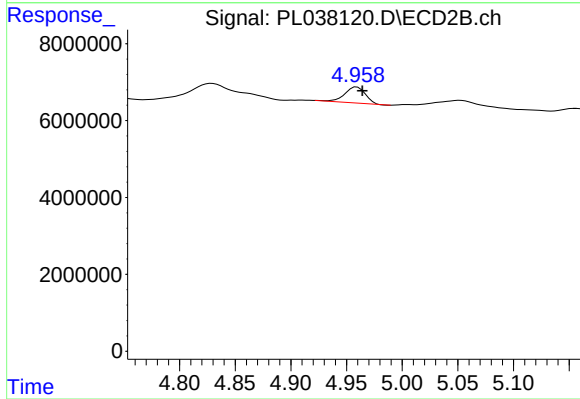


#7 delta-BHC

R.T.: 4.959 min
Delta R.T.: -0.005 min
Response: 5209937
Conc: 1.57 ng/ml

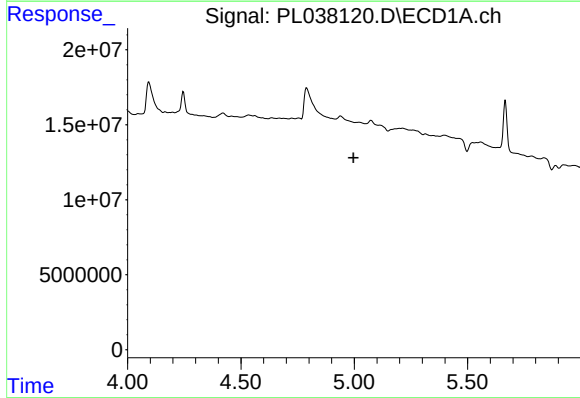


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

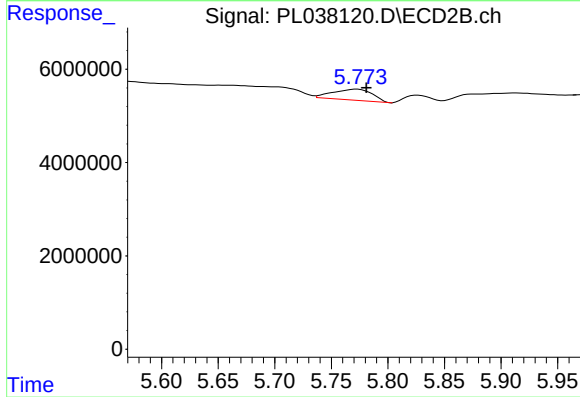

#8 Heptachlor epoxide


R.T.: 5.773 min
Delta R.T.: -0.008 min
Response: 5712173
Conc: 2.01 ng/ml

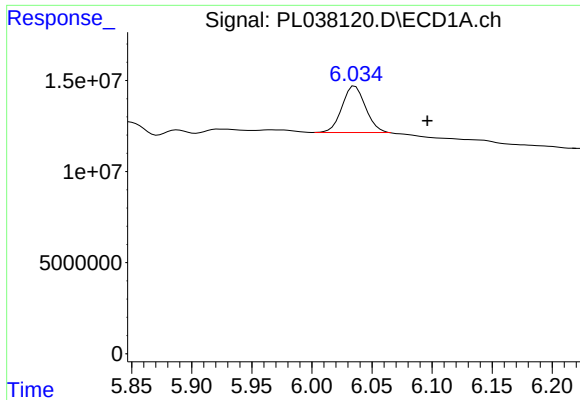

#15 Endosulfan II


R.T.: 6.036 min
Delta R.T.: -0.060 min
Response: 34617550
Conc: 4.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

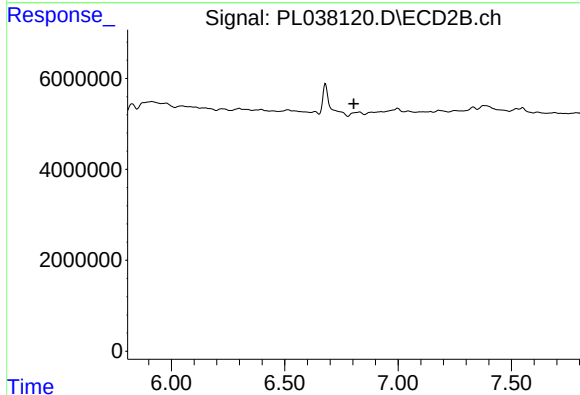


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

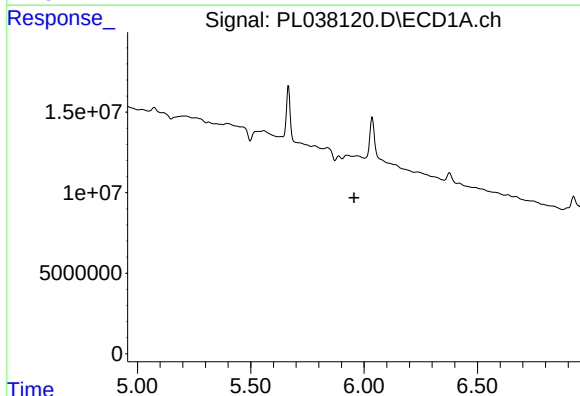


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

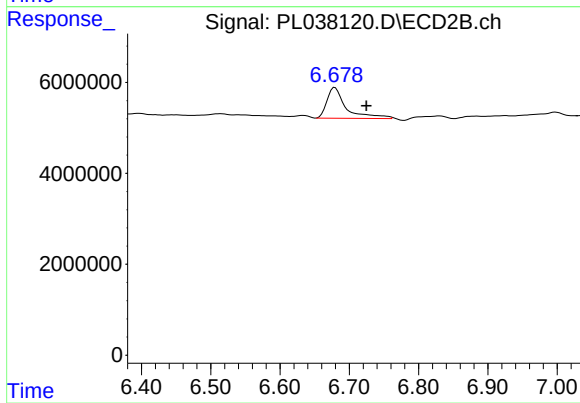

#16 4,4'-DDD


R.T.: 6.679 min
Delta R.T.: -0.045 min
Response: 13066259
Conc: 6.10 ng/ml

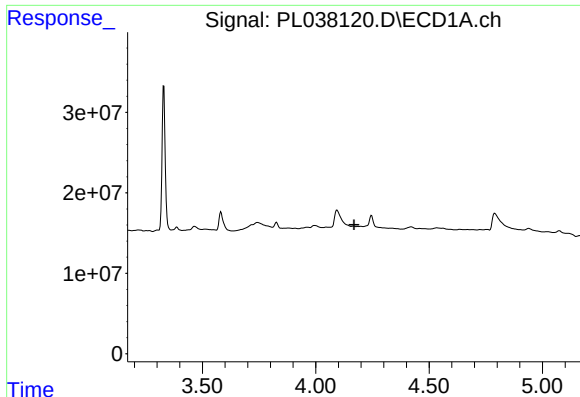

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

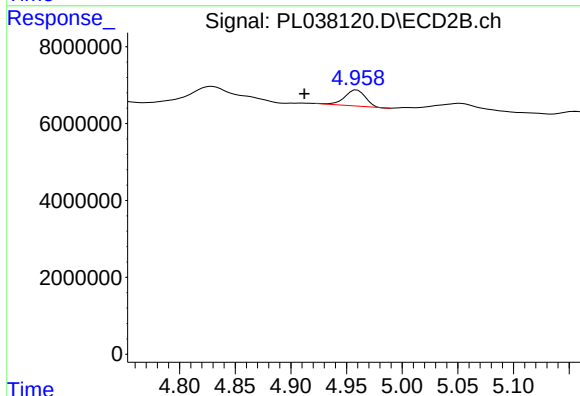


#23 Chlordane-1

R.T.: 4.959 min
Delta R.T.: 0.047 min
Response: 5209937
Conc: 44.96 ng/ml

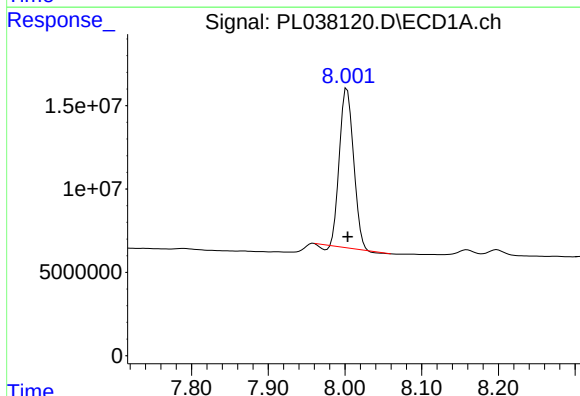

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 119962865
Conc: 15.81 ng/ml

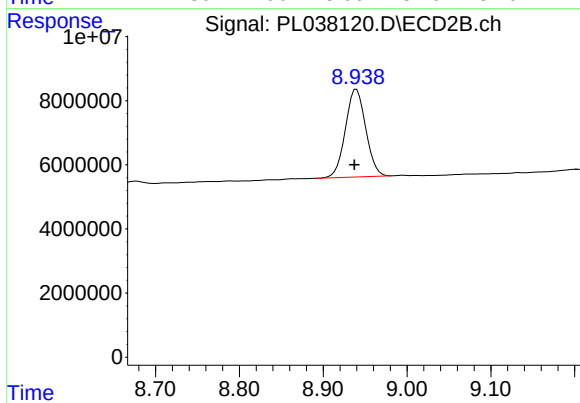

#28 Decachlorobiphenyl

R.T.: 8.940 min
Delta R.T.: 0.002 min
Response: 46374612
Conc: 18.97 ng/ml