

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071618\
 Data File : PL038136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2018 21:06
 Operator : AJ\SJ
 Sample : J3829-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:48:12 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.931	158.3E6	63882805	21.253	24.337
28)	SA Decachlor...	8.003	8.940	139.2E6	46867506	18.350	19.173
Target Compounds							
3)	MA gamma-BHC...	0.000	4.566	0	3320859	N.D.	0.919 #
6)	B beta-BHC	4.249f	0.000	10451505	0	2.214	N.D. #
7)	B delta-BHC	0.000	4.958	0	3812504	N.D.	1.150 #
15)	B Endosulfa...	6.036f	0.000	34411309	0	4.339	N.D. #
16)	A 4,4'-DDD	0.000	6.679f	0	11646844	N.D.	5.441 #
23)	Chlordane-1	4.101	4.958	22428456	3812504	64.775	32.899 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071618\
Data File : PL038136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2018 21:06
Operator : AJ\SJ
Sample : J3829-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:48:12 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

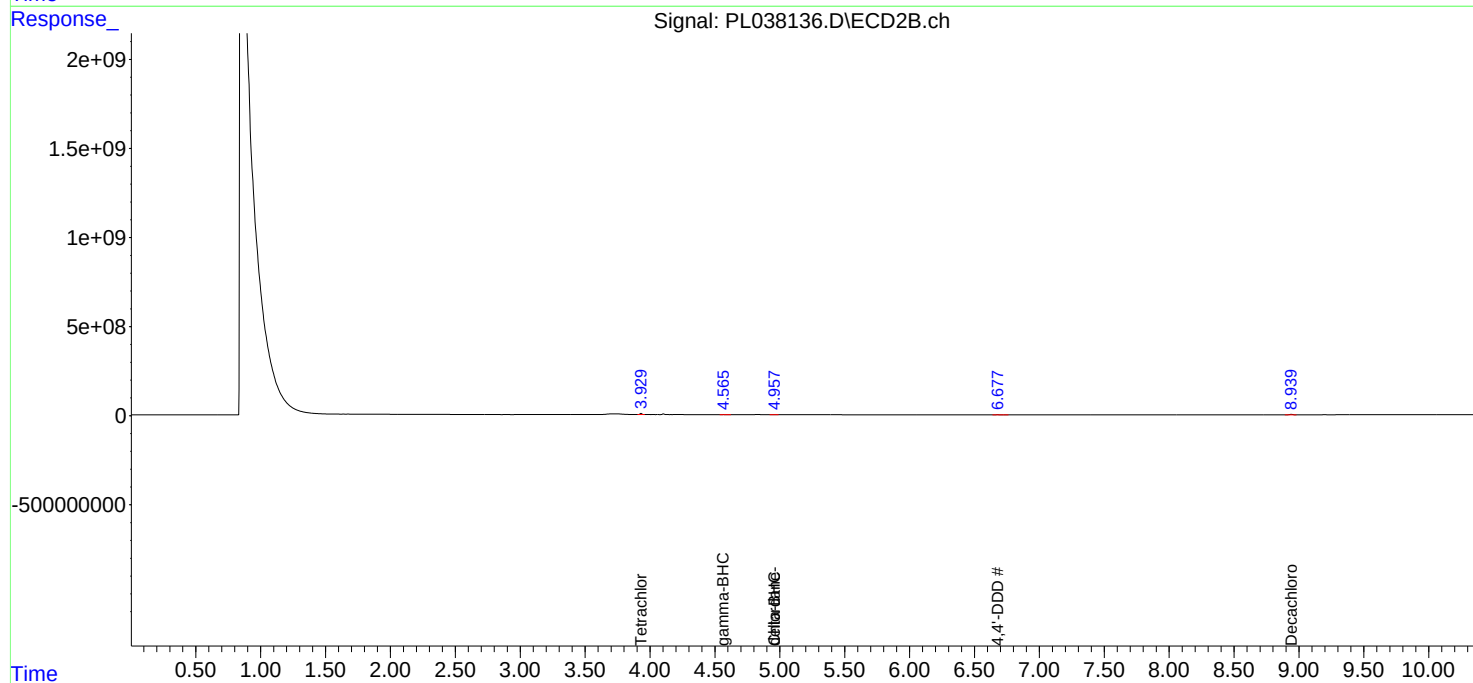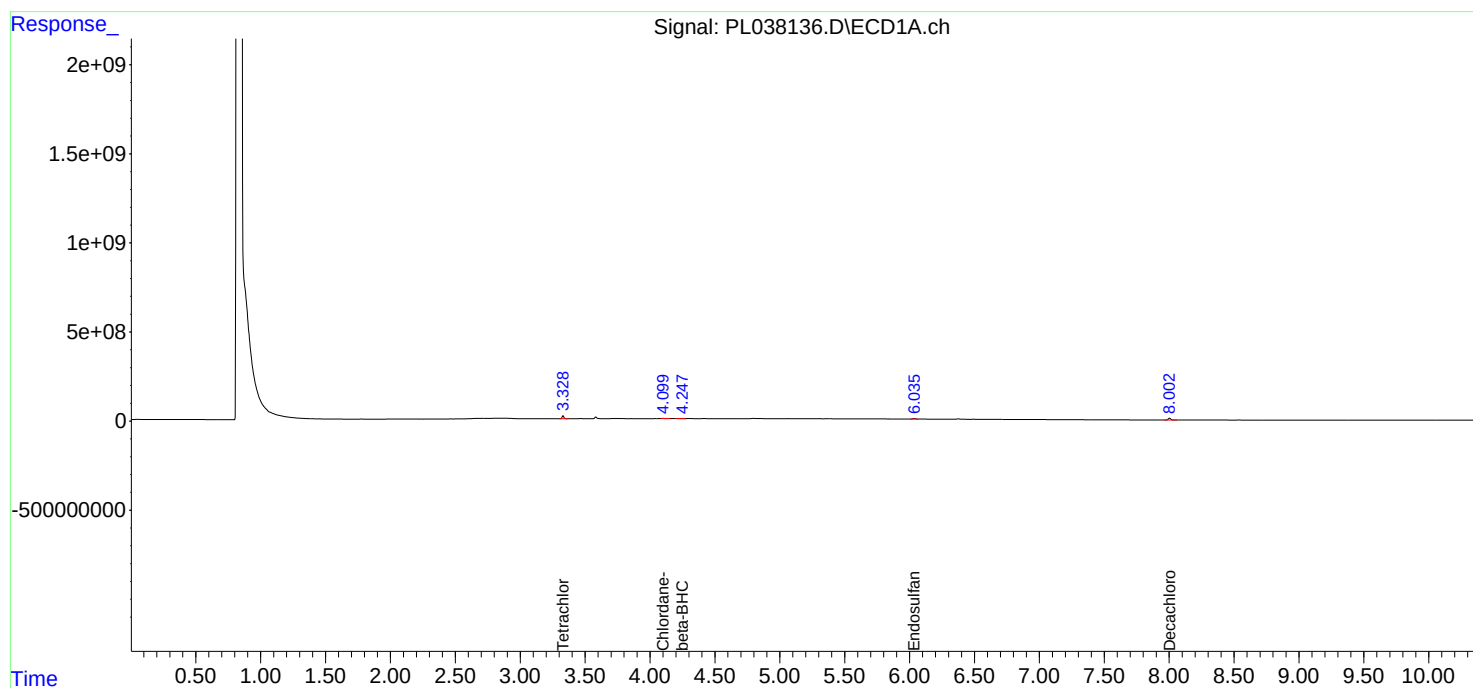


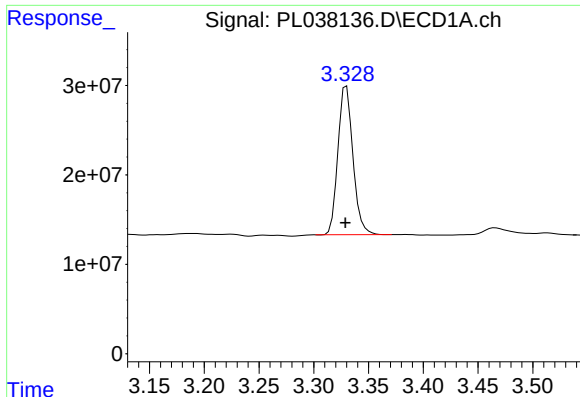

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 158261449
Conc: 21.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

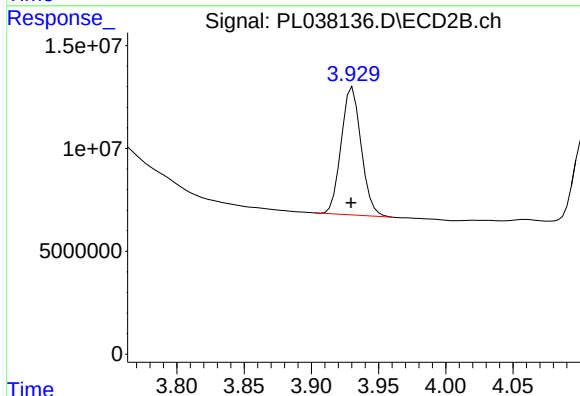


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 63882805
Conc: 24.34 ng/ml

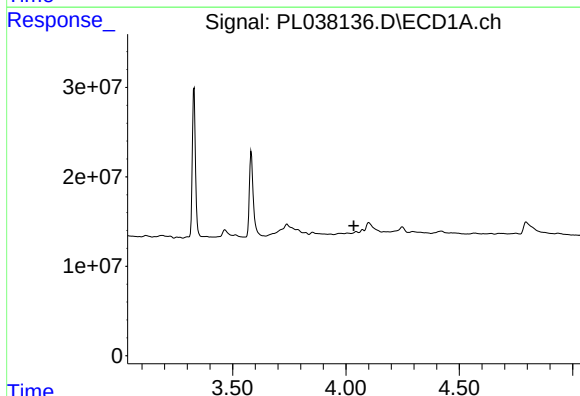


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

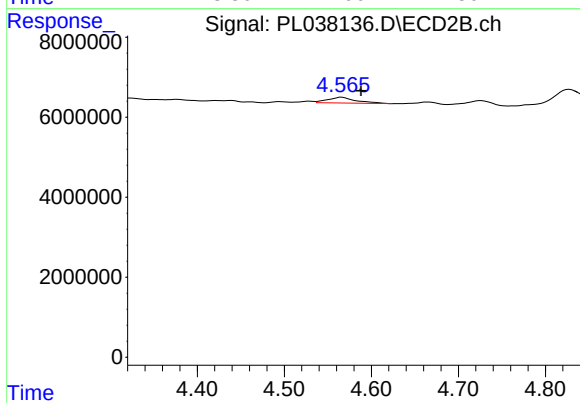

#3 gamma-BHC (Lindane)


R.T.: 4.566 min
Delta R.T.: -0.022 min
Response: 3320859
Conc: 0.92 ng/ml

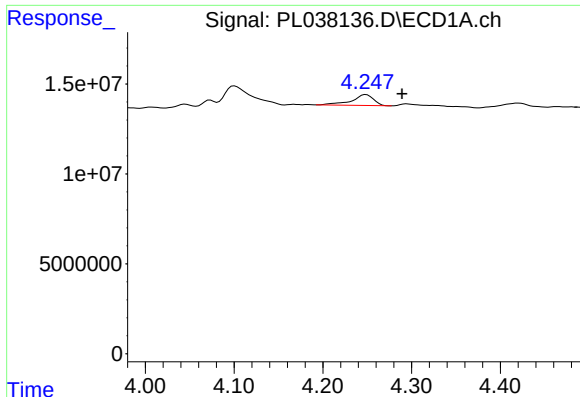

#6 beta-BHC


R.T.: 4.249 min
Delta R.T.: -0.041 min
Response: 10451505
Conc: 2.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

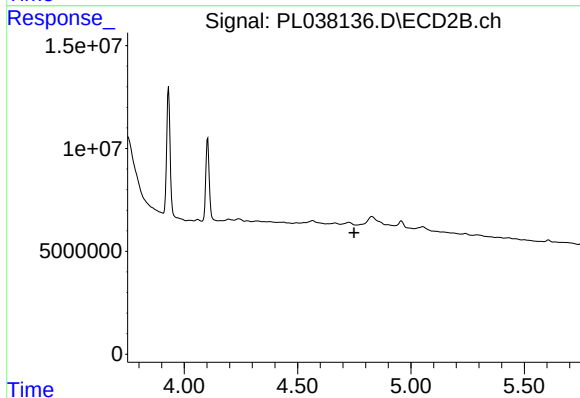


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

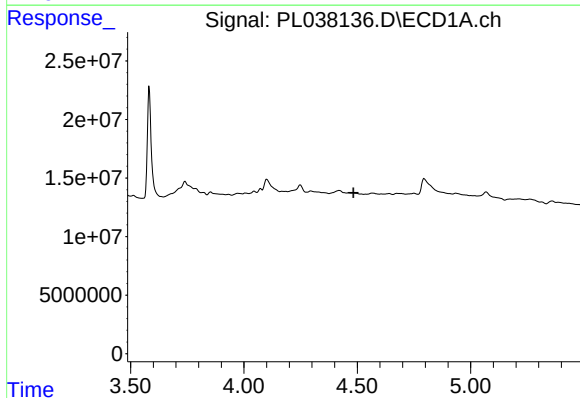


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

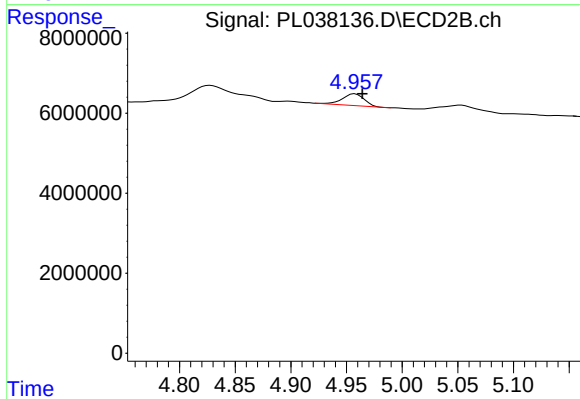

#7 delta-BHC


R.T.: 4.958 min
Delta R.T.: -0.007 min
Response: 3812504
Conc: 1.15 ng/ml

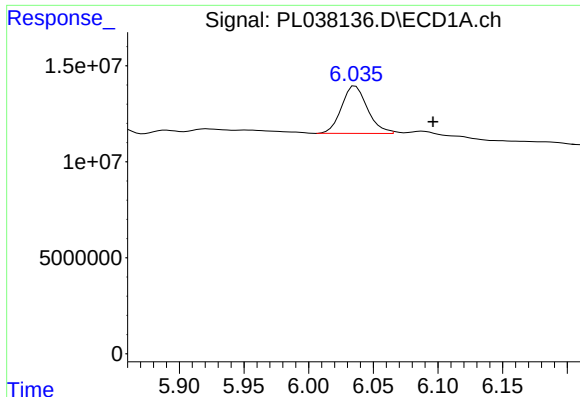

#15 Endosulfan II


R.T.: 6.036 min
Delta R.T.: -0.060 min
Response: 34411309
Conc: 4.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

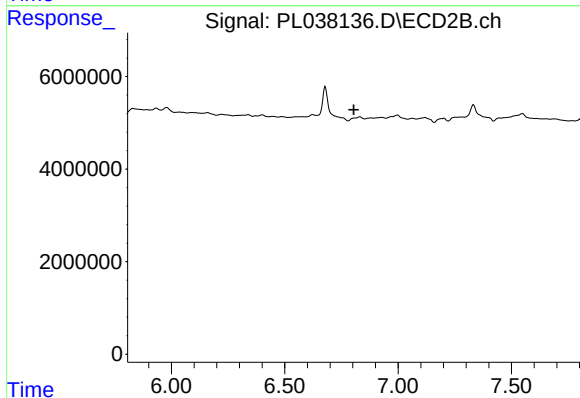


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

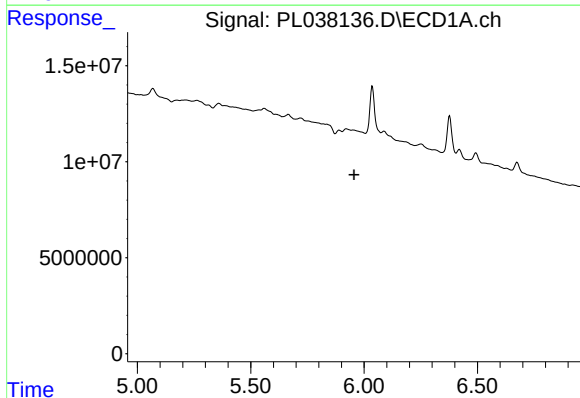


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

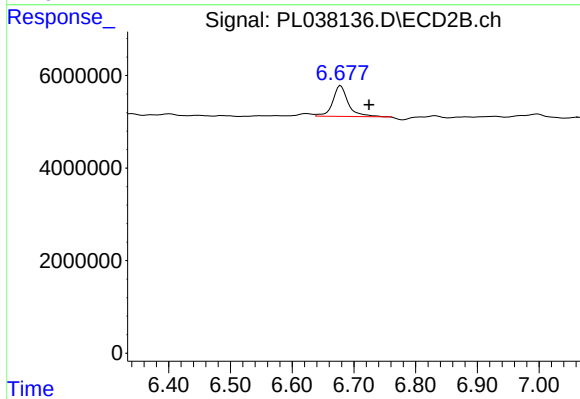

#16 4,4'-DDD


R.T.: 6.679 min
Delta R.T.: -0.046 min
Response: 11646844
Conc: 5.44 ng/ml

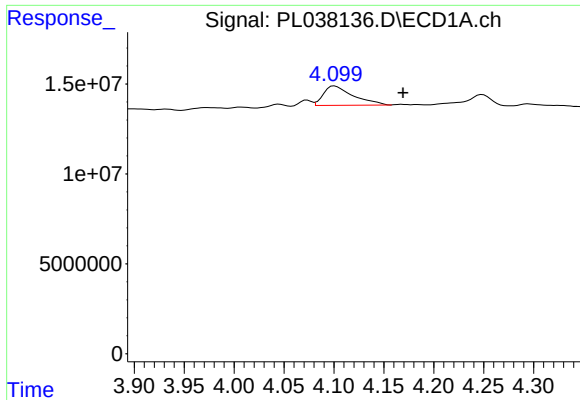

#23 Chlordane-1


R.T.: 4.101 min
Delta R.T.: -0.069 min
Response: 22428456
Conc: 64.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

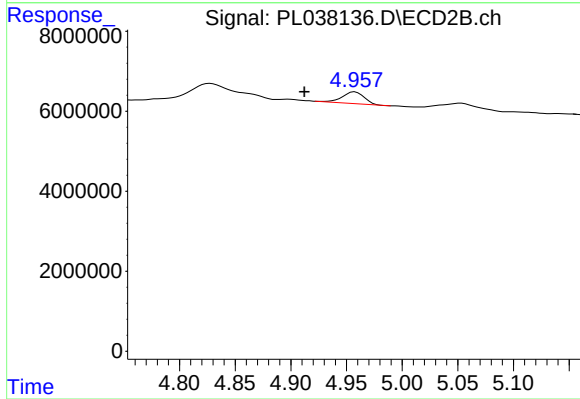


#23 Chlordane-1

R.T.: 4.958 min
Delta R.T.: 0.045 min
Response: 3812504
Conc: 32.90 ng/ml

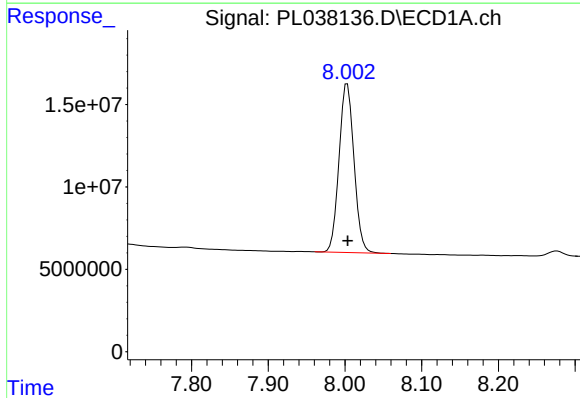

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 139204386
Conc: 18.35 ng/ml

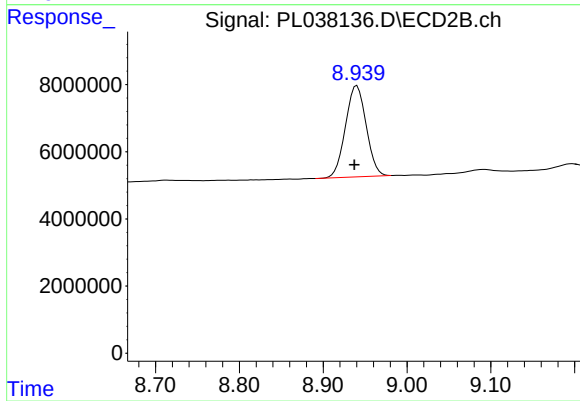

#28 Decachlorobiphenyl

R.T.: 8.940 min
Delta R.T.: 0.003 min
Response: 46867506
Conc: 19.17 ng/ml