

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071618\
 Data File : PL038162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 04:29
 Operator : AJ\SJ
 Sample : J3996-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 05:38:41 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.340	3.930	85540406	33440482	11.487	12.740
28)	SA Decachlor...	8.015	8.944	80702000	27855520	10.638	11.395
Target Compounds							
2)	A alpha-BHC	0.000	4.352f	0	19552690	N.D.	5.052 #
7)	B delta-BHC	4.496	0.000	5538186	0	0.510	N.D. #
14)	MA Endrin	0.000	6.596	0	49682291	N.D.	20.804 #
15)	B Endosulfa...	6.028f	6.812	119.6E6	3369773	15.083	1.403 #
16)	A 4,4'-DDD	5.957	0.000	230.1E6	0	31.365	N.D. #
21)	B Endrin ke...	0.000	7.619	0	1485258	N.D.	0.623 #
23)	Chlordane-1	4.106	0.000	27172421	0	78.476	N.D. #
27)	Chlordane-5	0.000	6.812	0	3369773	N.D.	37.618 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071618\
Data File : PL038162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 04:29
Operator : AJ\SJ
Sample : J3996-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 05:38:41 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

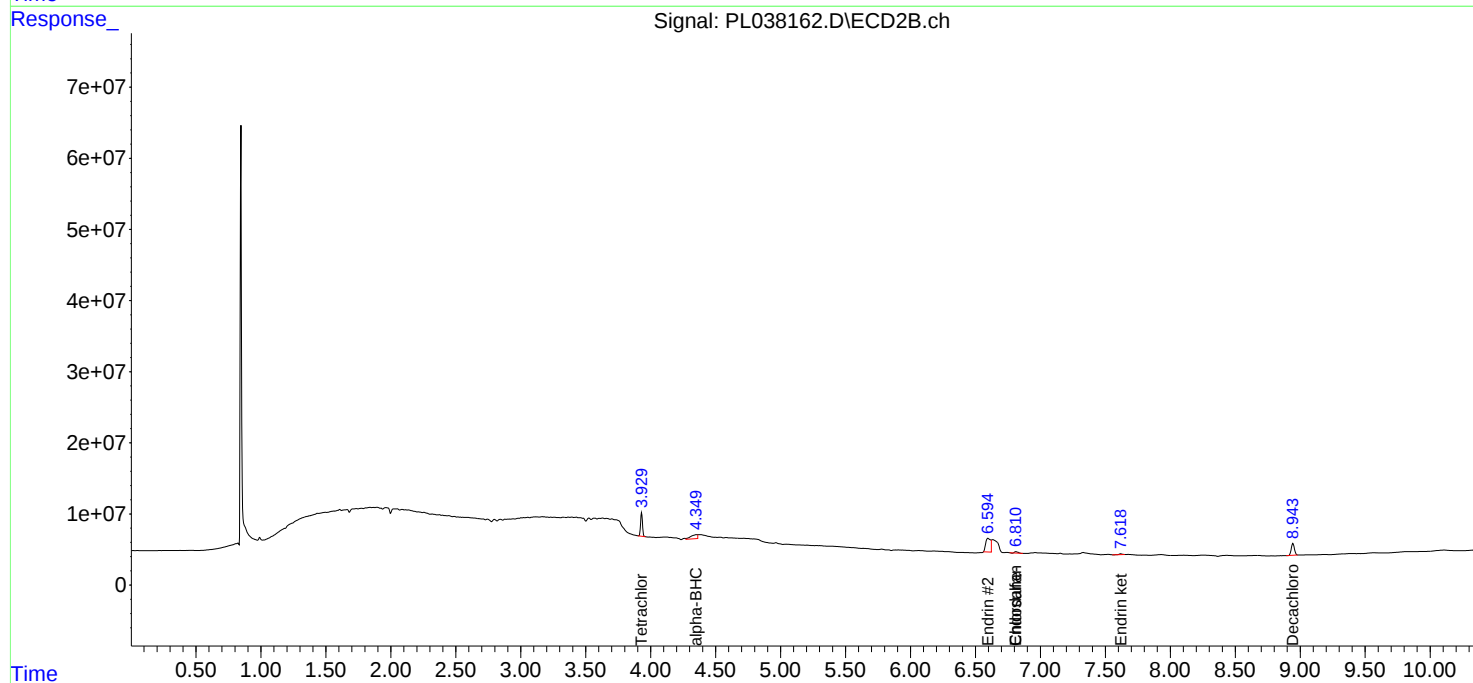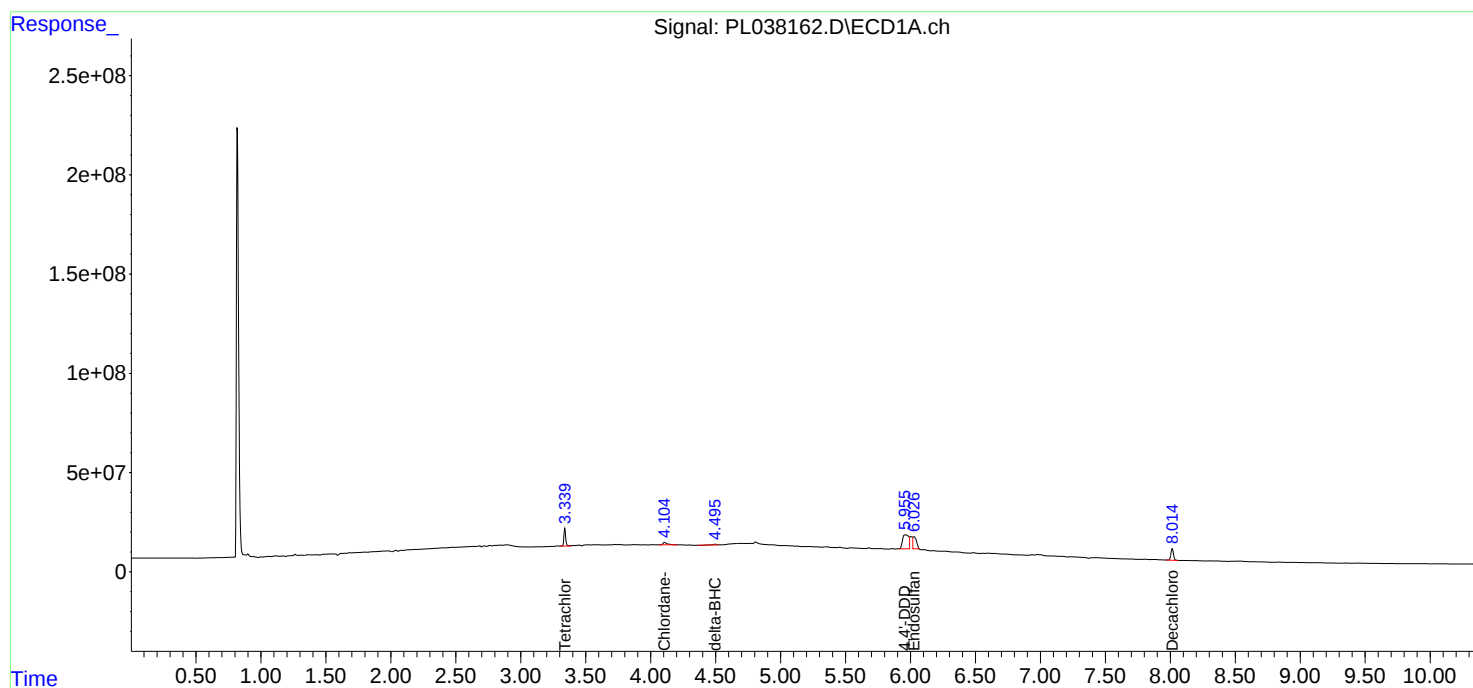


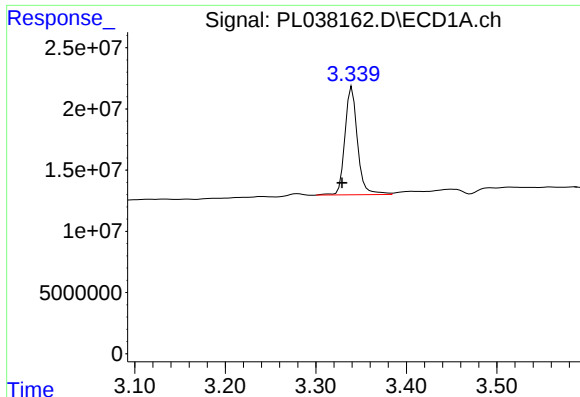

#1 Tetrachloro-m-xylene


R.T.: 3.340 min
Delta R.T.: 0.011 min
Response: 85540406
Conc: 11.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

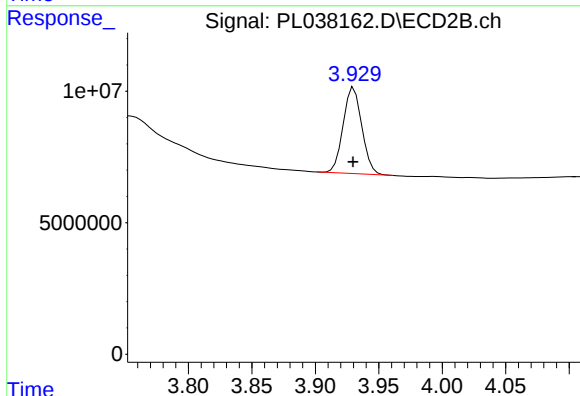


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 33440482
Conc: 12.74 ng/ml

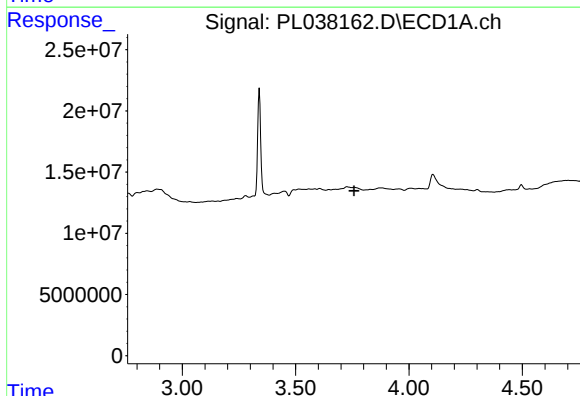


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

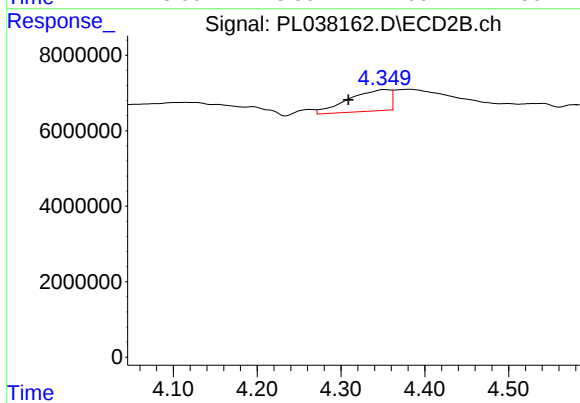

#2 alpha-BHC


R.T.: 4.352 min
Delta R.T.: 0.043 min
Response: 19552690
Conc: 5.05 ng/ml

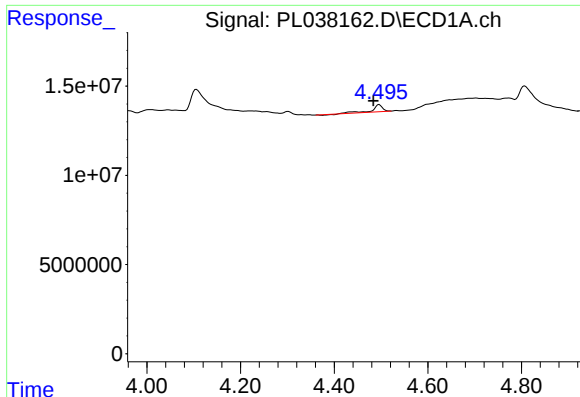

#7 delta-BHC


R.T.: 4.496 min
Delta R.T.: 0.012 min
Response: 5538186
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

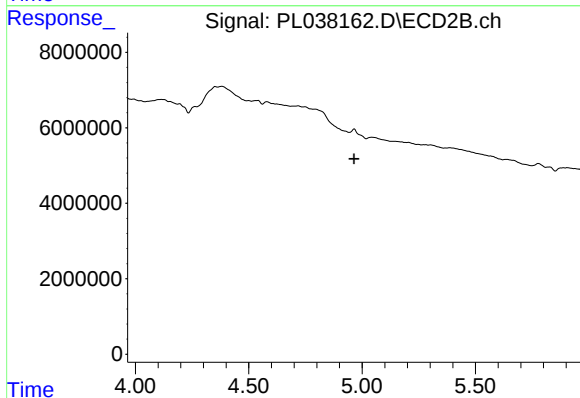


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.964 min
Response: 0
Conc: N.D.

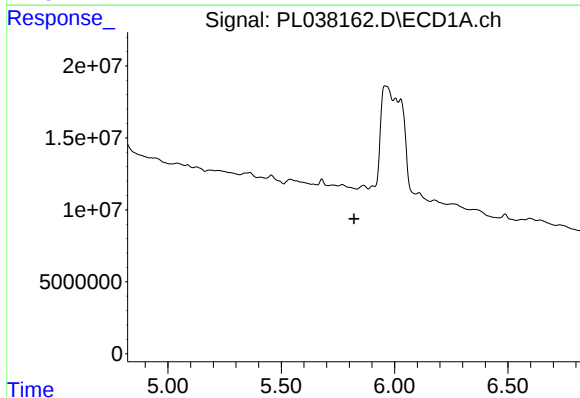


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.821 min
Response: 0
Conc: N.D.

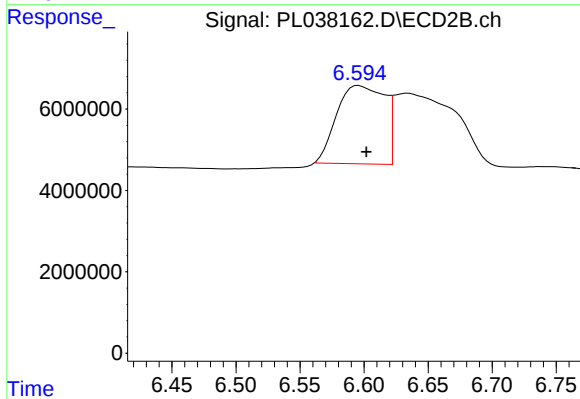

#14 Endrin


R.T.: 6.596 min
Delta R.T.: -0.006 min
Response: 49682291
Conc: 20.80 ng/ml

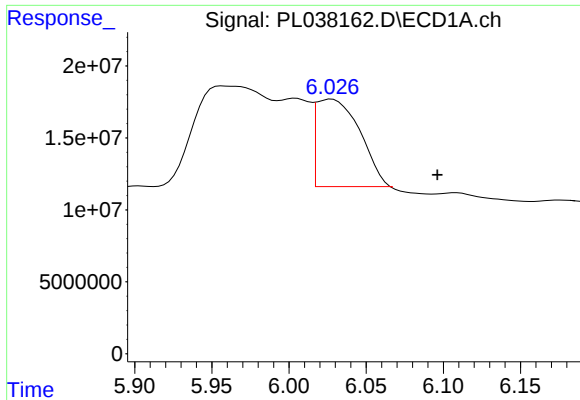

#15 Endosulfan II


R.T.: 6.028 min
Delta R.T.: -0.068 min
Response: 119610384
Conc: 15.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

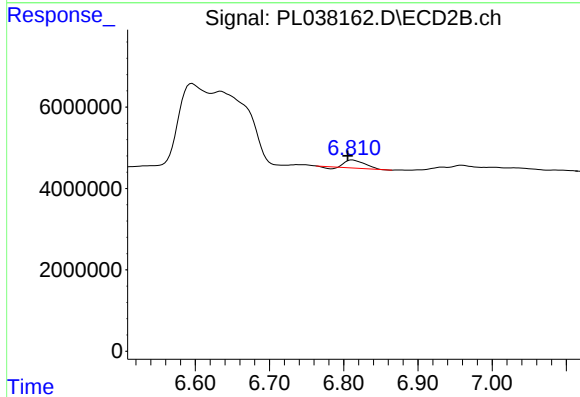


#15 Endosulfan II

R.T.: 6.812 min
Delta R.T.: 0.006 min
Response: 3369773
Conc: 1.40 ng/ml

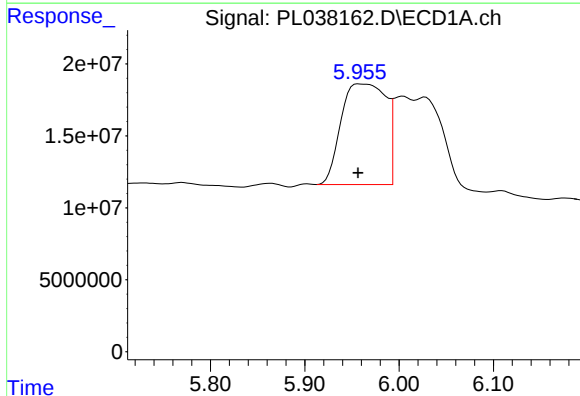


#16 4,4'-DDD

R.T.: 5.957 min
Delta R.T.: 0.000 min
Response: 230079752
Conc: 31.36 ng/ml

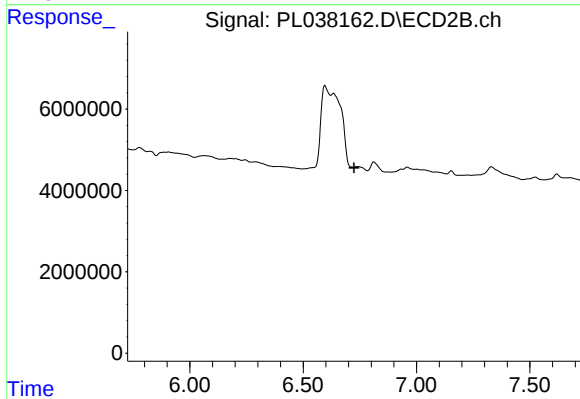

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.725 min
Response: 0
Conc: N.D.

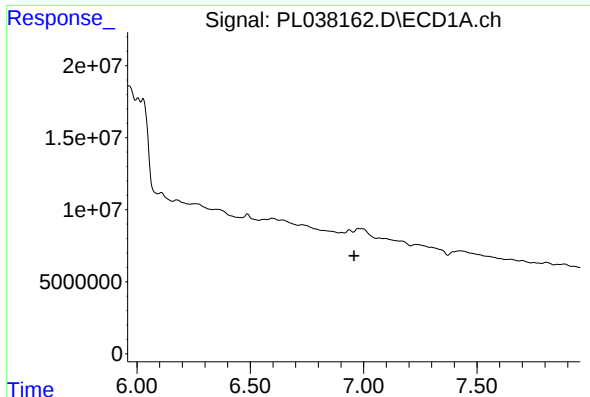

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.958 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

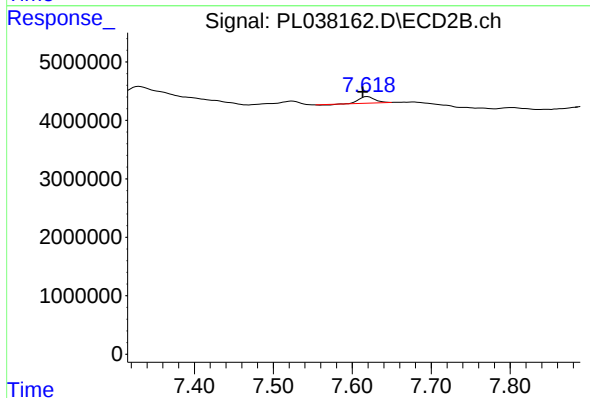


#21 Endrin ketone

R.T.: 7.619 min
Delta R.T.: 0.006 min
Response: 1485258
Conc: 0.62 ng/ml

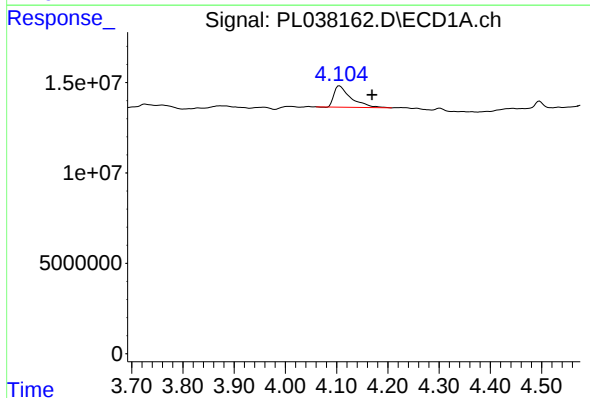


#23 Chlordane-1

R.T.: 4.106 min
Delta R.T.: -0.064 min
Response: 27172421
Conc: 78.48 ng/ml

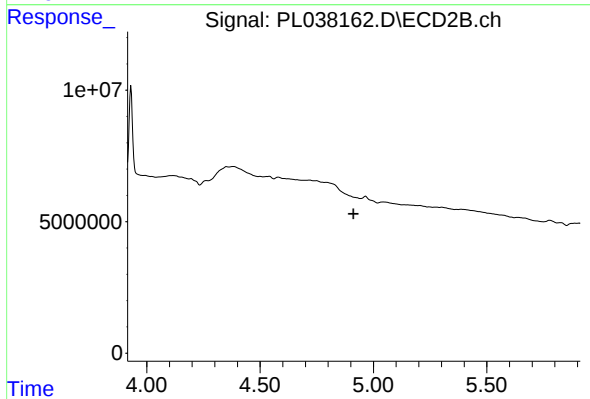

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.912 min
Response: 0
Conc: N.D.

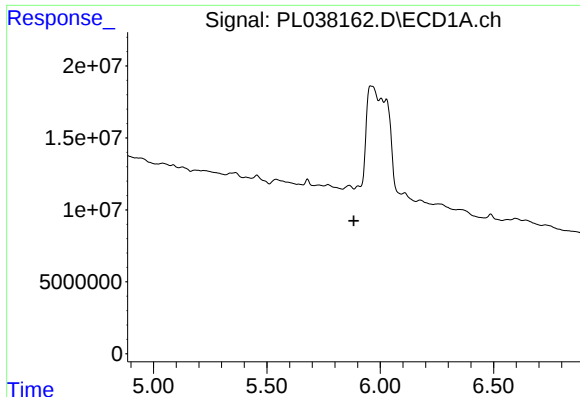

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

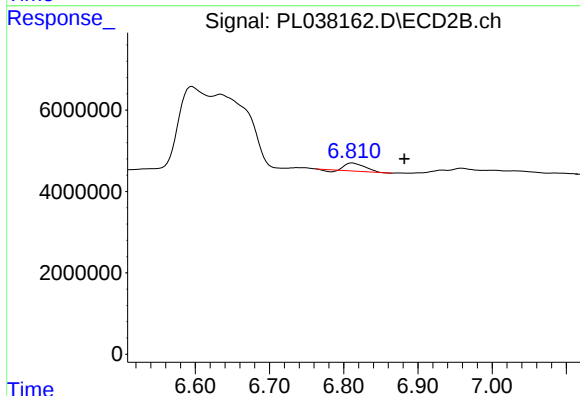


#27 Chlordane-5

R.T.: 6.812 min
Delta R.T.: -0.070 min
Response: 3369773
Conc: 37.62 ng/ml

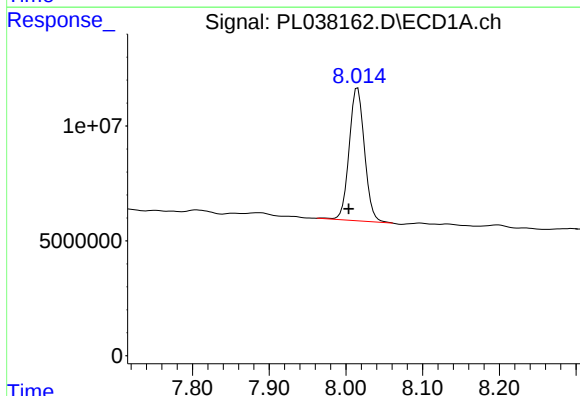

#28 Decachlorobiphenyl

R.T.: 8.015 min
Delta R.T.: 0.012 min
Response: 80702000
Conc: 10.64 ng/ml

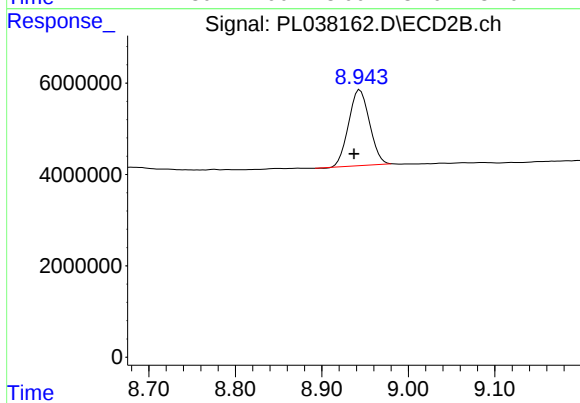

#28 Decachlorobiphenyl

R.T.: 8.944 min
Delta R.T.: 0.007 min
Response: 27855520
Conc: 11.40 ng/ml