

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071618\
 Data File : PL038163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 04:43
 Operator : AJ\SJ
 Sample : J3997-03
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 05:38:52 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.331	3.931	68566190	27537692	9.208	10.491
28)	SA Decachlor...	8.006	8.940	68251389	25456634	8.997	10.414
Target Compounds							
15)	B Endosulfa...	6.038f	0.000	26521562	0	3.344	N.D. #
16)	A 4,4'-DDD	0.000	6.679f	0	6541523	N.D.	3.056 #
20)	A Methoxychlor	0.000	7.422f	0	1387788	N.D.	1.219 #
23)	Chlordane-1	4.108	0.000	18601659	0	53.723	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071618\
Data File : PL038163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 04:43
Operator : AJ\SJ
Sample : J3997-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 05:38:52 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

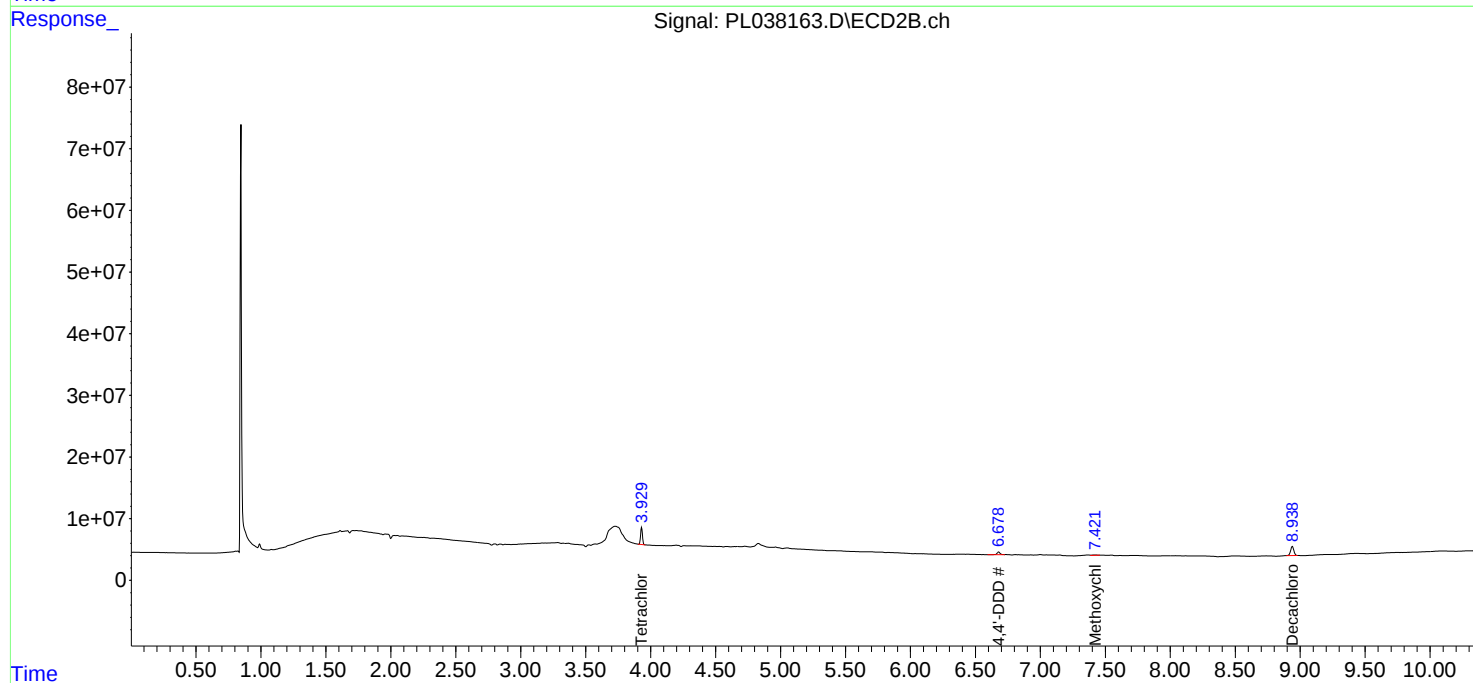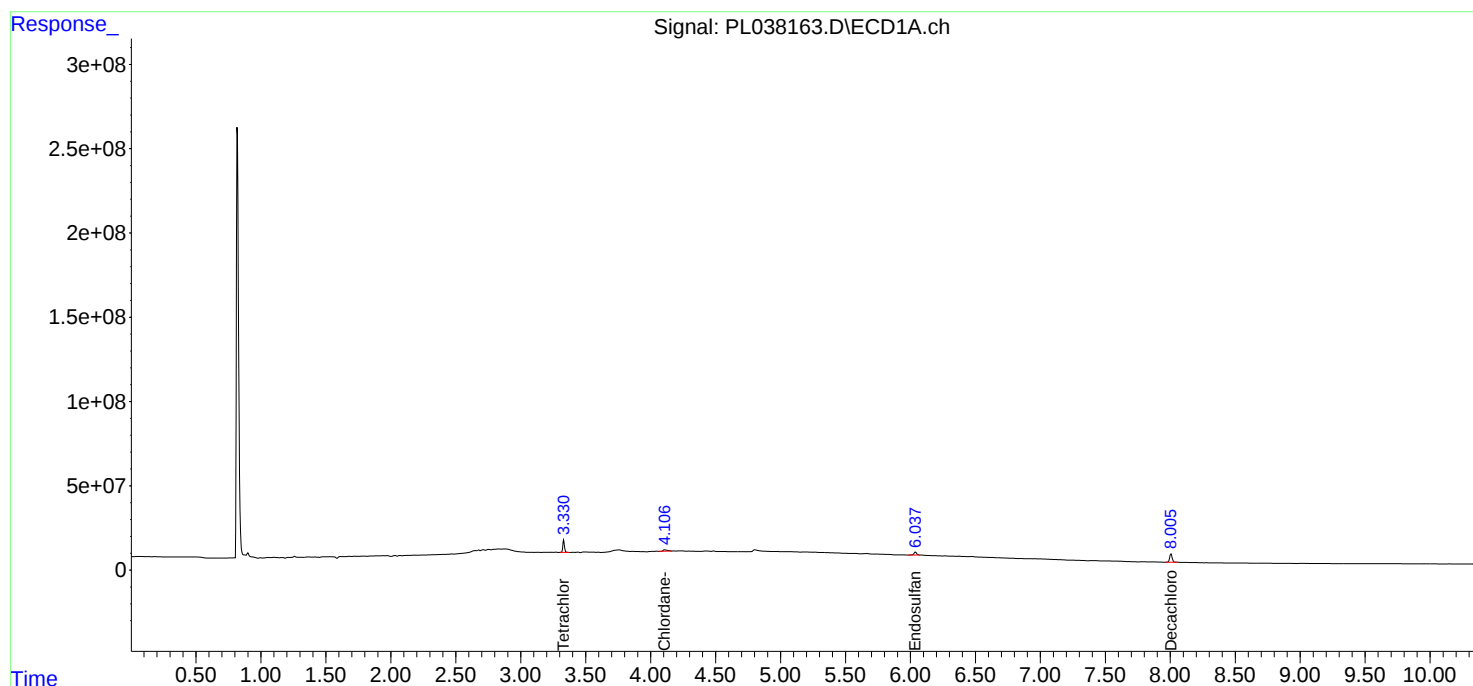


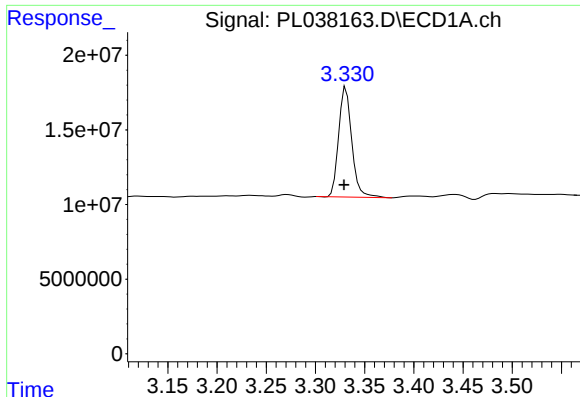

#1 Tetrachloro-m-xylene


R.T.: 3.331 min
Delta R.T.: 0.002 min
Response: 68566190
Conc: 9.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

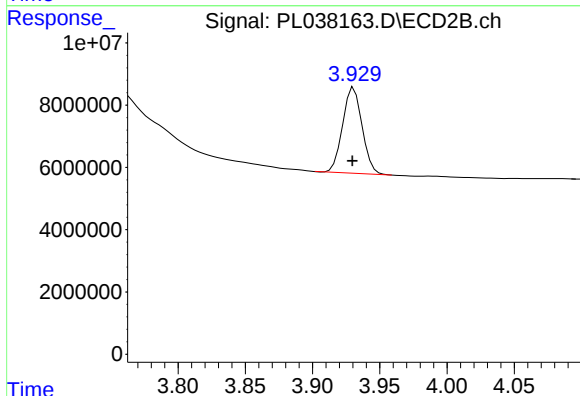


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.001 min
Response: 27537692
Conc: 10.49 ng/ml

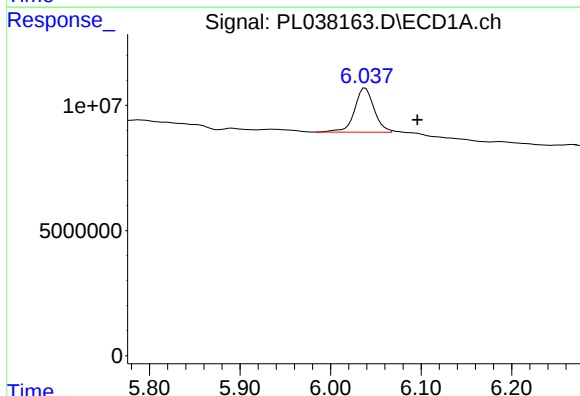


#15 Endosulfan II

R.T.: 6.038 min
Delta R.T.: -0.058 min
Response: 26521562
Conc: 3.34 ng/ml

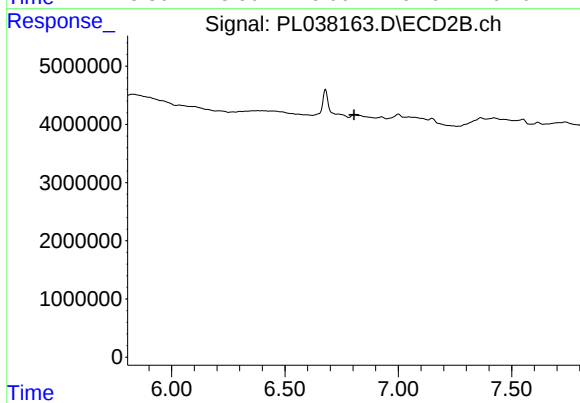

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.805 min
Response: 0
Conc: N.D.

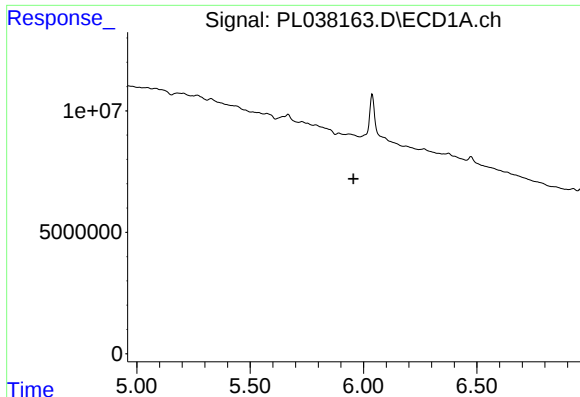

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

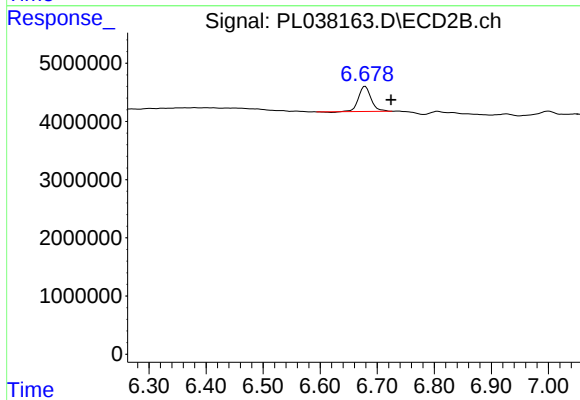


#16 4,4'-DDD

R.T.: 6.679 min
Delta R.T.: -0.046 min
Response: 6541523
Conc: 3.06 ng/ml

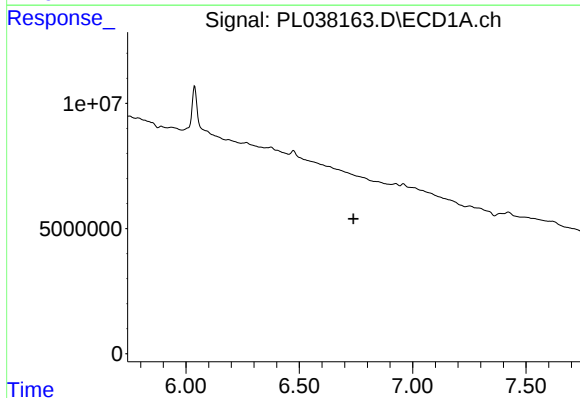


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.739 min
Response: 0
Conc: N.D.

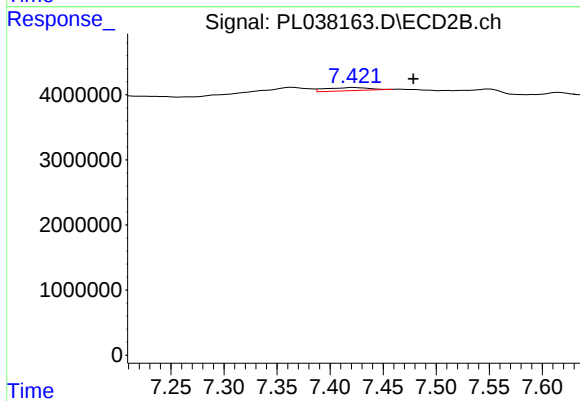

#20 Methoxychlor


R.T.: 7.422 min
Delta R.T.: -0.056 min
Response: 1387788
Conc: 1.22 ng/ml

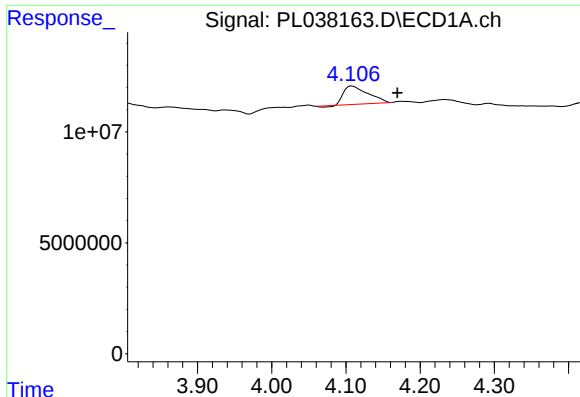

#23 Chlordane-1


R.T.: 4.108 min
Delta R.T.: -0.061 min
Response: 18601659
Conc: 53.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

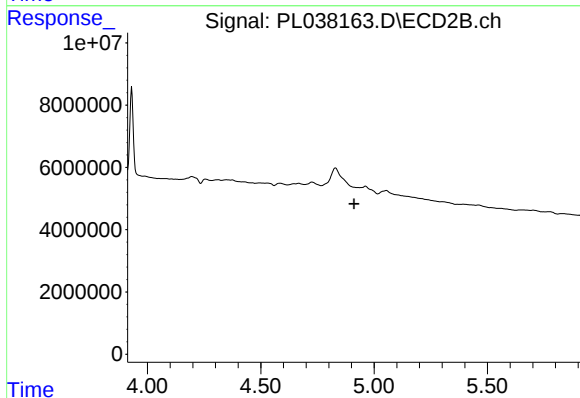


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.912 min
Response: 0
Conc: N.D.

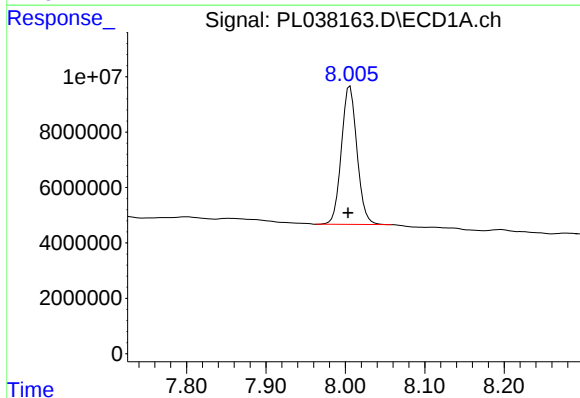

#28 Decachlorobiphenyl

R.T.: 8.006 min
Delta R.T.: 0.002 min
Response: 68251389
Conc: 9.00 ng/ml

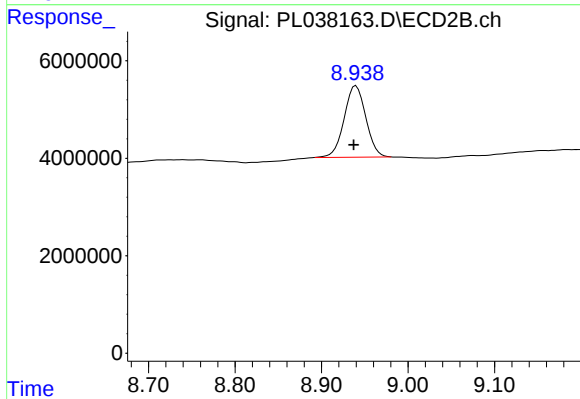

#28 Decachlorobiphenyl

R.T.: 8.940 min
Delta R.T.: 0.002 min
Response: 25456634
Conc: 10.41 ng/ml