

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
 Data File : PL050377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2019 09:10
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:06:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	0.000	5.791	0	42876349	N.D.	11.793 #
9) A	Endosulfan I	5.337f	0.000	26615386	0	1.720	N.D. #
10) B	gamma-Chl...	0.000	6.025	0	44966112	N.D.	12.067 #
11) B	alpha-Chl...	0.000	6.099	0	14303837	N.D.	3.868 #
12) B	4,4'-DDE	5.461f	0.000	51640923	0	3.100	N.D. #
14) MA	Endrin	5.820	6.629	49013764	13112756	3.061	4.153 #
15) B	Endosulfa...	6.070	0.000	53973484	0	3.704	N.D. #
24)	Chlordane-2	4.638f	0.000	263.8E6	0	451.618	N.D. #
25)	Chlordane-3	0.000	6.025	0	44966112	N.D.	90.361 #
26)	Chlordane-4	0.000	6.099	0	14303837	N.D.	24.067 #
27)	Chlordane-5	6.070f	0.000	53973484	0	96.174	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
Data File : PL050377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2019 09:10
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:06:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

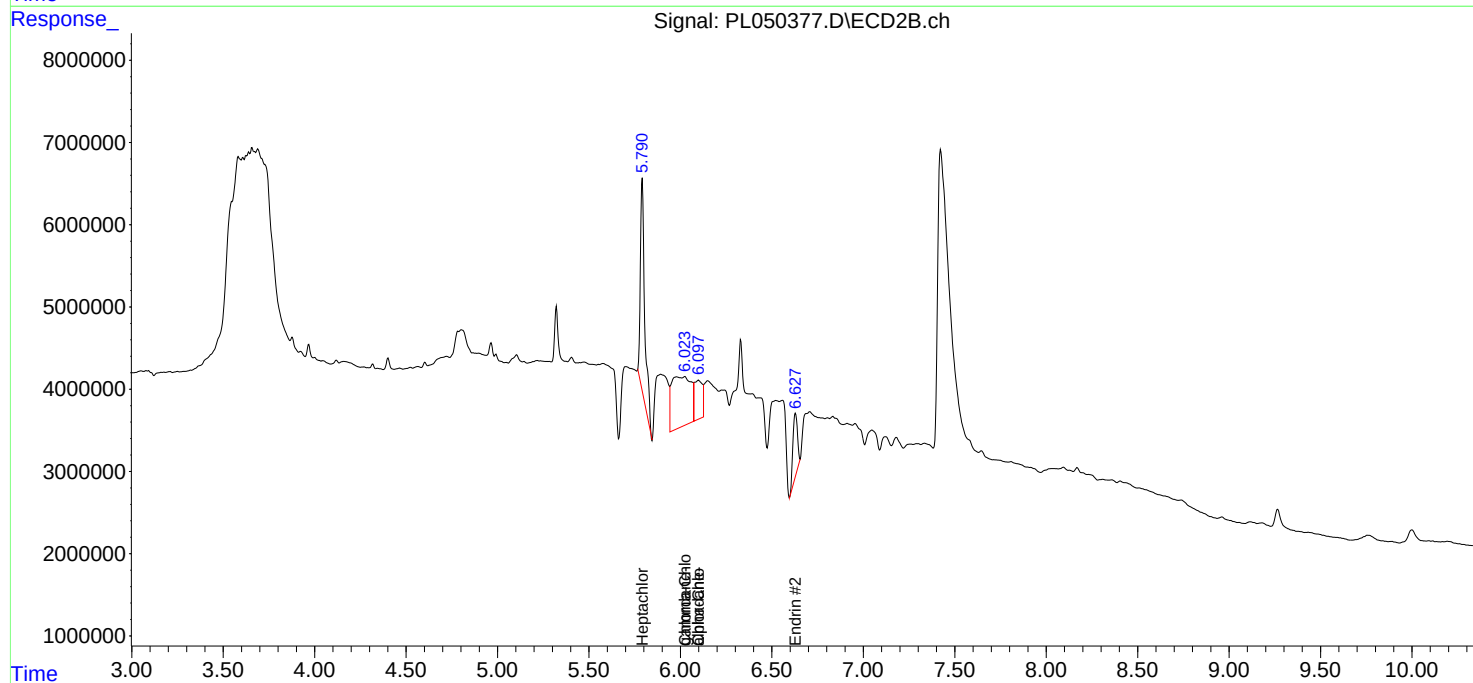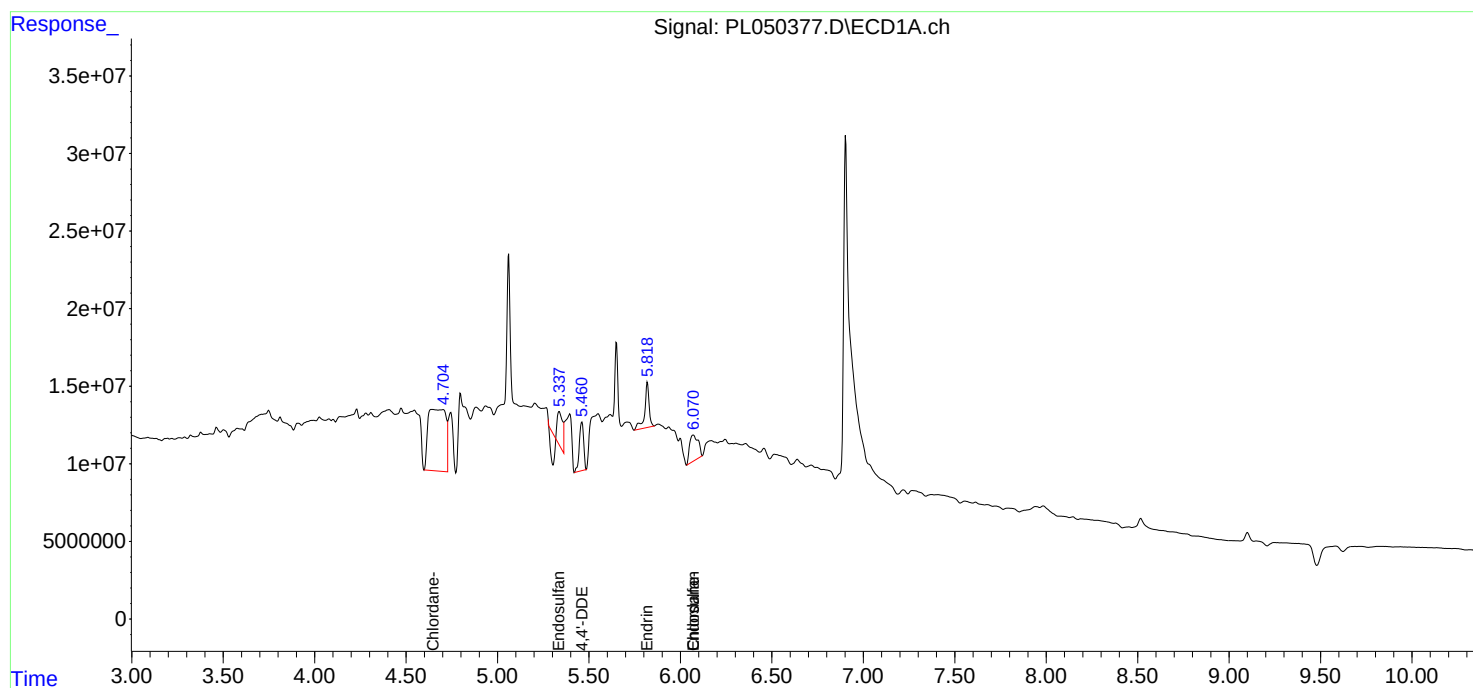


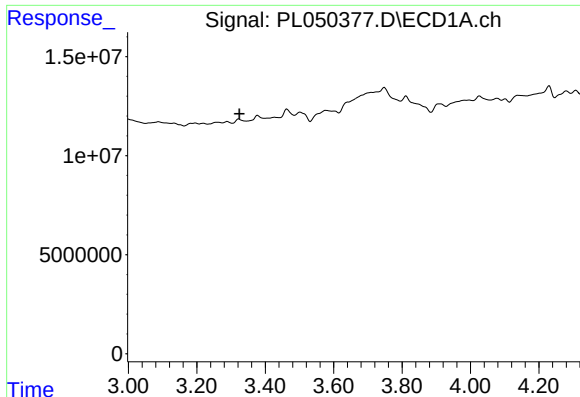

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

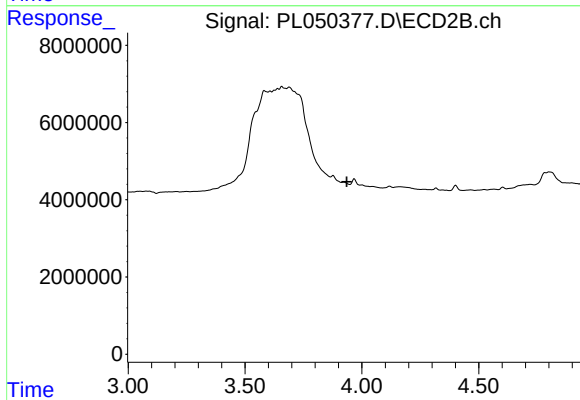


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.935 min
Response: 0
Conc: N.D.

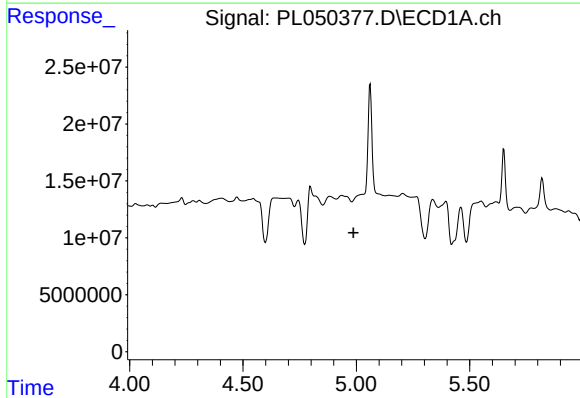


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

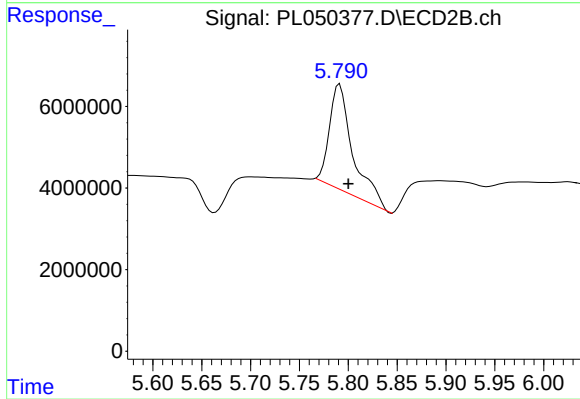

#8 Heptachlor epoxide


R.T.: 5.791 min
Delta R.T.: -0.009 min
Response: 42876349
Conc: 11.79 ng/ml

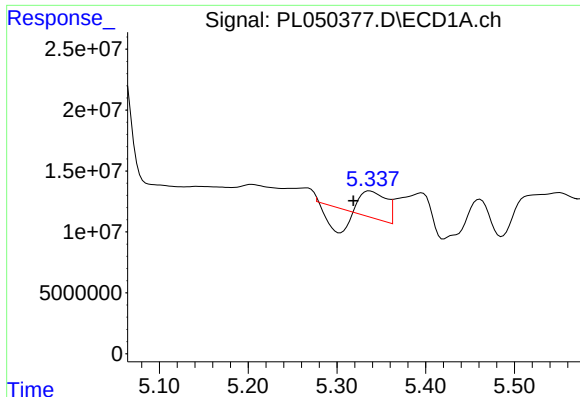

#9 Endosulfan I


R.T.: 5.337 min
Delta R.T.: 0.019 min
Response: 26615386
Conc: 1.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

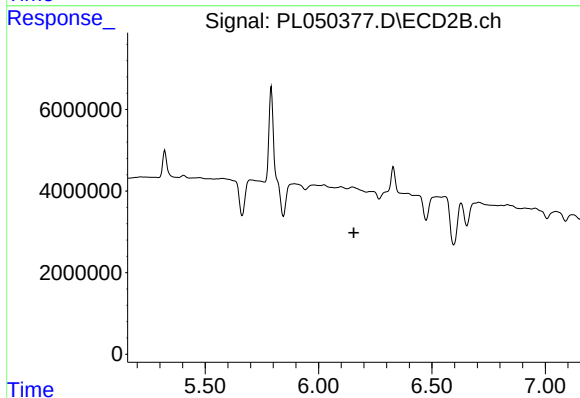


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

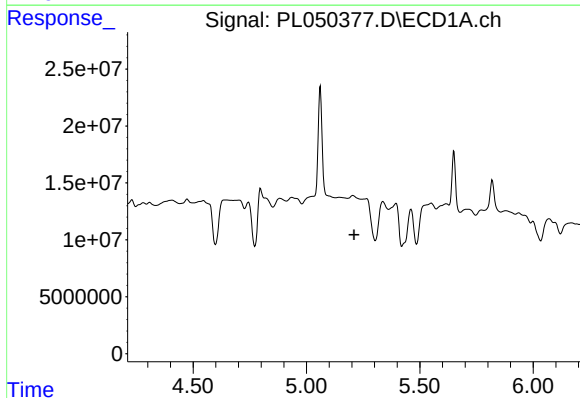


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.210 min
Response: 0
Conc: N.D.

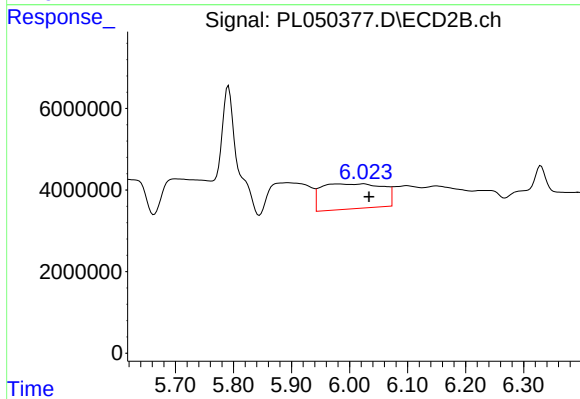

#10 gamma-Chlordane


R.T.: 6.025 min
Delta R.T.: -0.009 min
Response: 44966112
Conc: 12.07 ng/ml

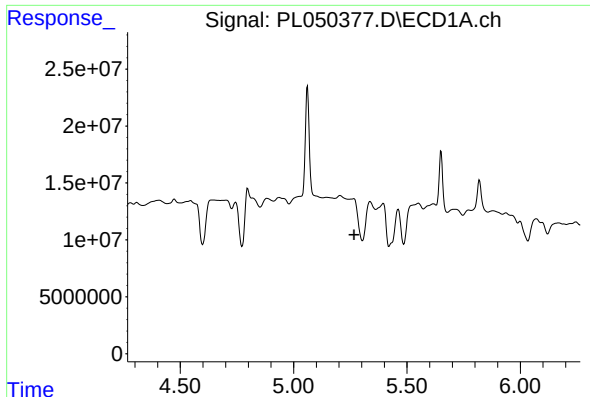

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

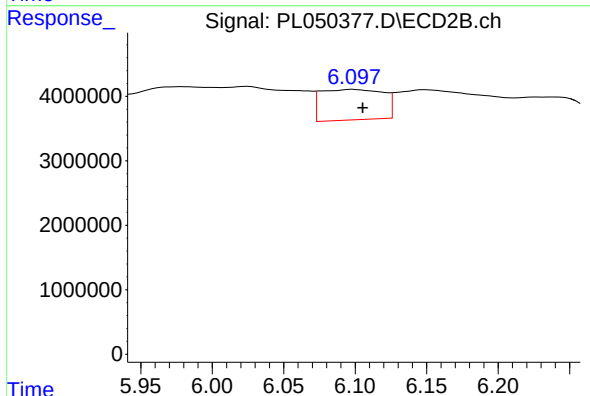


#11 alpha-Chlordane

R.T.: 6.099 min
Delta R.T.: -0.007 min
Response: 14303837
Conc: 3.87 ng/ml

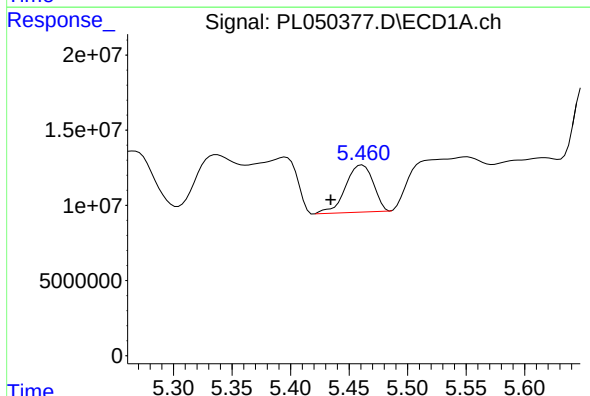


#12 4,4'-DDE

R.T.: 5.461 min
Delta R.T.: 0.027 min
Response: 51640923
Conc: 3.10 ng/ml

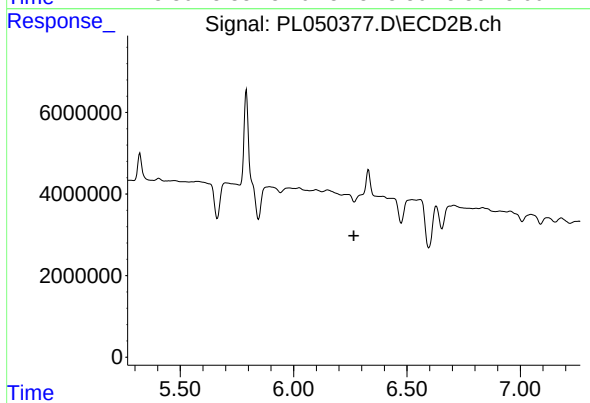

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

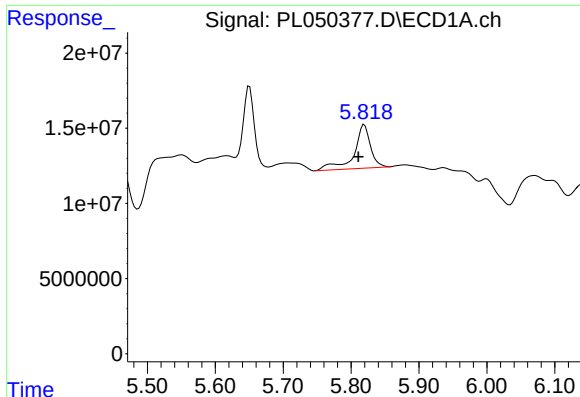

#14 Endrin


R.T.: 5.820 min
Delta R.T.: 0.009 min
Response: 49013764
Conc: 3.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

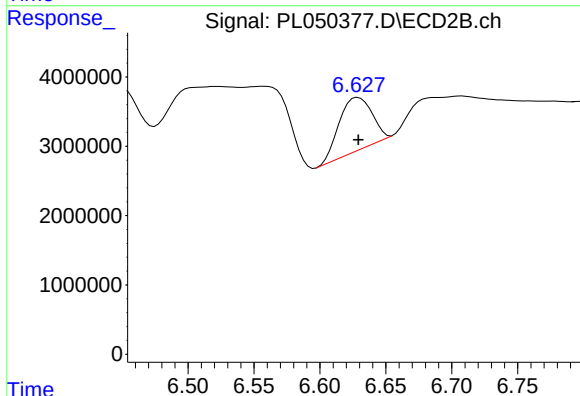


#14 Endrin

R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 13112756
Conc: 4.15 ng/ml

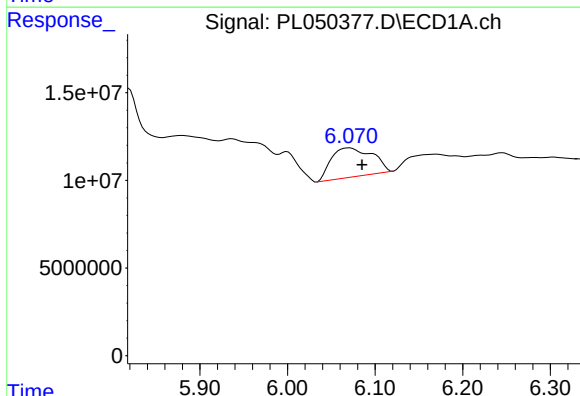


#15 Endosulfan II

R.T.: 6.070 min
Delta R.T.: -0.015 min
Response: 53973484
Conc: 3.70 ng/ml

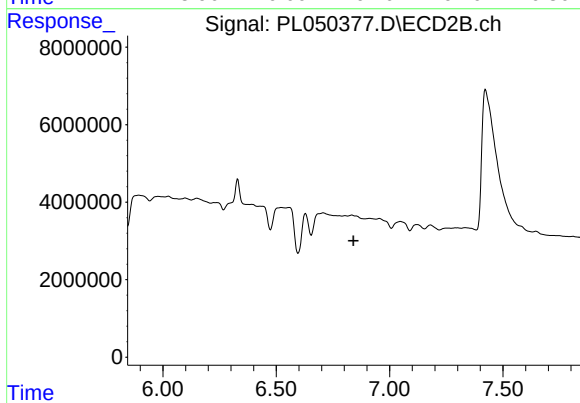

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.841 min
Response: 0
Conc: N.D.

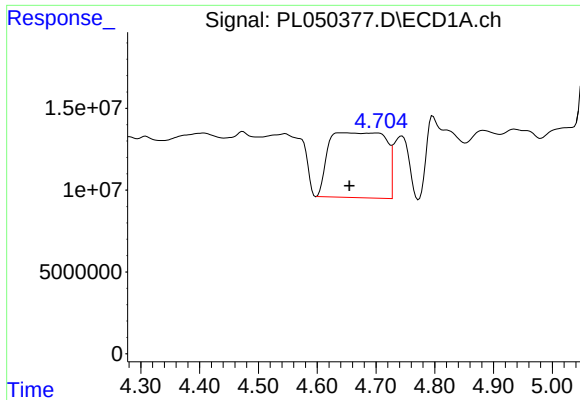

#24 Chlordane-2


R.T.: 4.638 min
Delta R.T.: -0.016 min
Response: 263760438
Conc: 451.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

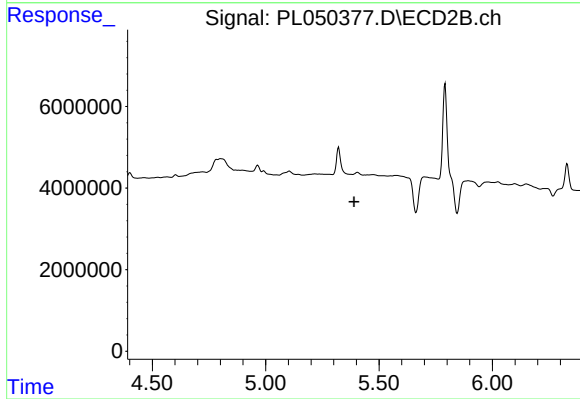


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.390 min
Response: 0
Conc: N.D.

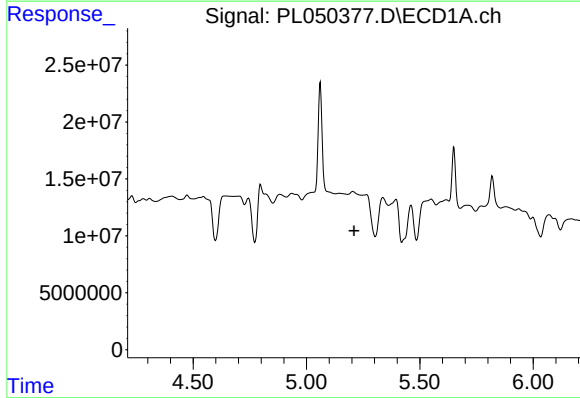


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.211 min
Response: 0
Conc: N.D.

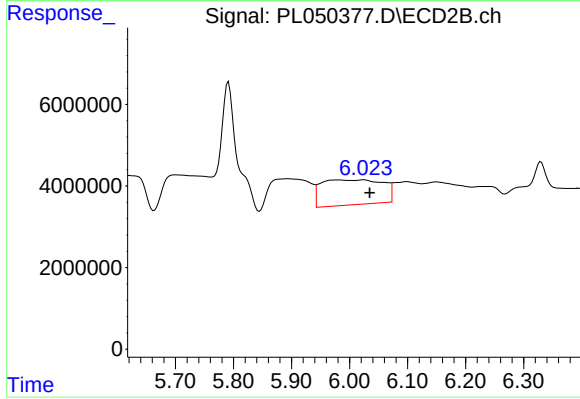

#25 Chlordane-3


R.T.: 6.025 min
Delta R.T.: -0.010 min
Response: 44966112
Conc: 90.36 ng/ml

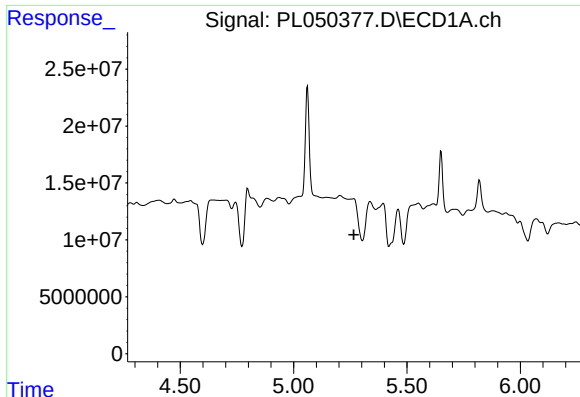

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

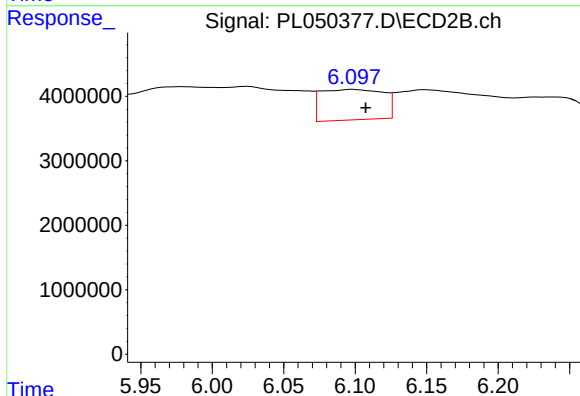


#26 Chlordane-4

R.T.: 6.099 min
Delta R.T.: -0.009 min
Response: 14303837
Conc: 24.07 ng/ml

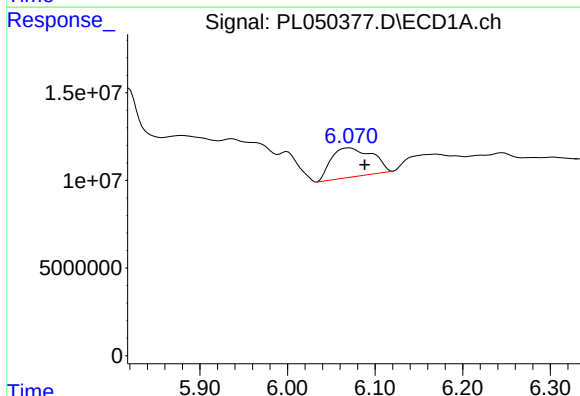


#27 Chlordane-5

R.T.: 6.070 min
Delta R.T.: -0.018 min
Response: 53973484
Conc: 96.17 ng/ml

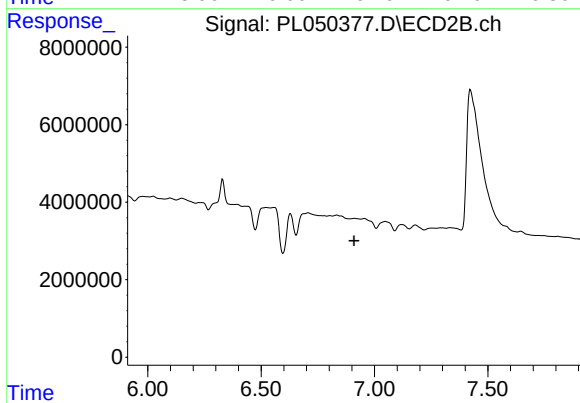

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.910 min
Response: 0
Conc: N.D.

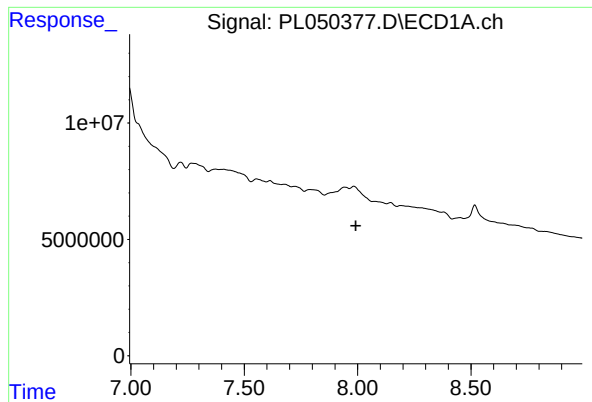

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

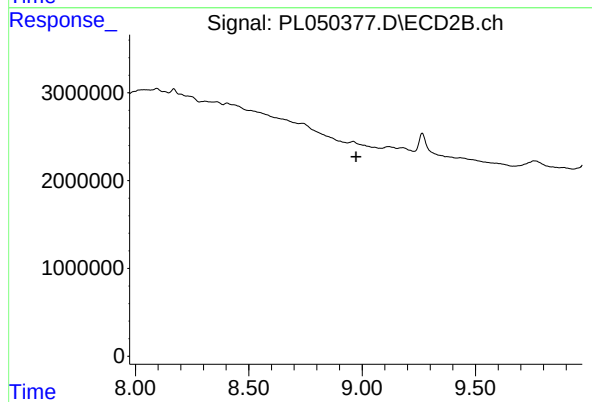

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.973 min
Response: 0
Conc: N.D.