

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
 Data File : PL050392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2019 12:50
 Operator : SM\AJ
 Sample : K3807-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-053

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:08:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.930	154.8E6	45519741	13.728	14.867
28)	SA Decachlor...	7.980	8.961	107.5E6	28397879	8.464	8.459
Target Compounds							
10)	B gamma-Chl...	5.202	6.025	41702563	7663025	2.440	2.056
11)	B alpha-Chl...	5.257	6.098	31132437	15057987	1.876	4.071 #
19)	B Endosulfa...	0.000	7.192	0	6638155	N.D.	2.206 #
25)	Chlordane-3	5.202	6.025	41702563	7663025	22.203	15.399 #
26)	Chlordane-4	5.257	6.098	31132437	15057987	17.840	25.336 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
Data File : PL050392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2019 12:50
Operator : SM\AJ
Sample : K3807-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-053

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:08:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

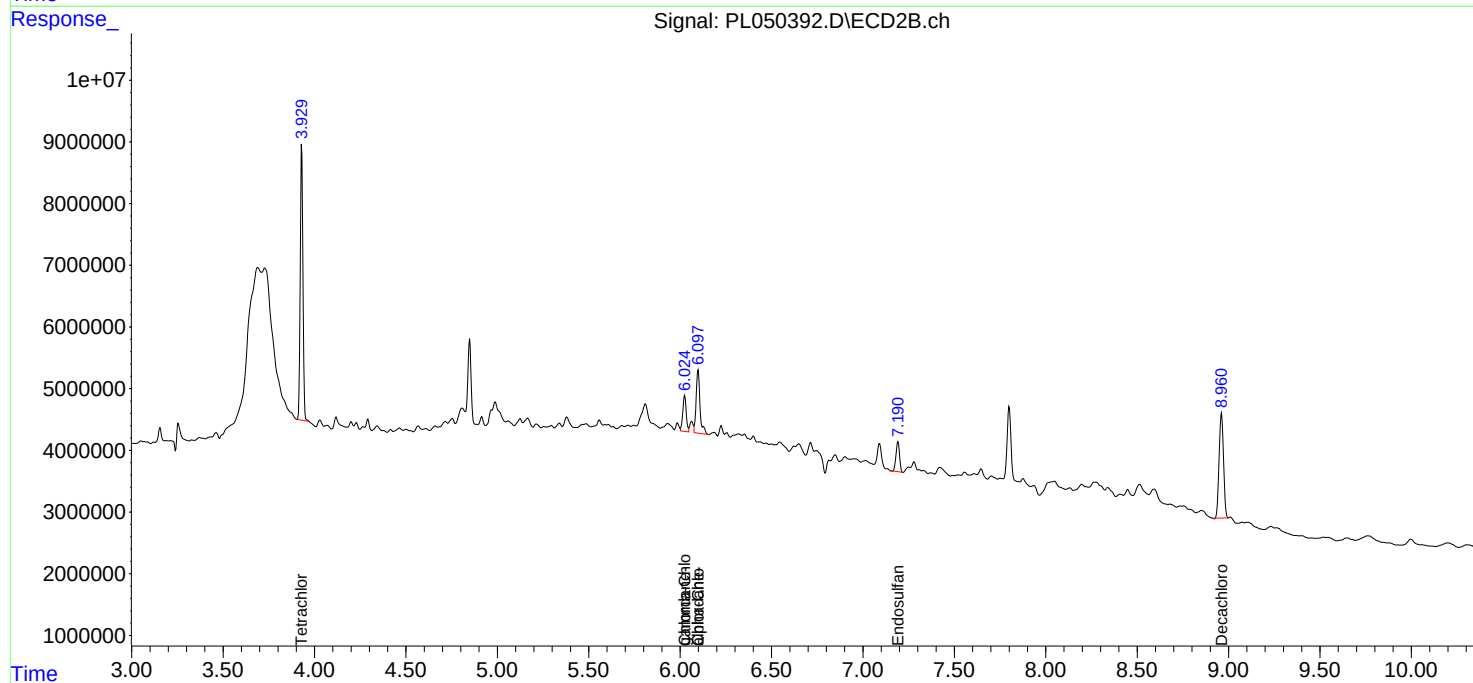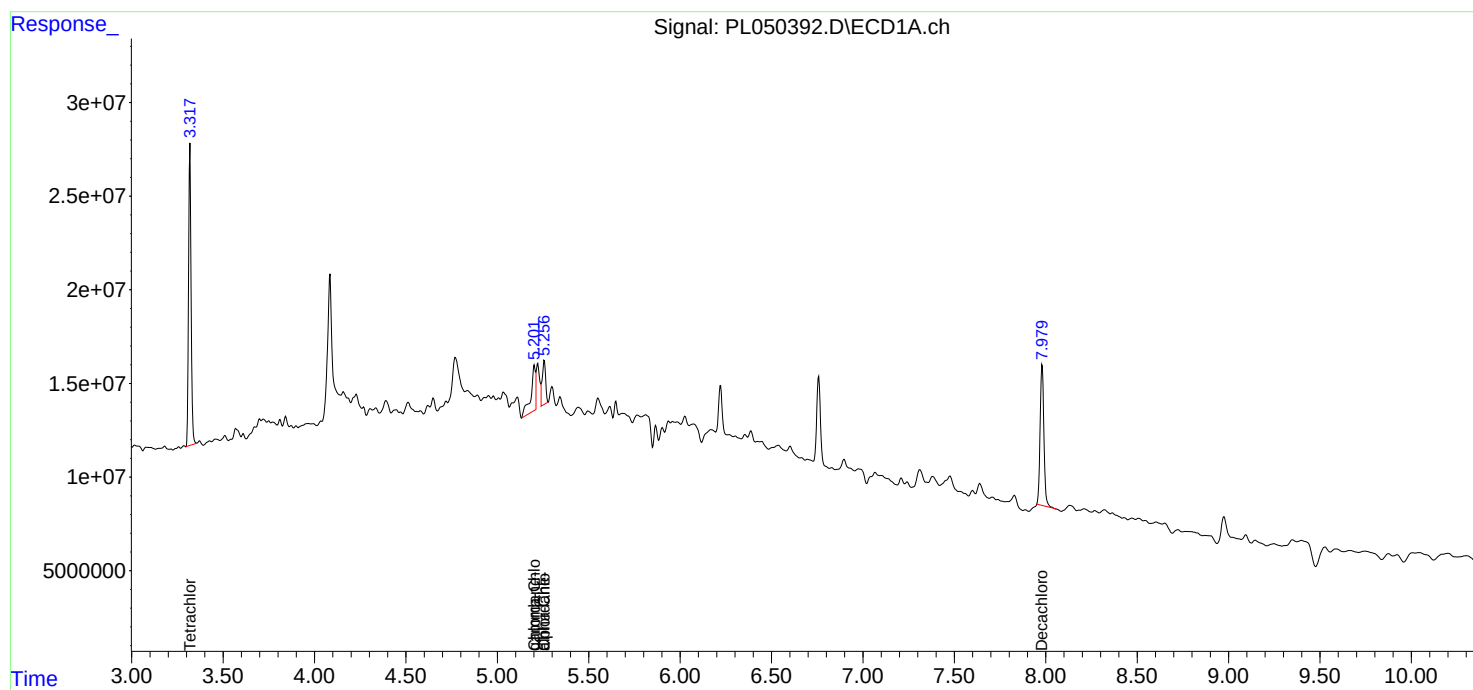


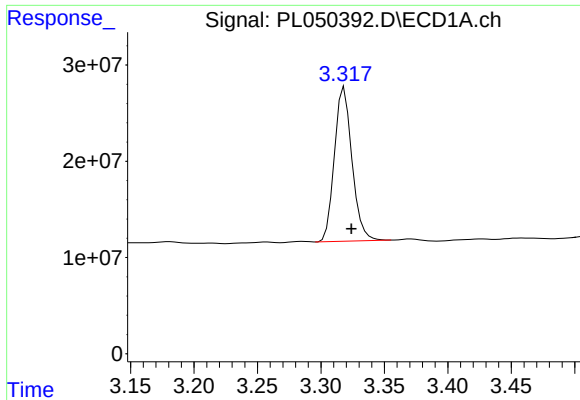

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: -0.006 min
Response: 154815406
Conc: 13.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-053

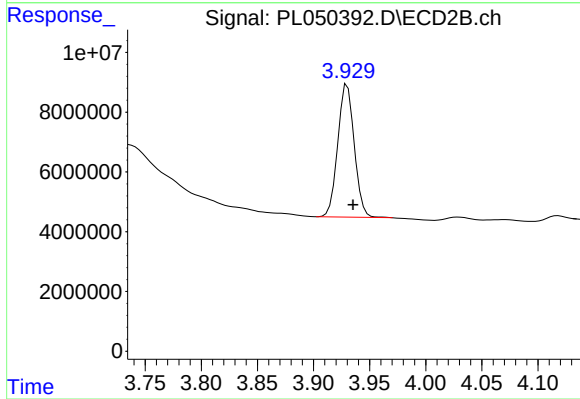


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.005 min
Response: 45519741
Conc: 14.87 ng/ml

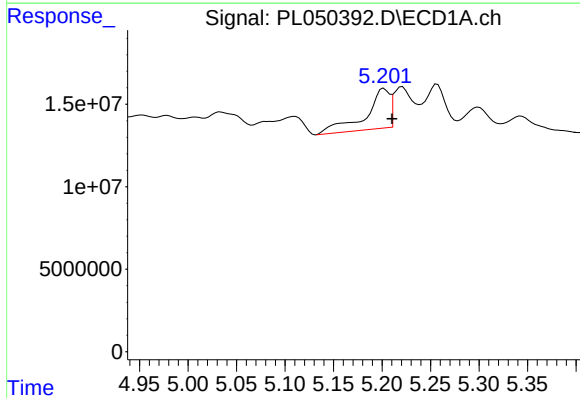


#10 gamma-Chlordane

R.T.: 5.202 min
Delta R.T.: -0.008 min
Response: 41702563
Conc: 2.44 ng/ml

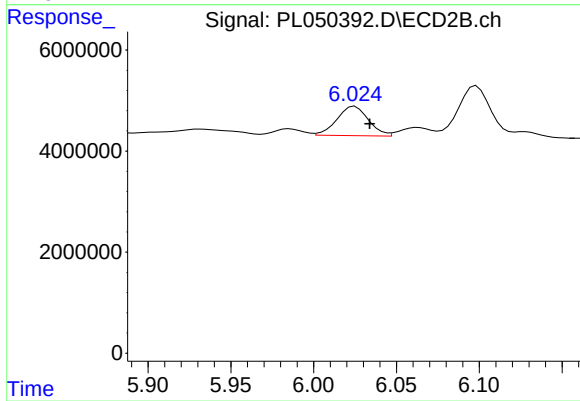

#10 gamma-Chlordane


R.T.: 6.025 min
Delta R.T.: -0.009 min
Response: 7663025
Conc: 2.06 ng/ml

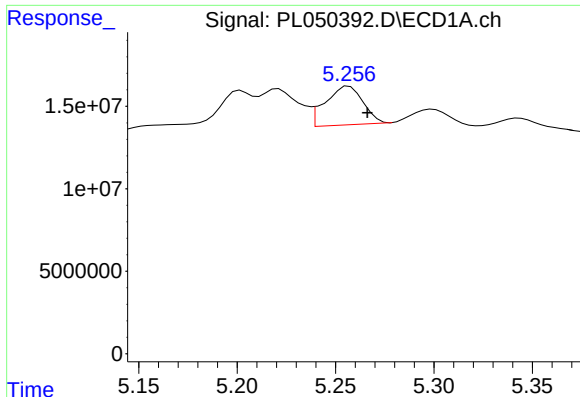

#11 alpha-Chlordane


R.T.: 5.257 min
Delta R.T.: -0.009 min
Response: 31132437
Conc: 1.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-053

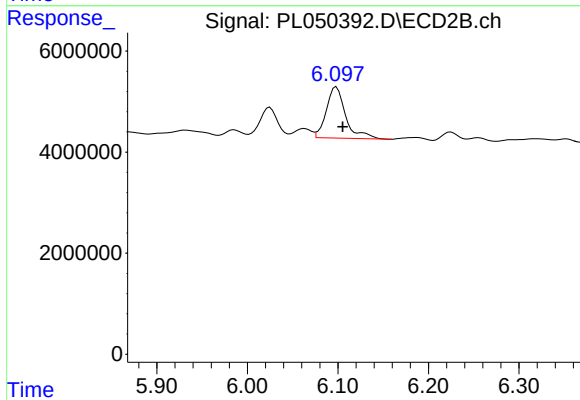


#11 alpha-Chlordane

R.T.: 6.098 min
Delta R.T.: -0.007 min
Response: 15057987
Conc: 4.07 ng/ml

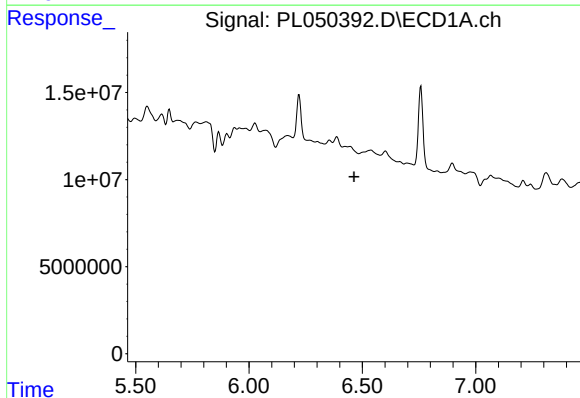


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.464 min
Response: 0
Conc: N.D.

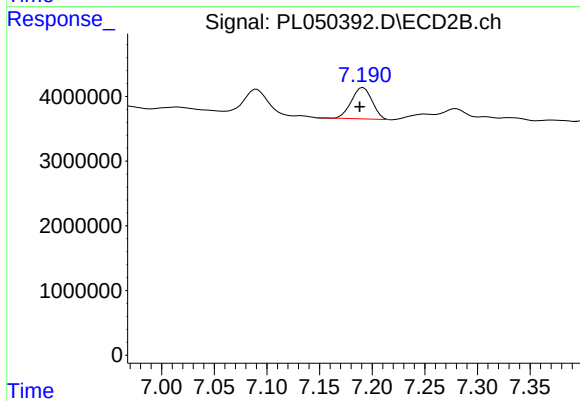

#19 Endosulfan Sulfate


R.T.: 7.192 min
Delta R.T.: 0.004 min
Response: 6638155
Conc: 2.21 ng/ml

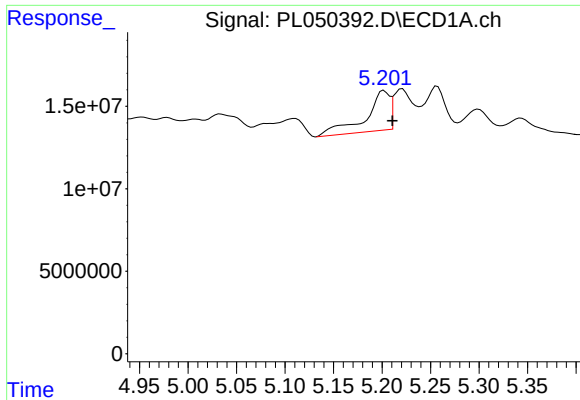

#25 Chlordane-3


R.T.: 5.202 min
Delta R.T.: -0.009 min
Response: 41702563
Conc: 22.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-053

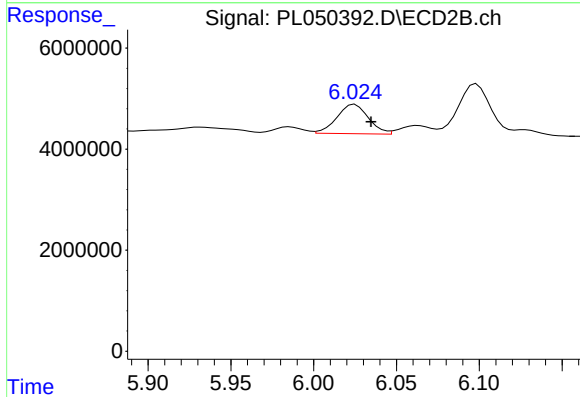


#25 Chlordane-3

R.T.: 6.025 min
Delta R.T.: -0.010 min
Response: 7663025
Conc: 15.40 ng/ml

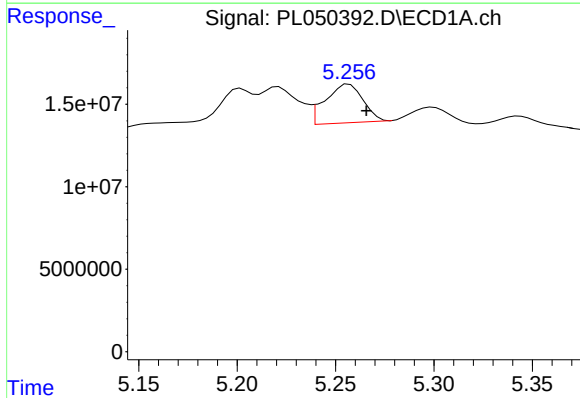


#26 Chlordane-4

R.T.: 5.257 min
Delta R.T.: -0.009 min
Response: 31132437
Conc: 17.84 ng/ml

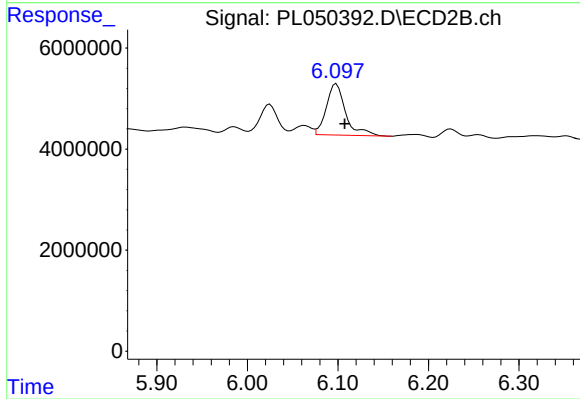

#26 Chlordane-4


R.T.: 6.098 min
Delta R.T.: -0.009 min
Response: 15057987
Conc: 25.34 ng/ml

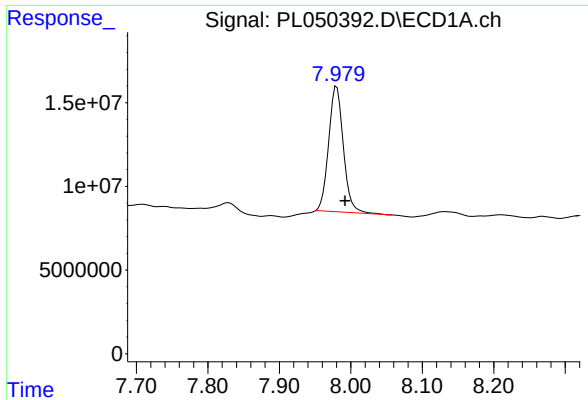

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.012 min
Response: 107545975
Conc: 8.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-053

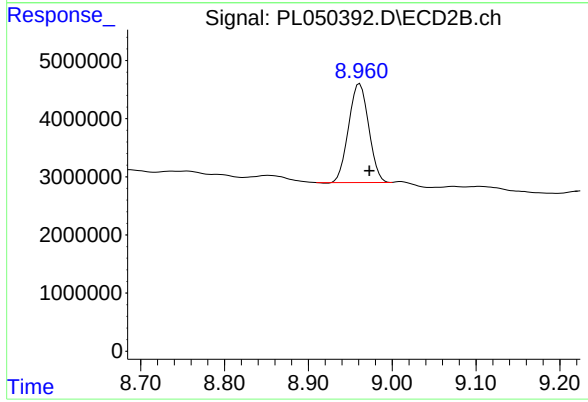

#28 Decachlorobiphenyl

R.T.: 8.961 min
Delta R.T.: -0.012 min
Response: 28397879
Conc: 8.46 ng/ml