

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
 Data File : PL050396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2019 13:48
 Operator : SM\AJ
 Sample : K3620-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-071219-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:09:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.930	105.0E6	29299789	9.315	9.570
28)	SA Decachlor...	7.980	8.960	95560030	29839017	7.521	8.888
Target Compounds							
5)	MB Aldrin	4.543	5.404	43153907	18460392	2.499	4.713 #
10)	B gamma-Chl...	5.221	6.026	70533502	8668673	4.127	2.326 #
11)	B alpha-Chl...	5.257	6.099	37814603	23202185	2.278	6.274 #
23)	Chlordane-1	4.157	4.915	23938662	5493993	42.029	37.383
24)	Chlordane-2	4.647	5.404	23237083	18460392	39.787	118.838 #
25)	Chlordane-3	5.221	6.026	70533502	8668673	37.553	17.420 #
26)	Chlordane-4	5.257	6.099	37814603	23202185	21.669	39.038 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
Data File : PL050396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2019 13:48
Operator : SM\AJ
Sample : K3620-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-01-071219-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:09:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

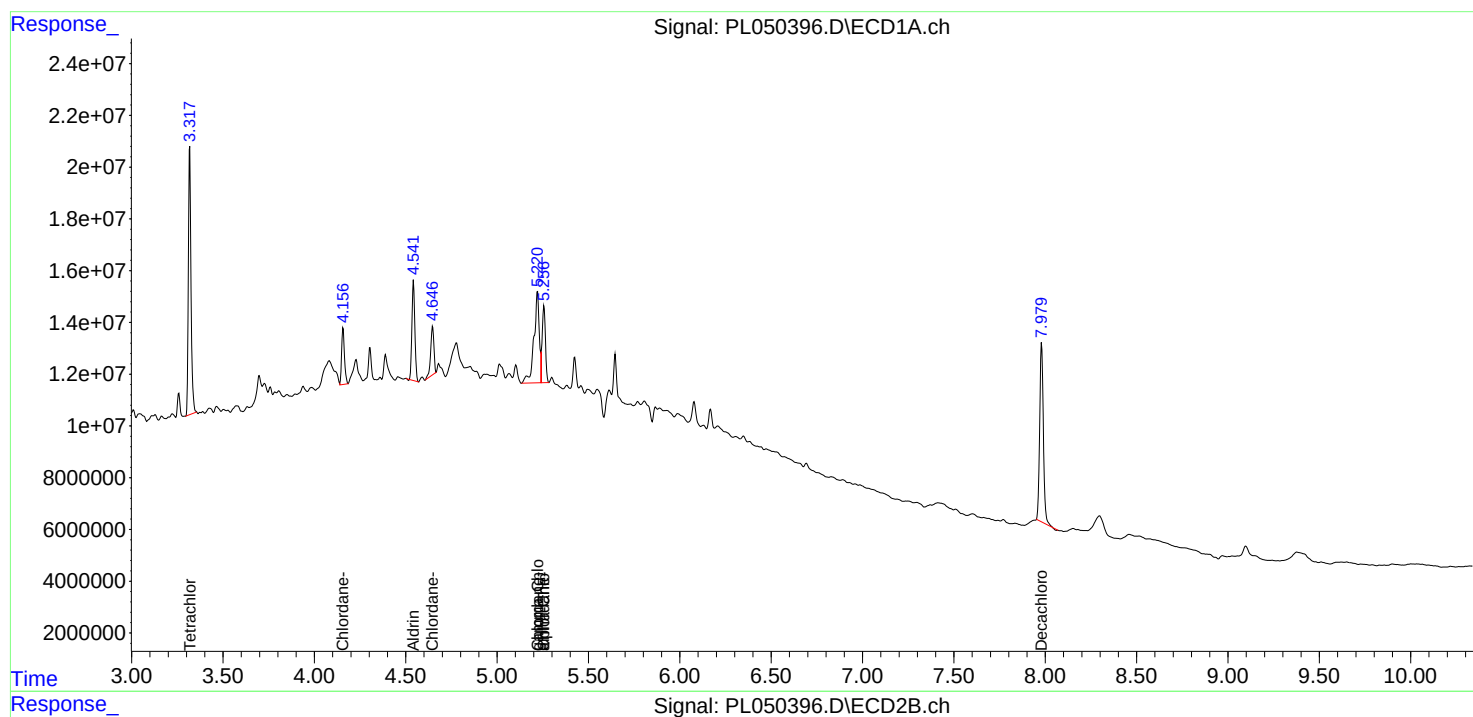


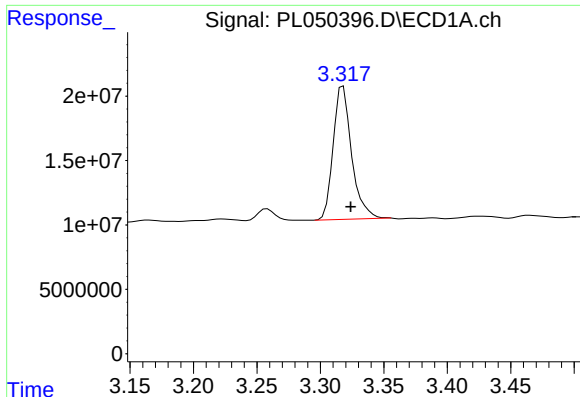

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: -0.006 min
Response: 105047096
Conc: 9.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-071219-A

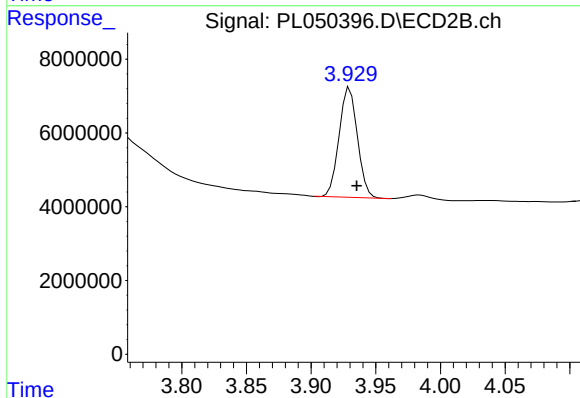


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.005 min
Response: 29299789
Conc: 9.57 ng/ml

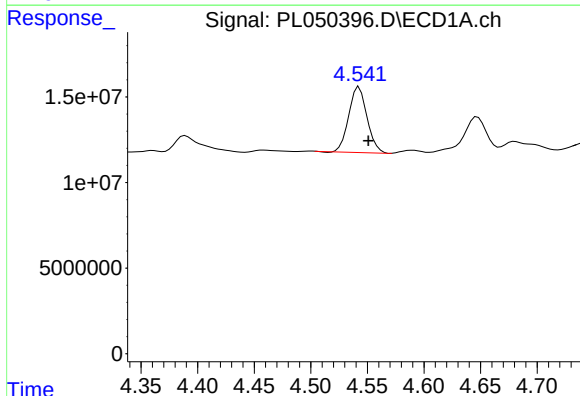


#5 Aldrin

R.T.: 4.543 min
Delta R.T.: -0.008 min
Response: 43153907
Conc: 2.50 ng/ml

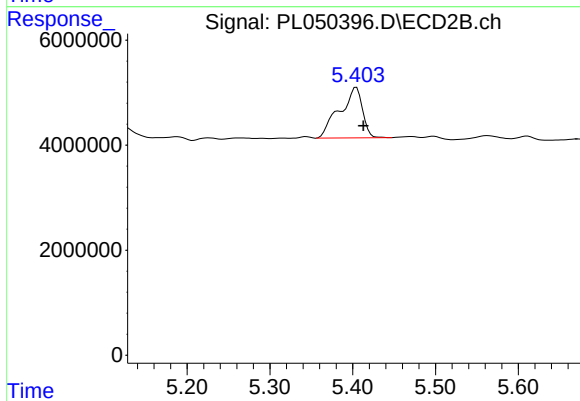

#5 Aldrin


R.T.: 5.404 min
Delta R.T.: -0.008 min
Response: 18460392
Conc: 4.71 ng/ml

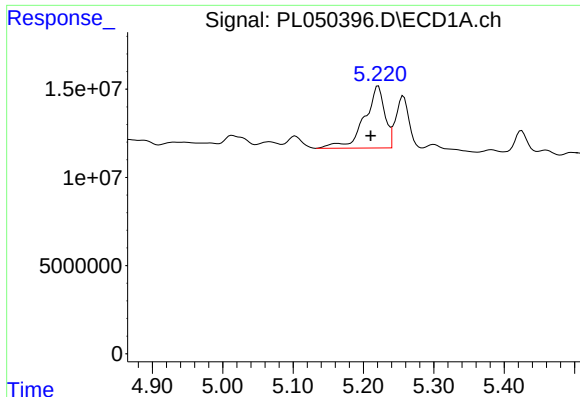

#10 gamma-Chlordane


R.T.: 5.221 min
Delta R.T.: 0.011 min
Response: 70533502
Conc: 4.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-071219-A

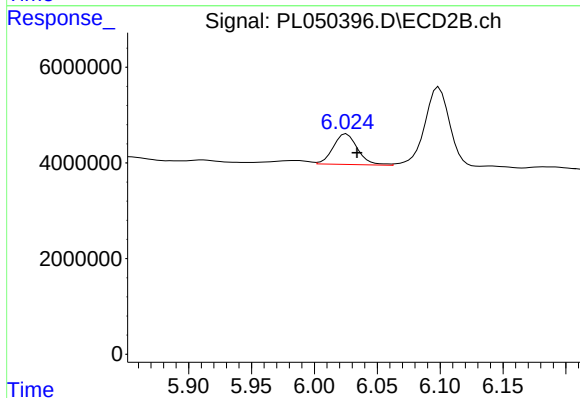


#10 gamma-Chlordane

R.T.: 6.026 min
Delta R.T.: -0.008 min
Response: 8668673
Conc: 2.33 ng/ml

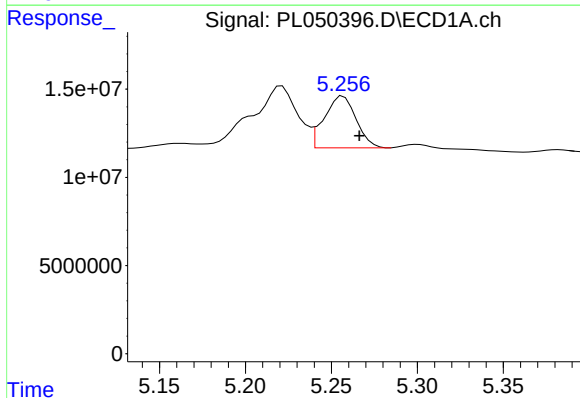


#11 alpha-Chlordane

R.T.: 5.257 min
Delta R.T.: -0.009 min
Response: 37814603
Conc: 2.28 ng/ml

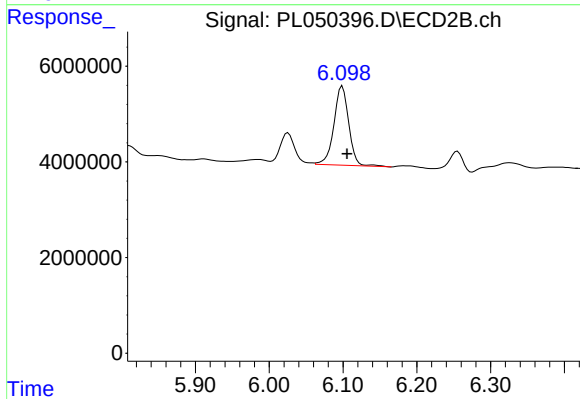

#11 alpha-Chlordane


R.T.: 6.099 min
Delta R.T.: -0.006 min
Response: 23202185
Conc: 6.27 ng/ml

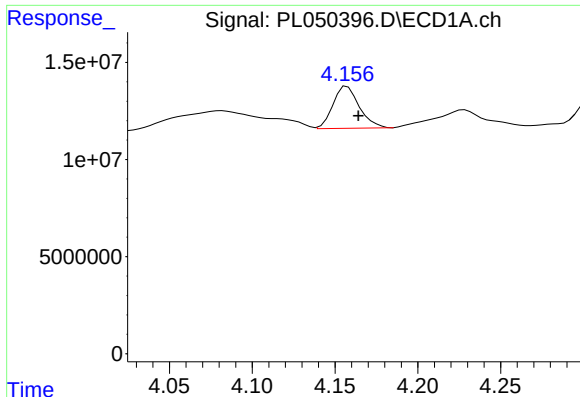

#23 Chlordane-1


R.T.: 4.157 min
Delta R.T.: -0.007 min
Response: 23938662
Conc: 42.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-071219-A

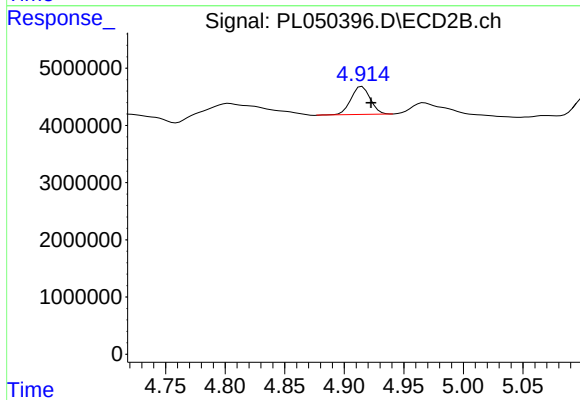


#23 Chlordane-1

R.T.: 4.915 min
Delta R.T.: -0.007 min
Response: 5493993
Conc: 37.38 ng/ml

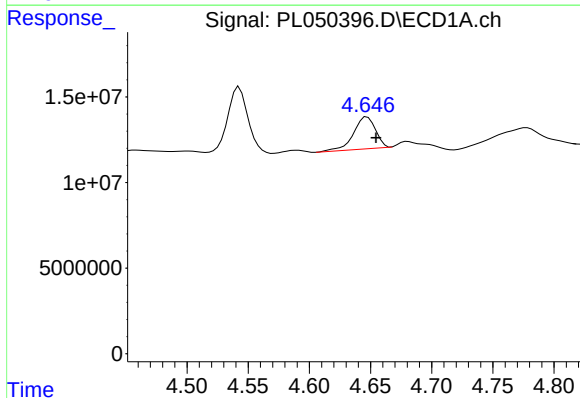


#24 Chlordane-2

R.T.: 4.647 min
Delta R.T.: -0.007 min
Response: 23237083
Conc: 39.79 ng/ml

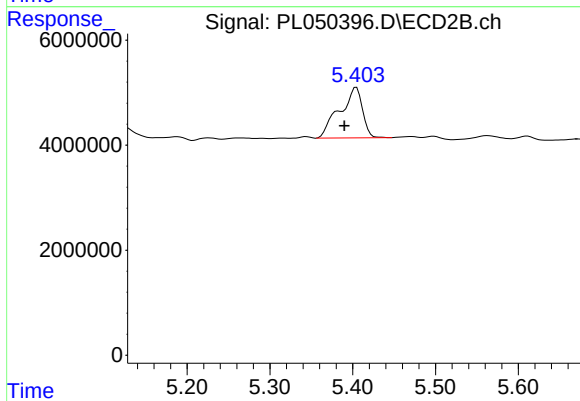

#24 Chlordane-2


R.T.: 5.404 min
Delta R.T.: 0.014 min
Response: 18460392
Conc: 118.84 ng/ml

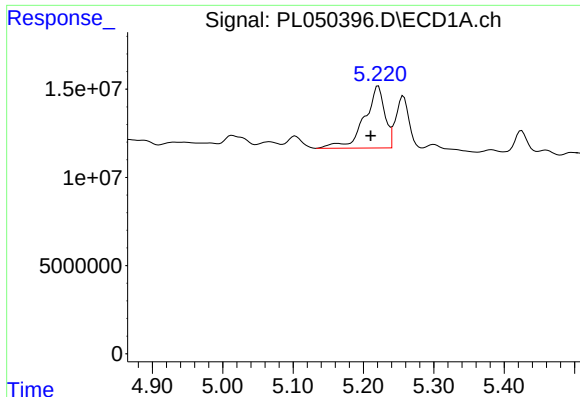

#25 Chlordane-3


R.T.: 5.221 min
Delta R.T.: 0.011 min
Response: 70533502
Conc: 37.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-071219-A

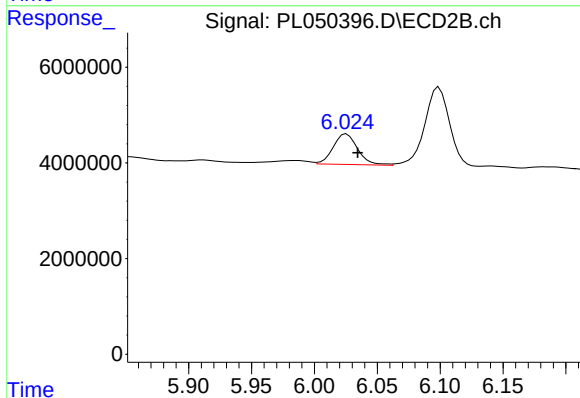


#25 Chlordane-3

R.T.: 6.026 min
Delta R.T.: -0.009 min
Response: 8668673
Conc: 17.42 ng/ml

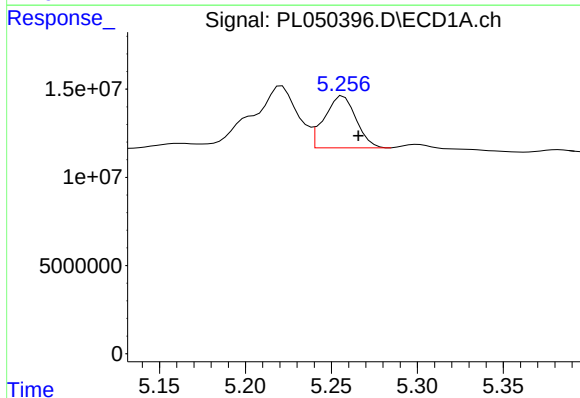


#26 Chlordane-4

R.T.: 5.257 min
Delta R.T.: -0.009 min
Response: 37814603
Conc: 21.67 ng/ml

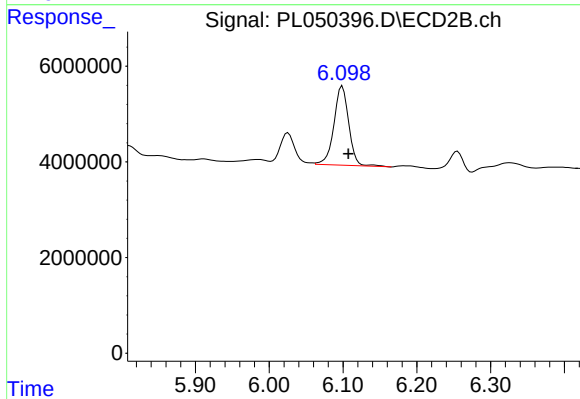

#26 Chlordane-4


R.T.: 6.099 min
Delta R.T.: -0.008 min
Response: 23202185
Conc: 39.04 ng/ml

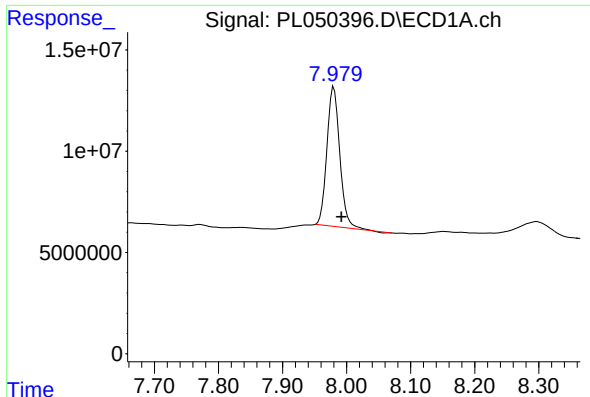

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.012 min
Response: 95560030
Conc: 7.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-071219-A

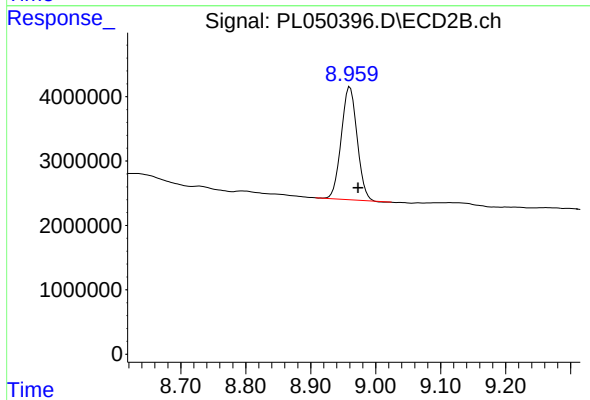

#28 Decachlorobiphenyl

R.T.: 8.960 min
Delta R.T.: -0.013 min
Response: 29839017
Conc: 8.89 ng/ml