

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
 Data File : PL050423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2019 21:17
 Operator : SM\AJ
 Sample : K3623-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-071519-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:13:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.318	3.930	105.0E6	29276687	9.308	9.562
28) SA Decachlor...	7.980	8.962	95430800	32667911	7.510	9.731 #
Target Compounds						
6) B beta-BHC	0.000	4.801f	0	3624050	N.D.	1.871 #
24) Chlordane-2	4.680f	0.000	25130321	0	43.029	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
Data File : PL050423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2019 21:17
Operator : SM\AJ
Sample : K3623-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-02-071519-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:13:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

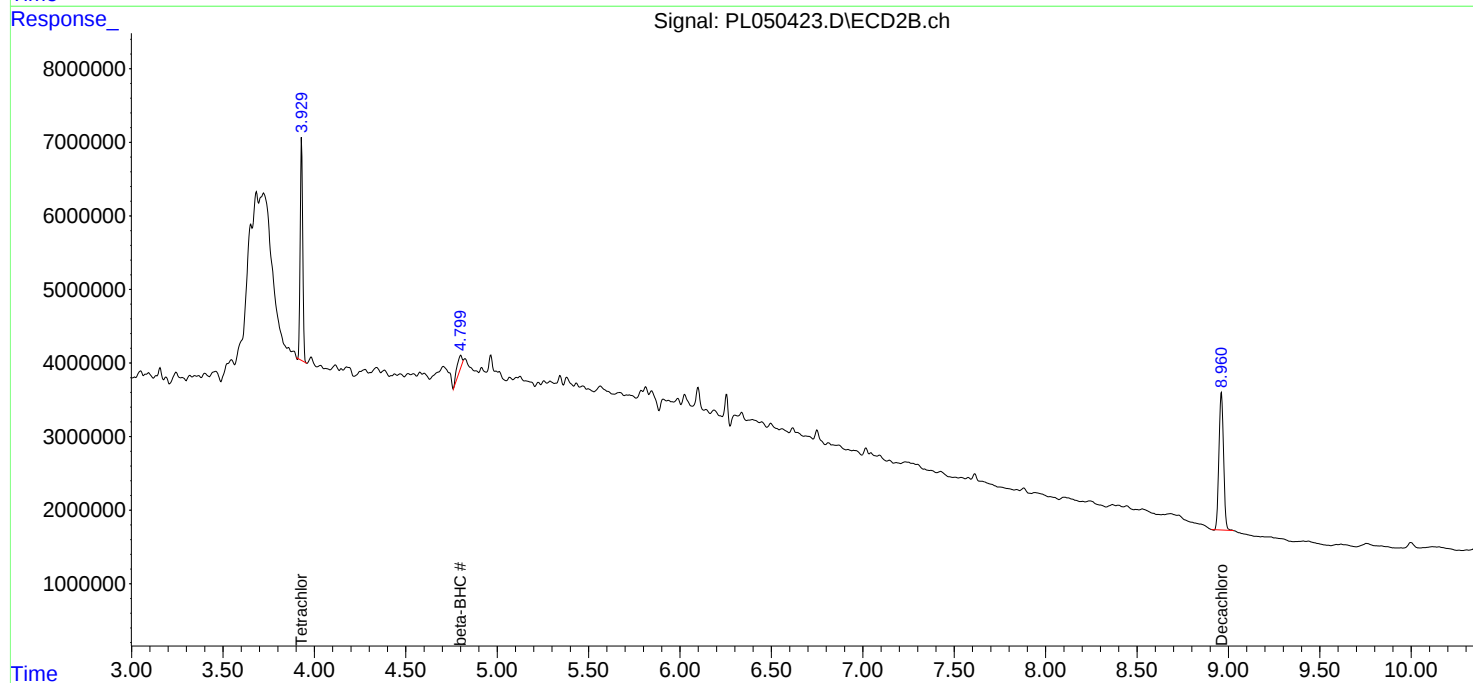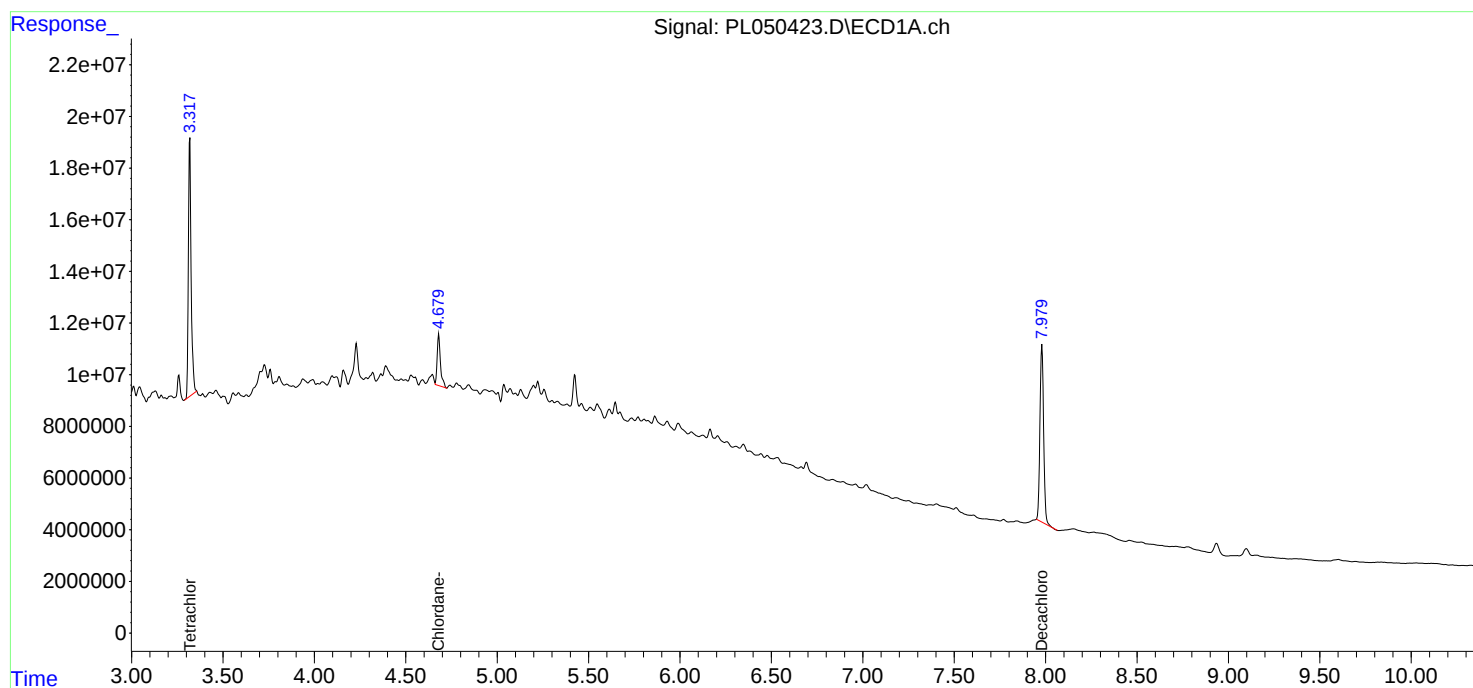


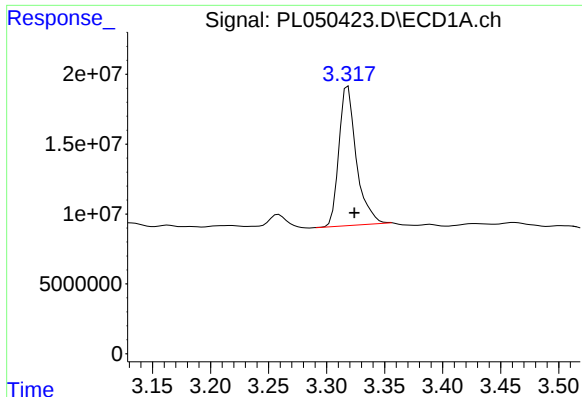

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: -0.006 min
Response: 104975736
Conc: 9.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-071519-A

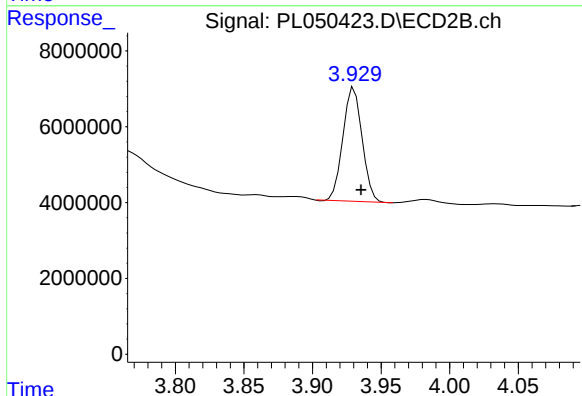


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.005 min
Response: 29276687
Conc: 9.56 ng/ml

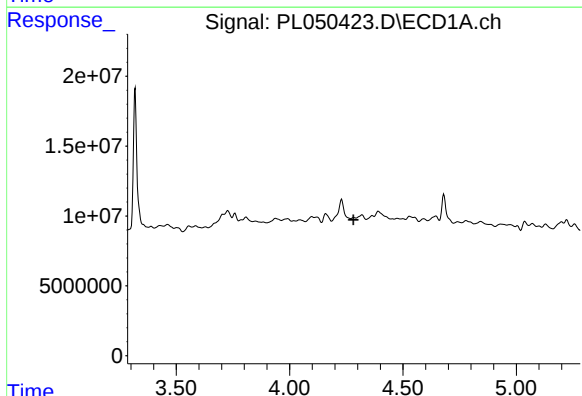


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

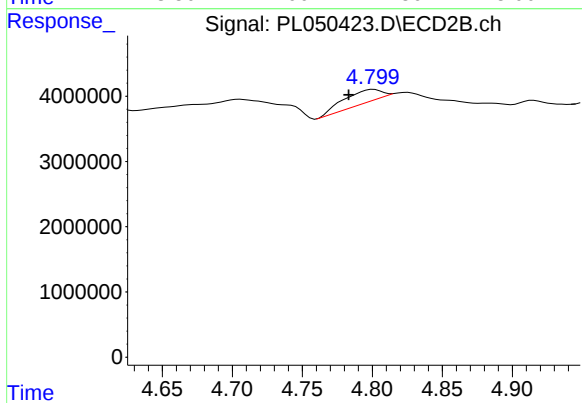

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.018 min
Response: 3624050
Conc: 1.87 ng/ml

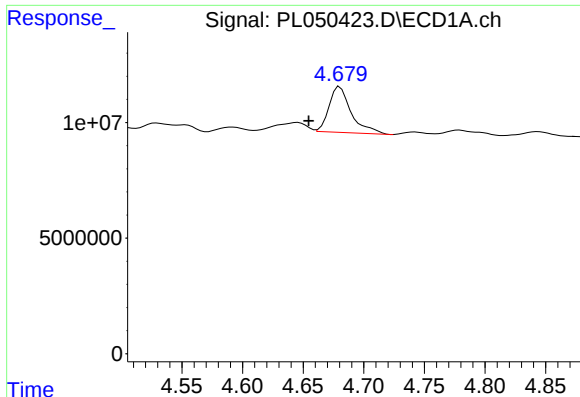

#24 Chlordane-2


R.T.: 4.680 min
Delta R.T.: 0.026 min
Response: 25130321
Conc: 43.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-071519-A

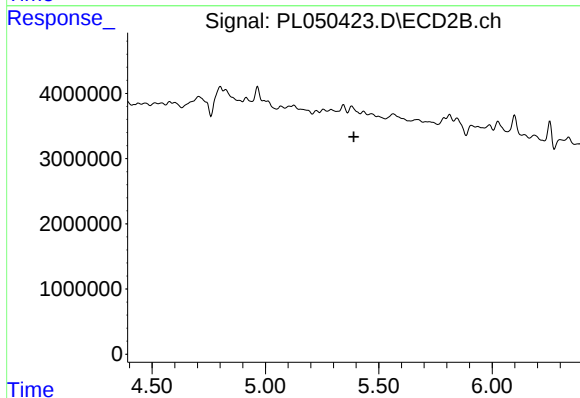


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.390 min
Response: 0
Conc: N.D.

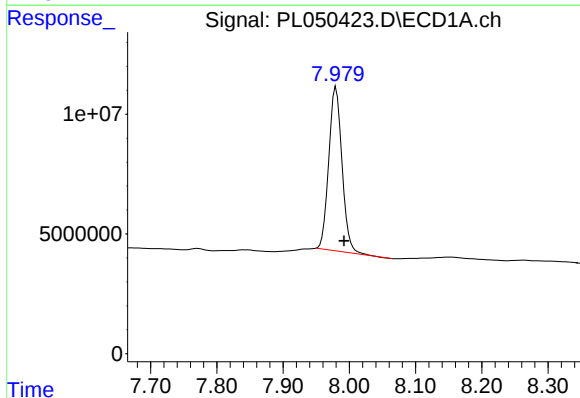

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.012 min
Response: 95430800
Conc: 7.51 ng/ml

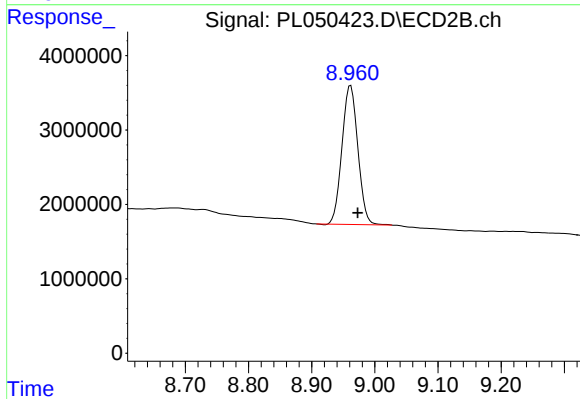

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: -0.011 min
Response: 32667911
Conc: 9.73 ng/ml