

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
 Data File : PL050435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 00:09
 Operator : SM\AJ
 Sample : K3627-04
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-071219-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:15:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.931	193.6E6	62755460	17.163	20.497
28)	SA Decachlor...	7.982	8.963	162.9E6	51328587	12.820	15.290
Target Compounds							
15)	B Endosulfa...	0.000	6.846	0	13407920	N.D.	4.163 #
19)	B Endosulfa...	6.477	7.190	75005269	828502	5.785	0.275 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
Data File : PL050435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 00:09
Operator : SM\AJ
Sample : K3627-04
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-01-071219-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:15:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

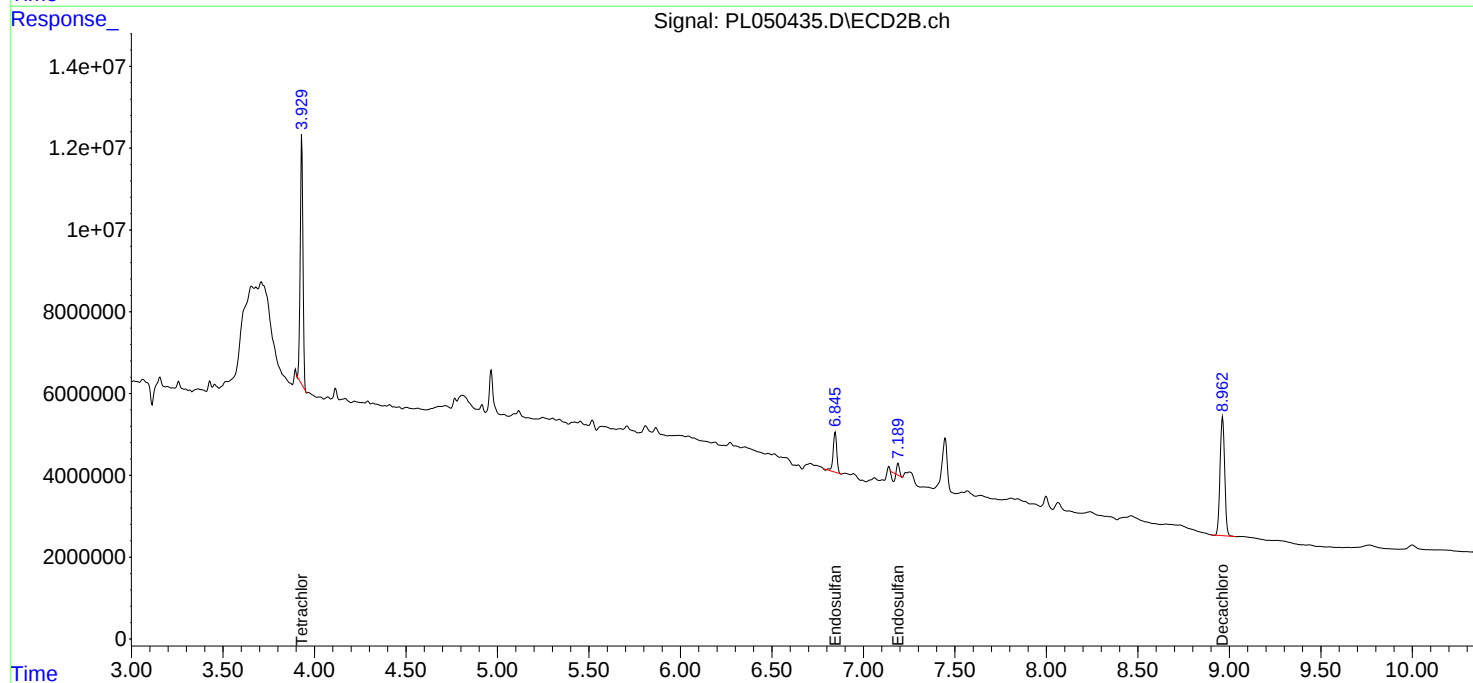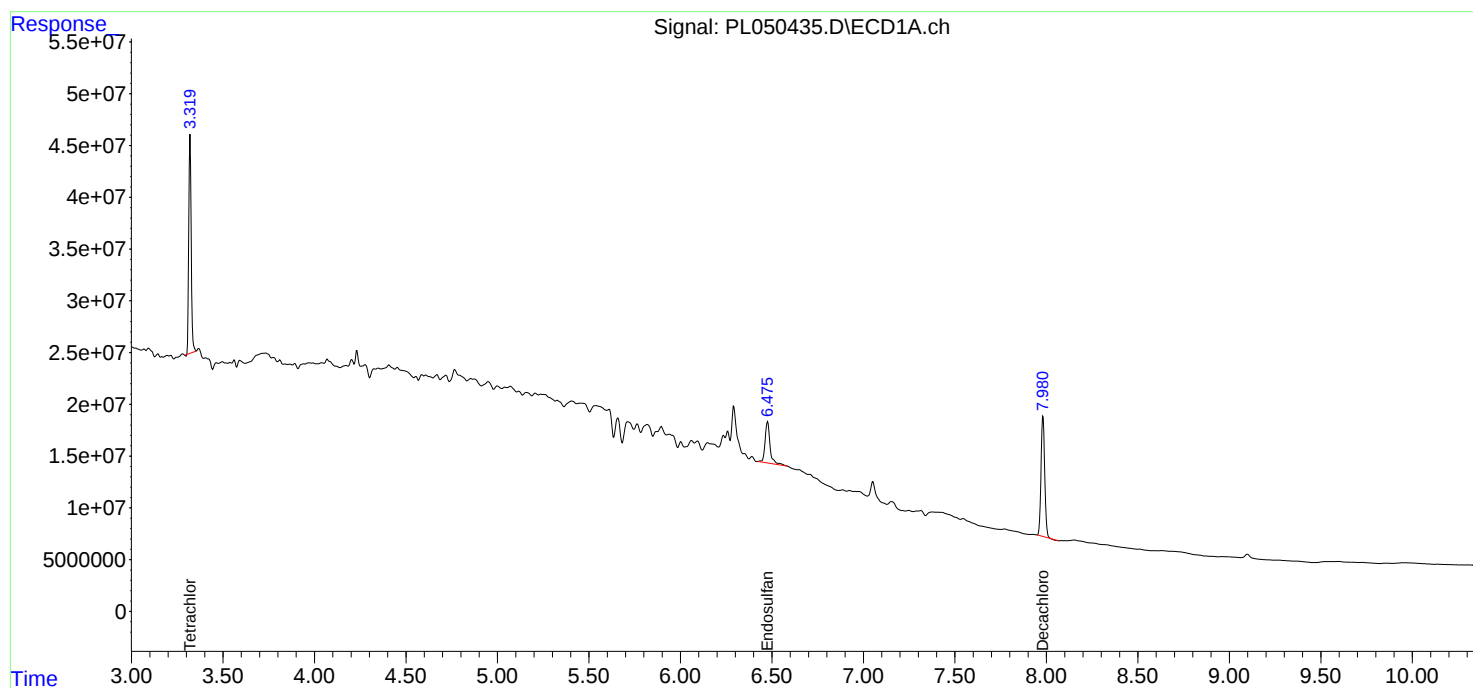


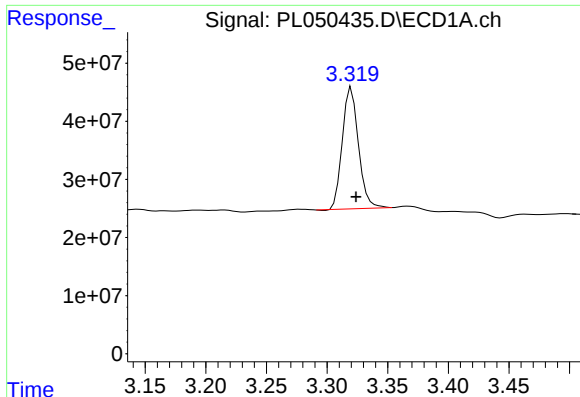

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 193554714
Conc: 17.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-071219-D

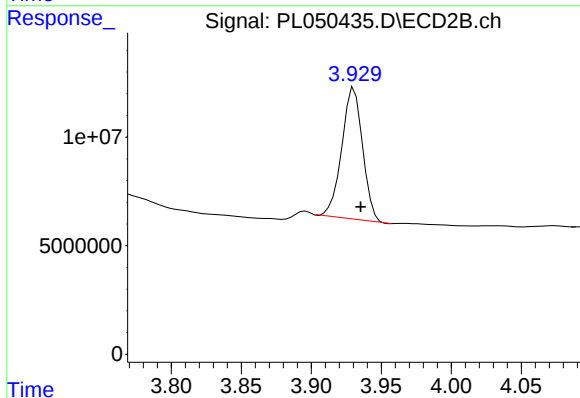


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.004 min
Response: 62755460
Conc: 20.50 ng/ml

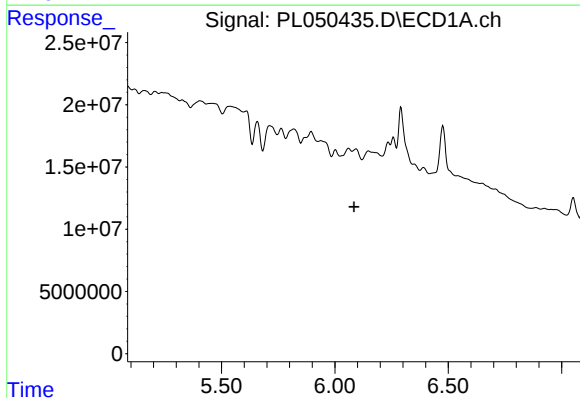


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.085 min
Response: 0
Conc: N.D.

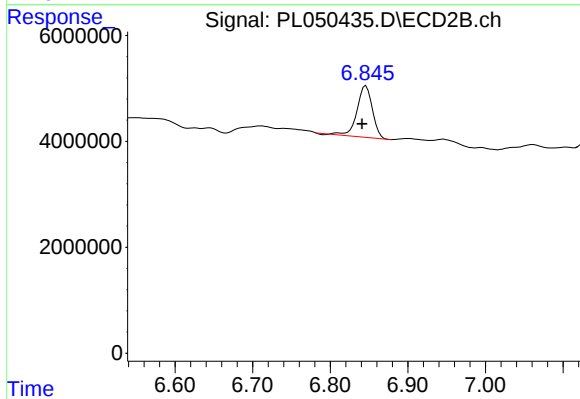

#15 Endosulfan II


R.T.: 6.846 min
Delta R.T.: 0.005 min
Response: 13407920
Conc: 4.16 ng/ml

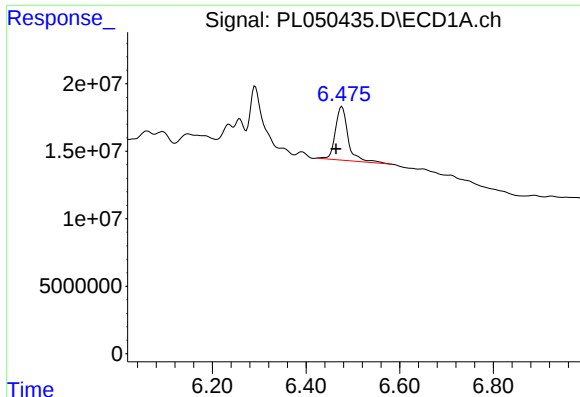

#19 Endosulfan Sulfate


R.T.: 6.477 min
Delta R.T.: 0.013 min
Response: 75005269
Conc: 5.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-071219-D

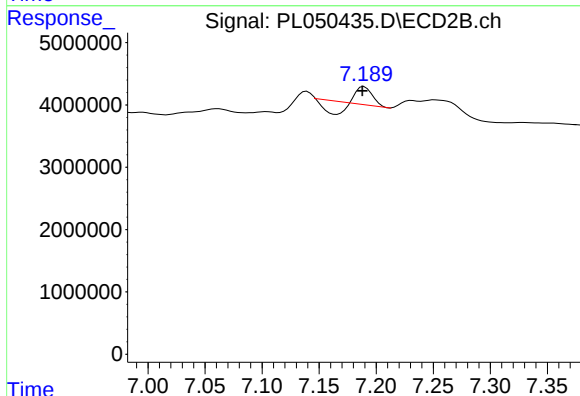


#19 Endosulfan Sulfate

R.T.: 7.190 min
Delta R.T.: 0.001 min
Response: 828502
Conc: 0.28 ng/ml

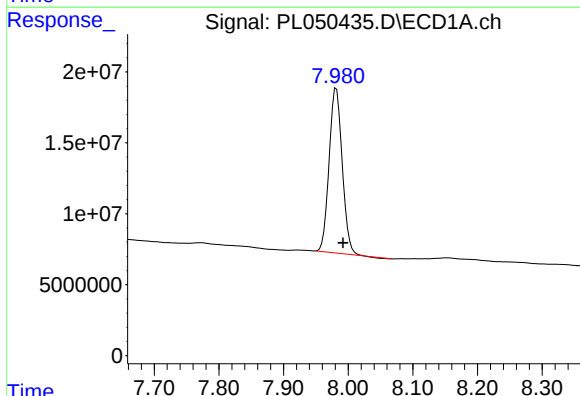

#28 Decachlorobiphenyl

R.T.: 7.982 min
Delta R.T.: -0.010 min
Response: 162893249
Conc: 12.82 ng/ml

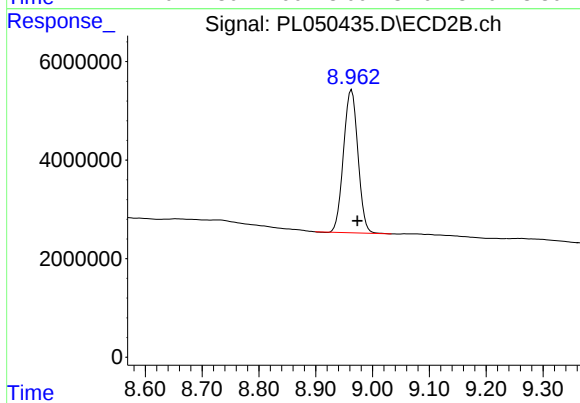

#28 Decachlorobiphenyl

R.T.: 8.963 min
Delta R.T.: -0.010 min
Response: 51328587
Conc: 15.29 ng/ml