

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
 Data File : PL050392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2019 12:50
 Operator : SM\AJ
 Sample : K3807-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-053

Manual Integrations
 APPROVED

Ankita
 7/18/2019 8:36:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:08:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.930	154.8E6	45519741	13.728	14.867
28)	SA Decachlor...	7.980	8.961	107.5E6	28397879	8.464	8.459
Target Compounds							
10)	B gamma-Chl...	5.201	6.025	27639068	7663025	1.617m	2.056 #
11)	B alpha-Chl...	5.257	6.097	31132437	13188922	1.876	3.566m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
Data File : PL050392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2019 12:50
Operator : SM\AJ
Sample : K3807-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FK-PS-01-053


Manual Integrations
APPROVED

Ankita
7/18/2019 8:36:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:08:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

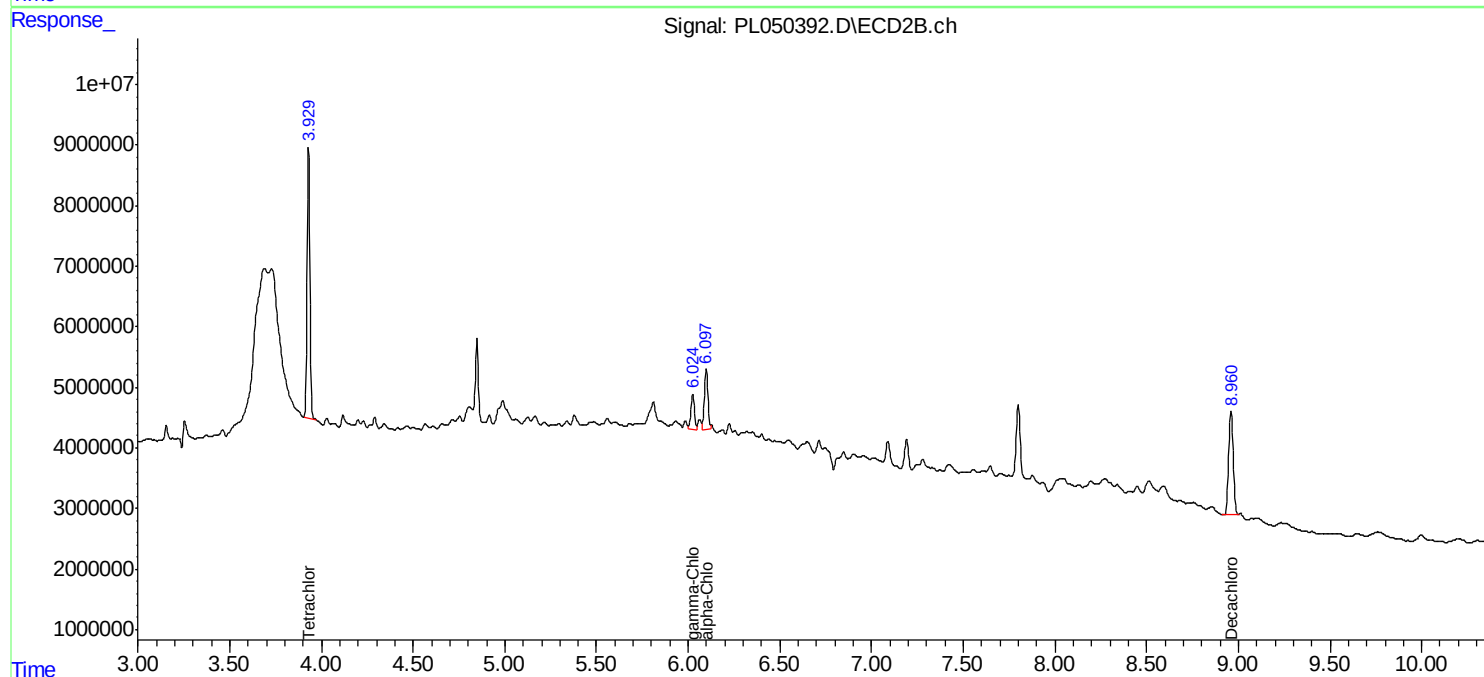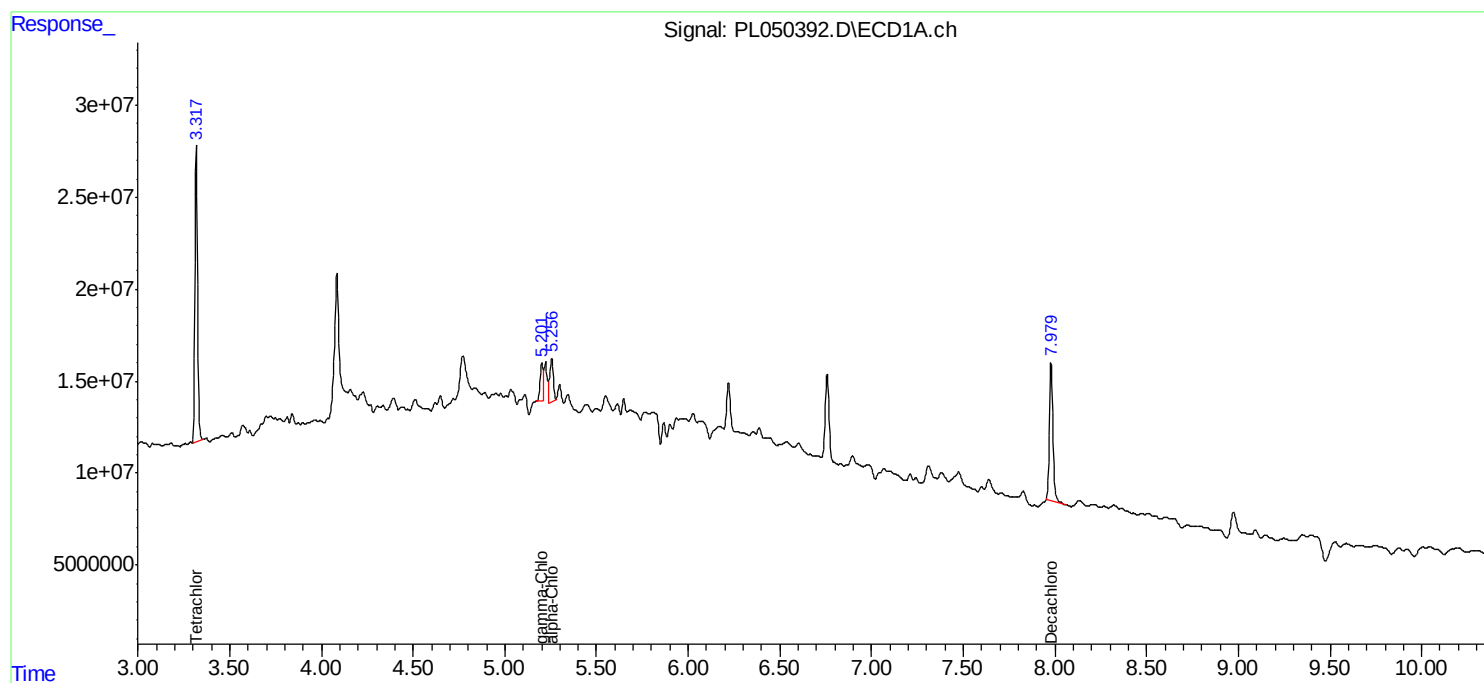

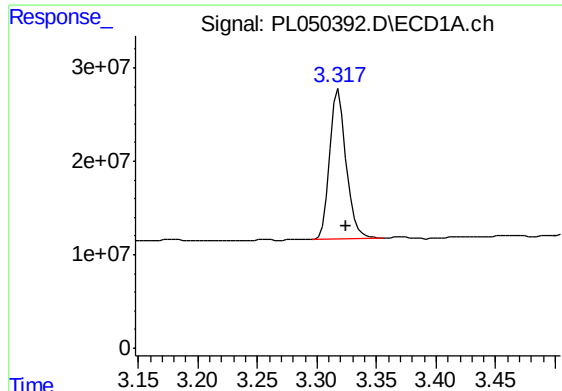


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: -0.006 min
Response: 154815406
Conc: 13.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-053


Manual Integrations
APPROVED

Ankita
7/18/2019 8:36:36 AM

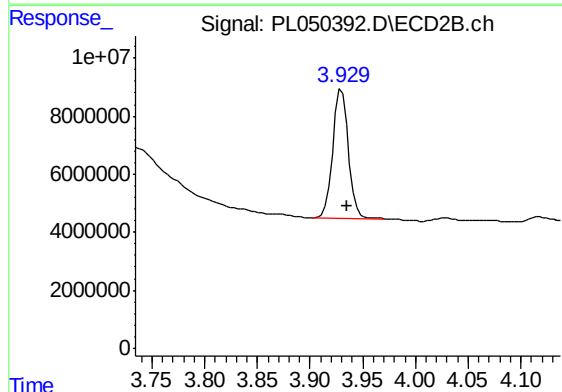


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.005 min
Response: 45519741
Conc: 14.87 ng/ml

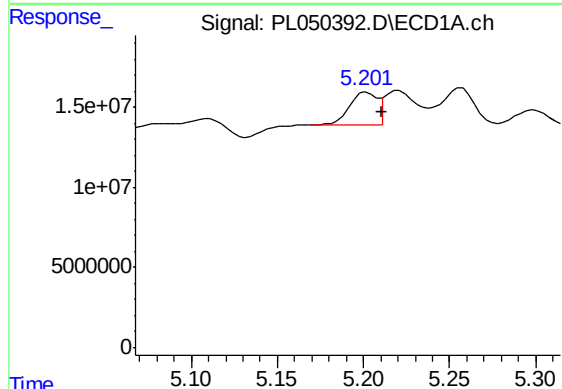


#10 gamma-Chlordane

R.T.: 5.201 min
Delta R.T.: -0.010 min
Response: 27639068
Conc: 1.62 ng/ml m

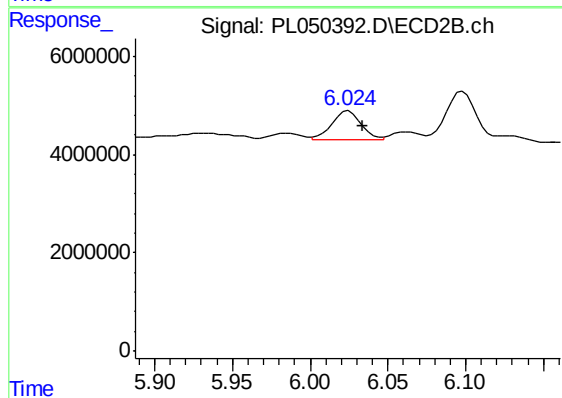

#10 gamma-Chlordane

R.T.: 6.025 min
Delta R.T.: -0.009 min
Response: 7663025
Conc: 2.06 ng/ml

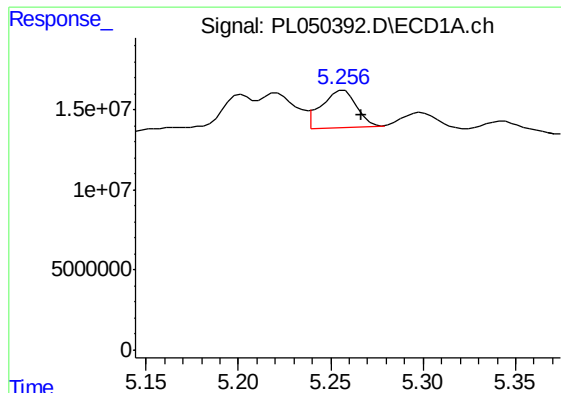


#11 alpha-Chlordane

R.T.: 5.257 min
Delta R.T.: -0.009 min
Response: 31132437
Conc: 1.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-053


Manual Integrations
APPROVED

Ankita
7/18/2019 8:36:36 AM

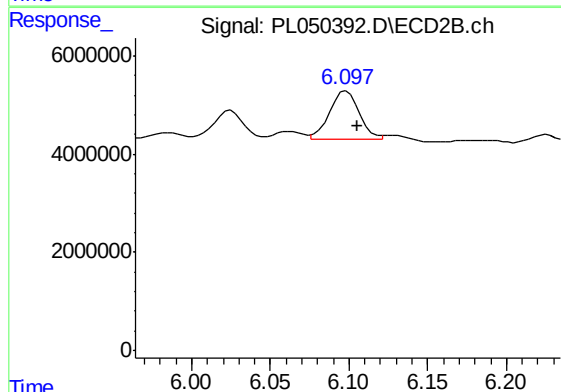


#11 alpha-Chlordane

R.T.: 6.097 min
Delta R.T.: -0.008 min
Response: 13188922
Conc: 3.57 ng/ml m

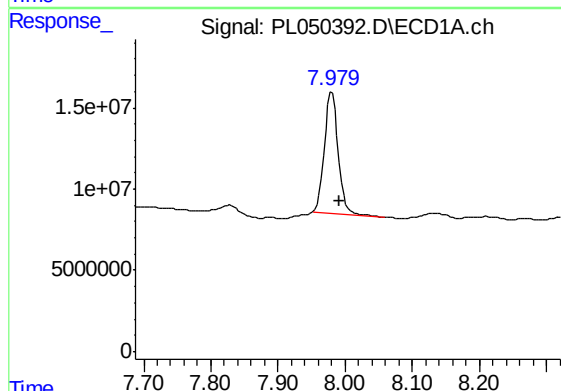

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.012 min
Response: 107545975
Conc: 8.46 ng/ml

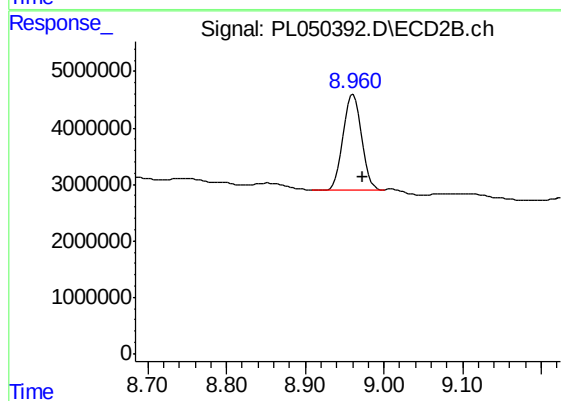

#28 Decachlorobiphenyl

R.T.: 8.961 min
Delta R.T.: -0.012 min
Response: 28397879
Conc: 8.46 ng/ml