

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
 Data File : PL050403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2019 16:13
 Operator : SM\AJ
 Sample : K3810-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-1

Manual Integrations
 APPROVED

Ankita
 7/18/2019 8:37:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:10:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.931	192.4E6	56287466	17.064	18.384
28)	SA Decachlor...	7.981	8.960	162.3E6	53455855	12.774	15.923m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
Data File : PL050403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2019 16:13
Operator : SM\AJ
Sample : K3810-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
S-1


Manual Integrations
APPROVED

Ankita
7/18/2019 8:37:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:10:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

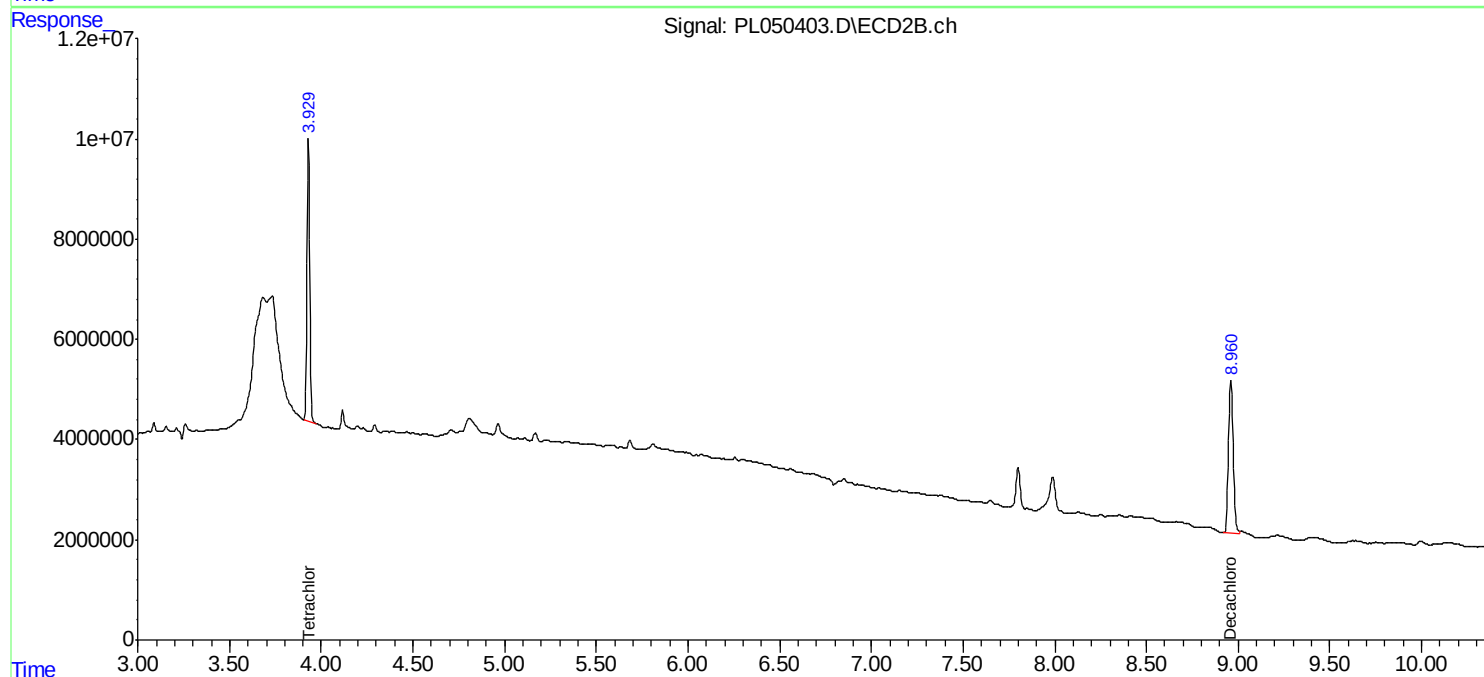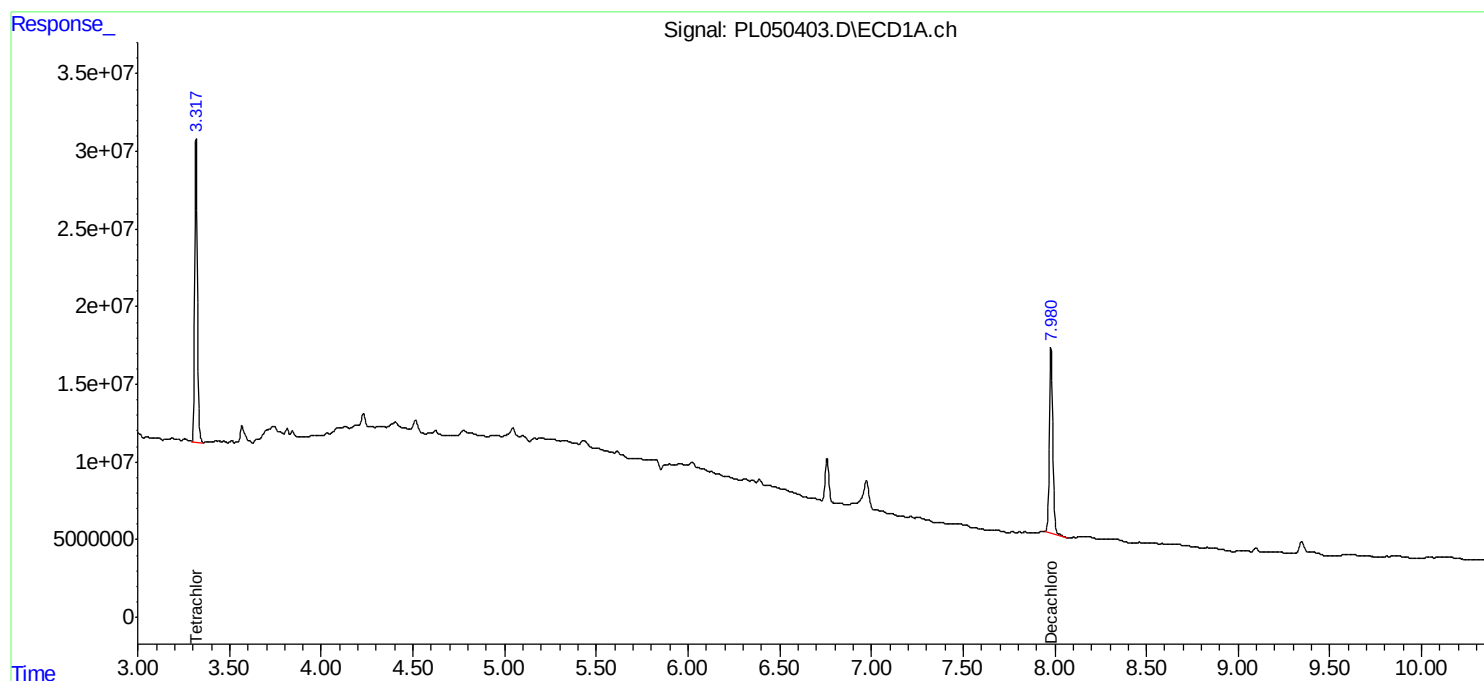

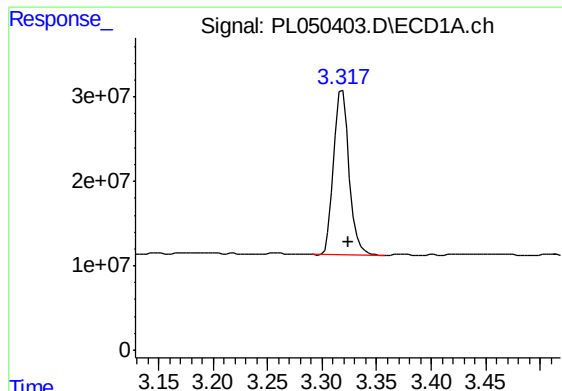


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: -0.006 min
Response: 192445113
Conc: 17.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1


Manual Integrations
APPROVED

Ankita
7/18/2019 8:37:00 AM

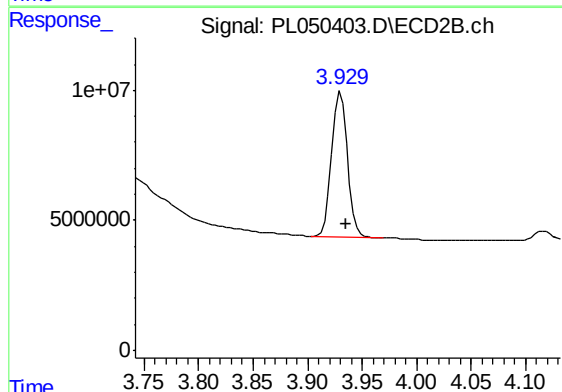


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.005 min
Response: 56287466
Conc: 18.38 ng/ml

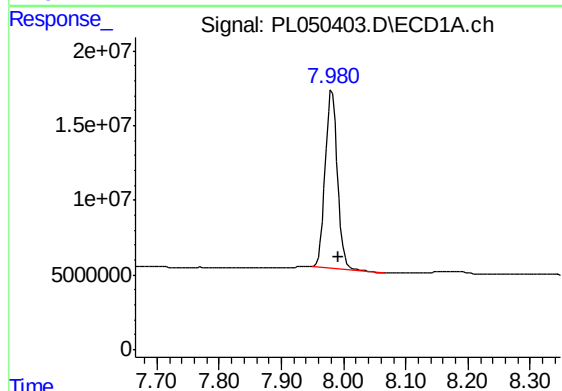

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: -0.011 min
Response: 162310019
Conc: 12.77 ng/ml

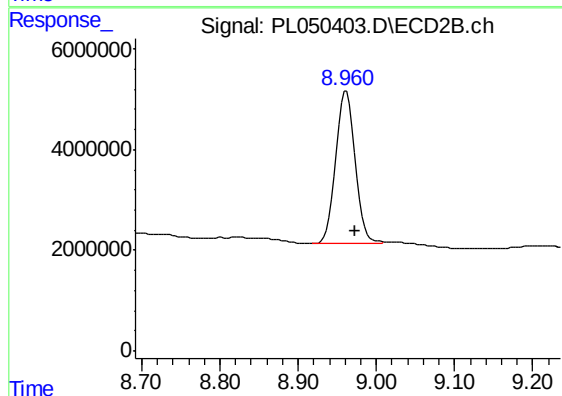

#28 Decachlorobiphenyl

R.T.: 8.960 min
Delta R.T.: -0.013 min
Response: 53455855
Conc: 15.92 ng/ml m