

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
 Data File : PL050429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2019 22:42
 Operator : SM\AJ
 Sample : K3622-05
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-071519-A

Manual Integrations
 APPROVED

Ankita
 7/18/2019 8:37:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:14:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	3.929	121.8E6	29605671	10.800m	9.669m
28)	SA Decachlor...	7.980	8.961	100.2E6	31741790	7.887	9.455
Target Compounds							
10)	B gamma-Chl...	5.194f	6.025	10388469	2871473	0.608m	0.771m#
11)	B alpha-Chl...	5.255	6.099	10789835	8793457	0.650m	2.378m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071619\
Data File : PL050429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2019 22:42
Operator : SM\AJ
Sample : K3622-05
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
OR-03-071519-A


Manual Integrations
APPROVED

Ankita
7/18/2019 8:37:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:14:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

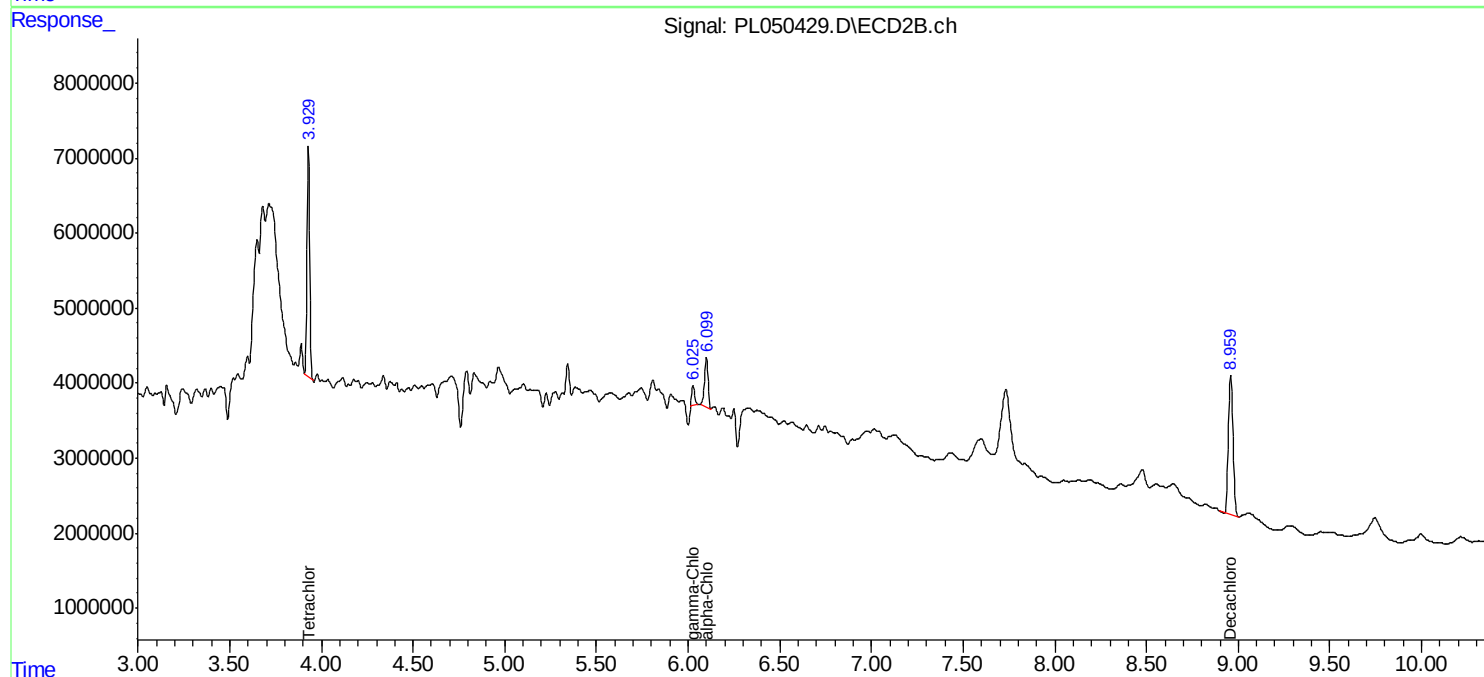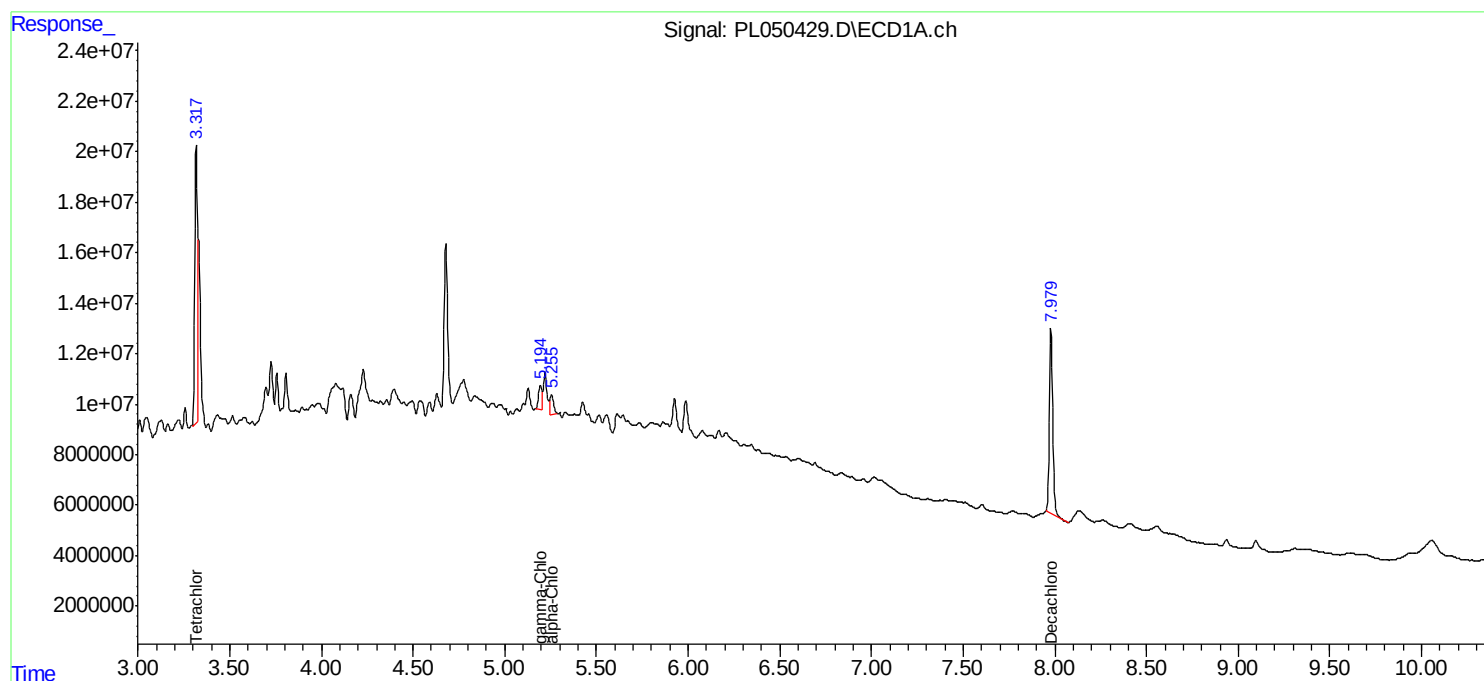

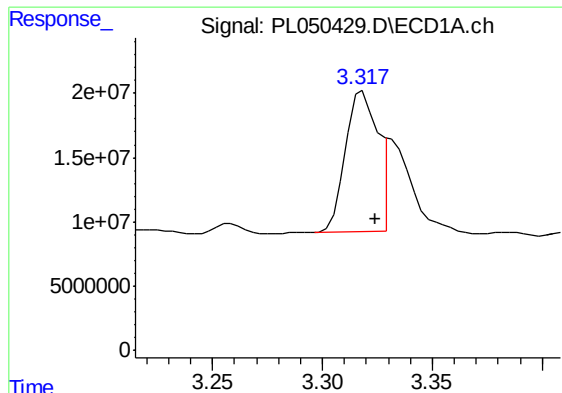


#1 Tetrachloro-m-xylene

R.T.: 3.317 min
Delta R.T.: -0.007 min
Response: 121798422
Conc: 10.80 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OR-03-071519-A


Manual Integrations
APPROVED

Ankita
7/18/2019 8:37:40 AM

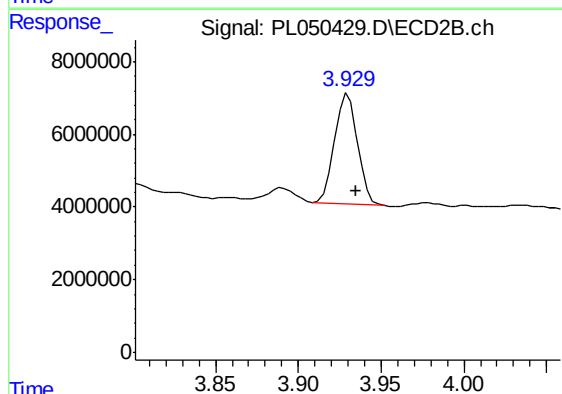


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.007 min
Response: 29605671
Conc: 9.67 ng/ml m

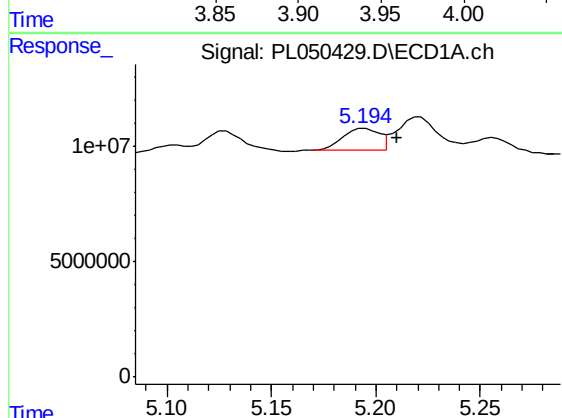


#10 gamma-Chlordane

R.T.: 5.194 min
Delta R.T.: -0.017 min
Response: 10388469
Conc: 0.61 ng/ml m

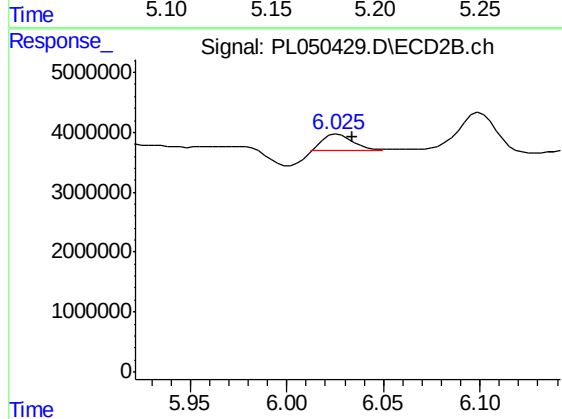

#10 gamma-Chlordane

R.T.: 6.025 min
Delta R.T.: -0.009 min
Response: 2871473
Conc: 0.77 ng/ml m

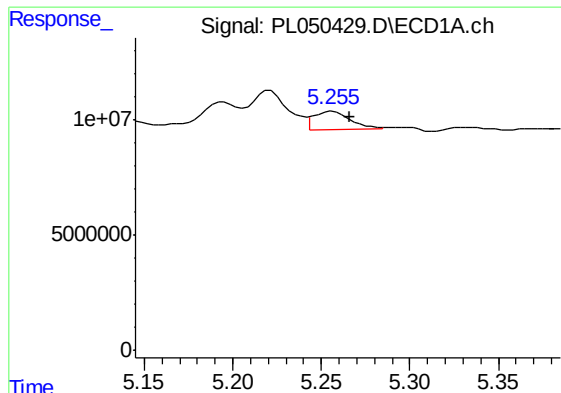


#11 alpha-Chlordane

R.T.: 5.255 min
Delta R.T.: -0.011 min
Response: 10789835
Conc: 0.65 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OR-03-071519-A


Manual Integrations
APPROVED

Ankita
7/18/2019 8:37:40 AM

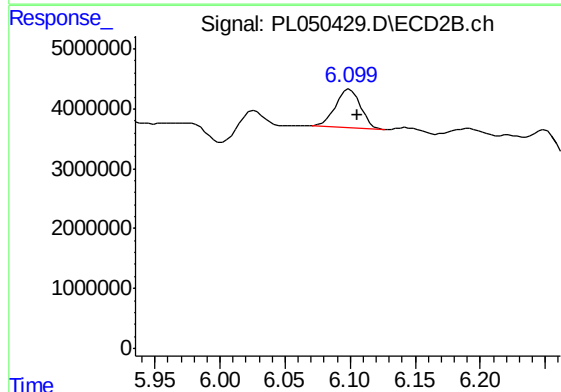


#11 alpha-Chlordane

R.T.: 6.099 min
Delta R.T.: -0.007 min
Response: 8793457
Conc: 2.38 ng/ml m

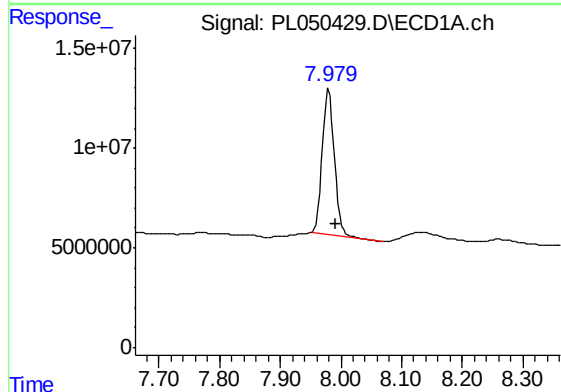

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.012 min
Response: 100218007
Conc: 7.89 ng/ml

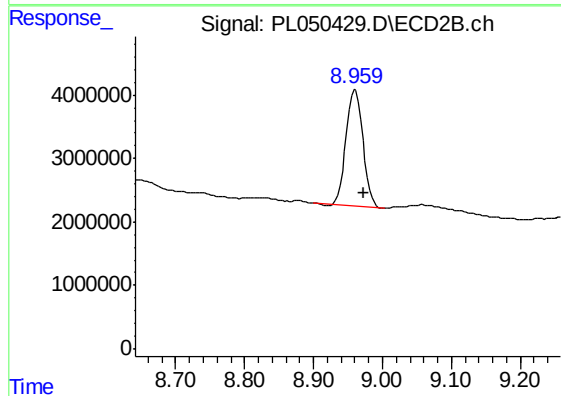

#28 Decachlorobiphenyl

R.T.: 8.961 min
Delta R.T.: -0.012 min
Response: 31741790
Conc: 9.46 ng/ml