

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071620\
 Data File : PL059998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2020 00:58
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 04:59:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	42830675	56851007	22.144	21.452
28)	SA Decachlor...	8.225	9.100	30727720	38513150	18.678	18.415
Target Compounds							
8)	B Heptachlo...	0.000	5.884	0	29735437	N.D.	11.041 #
11)	B alpha-Chl...	0.000	6.180f	0	22119491	N.D.	7.736 #
12)	B 4,4'-DDE	0.000	6.335f	0	51249699	N.D.	19.147 #
14)	MA Endrin	6.021	6.719	996926	78506587	0.685	36.891 #
18)	B Endrin al...	0.000	7.037f	0	19303121	N.D.	8.888 #
26)	Chlordane-4	0.000	6.180f	0	22119491	N.D.	47.785 #
27)	Chlordane-5	0.000	7.037f	0	19303121	N.D.	248.543 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071620\
Data File : PL059998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2020 00:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 04:59:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

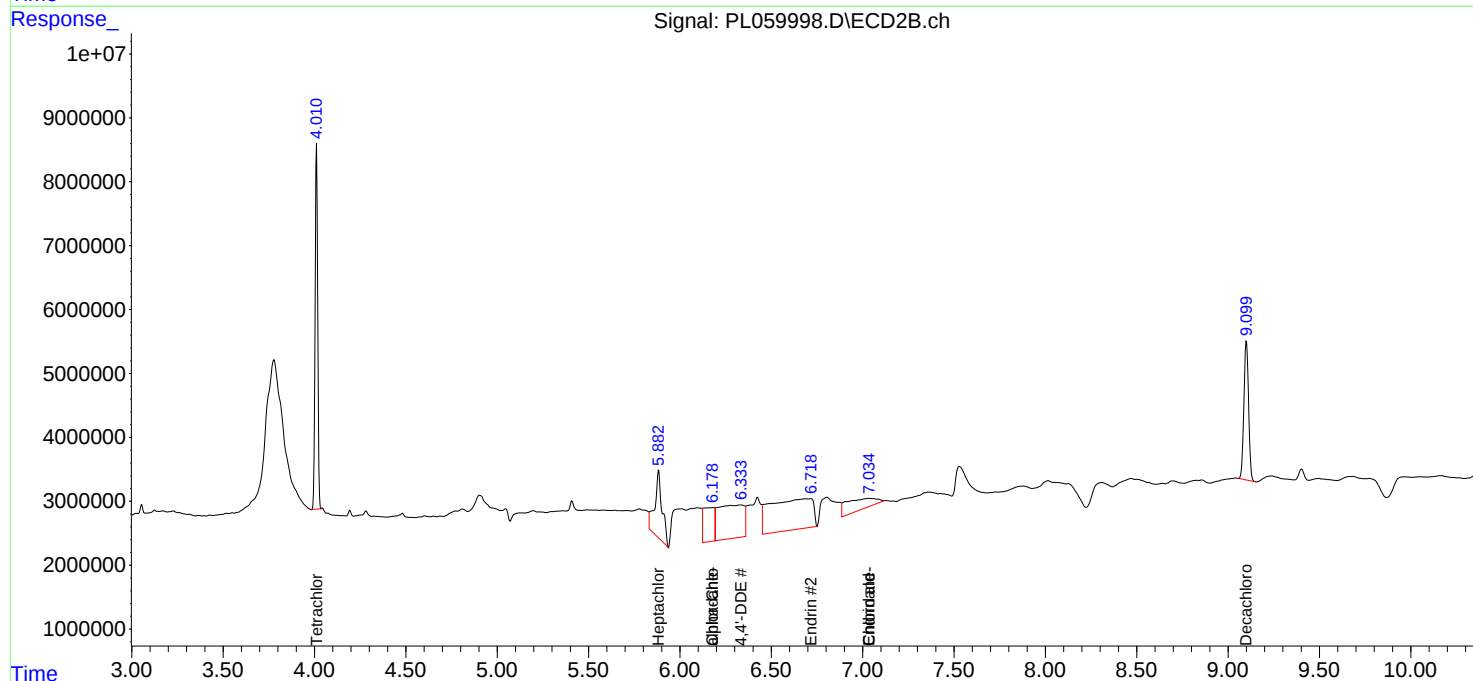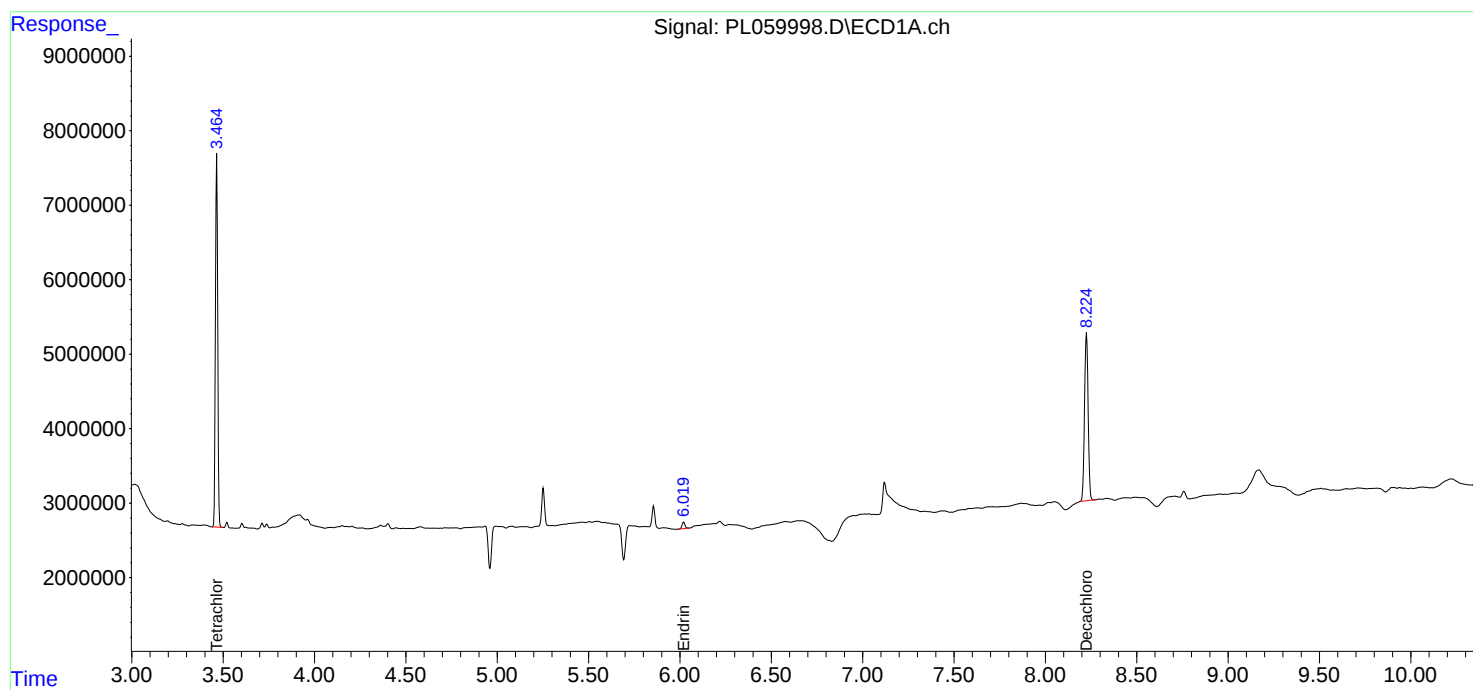


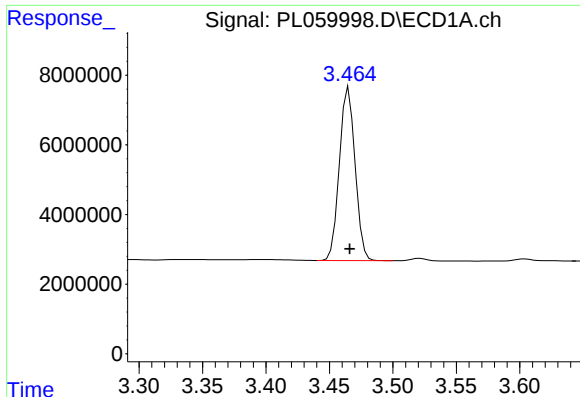

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 42830675
Conc: 22.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

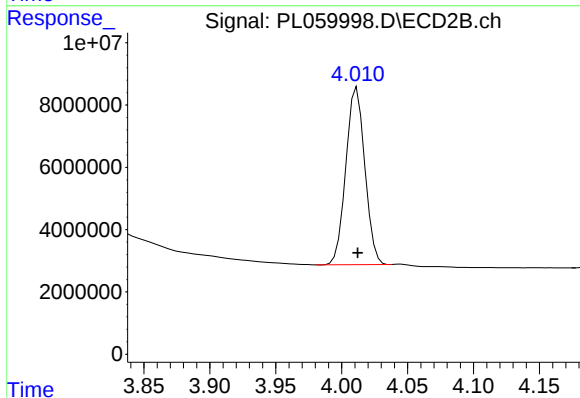


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 56851007
Conc: 21.45 ng/ml

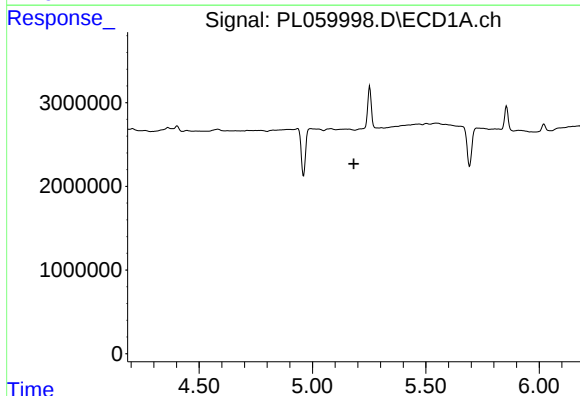


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.183 min
Response: 0
Conc: N.D.

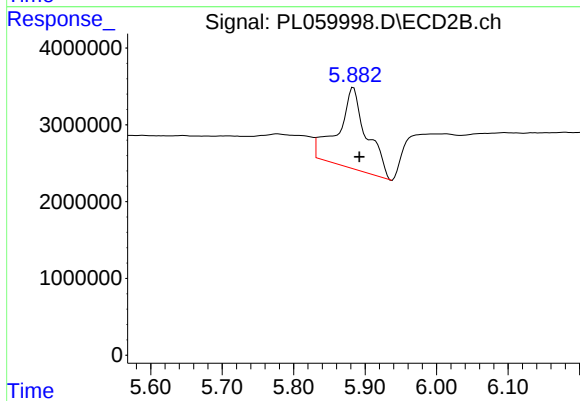

#8 Heptachlor epoxide


R.T.: 5.884 min
Delta R.T.: -0.008 min
Response: 29735437
Conc: 11.04 ng/ml

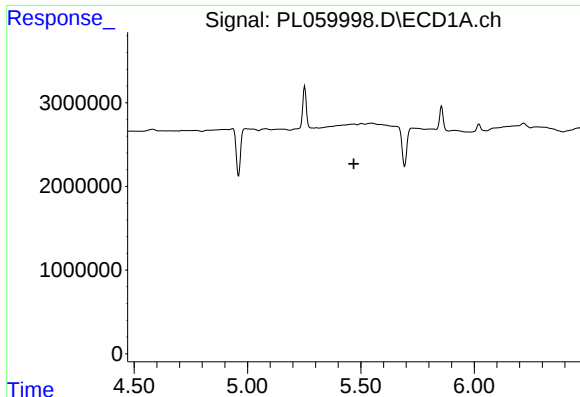

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

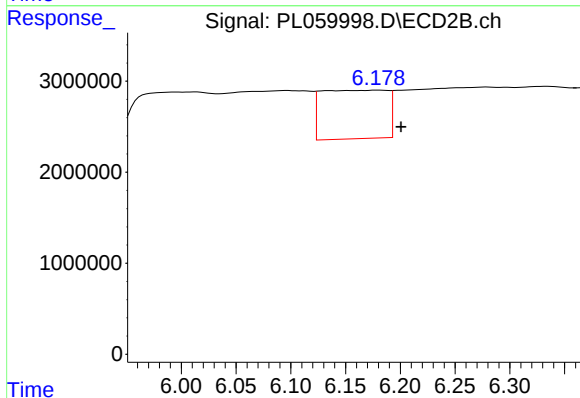


#11 alpha-Chlordane

R.T.: 6.180 min
Delta R.T.: -0.020 min
Response: 22119491
Conc: 7.74 ng/ml

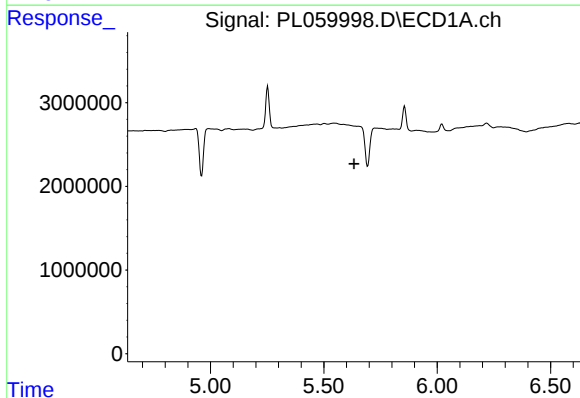


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.634 min
Response: 0
Conc: N.D.

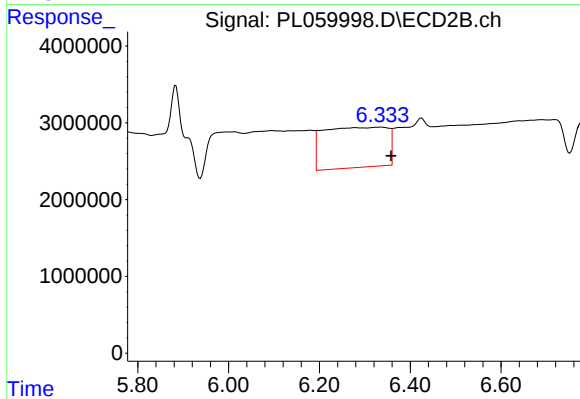

#12 4,4'-DDE


R.T.: 6.335 min
Delta R.T.: -0.023 min
Response: 51249699
Conc: 19.15 ng/ml

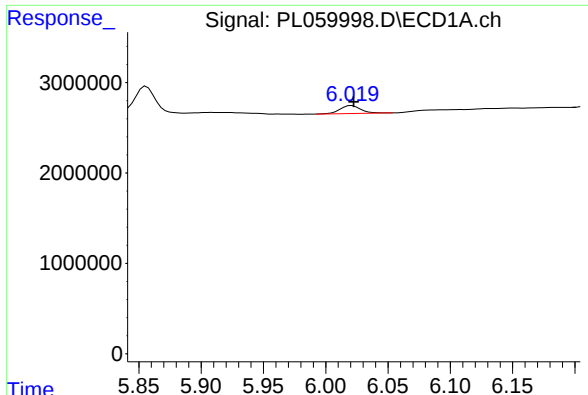

#14 Endrin


R.T.: 6.021 min
Delta R.T.: -0.002 min
Response: 996926
Conc: 0.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

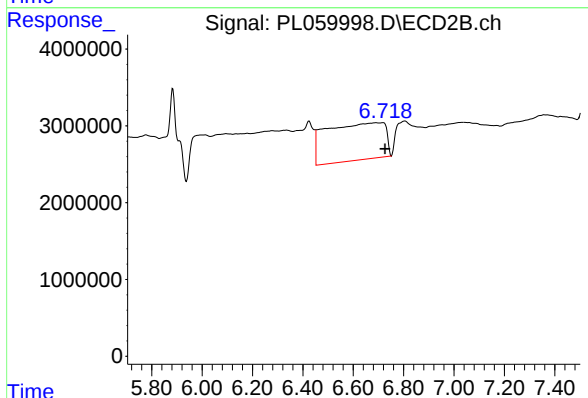


#14 Endrin

R.T.: 6.719 min
Delta R.T.: -0.008 min
Response: 78506587
Conc: 36.89 ng/ml

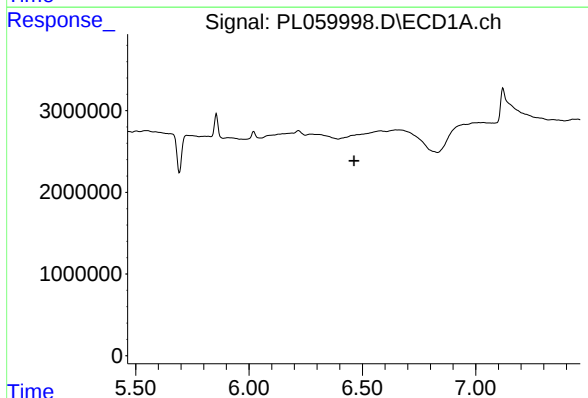


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.464 min
Response: 0
Conc: N.D.

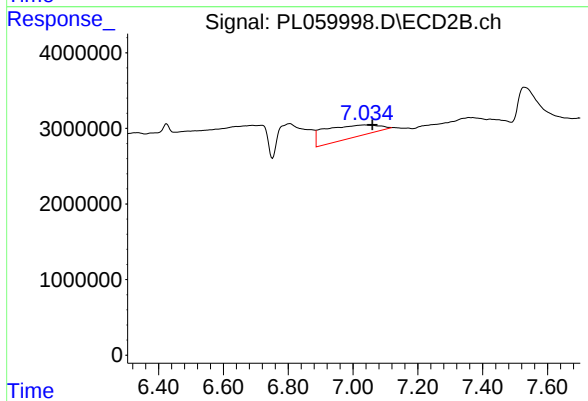

#18 Endrin aldehyde


R.T.: 7.037 min
Delta R.T.: -0.023 min
Response: 19303121
Conc: 8.89 ng/ml

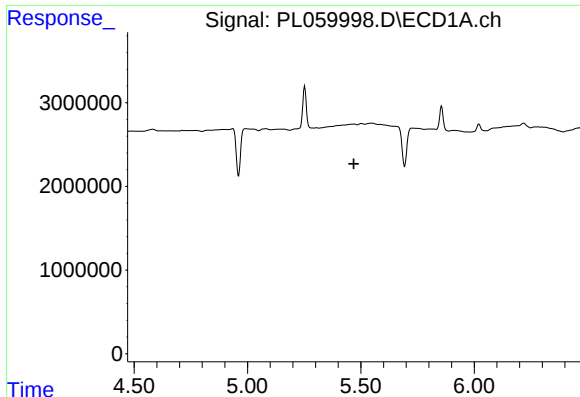

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

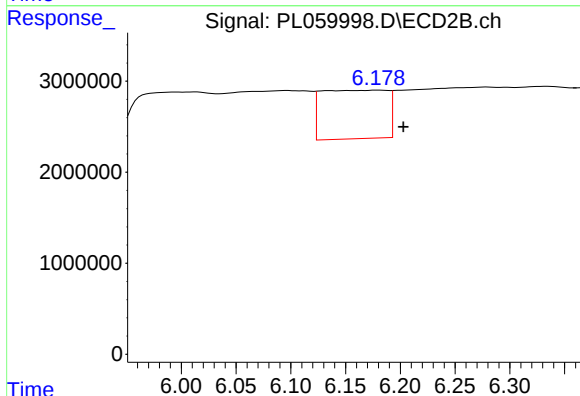


#26 Chlordane-4

R.T.: 6.180 min
Delta R.T.: -0.023 min
Response: 22119491
Conc: 47.78 ng/ml

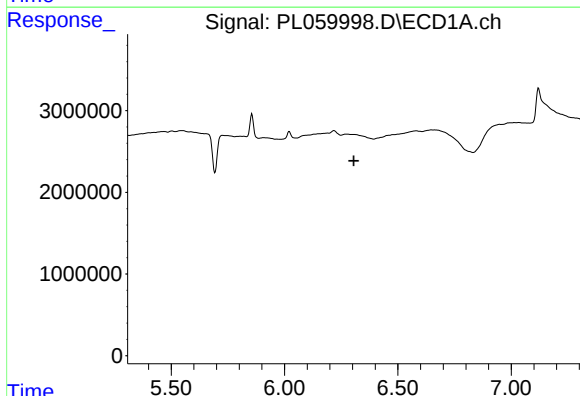


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.306 min
Response: 0
Conc: N.D.

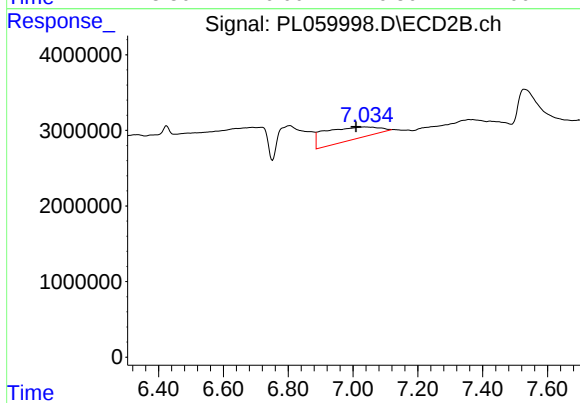

#27 Chlordane-5


R.T.: 7.037 min
Delta R.T.: 0.027 min
Response: 19303121
Conc: 248.54 ng/ml

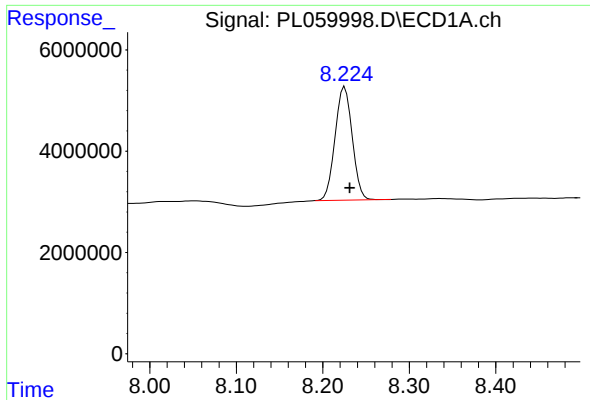

#28 Decachlorobiphenyl

R.T.: 8.225 min
Delta R.T.: -0.006 min
Response: 30727720
Conc: 18.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

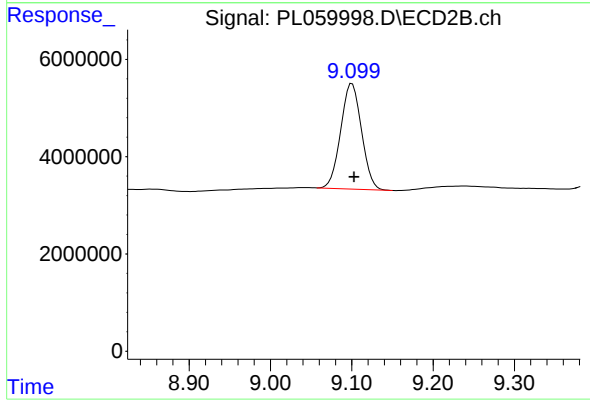

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.002 min
Response: 38513150
Conc: 18.42 ng/ml