

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071620\
 Data File : PL059943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 10:57
 Operator : DD\AJ
 Sample : L3183-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-071420

Manual Integrations
 APPROVED

Ankita
 7/17/2020 11:42:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 12:16:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.010	26273440	31613582	13.583	11.929
28)	SA Decachlor...	8.225	9.098	17207135	22895683	10.460	10.948m
Target Compounds							
10)	B gamma-Chl...	5.406	6.123	3870458	3918453	2.133m	1.368m#
11)	B alpha-Chl...	5.466	6.196	7967776	8065963	4.418	2.821m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071620\
Data File : PL059943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 10:57
Operator : DD\AJ
Sample : L3183-06
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-01-071420


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 12:16:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

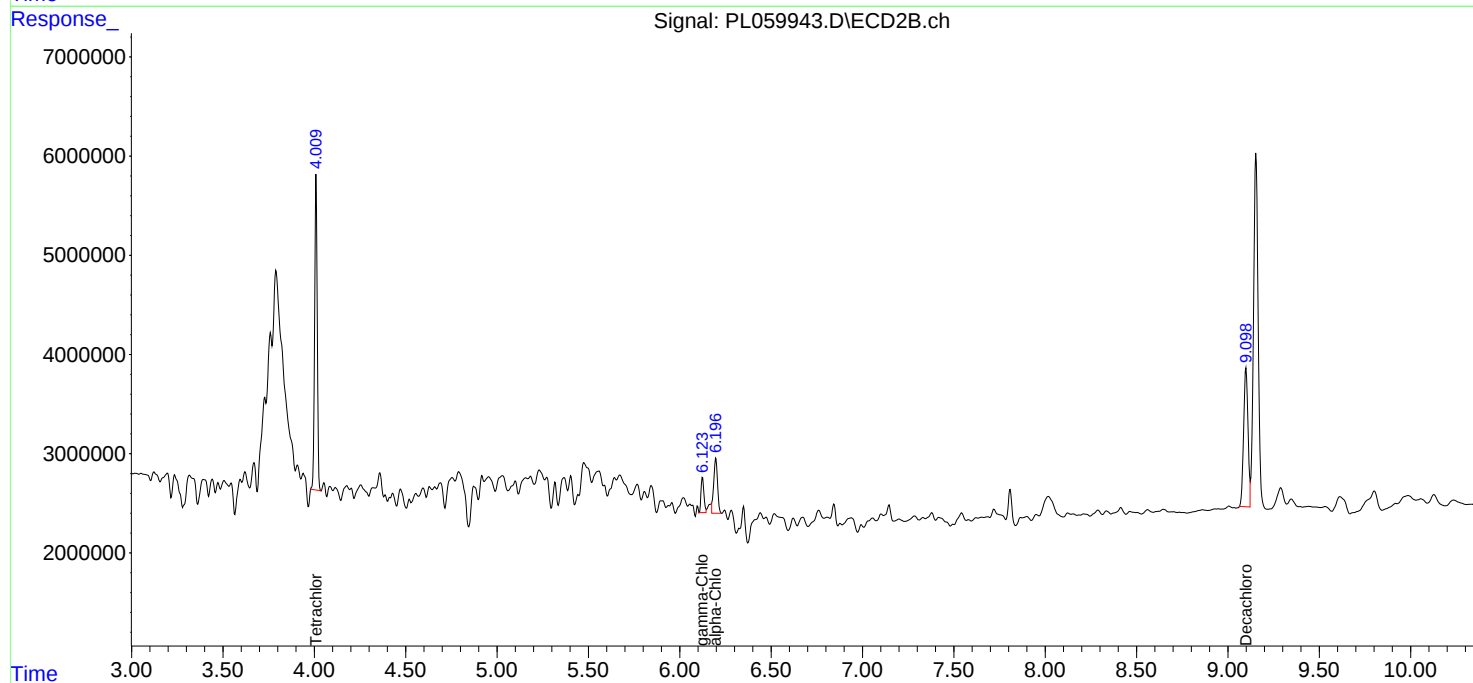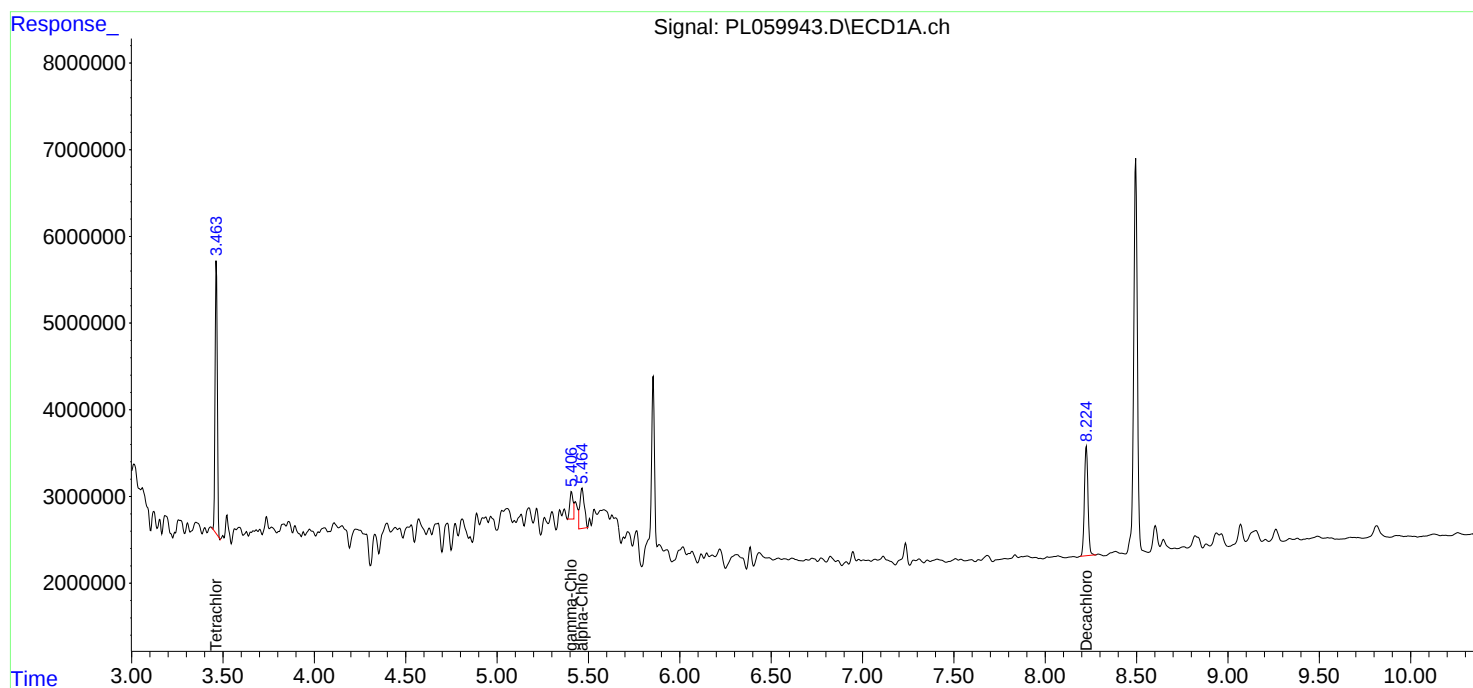

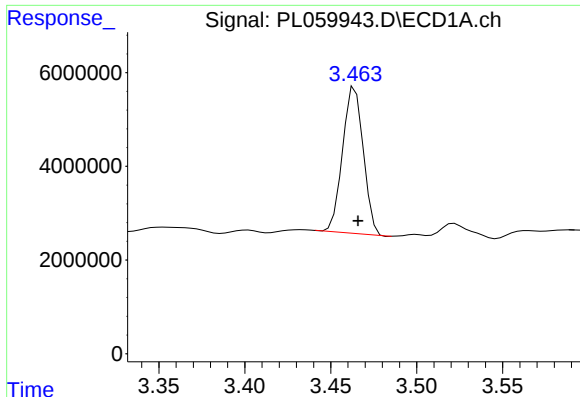


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: -0.002 min
Response: 26273440
Conc: 13.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-071420


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:50 AM

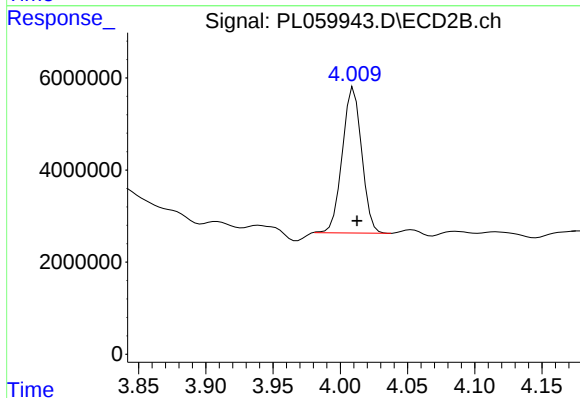


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: -0.002 min
Response: 31613582
Conc: 11.93 ng/ml

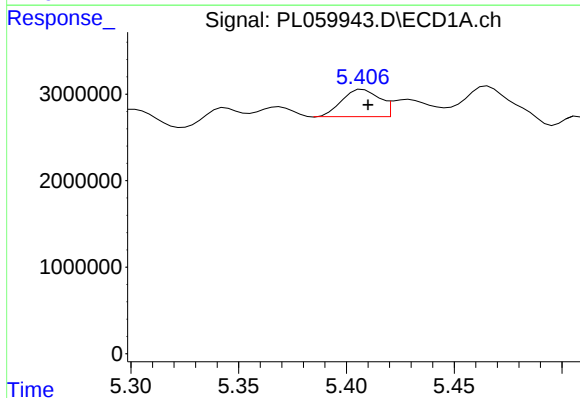


#10 gamma-Chlordane

R.T.: 5.406 min
Delta R.T.: -0.004 min
Response: 3870458
Conc: 2.13 ng/ml m

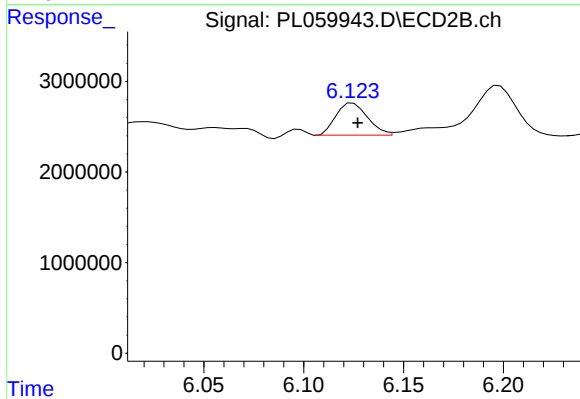

#10 gamma-Chlordane

R.T.: 6.123 min
Delta R.T.: -0.004 min
Response: 3918453
Conc: 1.37 ng/ml m

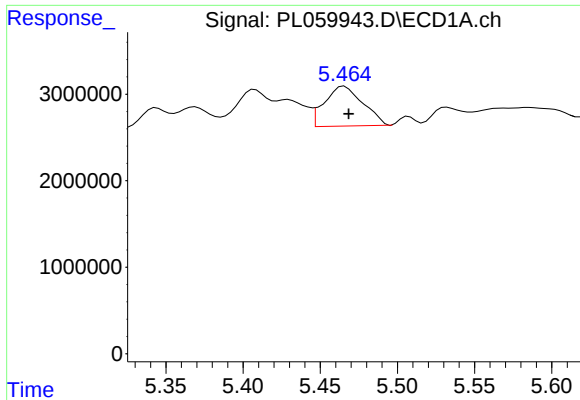


#11 alpha-Chlordane

R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 7967776
Conc: 4.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-071420


Manual Integrations
APPROVED

Ankita
7/17/2020 11:42:50 AM

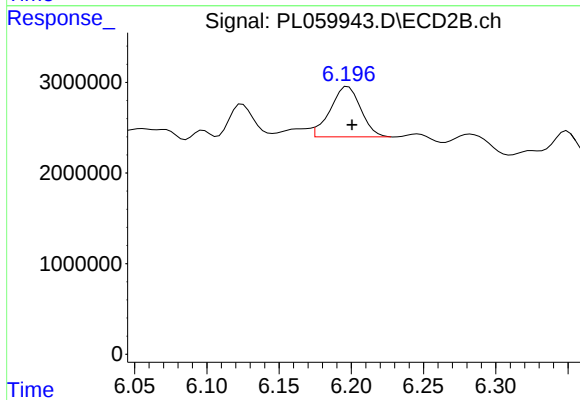


#11 alpha-Chlordane

R.T.: 6.196 min
Delta R.T.: -0.004 min
Response: 8065963
Conc: 2.82 ng/ml m

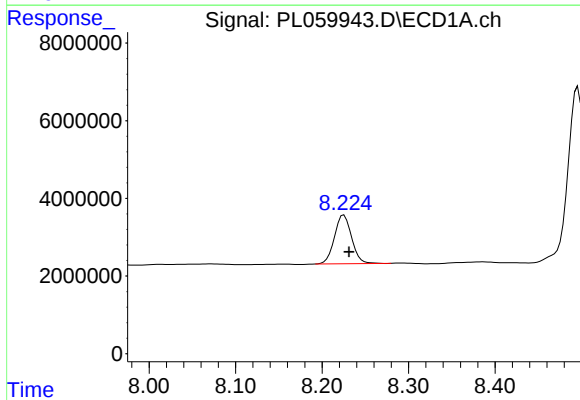

#28 Decachlorobiphenyl

R.T.: 8.225 min
Delta R.T.: -0.006 min
Response: 17207135
Conc: 10.46 ng/ml

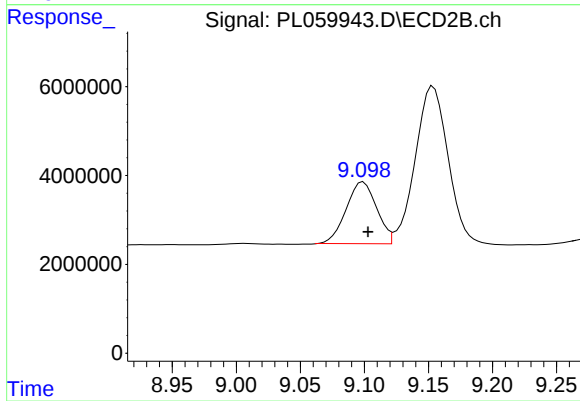

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: -0.005 min
Response: 22895683
Conc: 10.95 ng/ml m