

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071620\
 Data File : PL059958.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 15:05
 Operator : DD\AJ
 Sample : L3183-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-071520

Manual Integrations
 APPROVED

Ankita
 7/17/2020 11:43:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 17:52:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.469	4.012	26271495	32247623	13.582	12.168
28)	SA Decachlor...	8.230	9.104	17297562	20153997	10.515	9.637
Target Compounds							
11)	B alpha-Chl...	5.472	6.200	8014292	8647895	4.444	3.025m#
17)	MA 4,4'-DDT	6.393	7.150	1758681	1849157	1.353	0.939 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071620\
Data File : PL059958.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 15:05
Operator : DD\AJ
Sample : L3183-11
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-03-071520


Manual Integrations
APPROVED

Ankita
7/17/2020 11:43:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 17:52:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

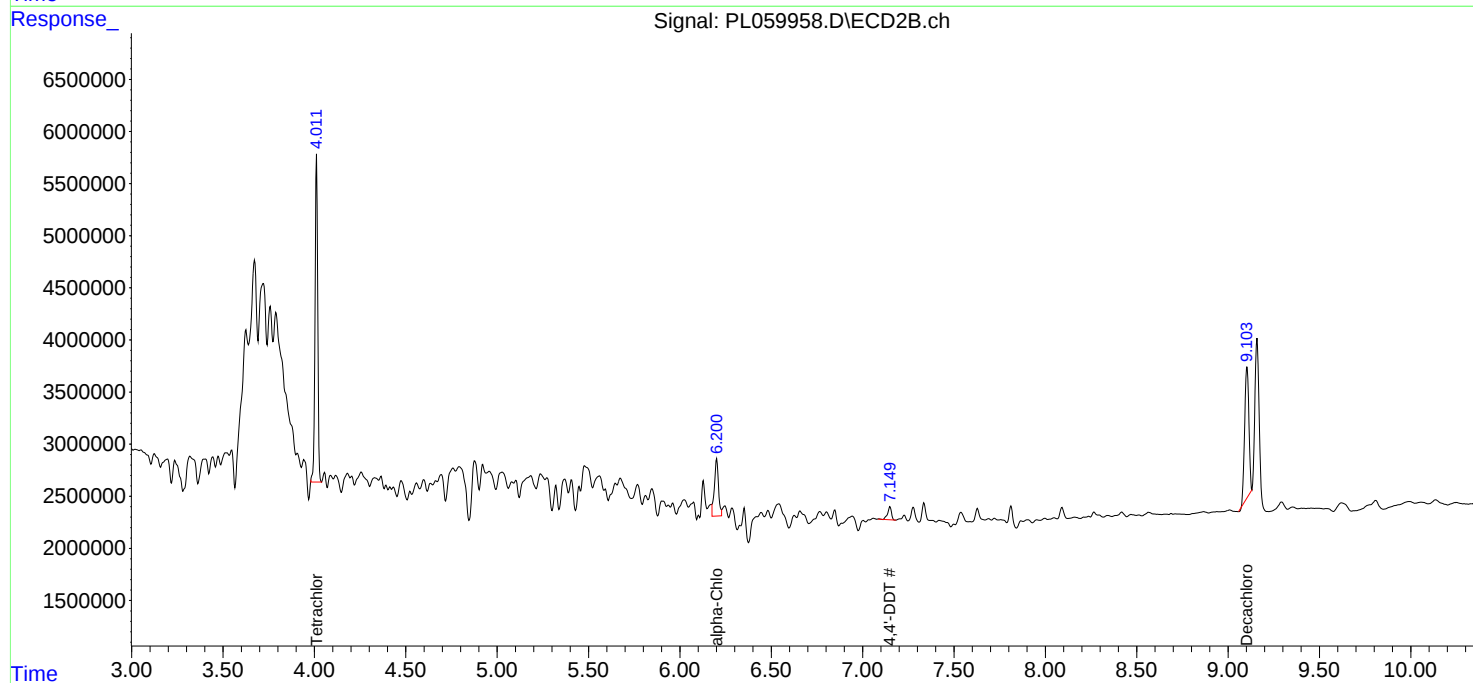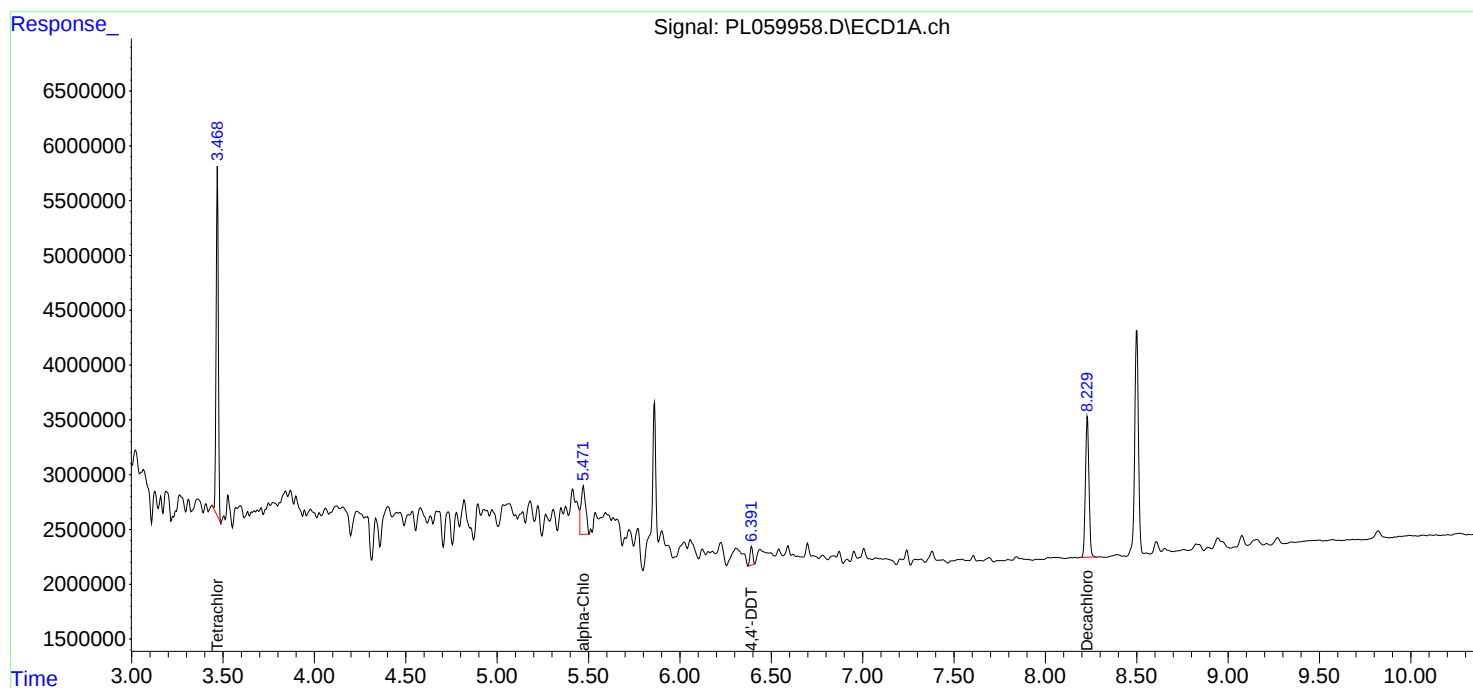

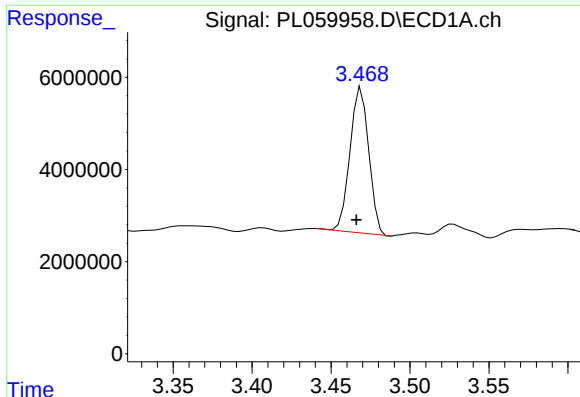


#1 Tetrachloro-m-xylene

R.T.: 3.469 min
Delta R.T.: 0.003 min
Response: 26271495
Conc: 13.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-071520


Manual Integrations
APPROVED

Ankita
7/17/2020 11:43:07 AM

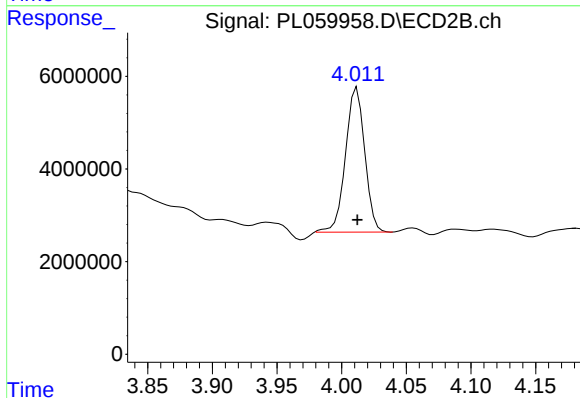


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 32247623
Conc: 12.17 ng/ml

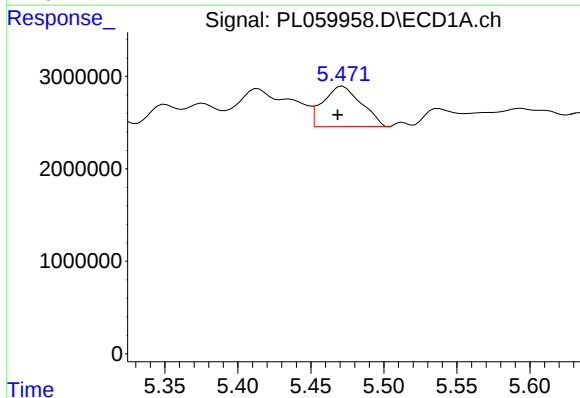


#11 alpha-Chlordane

R.T.: 5.472 min
Delta R.T.: 0.003 min
Response: 8014292
Conc: 4.44 ng/ml

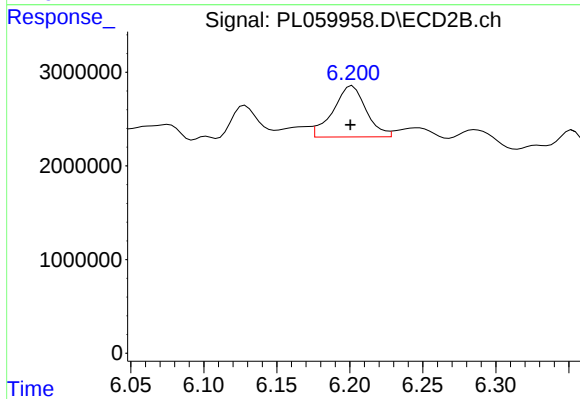

#11 alpha-Chlordane

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 8647895
Conc: 3.02 ng/ml m

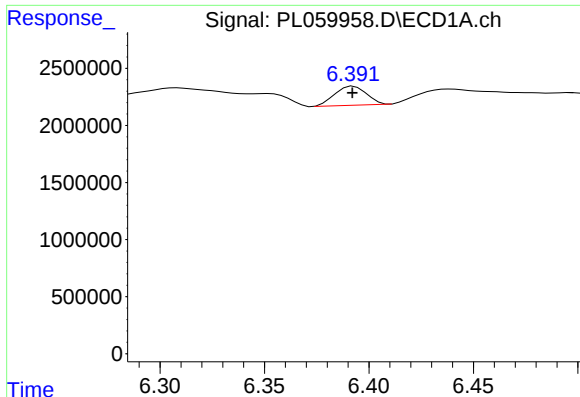


#17 4,4'-DDT

R.T.: 6.393 min
Delta R.T.: 0.000 min
Response: 1758681
Conc: 1.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-071520


Manual Integrations
APPROVED

Ankita
7/17/2020 11:43:07 AM

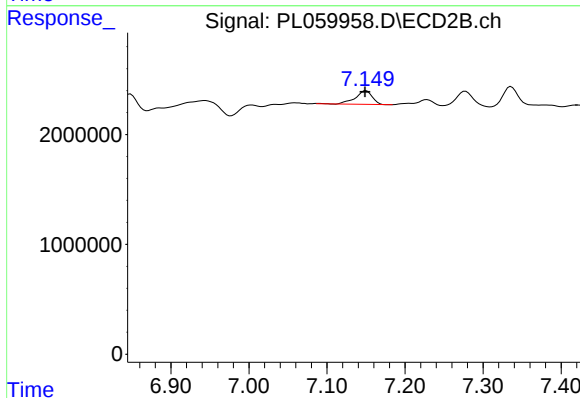


#17 4,4'-DDT

R.T.: 7.150 min
Delta R.T.: 0.001 min
Response: 1849157
Conc: 0.94 ng/ml

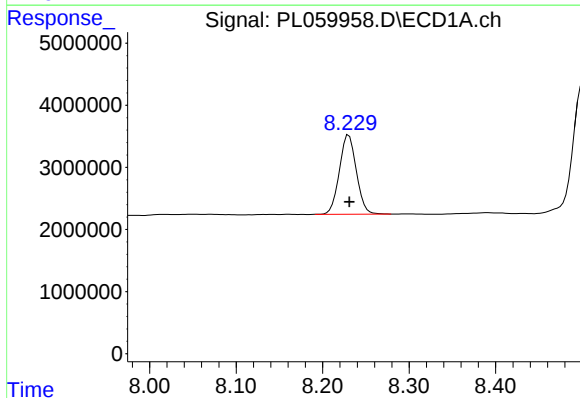

#28 Decachlorobiphenyl

R.T.: 8.230 min
Delta R.T.: 0.000 min
Response: 17297562
Conc: 10.51 ng/ml

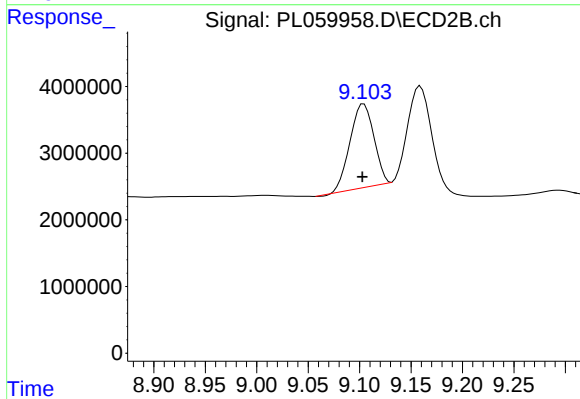

#28 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.001 min
Response: 20153997
Conc: 9.64 ng/ml