

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071620\
 Data File : PL059985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 21:55
 Operator : DD\AJ
 Sample : L3308-12
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 12

Manual Integrations
 APPROVED

Ankita
 7/17/2020 11:43:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 04:55:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.465	4.012	22167906	30449888	11.461	11.490
28) SA Decachlor...	8.225	9.099	17642507	21635581	10.724	10.345
Target Compounds						
10) B gamma-Chl...	5.407	6.124	2589682	5403065	1.427m	1.887m#
11) B alpha-Chl...	5.465	6.199	2352113	8058080	1.304m	2.818m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071620\
Data File : PL059985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 21:55
Operator : DD\AJ
Sample : L3308-12
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
12


Manual Integrations
APPROVED

Ankita
7/17/2020 11:43:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 04:55:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

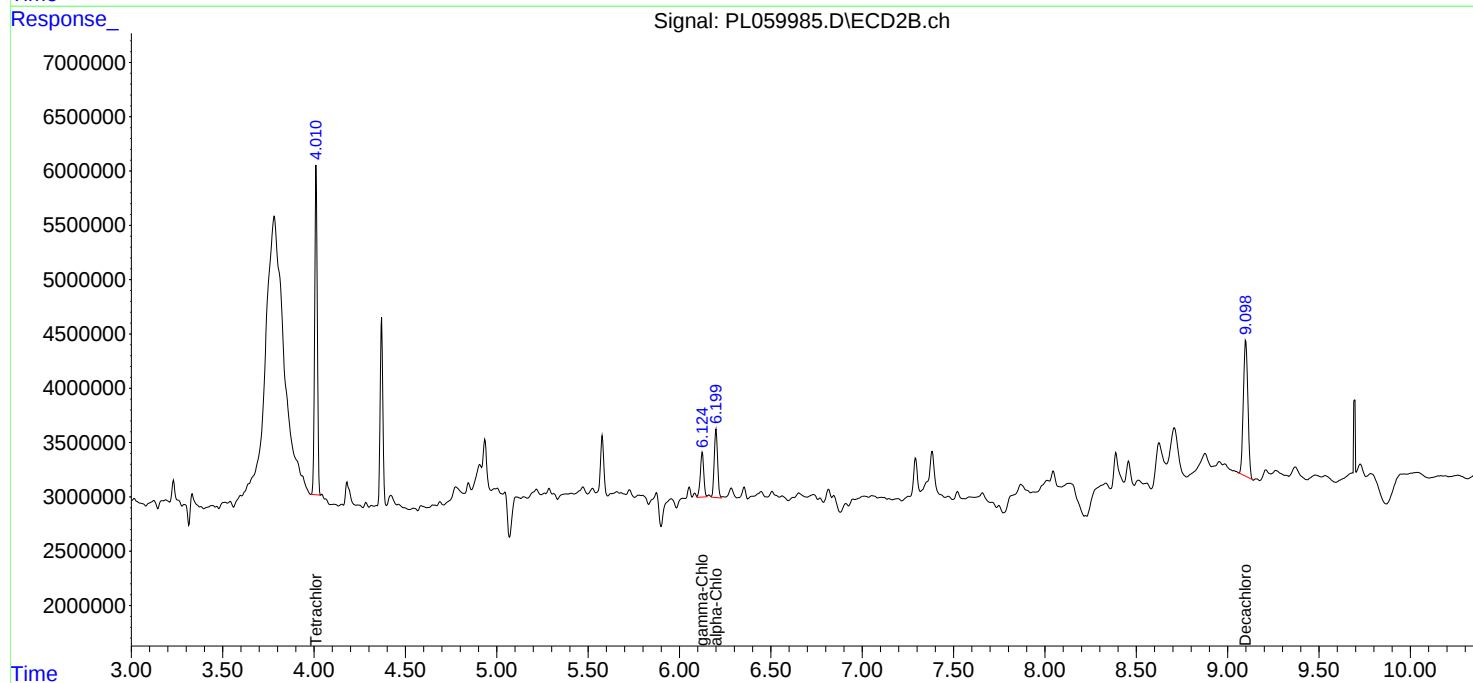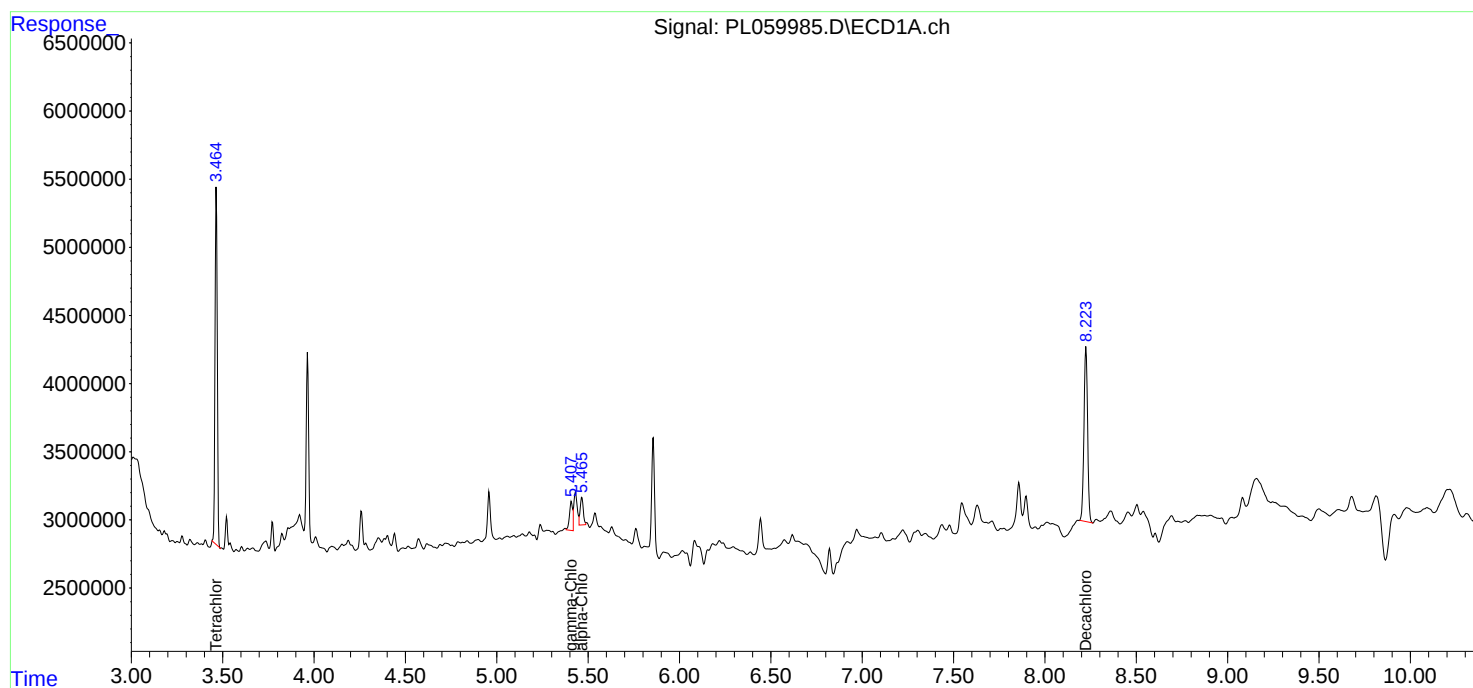

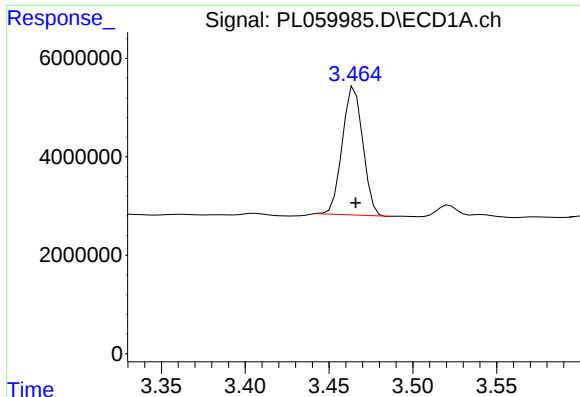


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 22167906
Conc: 11.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
12


Manual Integrations
APPROVED

Ankita
7/17/2020 11:43:53 AM

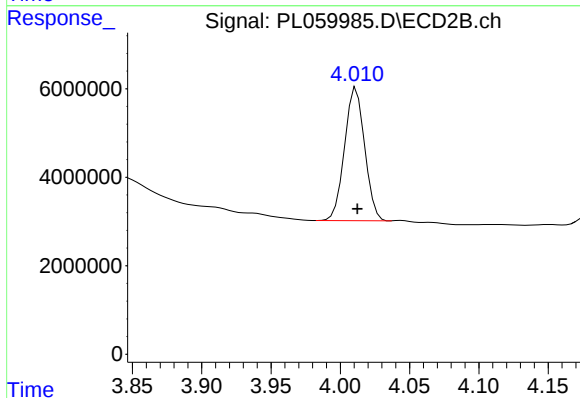


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 30449888
Conc: 11.49 ng/ml

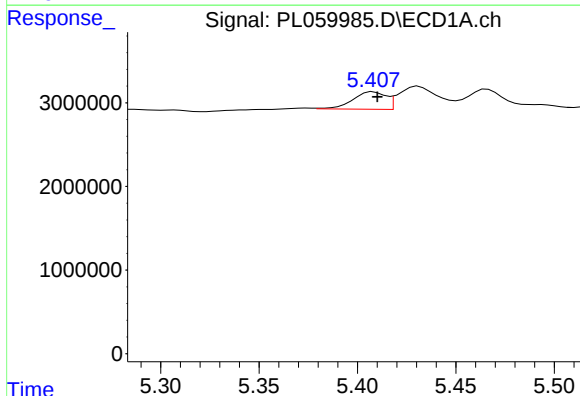


#10 gamma-Chlordane

R.T.: 5.407 min
Delta R.T.: -0.003 min
Response: 2589682
Conc: 1.43 ng/ml m

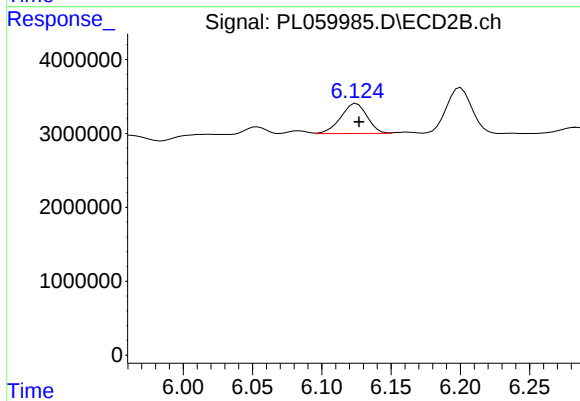

#10 gamma-Chlordane

R.T.: 6.124 min
Delta R.T.: -0.003 min
Response: 5403065
Conc: 1.89 ng/ml m

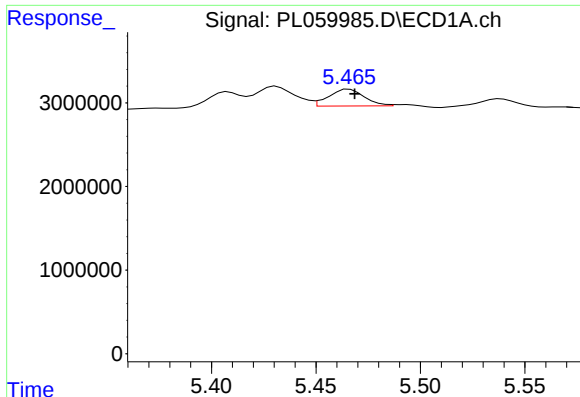


#11 alpha-Chlordane

R.T.: 5.465 min
Delta R.T.: -0.004 min
Response: 2352113
Conc: 1.30 ng/ml m

Instrument :
ECD_L
ClientSampleId :
12


Manual Integrations
APPROVED

Ankita
7/17/2020 11:43:53 AM

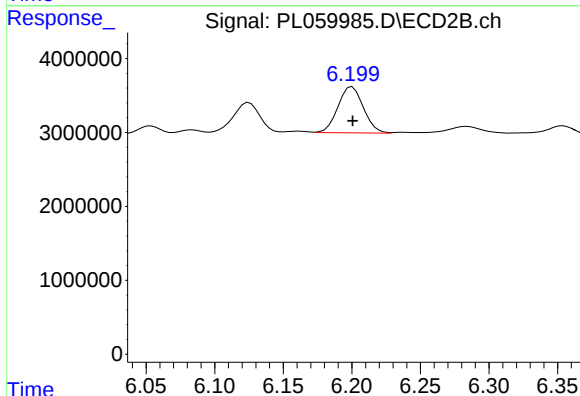


#11 alpha-Chlordane

R.T.: 6.199 min
Delta R.T.: -0.002 min
Response: 8058080
Conc: 2.82 ng/ml m

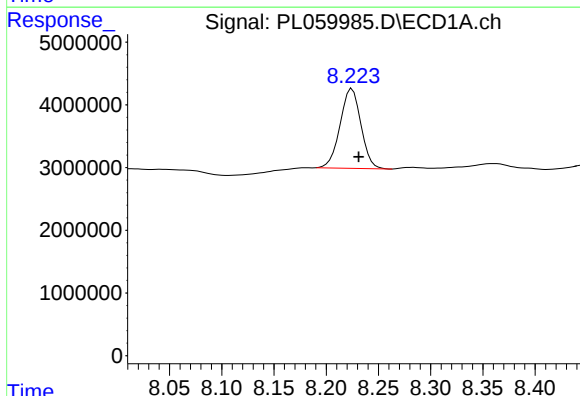

#28 Decachlorobiphenyl

R.T.: 8.225 min
Delta R.T.: -0.006 min
Response: 17642507
Conc: 10.72 ng/ml

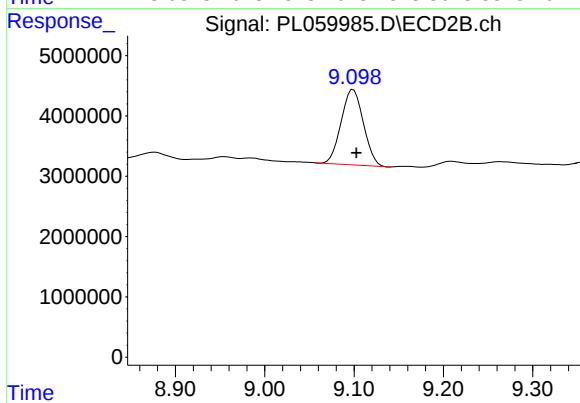

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.004 min
Response: 21635581
Conc: 10.35 ng/ml