

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071620\
 Data File : PL059993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2020 23:48
 Operator : DD\AJ
 Sample : L3308-20
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20

Manual Integrations
 APPROVED

Ankita
 7/17/2020 11:44:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 04:57:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.012	20487092	28896626	10.592	10.904
28)	SA Decachlor...	8.224	9.100	16861191	19202070	10.249	9.181
Target Compounds							
10)	B gamma-Chl...	5.406	6.123	1540316	3436861	0.849m	1.200m#
11)	B alpha-Chl...	5.465	6.199	1204744	4432582	0.668m	1.550m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071620\
Data File : PL059993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2020 23:48
Operator : DD\AJ
Sample : L3308-20
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
20


Manual Integrations
APPROVED

Ankita
7/17/2020 11:44:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 04:57:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

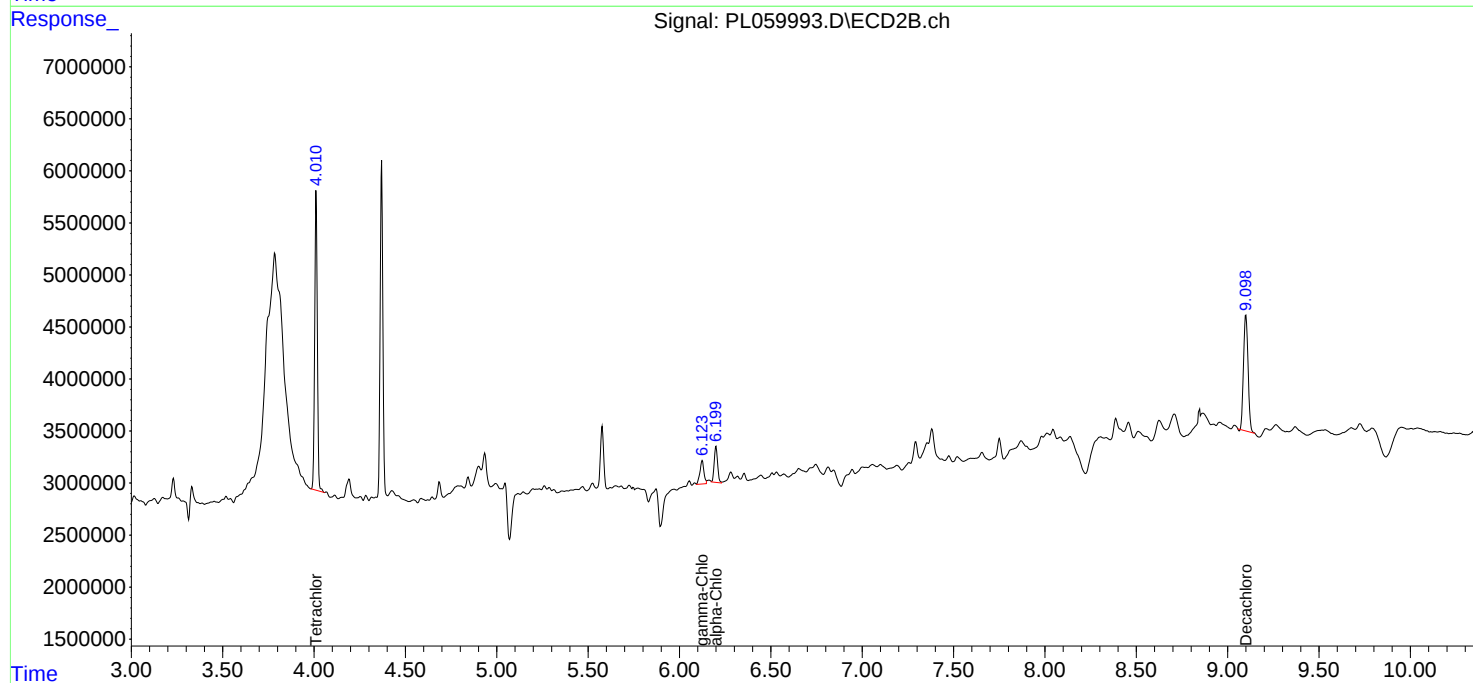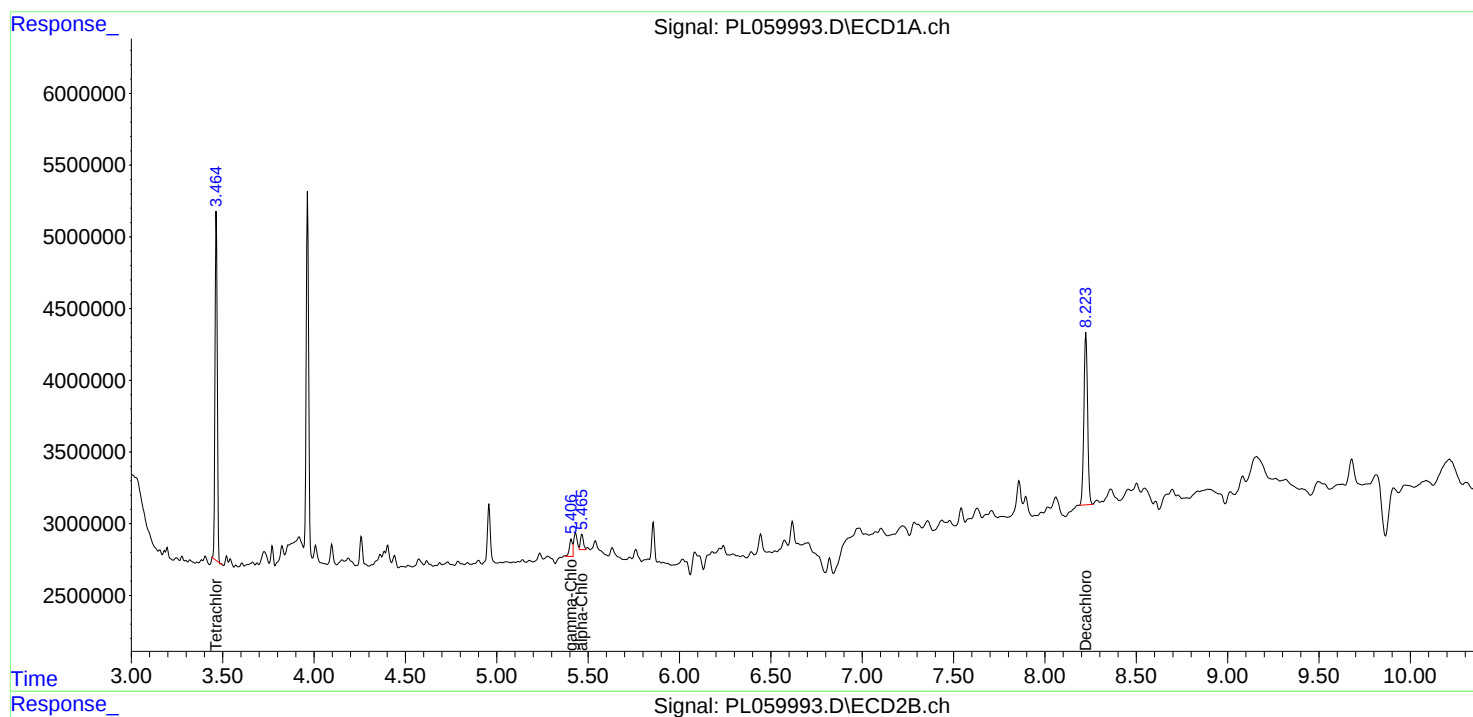

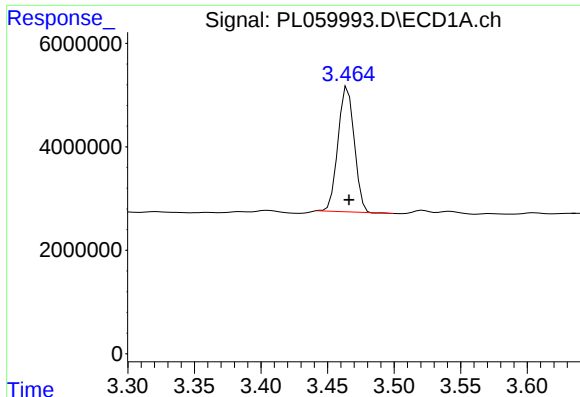


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 20487092
Conc: 10.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
20


Manual Integrations
APPROVED

Ankita
7/17/2020 11:44:02 AM

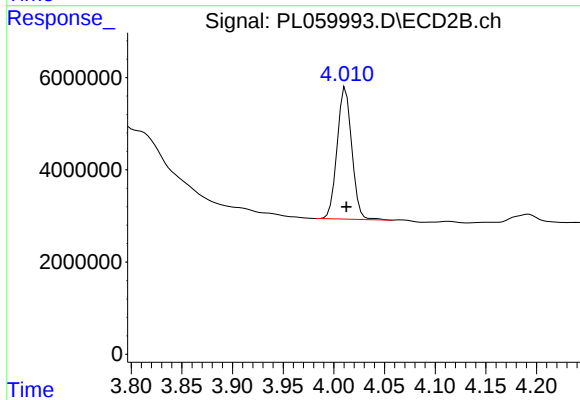


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 28896626
Conc: 10.90 ng/ml

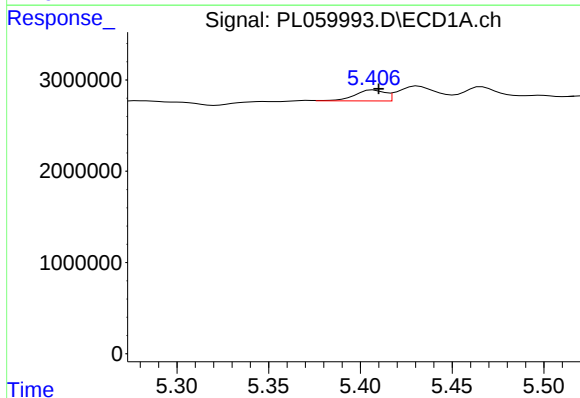


#10 gamma-Chlordane

R.T.: 5.406 min
Delta R.T.: -0.004 min
Response: 1540316
Conc: 0.85 ng/ml m

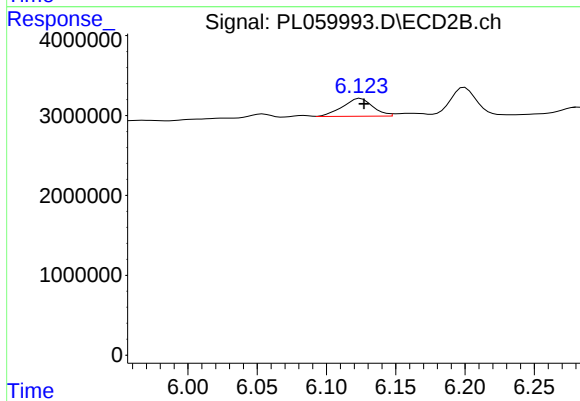

#10 gamma-Chlordane

R.T.: 6.123 min
Delta R.T.: -0.004 min
Response: 3436861
Conc: 1.20 ng/ml m

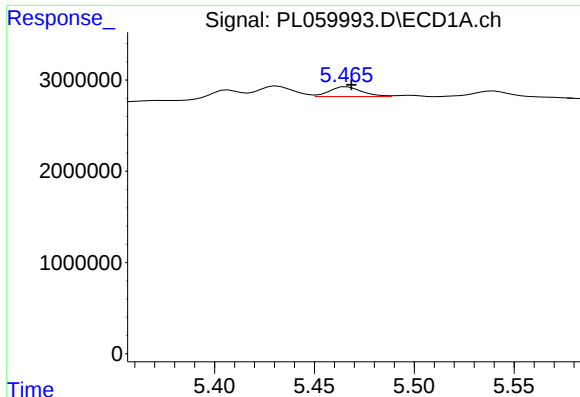


#11 alpha-Chlordane

R.T.: 5.465 min
Delta R.T.: -0.004 min
Response: 1204744
Conc: 0.67 ng/ml m

Instrument :
ECD_L
ClientSampleId :
20


Manual Integrations
APPROVED

Ankita
7/17/2020 11:44:02 AM

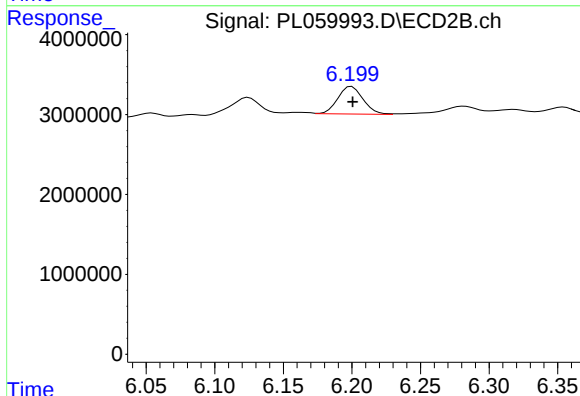


#11 alpha-Chlordane

R.T.: 6.199 min
Delta R.T.: -0.002 min
Response: 4432582
Conc: 1.55 ng/ml m

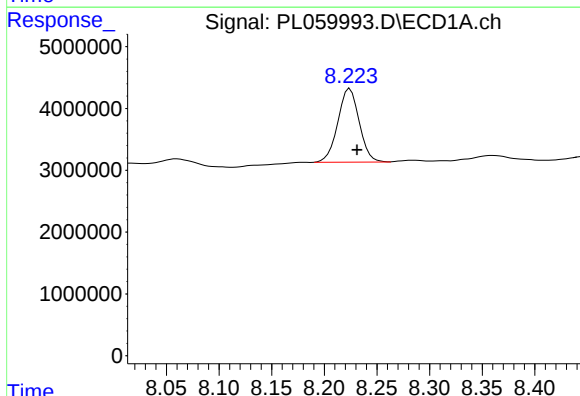

#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 16861191
Conc: 10.25 ng/ml

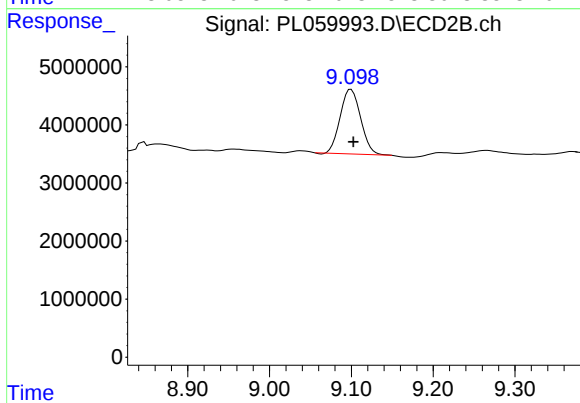

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.003 min
Response: 19202070
Conc: 9.18 ng/ml