

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
 Data File : PL068183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 14:18
 Operator : AR\AJ
 Sample : M3047-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 04:20:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.655	5.585	4071913	10128406	10.101	9.821
28)	SA Decachlor...	10.432	11.508	5695208	10552023	13.801	11.728
Target Compounds							
5)	MB Aldrin	0.000	7.558f	0	746118	N.D.	0.619 #
10)	B gamma-Chl...	0.000	8.315	0	390916	N.D.	0.352 #
11)	B alpha-Chl...	0.000	8.399	0	1164985	N.D.	1.045 #
12)	B 4,4'-DDE	7.661	8.580	369221	629224	0.854	0.620 #
16)	A 4,4'-DDD	0.000	9.122	0	864958	N.D.	1.009 #
17)	MA 4,4'-DDT	8.508	9.440	513259	802674	1.269	0.851 #
24)	Chlordane-2	0.000	7.558	0	746118	N.D.	16.278 #
25)	Chlordane-3	0.000	8.315	0	390916	N.D.	2.422 #
26)	Chlordane-4	0.000	8.399	0	1164985	N.D.	5.904 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
Data File : PL068183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 14:18
Operator : AR\AJ
Sample : M3047-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 04:20:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

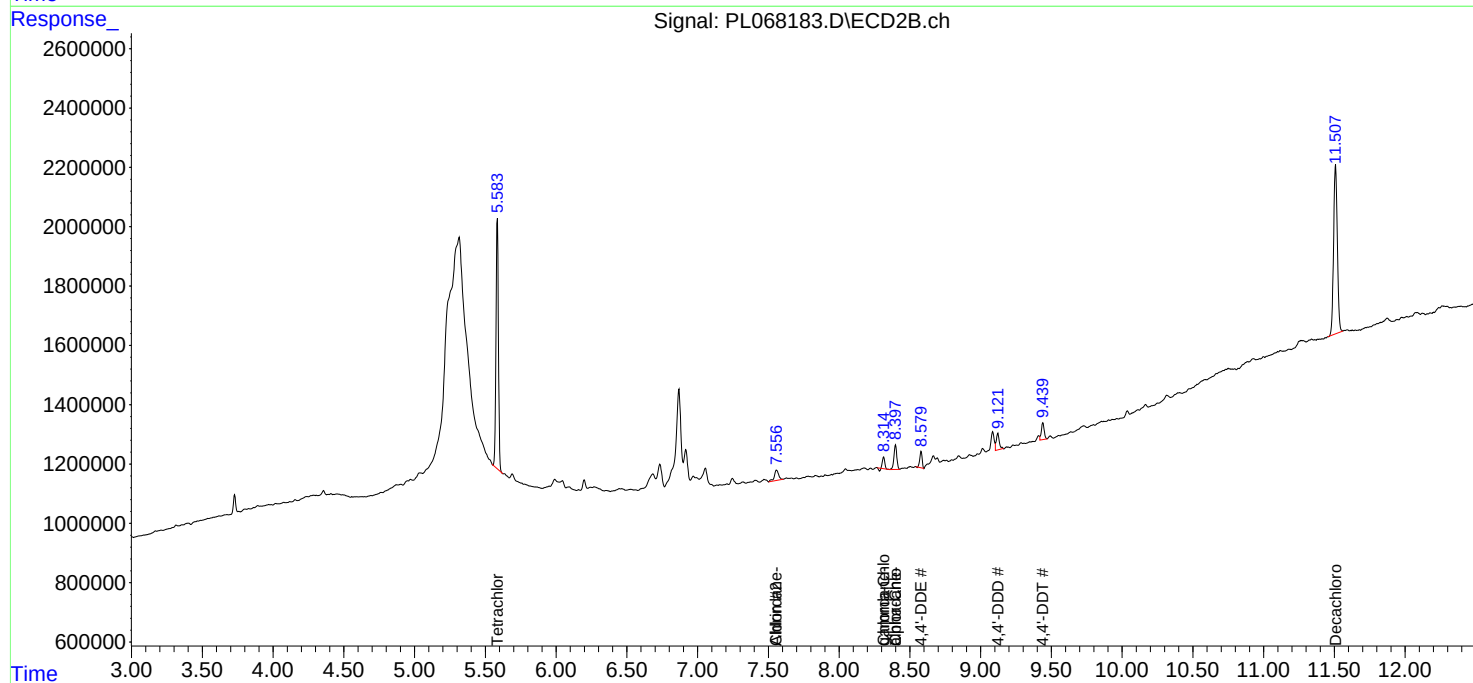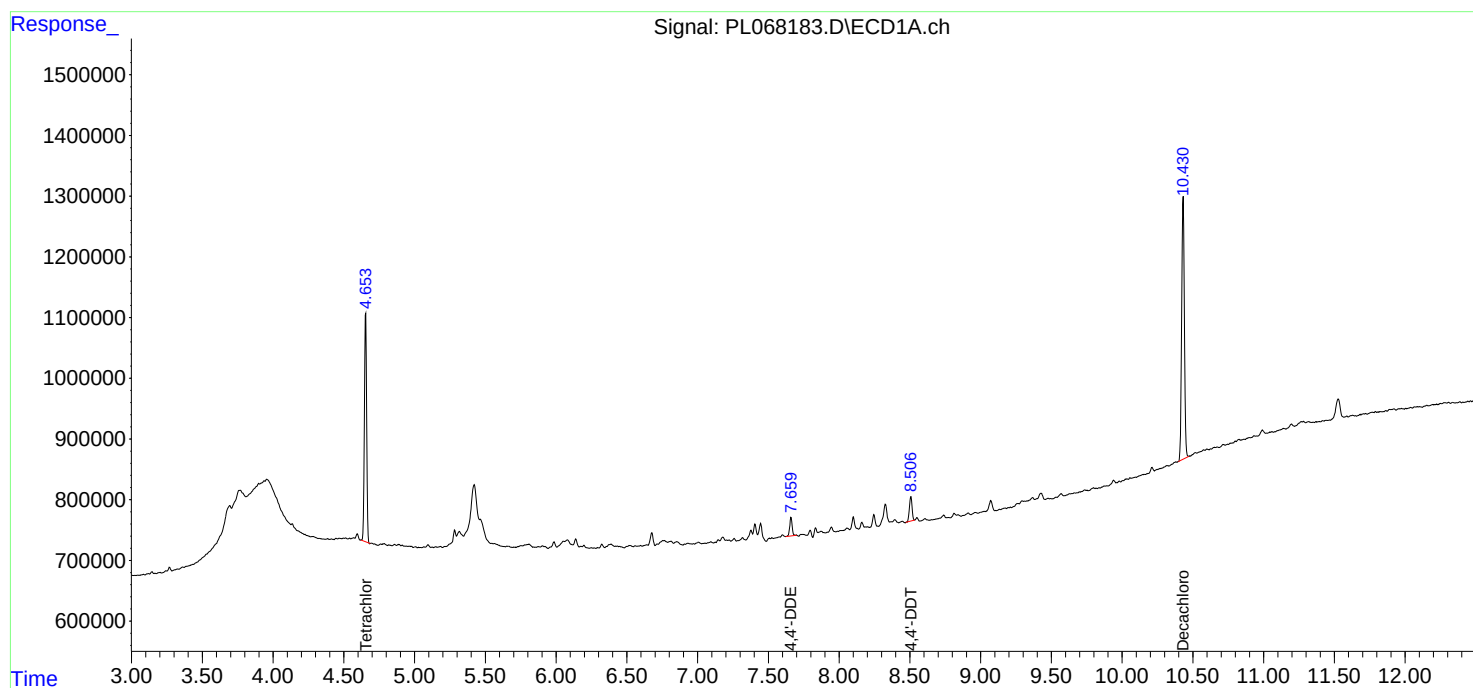


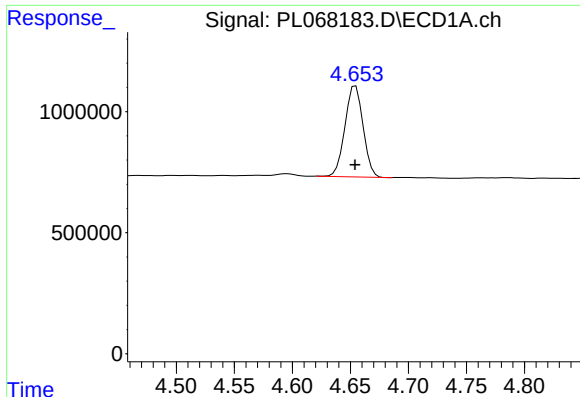

#1 Tetrachloro-m-xylene


R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 4071913
Conc: 10.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

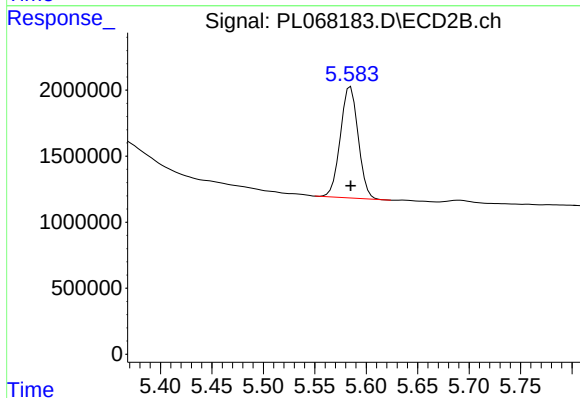


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 10128406
Conc: 9.82 ng/ml

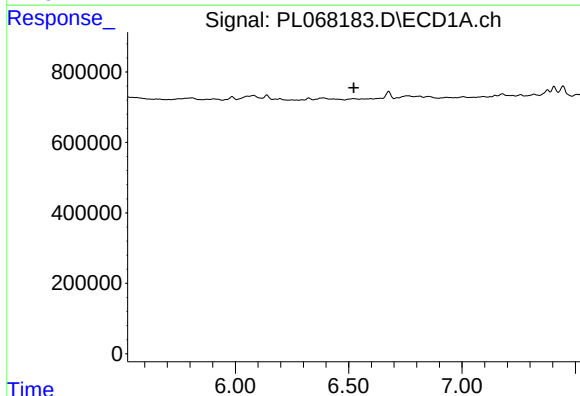


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.523 min
Response: 0
Conc: N.D.

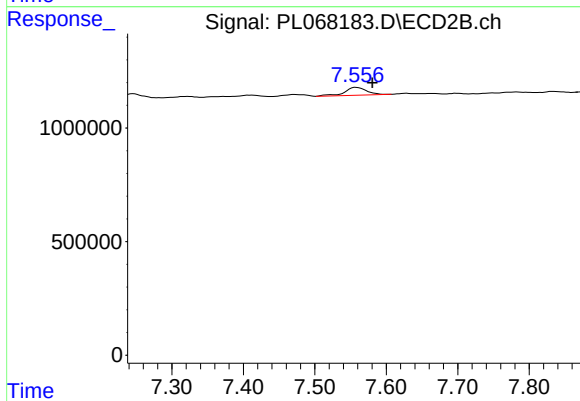

#5 Aldrin


R.T.: 7.558 min
Delta R.T.: -0.023 min
Response: 746118
Conc: 0.62 ng/ml

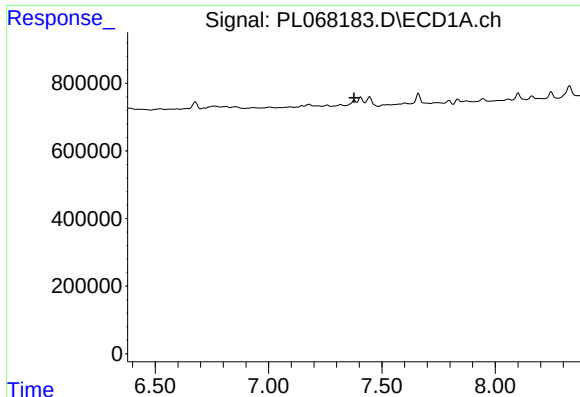

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

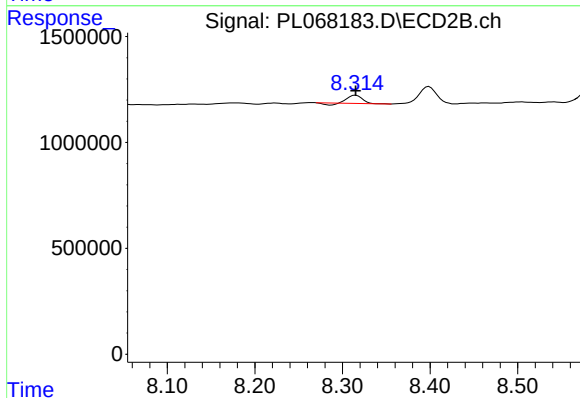


#10 gamma-Chlordane

R.T.: 8.315 min
Delta R.T.: 0.000 min
Response: 390916
Conc: 0.35 ng/ml

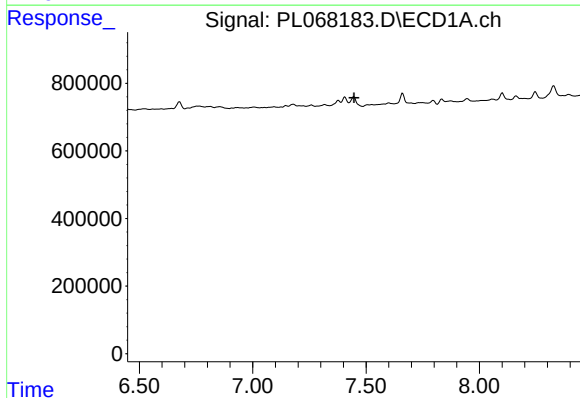


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.448 min
Response: 0
Conc: N.D.

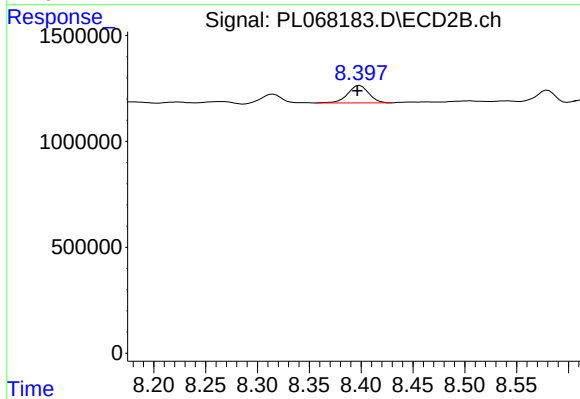

#11 alpha-Chlordane


R.T.: 8.399 min
Delta R.T.: 0.002 min
Response: 1164985
Conc: 1.05 ng/ml

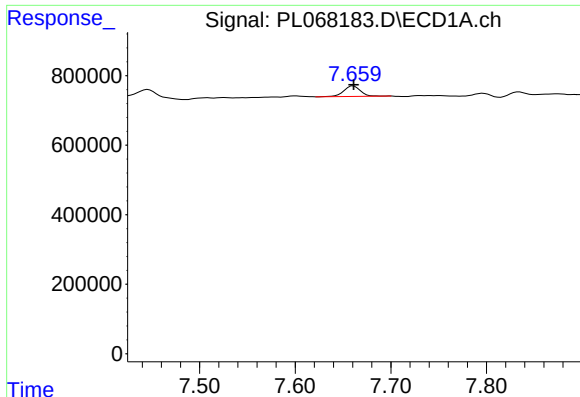

#12 4,4'-DDE


R.T.: 7.661 min
Delta R.T.: 0.000 min
Response: 369221
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

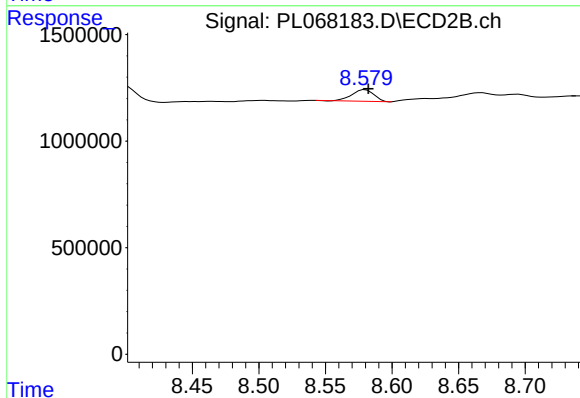


#12 4,4'-DDE

R.T.: 8.580 min
Delta R.T.: -0.002 min
Response: 629224
Conc: 0.62 ng/ml

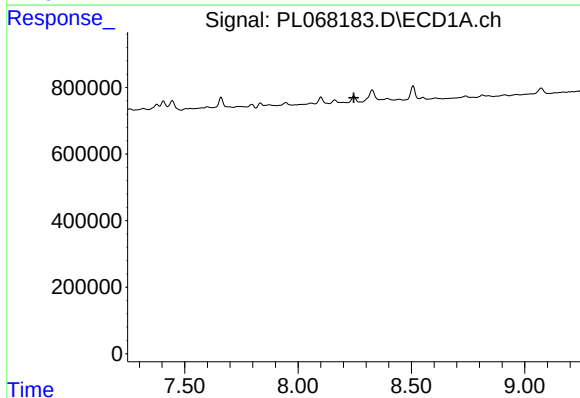


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.246 min
Response: 0
Conc: N.D.

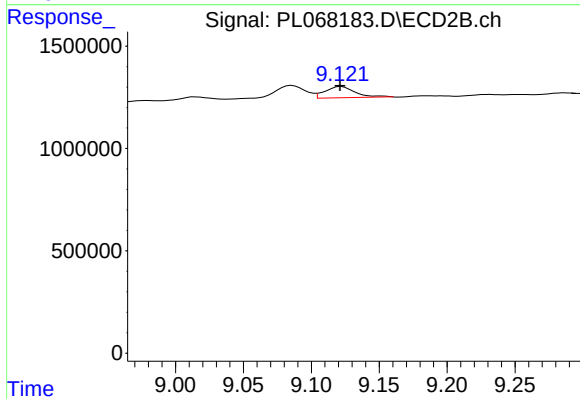

#16 4,4'-DDD


R.T.: 9.122 min
Delta R.T.: 0.001 min
Response: 864958
Conc: 1.01 ng/ml

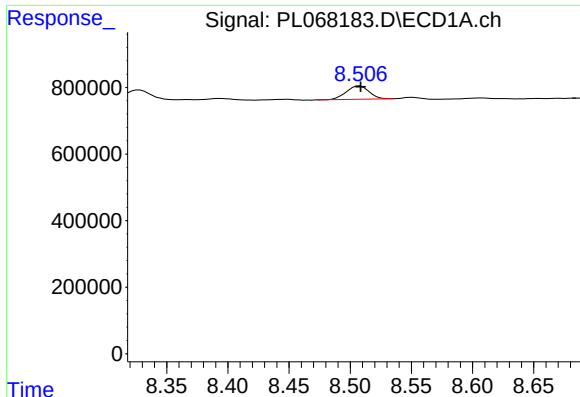

#17 4,4'-DDT


R.T.: 8.508 min
Delta R.T.: 0.000 min
Response: 513259
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

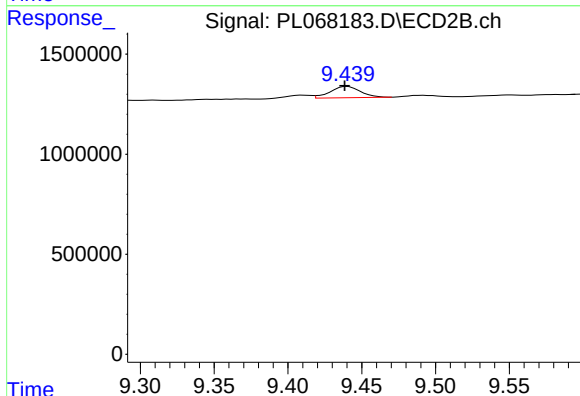


#17 4,4'-DDT

R.T.: 9.440 min
Delta R.T.: 0.002 min
Response: 802674
Conc: 0.85 ng/ml

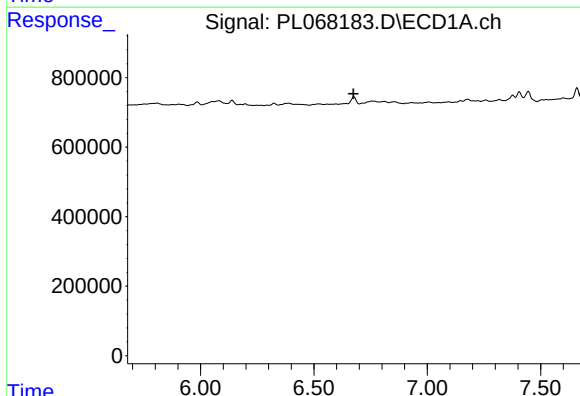


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.675 min
Response: 0
Conc: N.D.

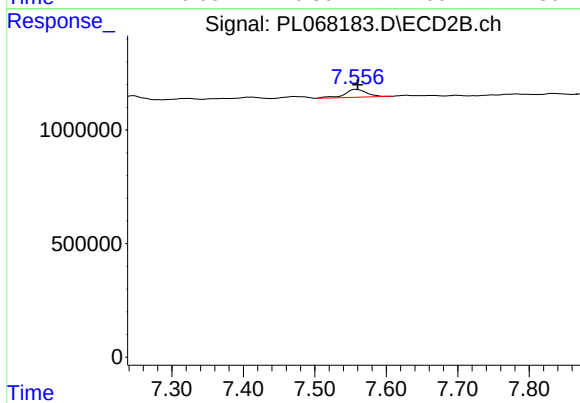

#24 Chlordane-2


R.T.: 7.558 min
Delta R.T.: -0.003 min
Response: 746118
Conc: 16.28 ng/ml

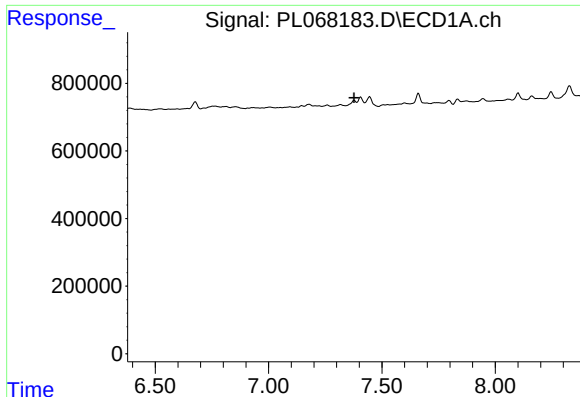

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.378 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

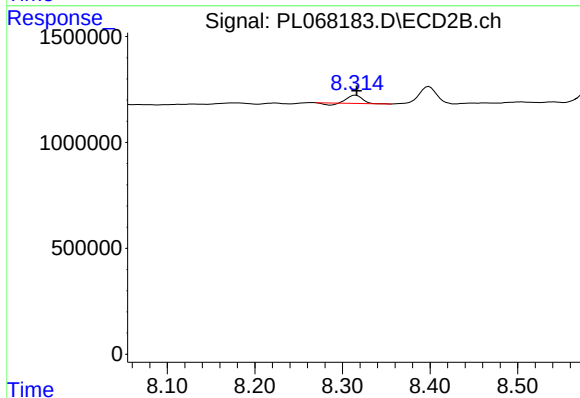


#25 Chlordane-3

R.T.: 8.315 min
Delta R.T.: 0.000 min
Response: 390916
Conc: 2.42 ng/ml

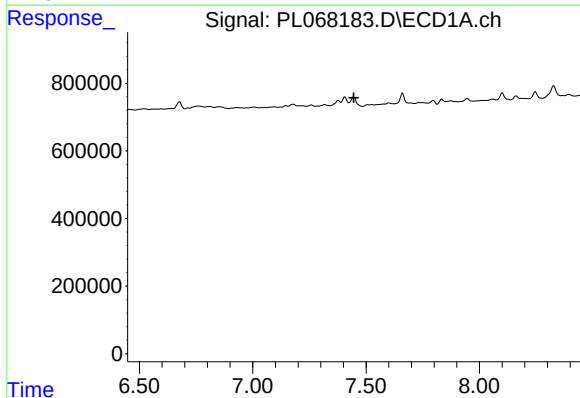


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.446 min
Response: 0
Conc: N.D.

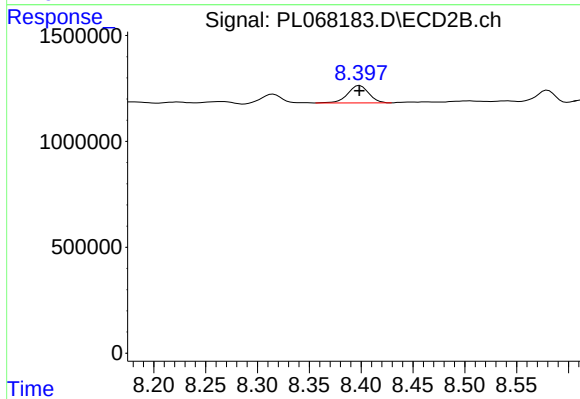

#26 Chlordane-4


R.T.: 8.399 min
Delta R.T.: 0.000 min
Response: 1164985
Conc: 5.90 ng/ml

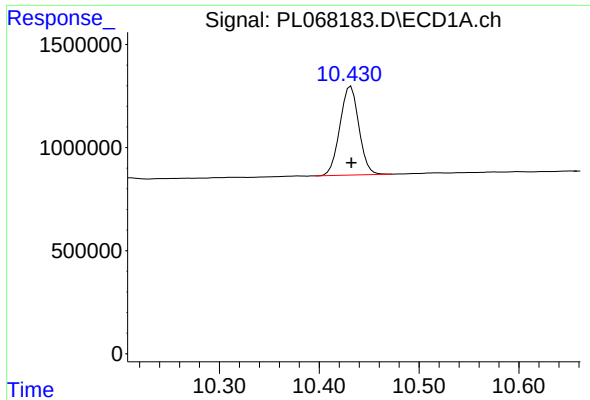

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 5695208
Conc: 13.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

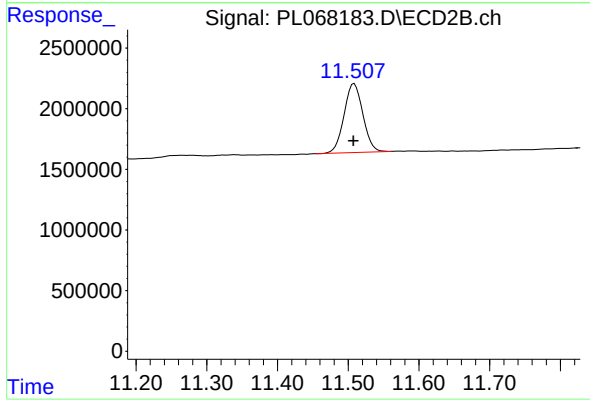

#28 Decachlorobiphenyl

R.T.: 11.508 min
Delta R.T.: 0.001 min
Response: 10552023
Conc: 11.73 ng/ml