

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
 Data File : PL068184.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 14:35
 Operator : AR\AJ
 Sample : M3048-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 04:20:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.655	5.585	7921051	20508782	19.650	19.887
28)	SA Decachlor...	10.431	11.508	8910011	16685643	21.592	18.546
Target Compounds							
10)	B gamma-Chl...	0.000	8.316	0	442839	N.D.	0.398 #
11)	B alpha-Chl...	0.000	8.398	0	715953	N.D.	0.642 #
25)	Chlordane-3	0.000	8.316	0	442839	N.D.	2.743 #
26)	Chlordane-4	0.000	8.398	0	715953	N.D.	3.628 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
Data File : PL068184.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 14:35
Operator : AR\AJ
Sample : M3048-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 04:20:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

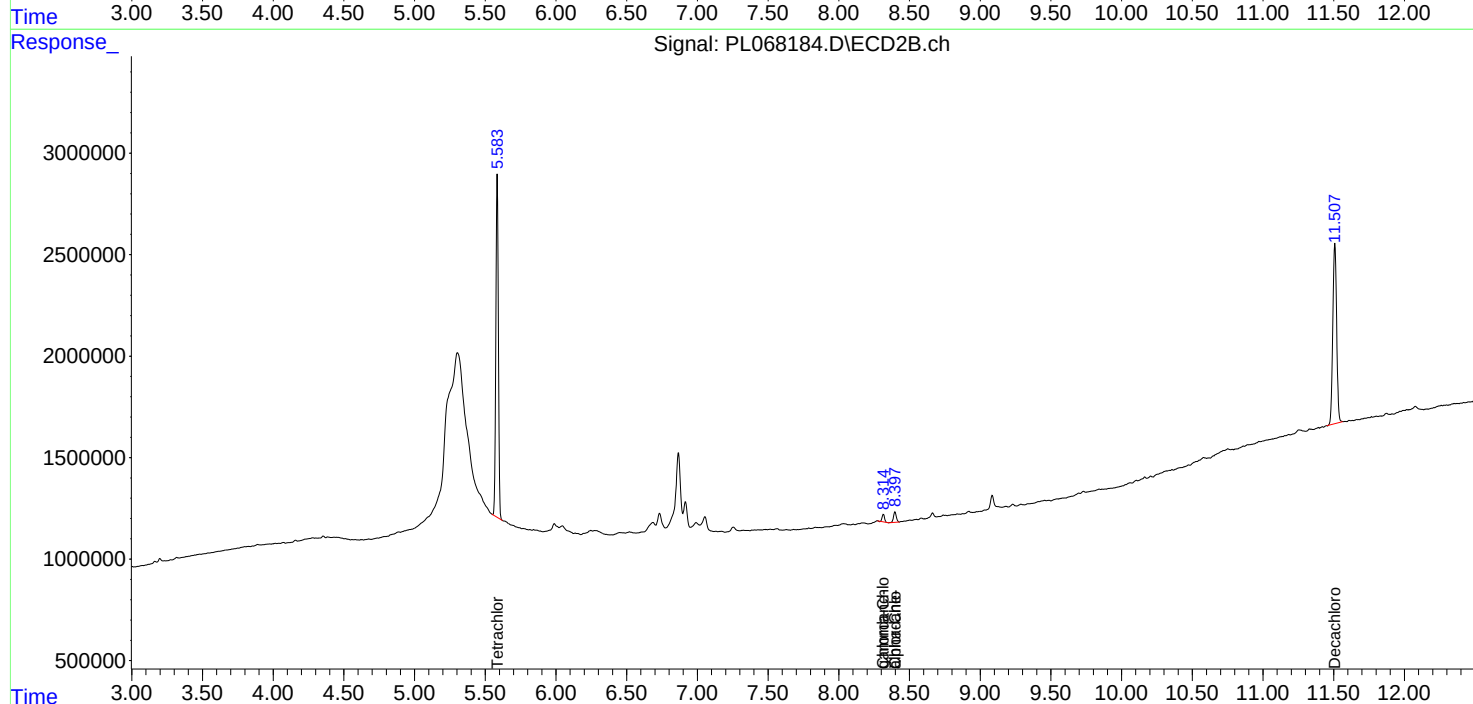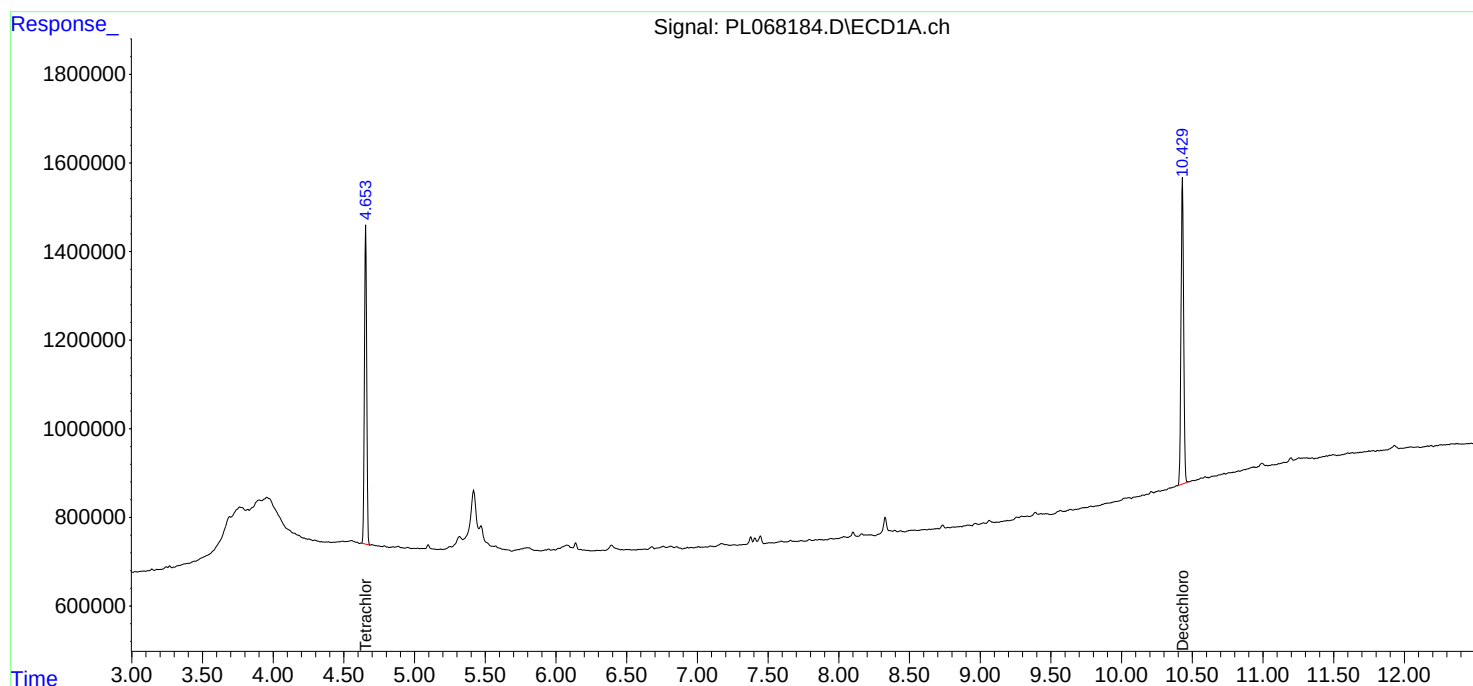


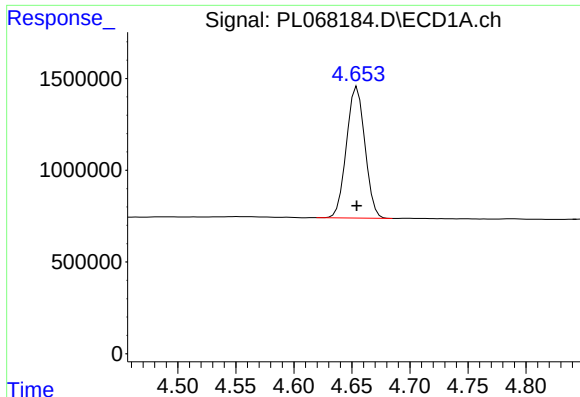

#1 Tetrachloro-m-xylene


R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 7921051
Conc: 19.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

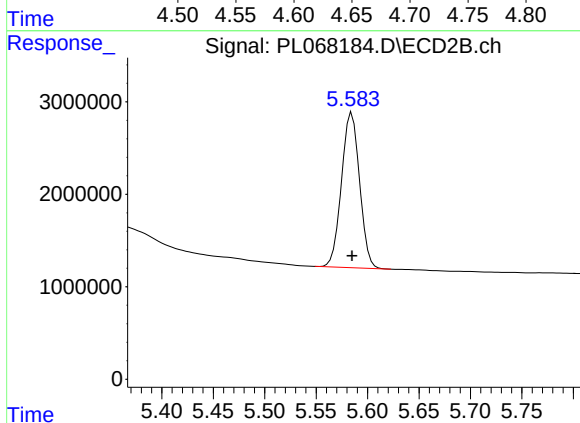


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 20508782
Conc: 19.89 ng/ml

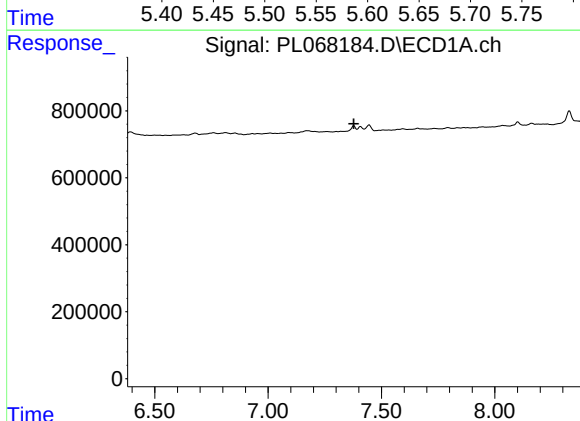


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.377 min
Response: 0
Conc: N.D.

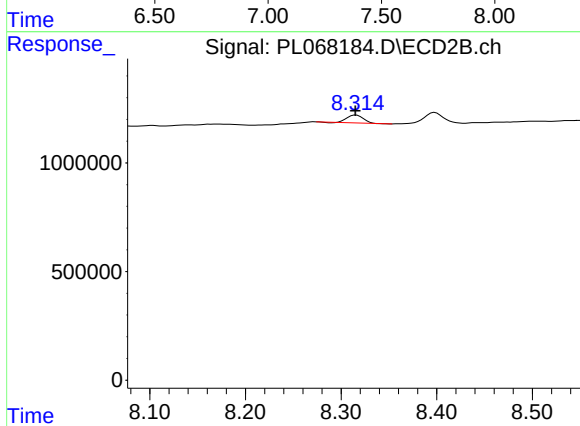

#10 gamma-Chlordane


R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 442839
Conc: 0.40 ng/ml

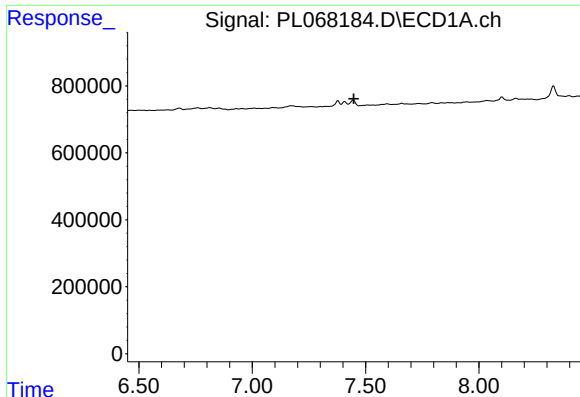

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

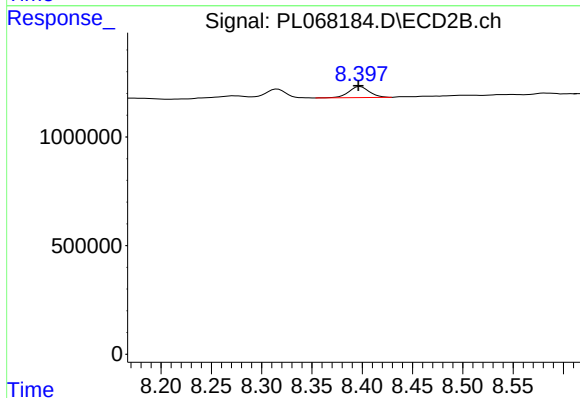


#11 alpha-Chlordane

R.T.: 8.398 min
Delta R.T.: 0.002 min
Response: 715953
Conc: 0.64 ng/ml

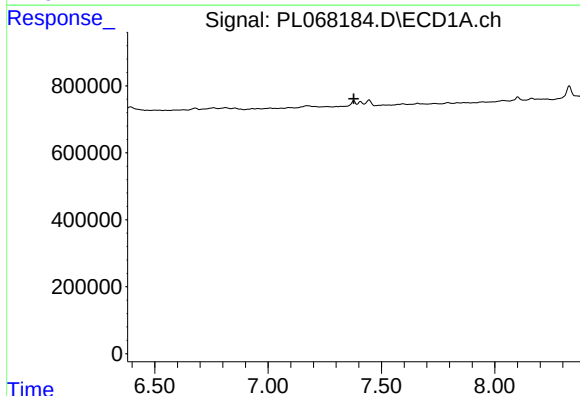


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.378 min
Response: 0
Conc: N.D.

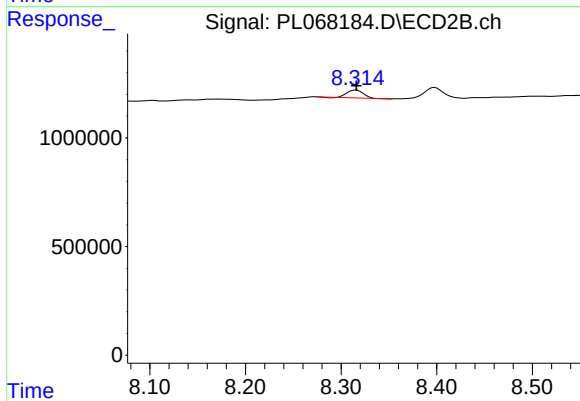

#25 Chlordane-3


R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 442839
Conc: 2.74 ng/ml

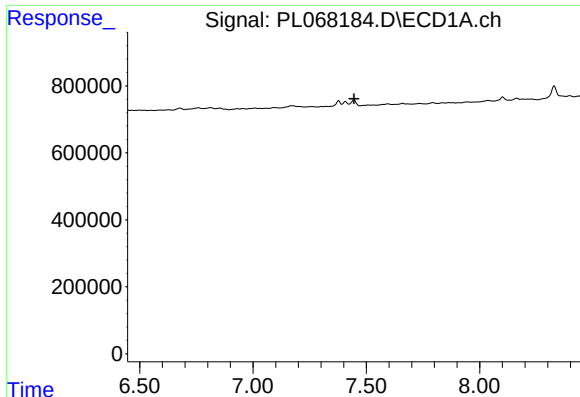

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.446 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

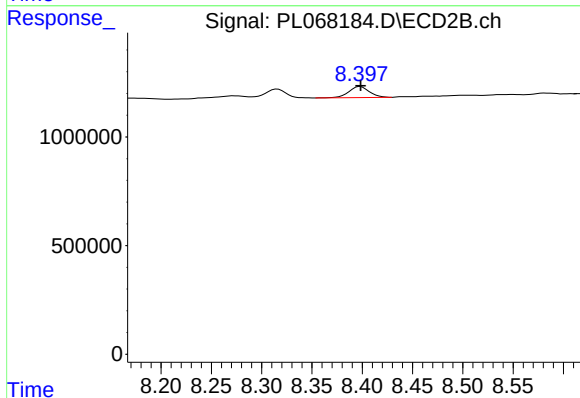


#26 Chlordane-4

R.T.: 8.398 min
Delta R.T.: 0.000 min
Response: 715953
Conc: 3.63 ng/ml

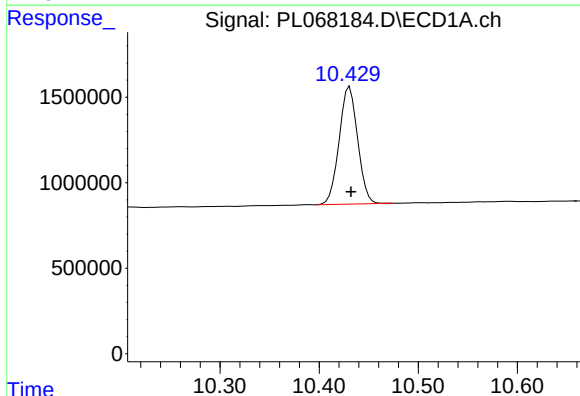

#28 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: -0.001 min
Response: 8910011
Conc: 21.59 ng/ml

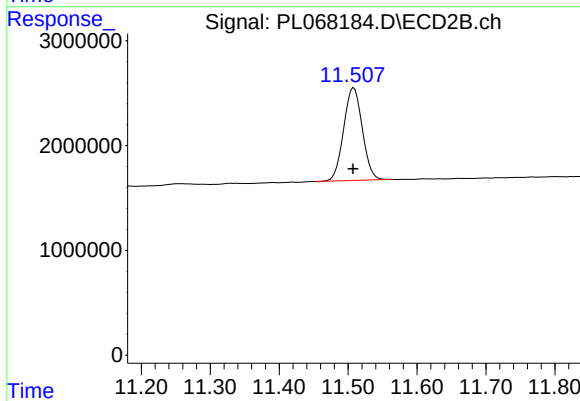

#28 Decachlorobiphenyl

R.T.: 11.508 min
Delta R.T.: 0.001 min
Response: 16685643
Conc: 18.55 ng/ml