

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
 Data File : PL068189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 16:34
 Operator : AR\AJ
 Sample : M3040-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 04:21:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.585	4675162	12059842	11.598	11.694
28)	SA Decachlor...	10.434	11.513	3886387	6934595	9.418	7.708
Target Compounds							
10)	B gamma-Chl...	0.000	8.317	0	726895	N.D.	0.654 #
11)	B alpha-Chl...	7.447	8.400	442575	1473360	0.925	1.322 #
12)	B 4,4'-DDE	0.000	8.583	0	341387	N.D.	0.336 #
16)	A 4,4'-DDD	0.000	9.124	0	278183	N.D.	0.325 #
25)	Chlordane-3	0.000	8.317	0	726895	N.D.	4.503 #
26)	Chlordane-4	7.447	8.400	442575	1473360	8.354	7.467



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
Data File : PL068189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 16:34
Operator : AR\AJ
Sample : M3040-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 04:21:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

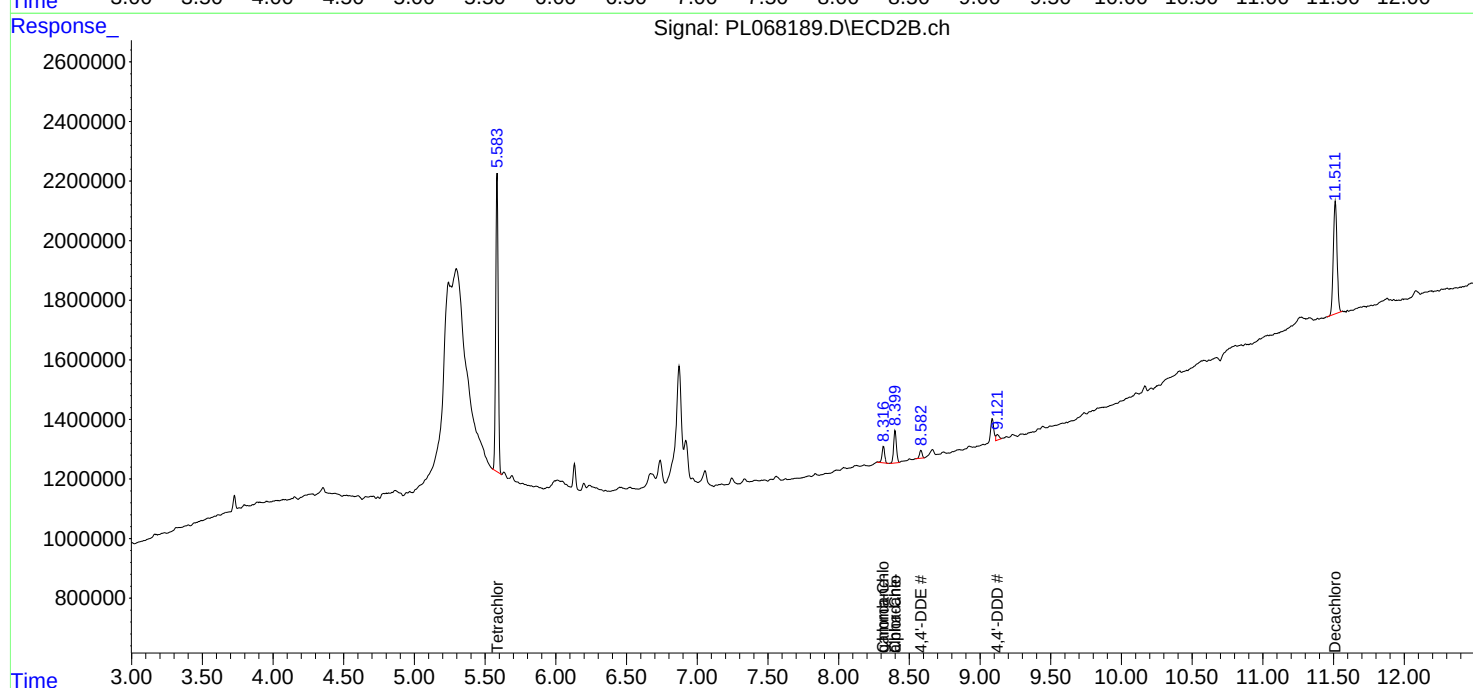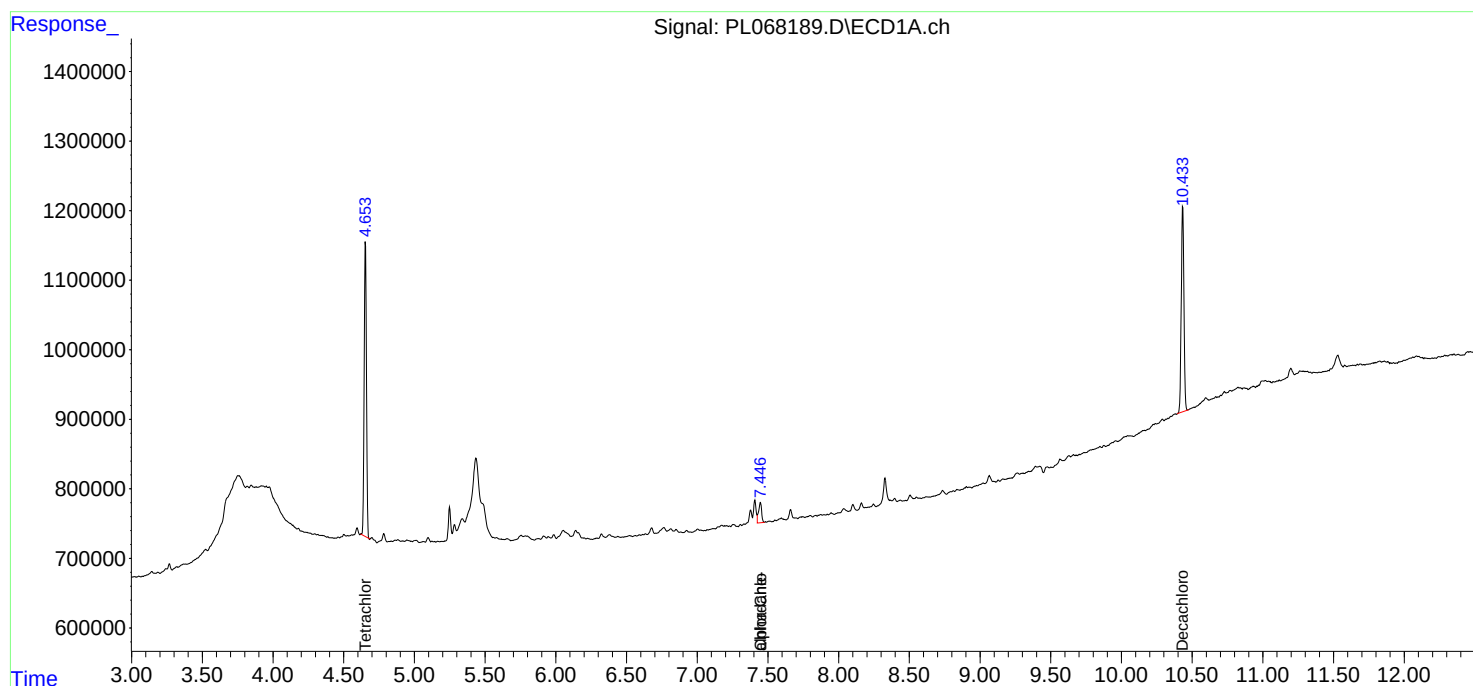


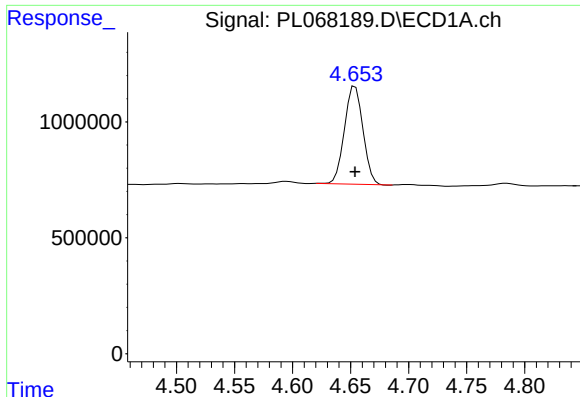

#1 Tetrachloro-m-xylene


R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 4675162
Conc: 11.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

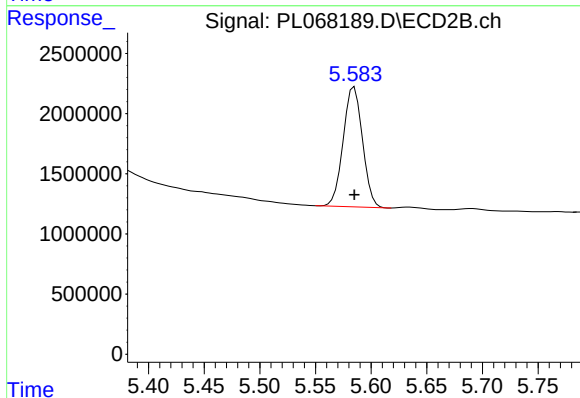


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 12059842
Conc: 11.69 ng/ml

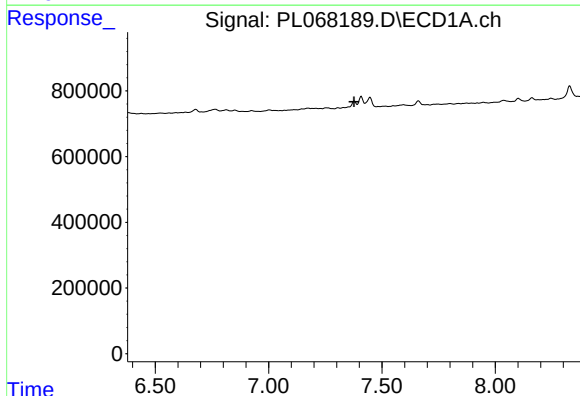


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.377 min
Response: 0
Conc: N.D.

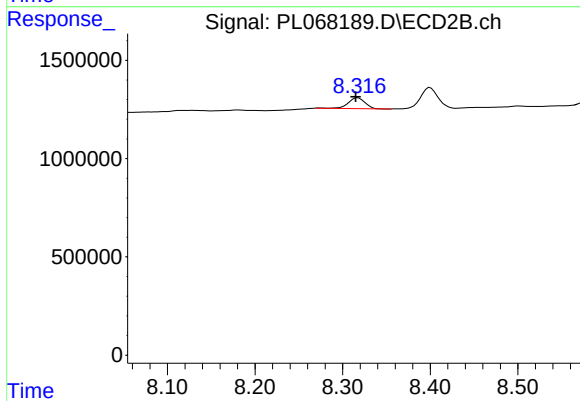

#10 gamma-Chlordane


R.T.: 8.317 min
Delta R.T.: 0.002 min
Response: 726895
Conc: 0.65 ng/ml

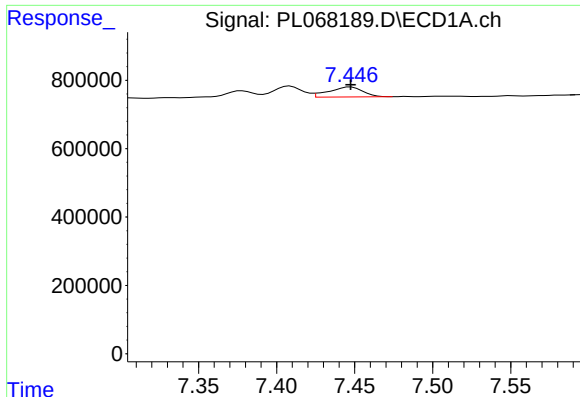

#11 alpha-Chlordane


R.T.: 7.447 min
Delta R.T.: 0.000 min
Response: 442575
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

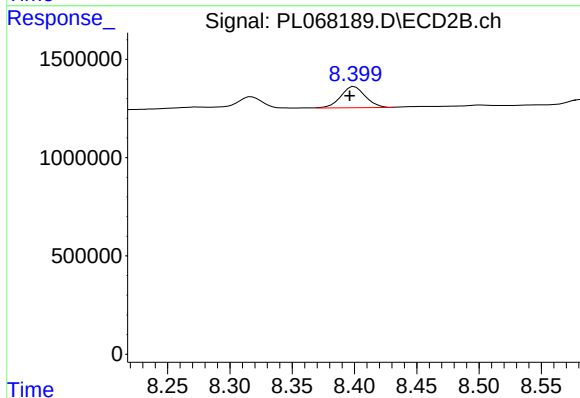


#11 alpha-Chlordane

R.T.: 8.400 min
Delta R.T.: 0.004 min
Response: 1473360
Conc: 1.32 ng/ml

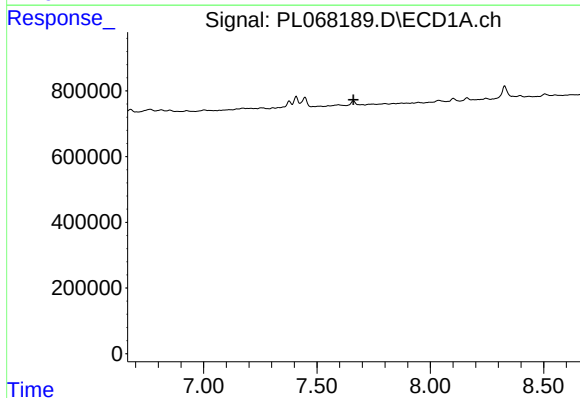


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 7.661 min
Response: 0
Conc: N.D.

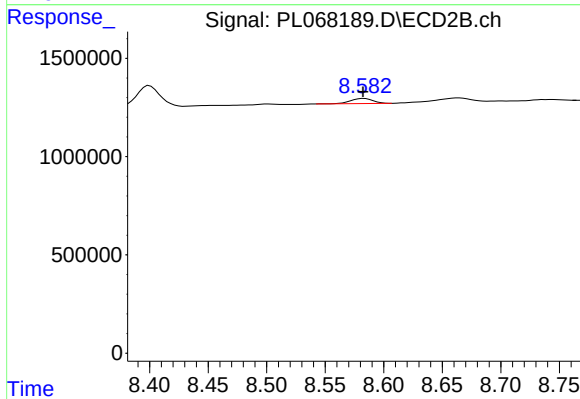

#12 4,4'-DDE


R.T.: 8.583 min
Delta R.T.: 0.000 min
Response: 341387
Conc: 0.34 ng/ml

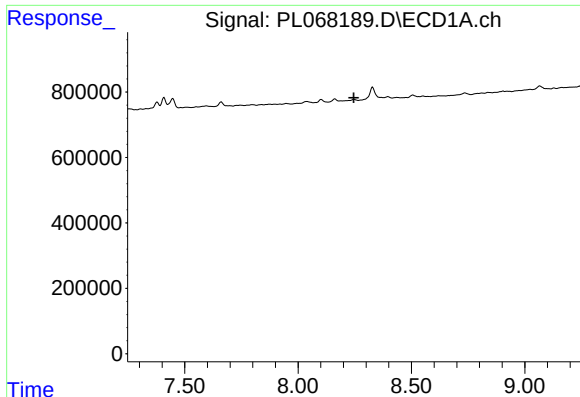

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

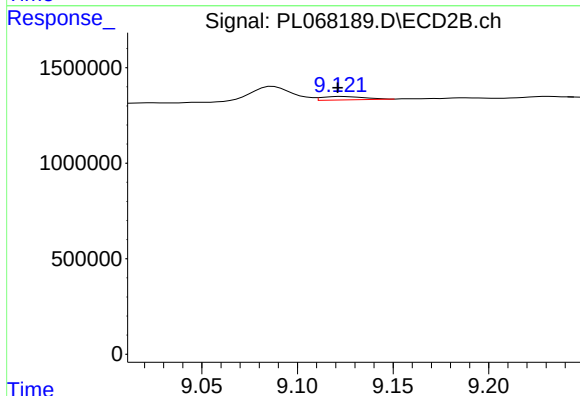


#16 4,4'-DDD

R.T.: 9.124 min
Delta R.T.: 0.002 min
Response: 278183
Conc: 0.32 ng/ml

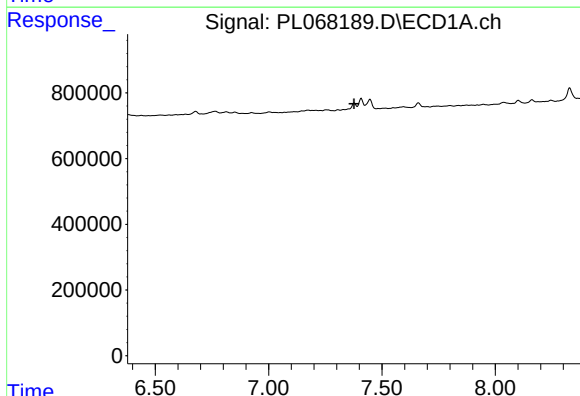


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.378 min
Response: 0
Conc: N.D.

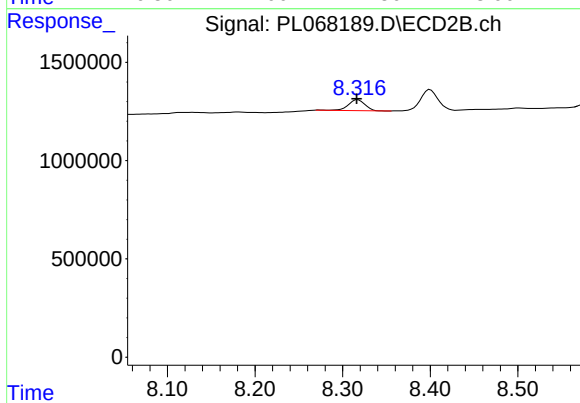

#25 Chlordane-3


R.T.: 8.317 min
Delta R.T.: 0.001 min
Response: 726895
Conc: 4.50 ng/ml

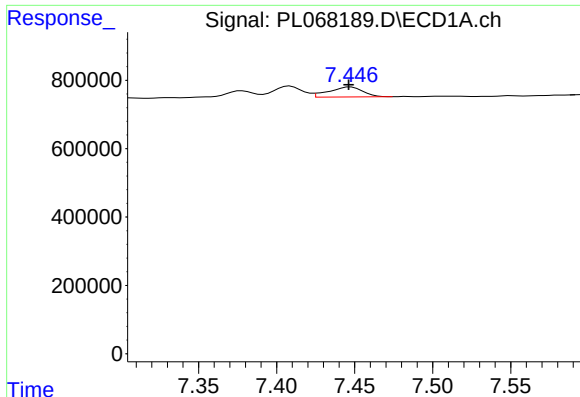

#26 Chlordane-4


R.T.: 7.447 min
Delta R.T.: 0.001 min
Response: 442575
Conc: 8.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

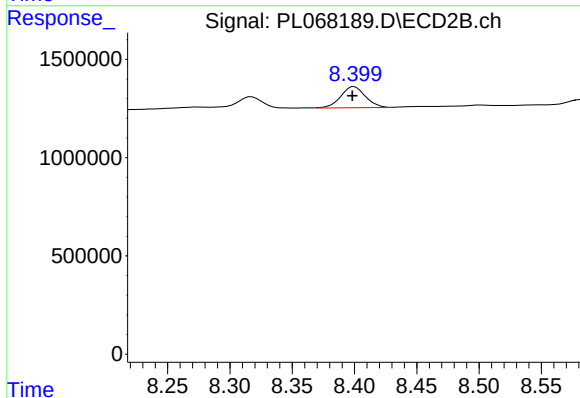


#26 Chlordane-4

R.T.: 8.400 min
Delta R.T.: 0.002 min
Response: 1473360
Conc: 7.47 ng/ml

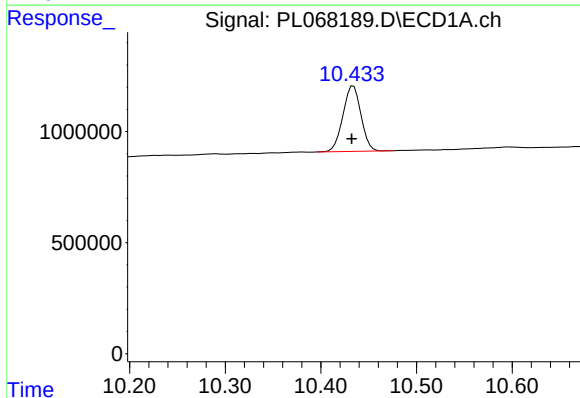

#28 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: 0.002 min
Response: 3886387
Conc: 9.42 ng/ml

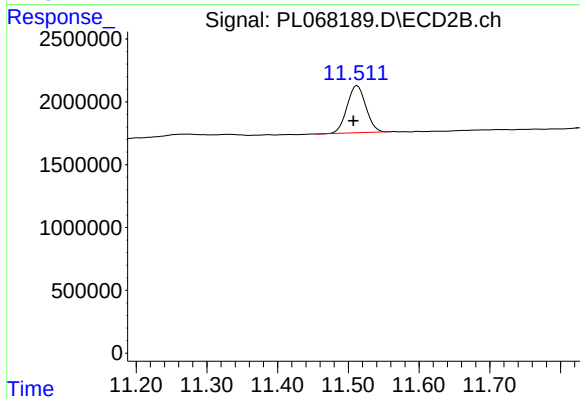

#28 Decachlorobiphenyl

R.T.: 11.513 min
Delta R.T.: 0.006 min
Response: 6934595
Conc: 7.71 ng/ml