

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
 Data File : PL068193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 17:40
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 04:22:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.585	8103367	20659532	20.102	20.033
28)	SA Decachlor...	10.431	11.509	9492861	17479427	23.004	19.428
Target Compounds							
4)	MA Heptachlor	6.173f	0.000	321182	0	0.582	N.D. #
6)	B beta-BHC	6.173	0.000	321182	0	1.235	N.D. #
14)	MA Endrin	8.102f	0.000	636252	0	1.477	N.D. #
15)	B Endosulfa...	0.000	9.231f	0	395779	N.D.	0.447 #
22)	Mirex	0.000	10.580f	0	439454	N.D.	0.577 #
23)	Chlordane-1	0.000	6.990f	0	810950	N.D.	21.068 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
Data File : PL068193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 17:40
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 04:22:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

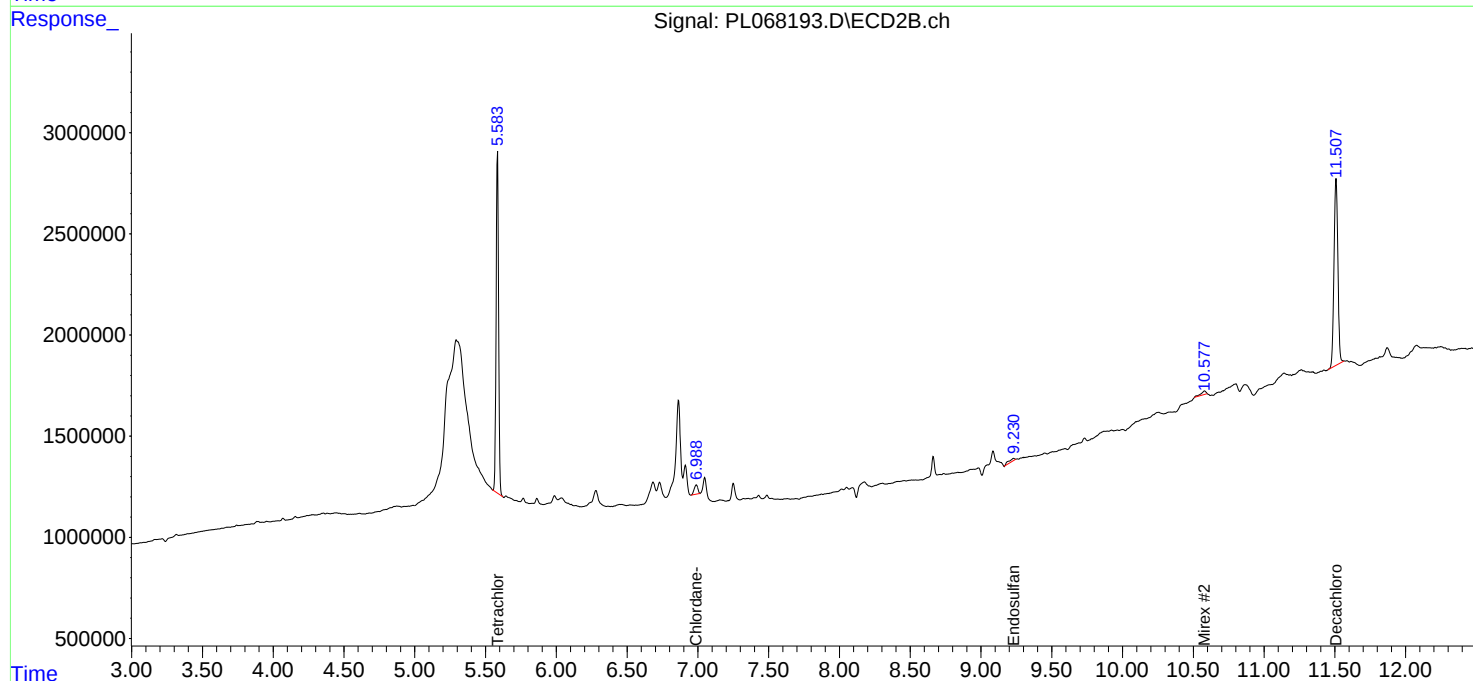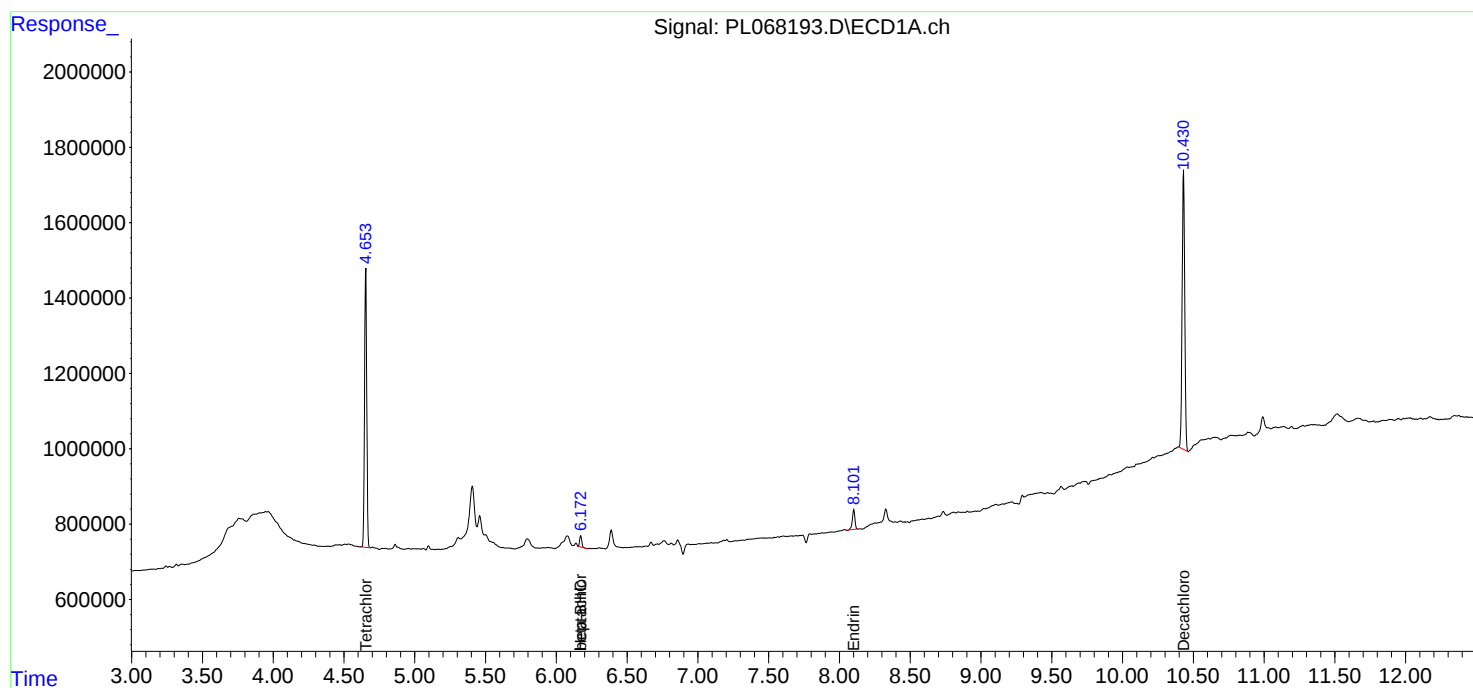


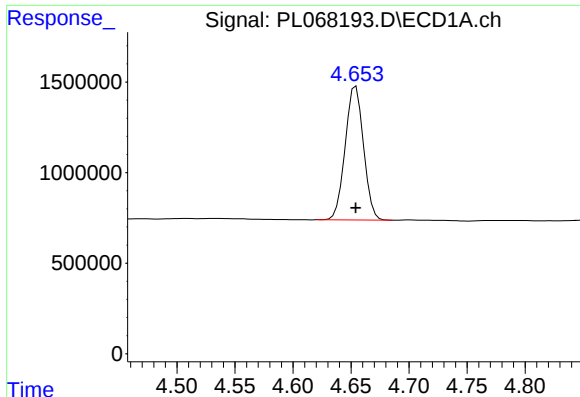

#1 Tetrachloro-m-xylene


R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 8103367
Conc: 20.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

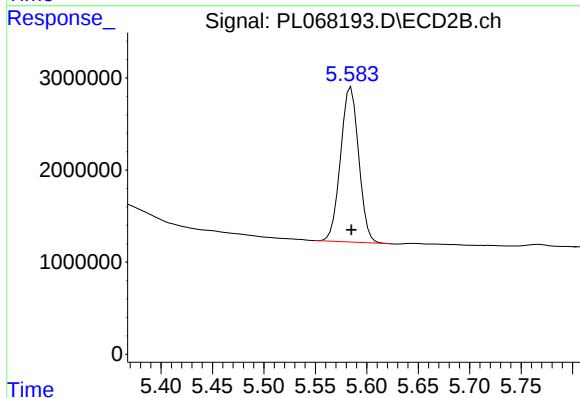


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 20659532
Conc: 20.03 ng/ml

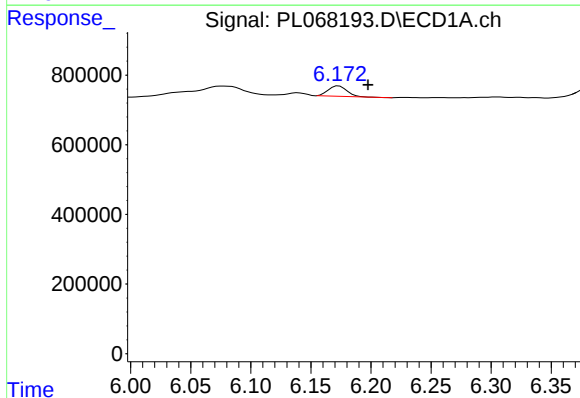


#4 Heptachlor

R.T.: 6.173 min
Delta R.T.: -0.024 min
Response: 321182
Conc: 0.58 ng/ml

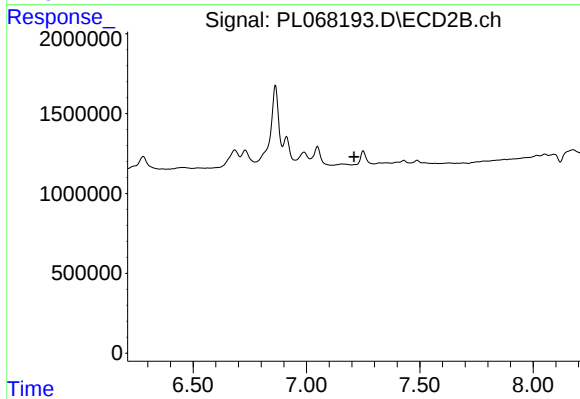

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.210 min
Response: 0
Conc: N.D.

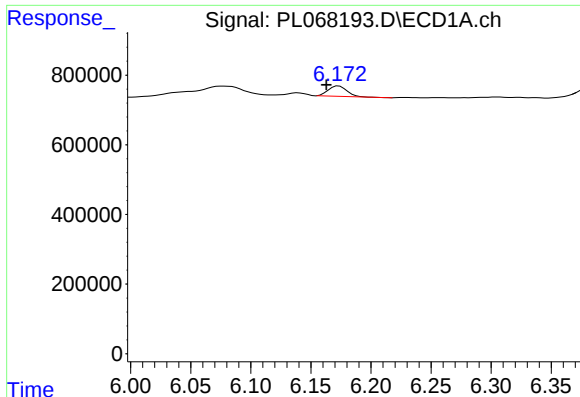

#6 beta-BHC


R.T.: 6.173 min
Delta R.T.: 0.010 min
Response: 321182
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

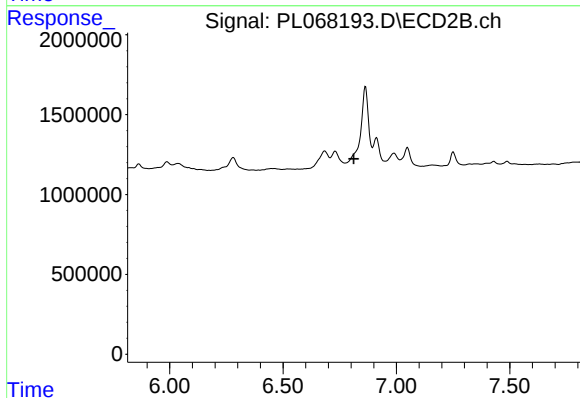


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.812 min
Response: 0
Conc: N.D.

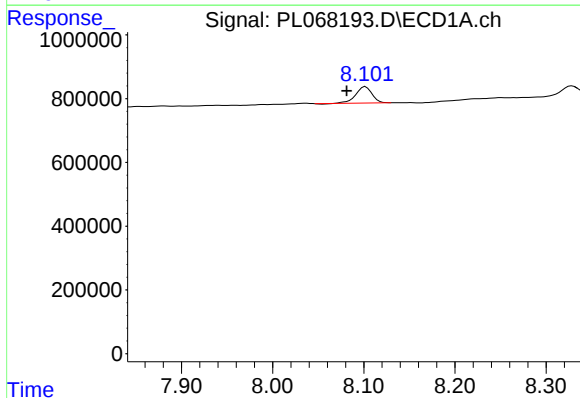


#14 Endrin

R.T.: 8.102 min
Delta R.T.: 0.021 min
Response: 636252
Conc: 1.48 ng/ml

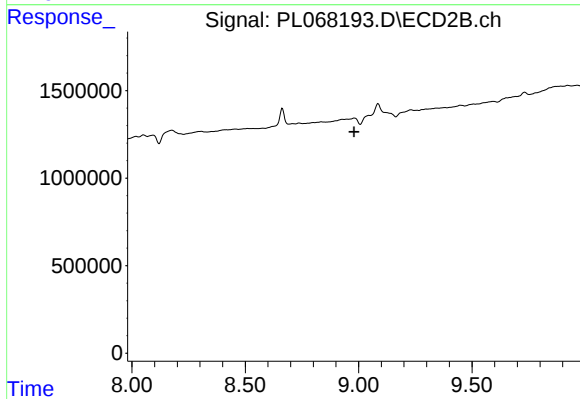

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.981 min
Response: 0
Conc: N.D.

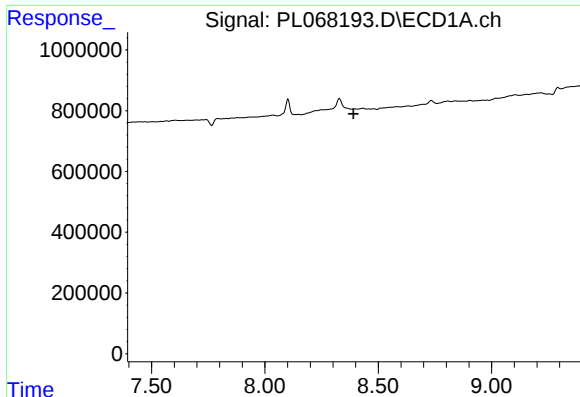

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

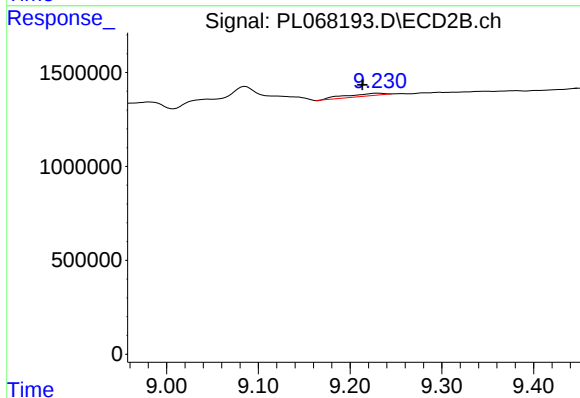


#15 Endosulfan II

R.T.: 9.231 min
Delta R.T.: 0.018 min
Response: 395779
Conc: 0.45 ng/ml

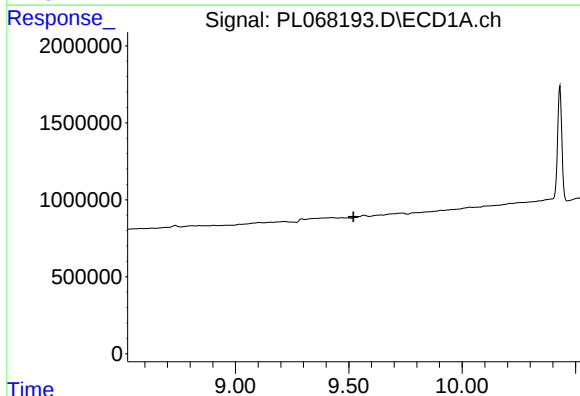


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.521 min
Response: 0
Conc: N.D.

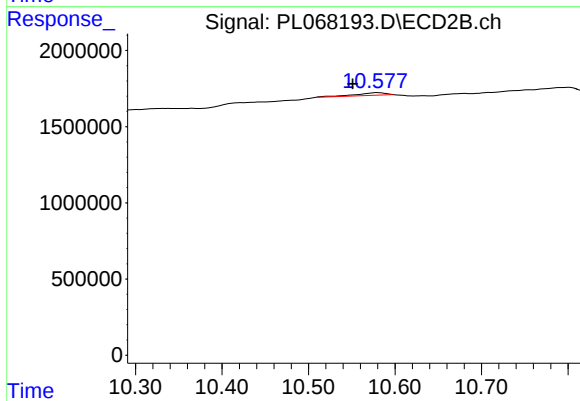

#22 Mirex


R.T.: 10.580 min
Delta R.T.: 0.029 min
Response: 439454
Conc: 0.58 ng/ml

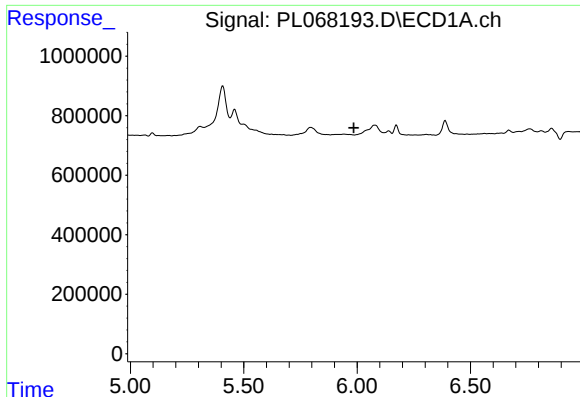

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.986 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

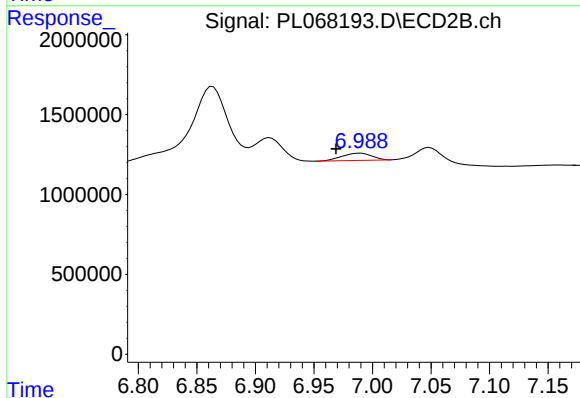


#23 Chlordane-1

R.T.: 6.990 min
Delta R.T.: 0.021 min
Response: 810950
Conc: 21.07 ng/ml

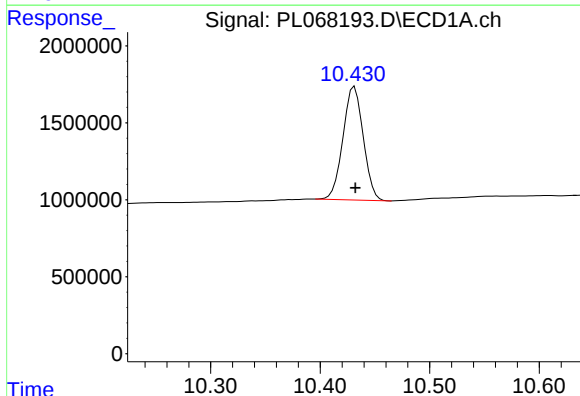

#28 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: 0.000 min
Response: 9492861
Conc: 23.00 ng/ml

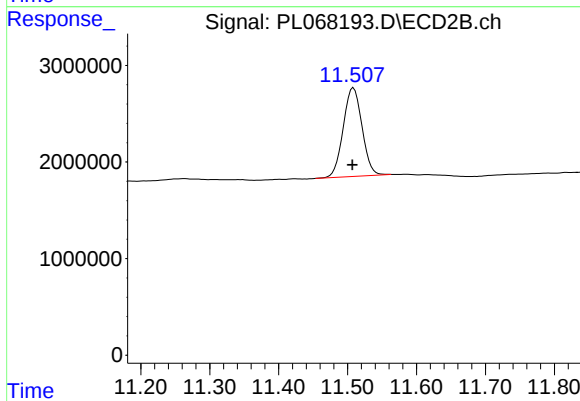

#28 Decachlorobiphenyl

R.T.: 11.509 min
Delta R.T.: 0.001 min
Response: 17479427
Conc: 19.43 ng/ml