

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
 Data File : PL068185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 14:52
 Operator : AR\AJ
 Sample : M3049-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-03-024-ABCD

Manual Integrations
 APPROVED

mohammad
 7/16/2021 9:22:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 04:46:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.653	5.585	8283934	21379795	20.550m	20.731
28) SA Decachlor...	10.431	11.509	8820460	16042656	21.375	17.831

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
Data File : PL068185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 14:52
Operator : AR\AJ
Sample : M3049-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-024-ABCD


Manual Integrations
APPROVED

mohammad
7/16/2021 9:22:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 04:46:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

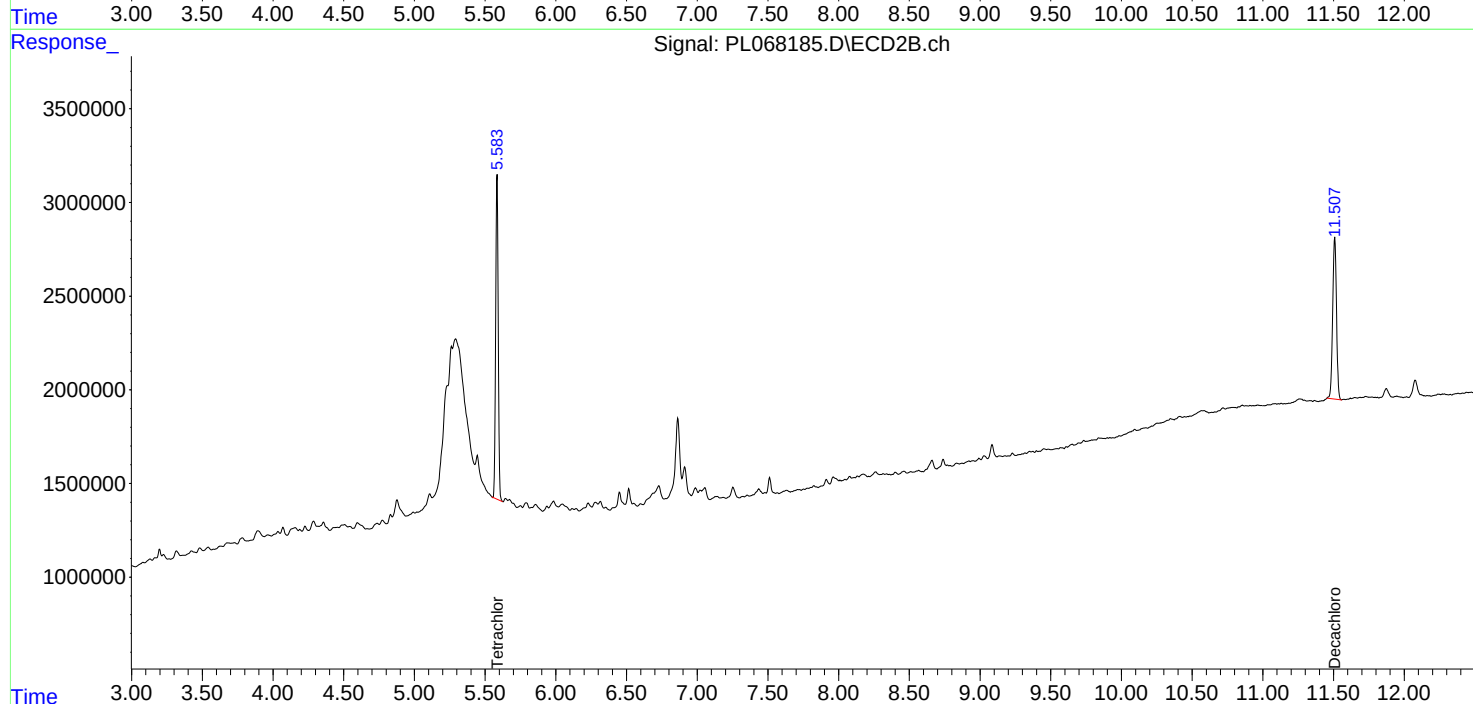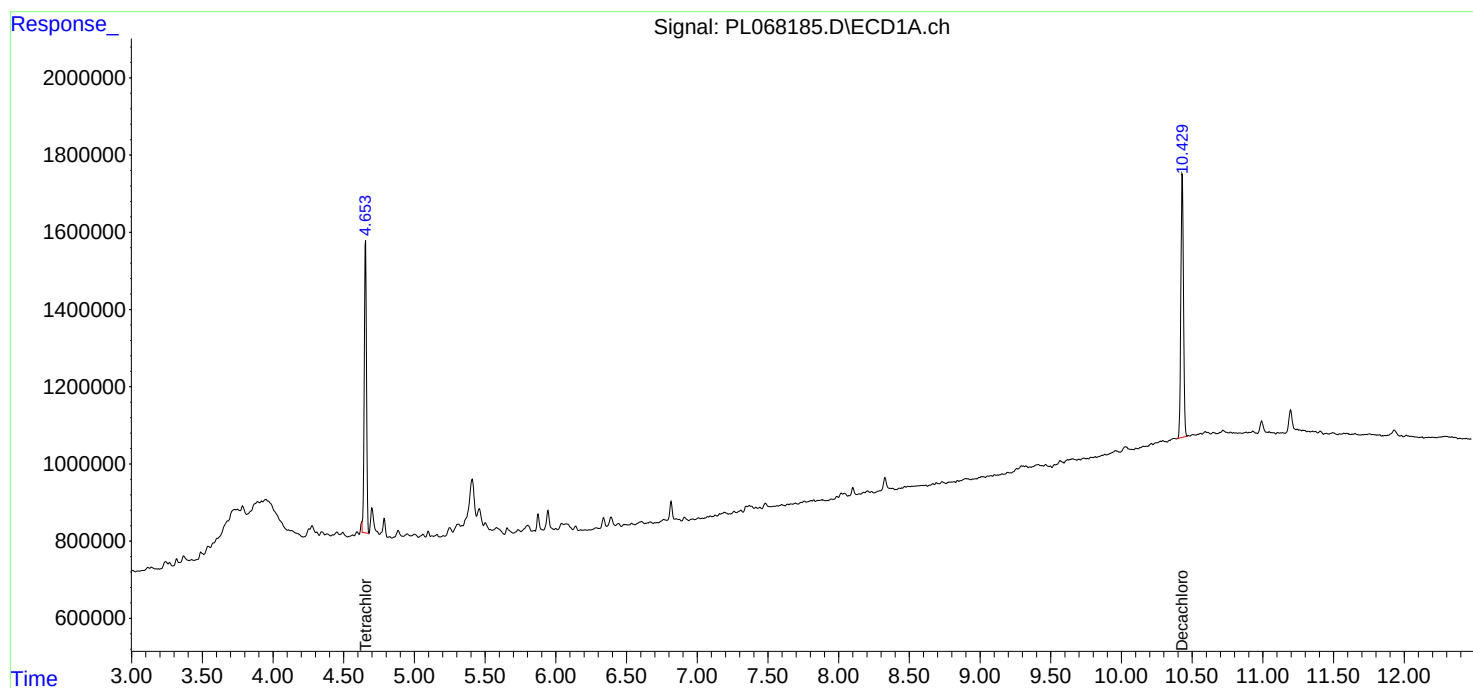

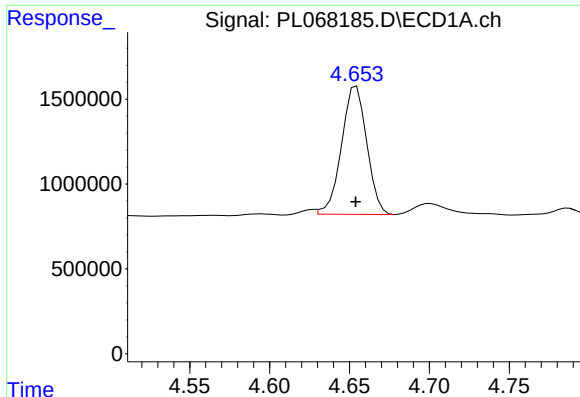


#1 Tetrachloro-m-xylene

R.T.: 4.653 min
Delta R.T.: -0.001 min
Response: 8283934
Conc: 20.55 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-024-ABCD


Manual Integrations
APPROVED

mohammad
7/16/2021 9:22:43 AM

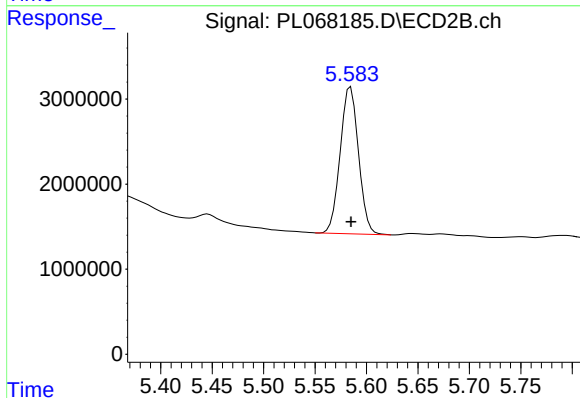


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 21379795
Conc: 20.73 ng/ml

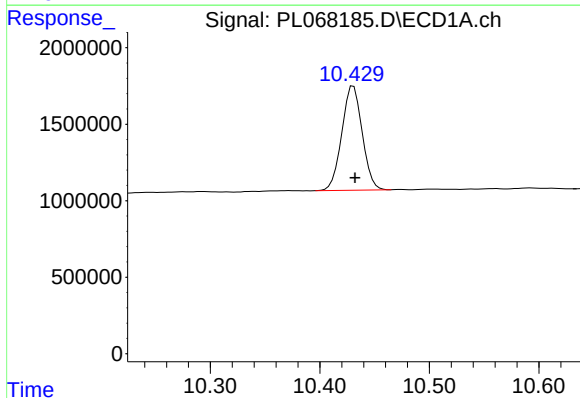

#28 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: -0.001 min
Response: 8820460
Conc: 21.37 ng/ml

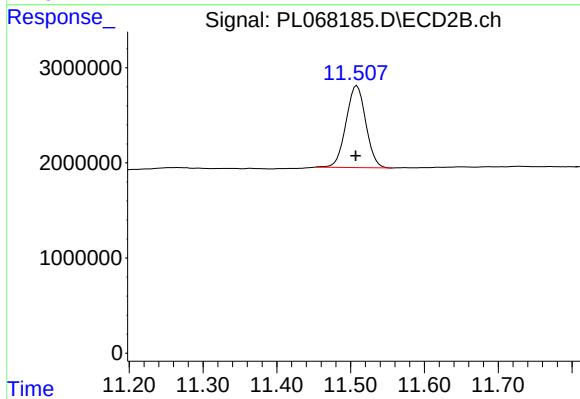

#28 Decachlorobiphenyl

R.T.: 11.509 min
Delta R.T.: 0.002 min
Response: 16042656
Conc: 17.83 ng/ml