

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
 Data File : PL068188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 16:17
 Operator : AR\AJ
 Sample : M3050-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-04-018-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 04:21:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.584	8237419	21473777	20.434	20.822
28)	SA Decachlor...	10.430	11.508	9675052	17051260	23.446	18.952

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071621\
Data File : PL068188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 16:17
Operator : AR\AJ
Sample : M3050-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-018-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 04:21:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

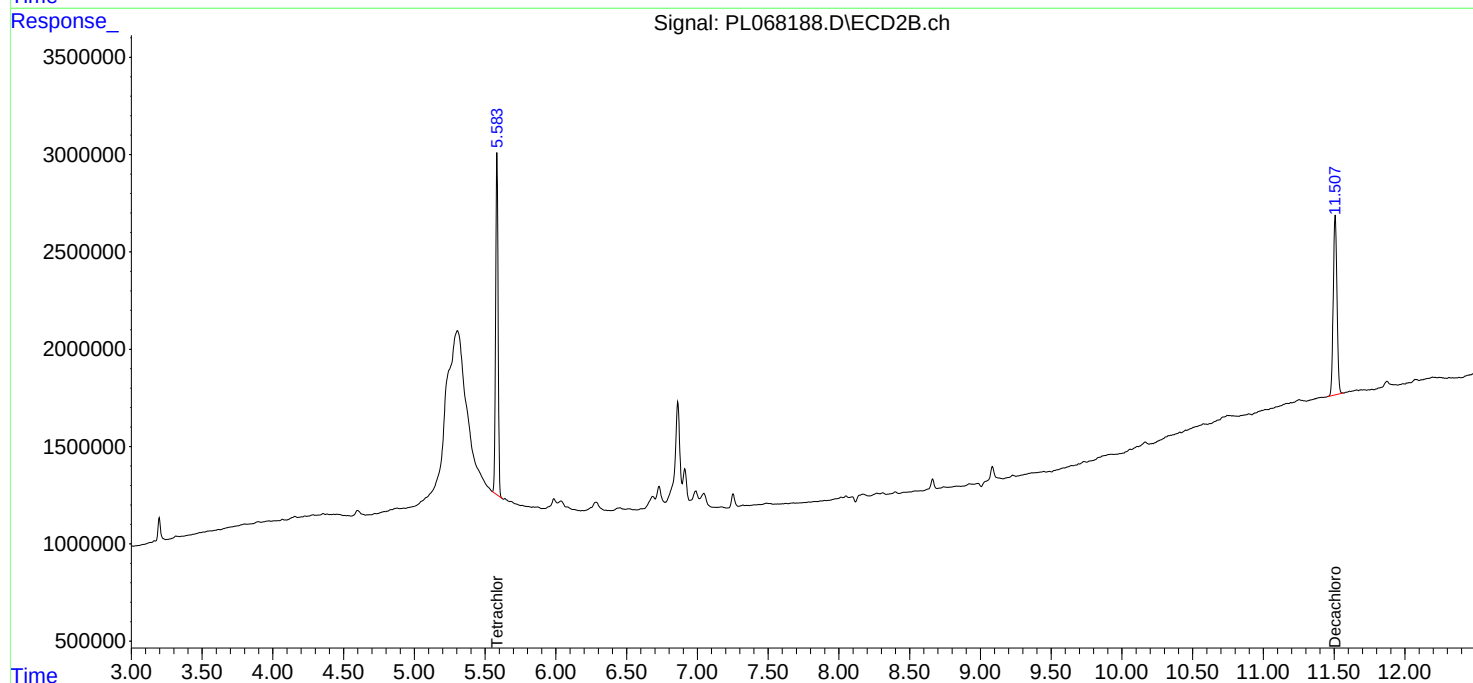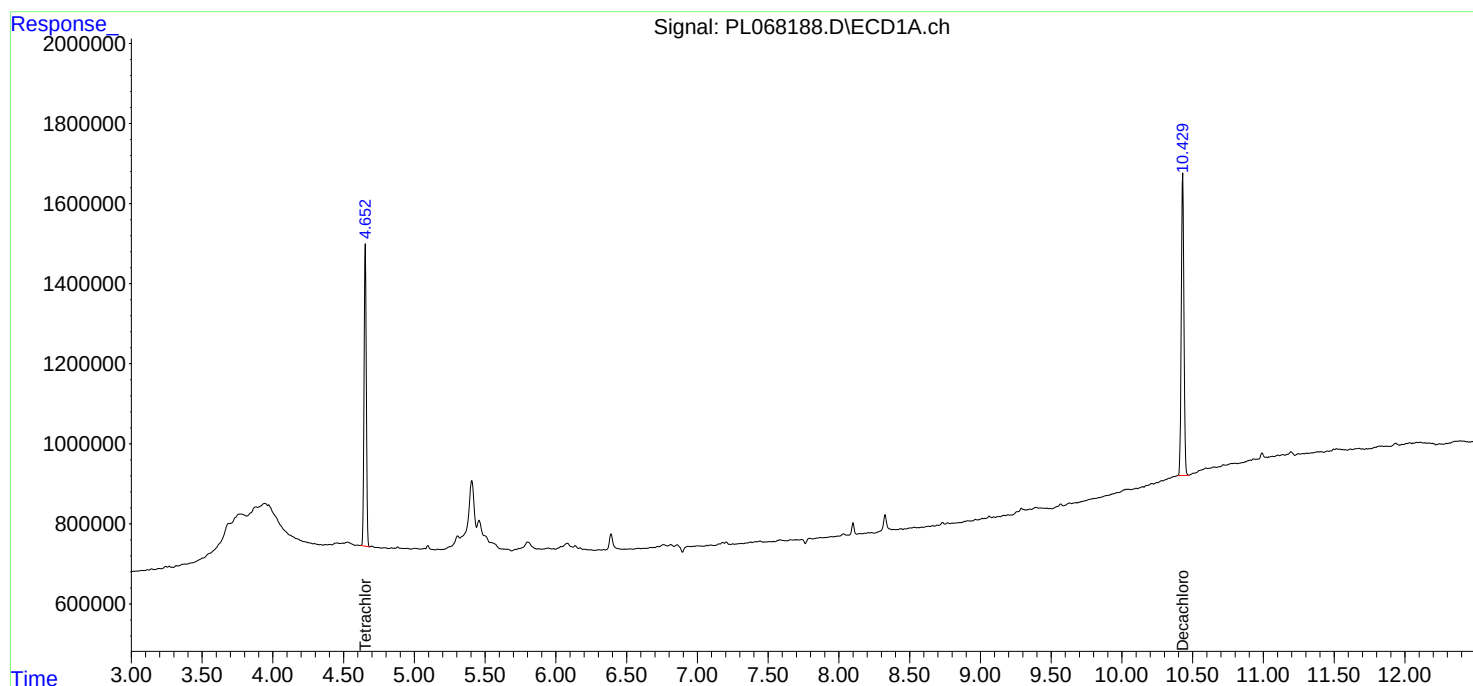


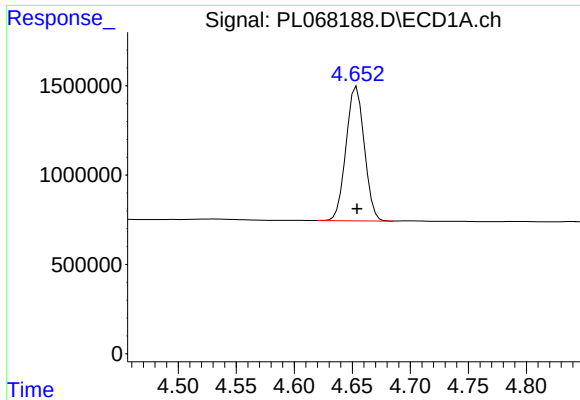

#1 Tetrachloro-m-xylene


R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 8237419
Conc: 20.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-04-018-ABCD

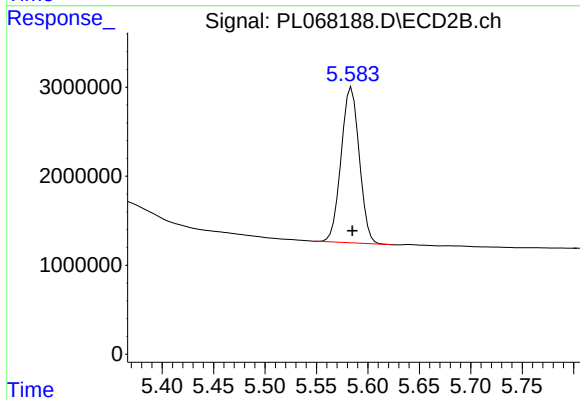


#1 Tetrachloro-m-xylene

R.T.: 5.584 min
Delta R.T.: 0.000 min
Response: 21473777
Conc: 20.82 ng/ml

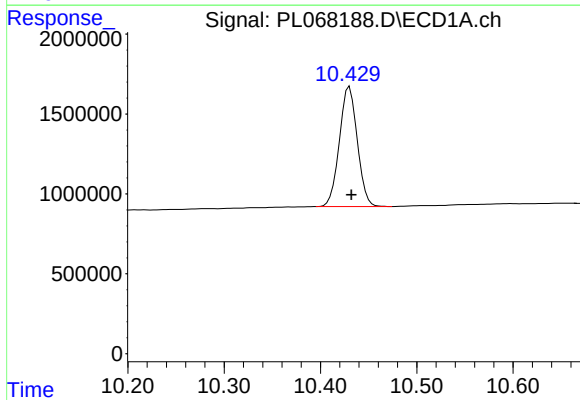

#28 Decachlorobiphenyl

R.T.: 10.430 min
Delta R.T.: -0.002 min
Response: 9675052
Conc: 23.45 ng/ml

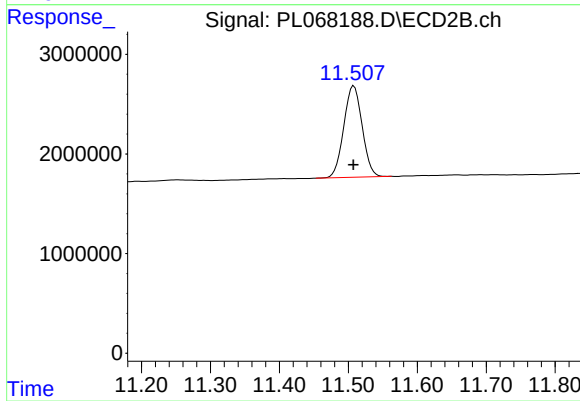

#28 Decachlorobiphenyl

R.T.: 11.508 min
Delta R.T.: 0.000 min
Response: 17051260
Conc: 18.95 ng/ml