

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071623\
 Data File : PL083955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 11:35
 Operator : AR\AJ
 Sample : 03501-16MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A46X7MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/19/2023
 Supervised By : Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:38:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 05:26:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.470	2.689	2783.1E6	11181757	1342.004	10.891 #
27)	SA Decachlor...	9.023	7.870	37995624	23954372	28.908	21.644 #
Target Compounds							
2)	A alpha-BHC	3.927	3.192	273.6E6	60687812	90.550m	41.991m#
3)	MA gamma-BHC...	4.273	3.505	2283.9E6	1743.8E6	809.545m	1262.722m#
4)	MA Heptachlor	4.857	3.886	77035413	4788.6E6	24.477m	3634.692 #
5)	MB Aldrin	5.201	4.129	62256131	543.2E6	20.954	416.092 #
6)	B beta-BHC	4.445	3.823	7215.4E6	35719966	5384.559m	53.022m#
7)	B delta-BHC	4.740f	4.061	3064.1E6	248.1E6	1082.119m	173.446m#
8)	B Heptachlo...	5.626	4.652	830.7E6	336.8E6	300.286m	269.090
9)	A Endosulfan I	6.009	5.021	259.1E6	27959774	107.341	24.694m#
10)	B trans-Chl...	5.911	4.890	294.1E6	254.3E6	112.472m	205.571m#
11)	B cis-Chlor...	5.971	4.962	240.8E6	77353061	90.684	60.384m#
12)	B 4,4'-DDE	6.144	5.168	361.4E6	104.9E6	174.488	86.937 #
13)	MA Dieldrin	6.295	5.295	306.9E6	527.8E6	126.398	403.541 #
14)	MA Endrin	6.525	5.563	482.6E6	151.7E6	248.955	133.222m#
15)	B Endosulfa...	6.742	5.861	183.6E6	156.5E6	96.217m	137.149 #
16)	A 4,4'-DDD	6.670	5.726	294.7E6	83254200	200.263	85.954 #
17)	MA 4,4'-DDT	6.950	5.972	345.4E6	275.4E6	223.627m	264.378
18)	B Endrin al...	6.874	6.041	144.3E6	42848182	109.279	52.217m#
19)	B Endosulfa...	7.108	6.270	193.4E6	113.5E6	110.270	102.882
20)	A Methoxychlor	7.462	6.560	341.5E6	269.5E6	447.917	480.752m
21)	B Endrin ke...	7.584	6.773	350.2E6	106.8E6	206.437	81.472 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071623\
Data File : PL083955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 11:35
Operator : AR\AJ
Sample : 03501-16MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:38:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 05:26:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

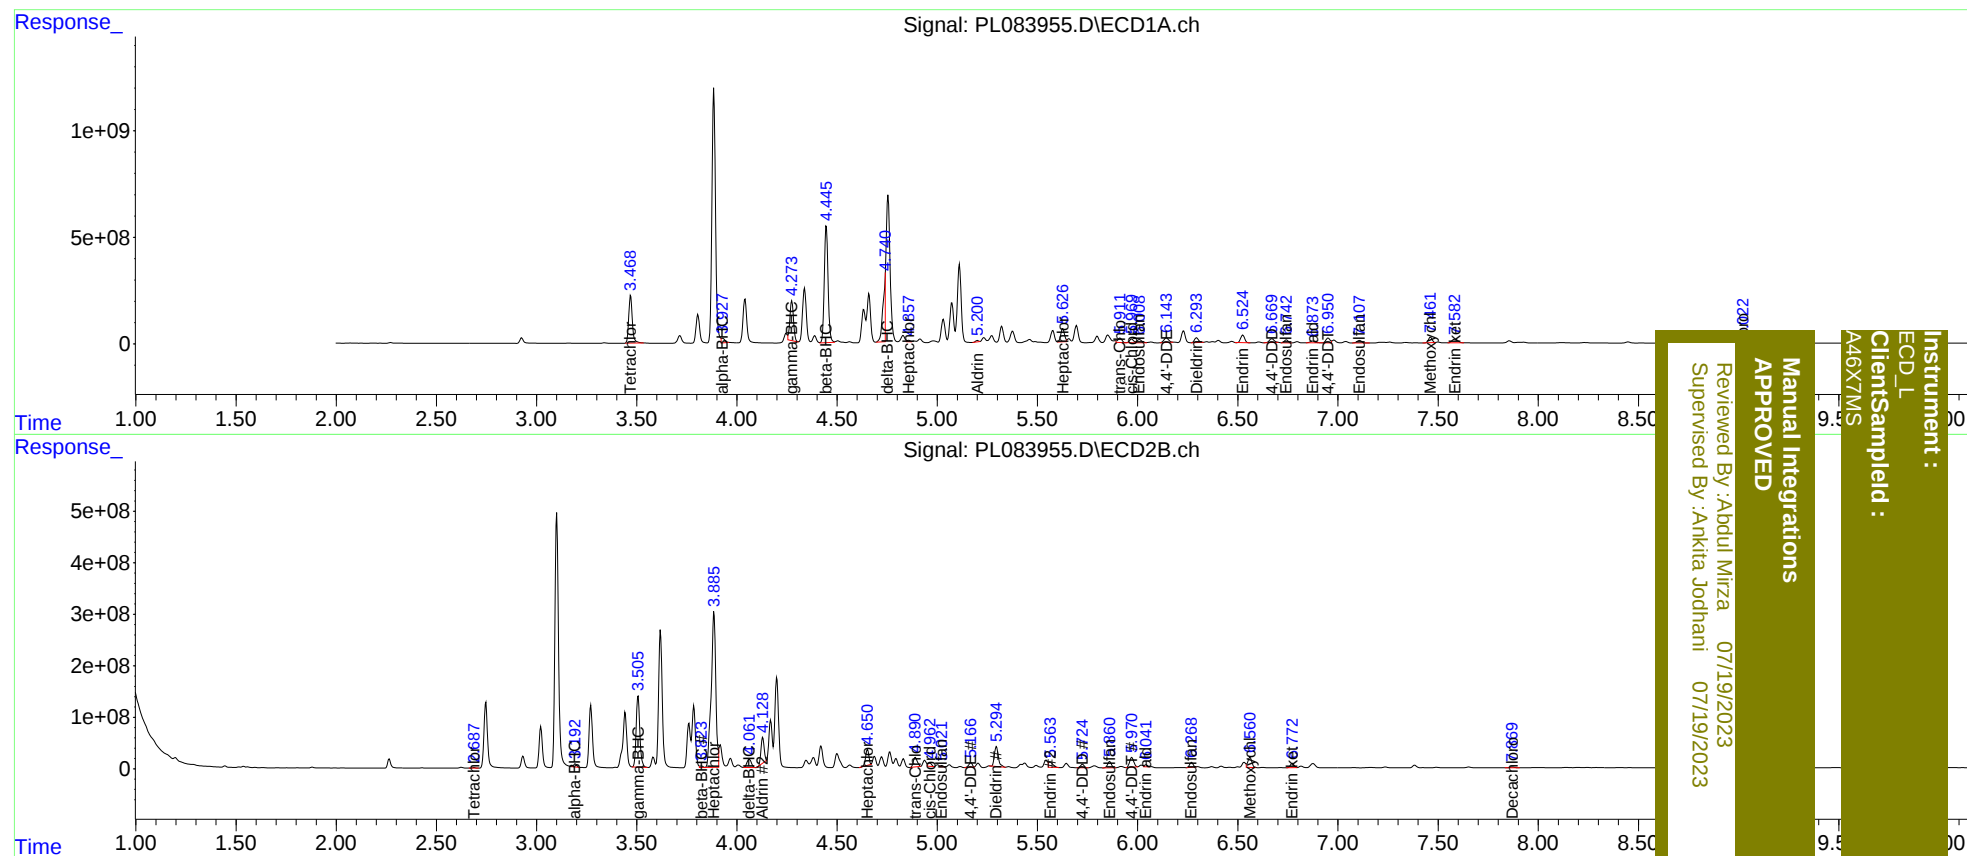

Reviewed By: Abdul Muzza 07/19/2023
Supervised By: Ankita Jodhani 07/19/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sampled :
A46XTMS