

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071623\
 Data File : PL083956.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2023 11:49
 Operator : AR\AJ
 Sample : 03501-17MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A46X7MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/19/2023
 Supervised By : Ankita Jodhani 07/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:46:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 05:26:27 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.470	2.688	2417.5E6	9440775	1165.715	9.195 #
27)	SA Decachlor...	9.024	7.870	34109263	20705903	25.951	18.709 #
Target Compounds							
2)	A alpha-BHC	3.929	3.192	206.6E6	52145925	68.399m	36.081m#
3)	MA gamma-BHC...	4.273	3.506	2034.0E6	1553.5E6	720.938m	1124.923m#
4)	MA Heptachlor	4.856	3.870	46382269	813.9E6	14.737m	617.806m#
5)	MB Aldrin	5.201	4.128	52292171	662.8E6	17.600	507.672m#
6)	B beta-BHC	4.446	3.823	6311.6E6	23531196	4710.118m	34.929m#
7)	B delta-BHC	4.736	4.062	1696.3E6	218.3E6	599.077m	152.593m#
8)	B Heptachlo...	5.626	4.652	730.2E6	298.4E6	263.960m	238.398
9)	A Endosulfan I	6.009	5.021	229.1E6	23173692	94.943	20.467m#
10)	B trans-Chl...	5.912	4.889	240.7E6	237.3E6	92.035m	191.837m#
11)	B cis-Chlor...	5.971	4.962	212.0E6	74303430	79.858	58.003m#
12)	B 4,4'-DDE	6.144	5.167	318.8E6	92194977	153.925	76.413 #
13)	MA Dieldrin	6.295	5.294	268.1E6	406.0E6	110.421	310.467m#
14)	MA Endrin	6.526	5.562	419.5E6	120.5E6	216.412	105.791m#
15)	B Endosulfa...	6.742	5.861	155.6E6	137.7E6	81.537m	120.715 #
16)	A 4,4'-DDD	6.671	5.725	254.8E6	73098439	173.103	75.469 #
17)	MA 4,4'-DDT	6.949	5.971	277.2E6	241.6E6	179.491m	231.929 #
18)	B Endrin al...	6.874	6.041	128.7E6	38867461	97.443	47.366m#
19)	B Endosulfa...	7.109	6.269	168.3E6	100.2E6	95.932	90.781
20)	A Methoxychlor	7.462	6.560	295.6E6	241.7E6	387.722	431.076m
21)	B Endrin ke...	7.583	6.773	297.6E6	93763207	175.410	71.553 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071623\
Data File : PL083956.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2023 11:49
Operator : AR\AJ
Sample : 03501-17MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:46:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071523CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 05:26:27 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

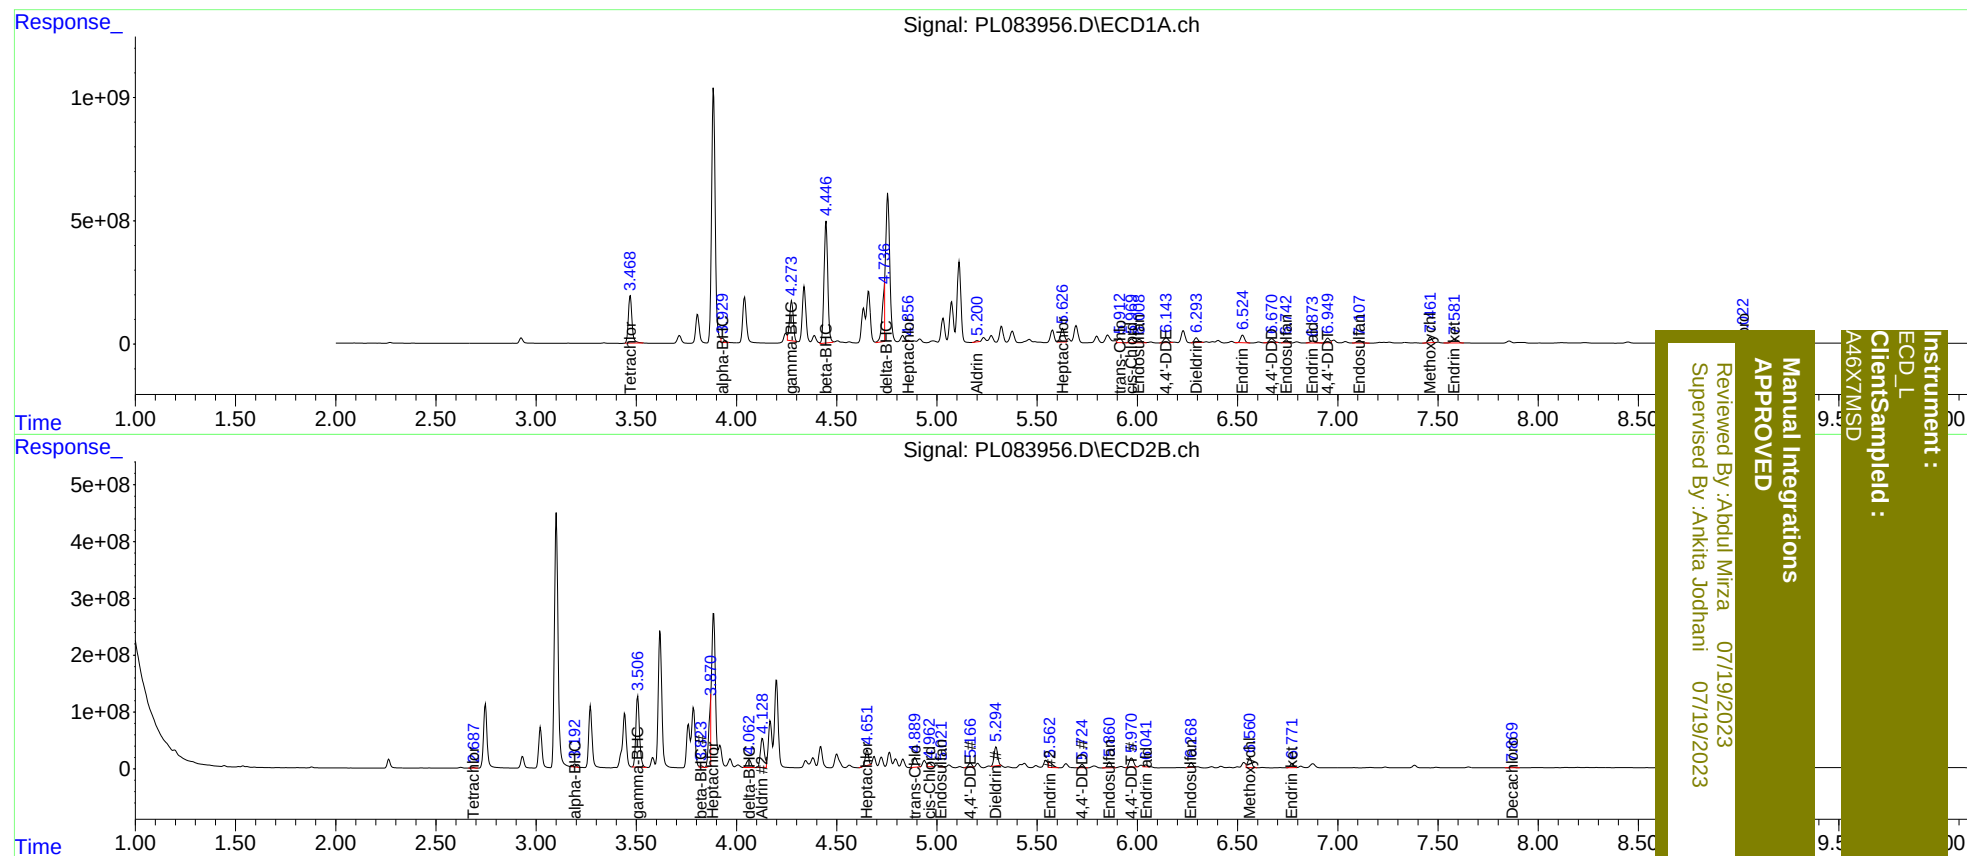

Instrument :
ECD_L
Client Sampled :
A46X7MSD

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/19/2023
Supervised By : Ankita Jodhani 07/19/2023