

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071625\
 Data File : PL096411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2025 18:25
 Operator : AR\AJ
 Sample : PB168867BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:45:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.829	79169621	134.6E6	21.696	23.317
28)	SA Decachlor...	9.020	7.994	59101088	100.6E6	21.010	20.171
Target Compounds							
8)	B Heptachlo...	5.657	0.000	123.9E6	0	29.861	N.D. #
11)	B alpha-Chl...	5.972f	0.000	12299881	0	2.809	N.D. #
14)	MA Endrin	0.000	5.719	0	231.2E6	N.D.	37.926 #
15)	B Endosulfa...	6.754	0.000	32033787	0	9.232	N.D. #
16)	A 4,4'-DDD	6.672	0.000	32012298	0	10.994	N.D. #
18)	B Endrin al...	0.000	6.178	0	18590320	N.D.	4.173 #
22)	Mirex	8.086	0.000	10423296	0	3.746	N.D. #
24)	Chlordane-2	0.000	4.416	0	31087238	N.D.	113.106 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071625\
Data File : PL096411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2025 18:25
Operator : AR\AJ
Sample : PB168867BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:45:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

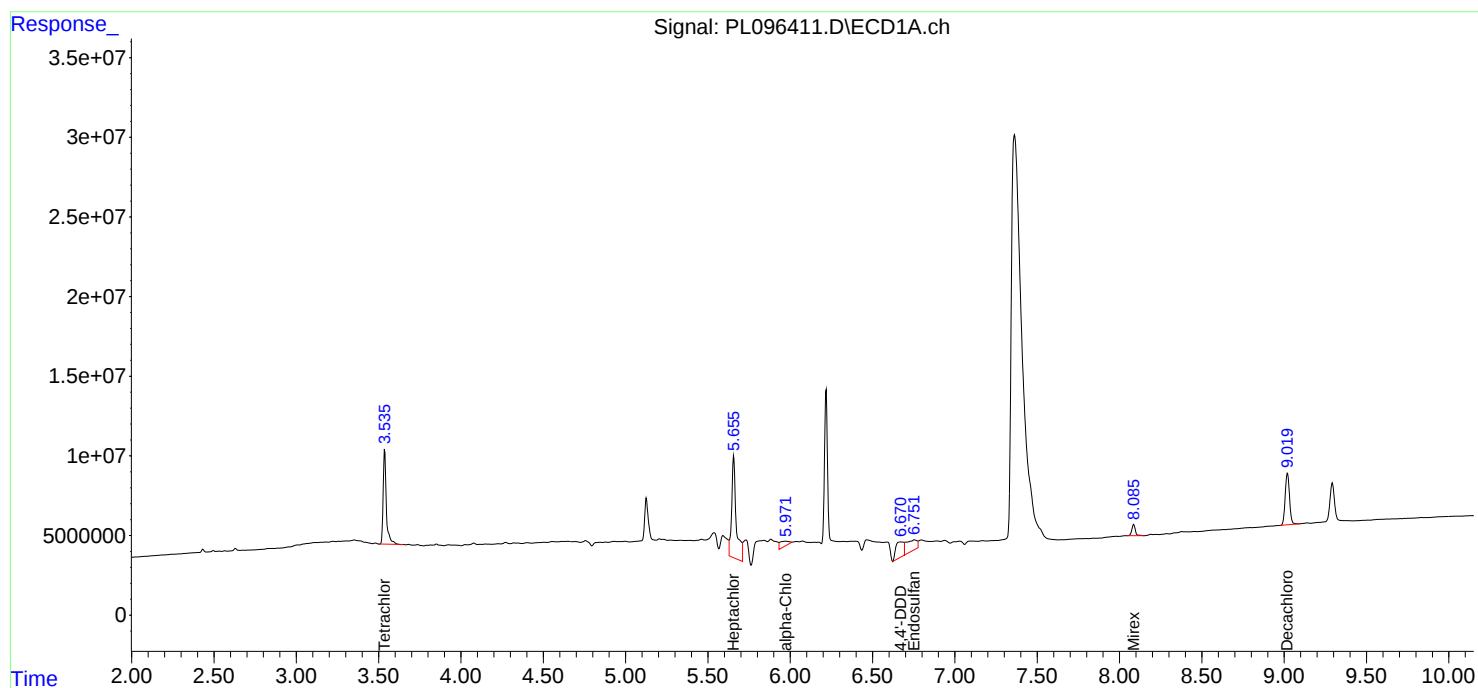


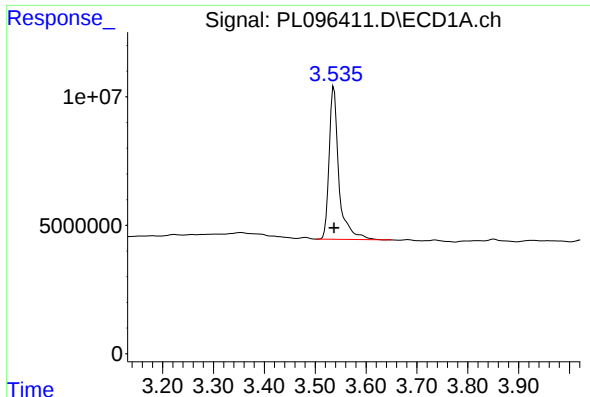

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 79169621
Conc: 21.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

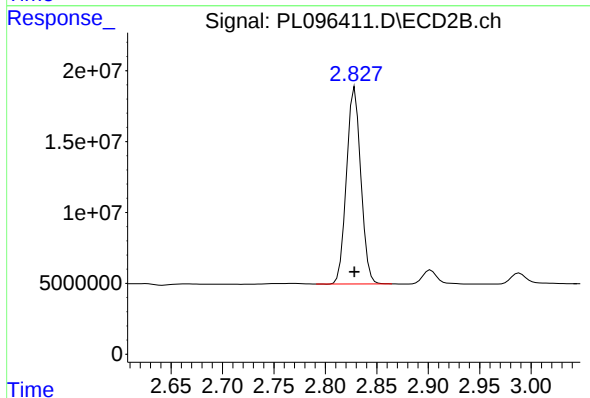


#1 Tetrachloro-m-xylene

R.T.: 2.829 min
Delta R.T.: 0.000 min
Response: 134569714
Conc: 23.32 ng/ml

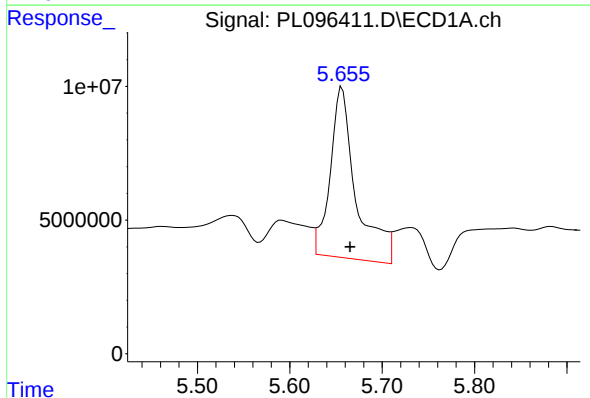


#8 Heptachlor epoxide

R.T.: 5.657 min
Delta R.T.: -0.009 min
Response: 123896339
Conc: 29.86 ng/ml

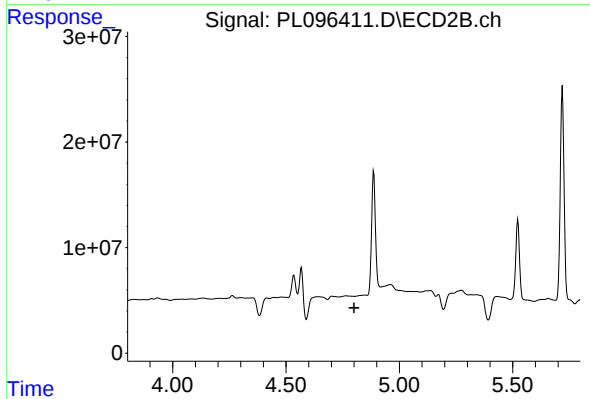

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

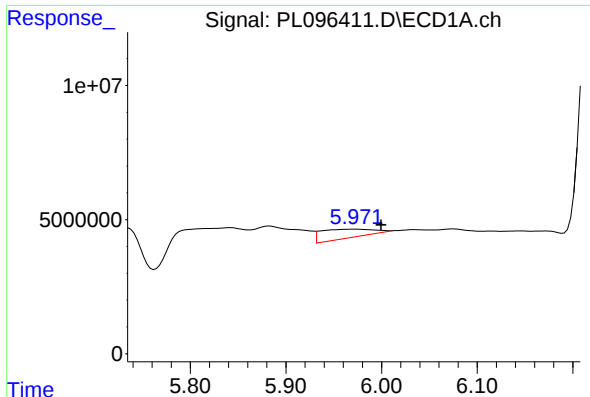

#11 alpha-Chlordane


R.T.: 5.972 min
Delta R.T.: -0.027 min
Response: 12299881
Conc: 2.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

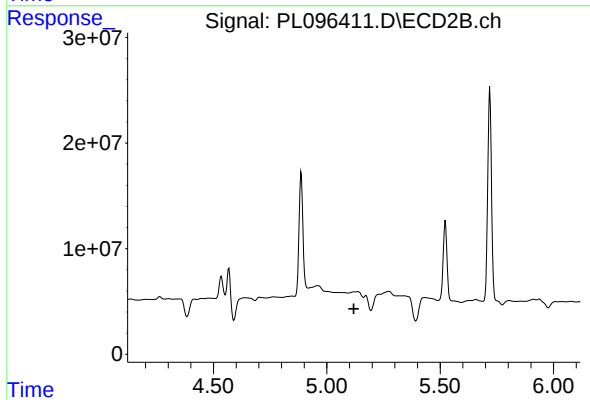


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

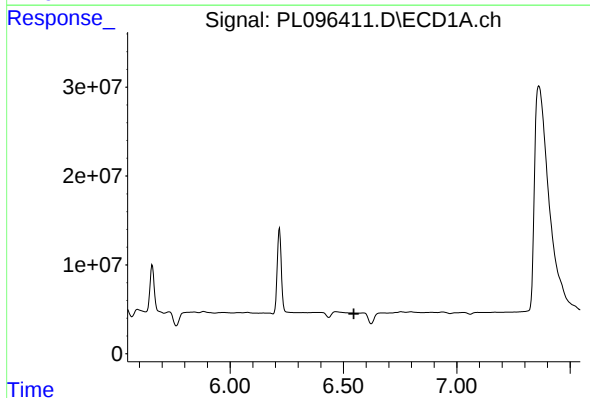


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.545 min
Response: 0
Conc: N.D.

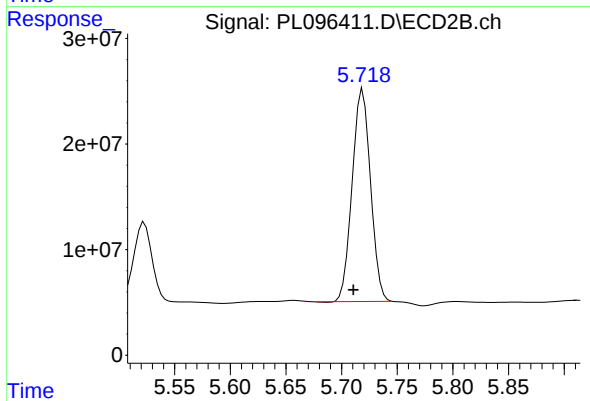

#14 Endrin


R.T.: 5.719 min
Delta R.T.: 0.008 min
Response: 231215822
Conc: 37.93 ng/ml

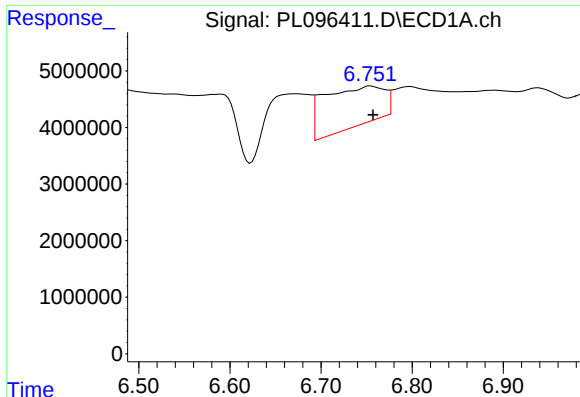

#15 Endosulfan II


R.T.: 6.754 min
Delta R.T.: -0.003 min
Response: 32033787
Conc: 9.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

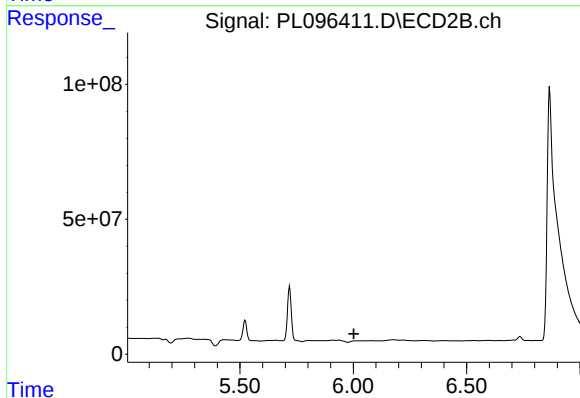


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.003 min
Response: 0
Conc: N.D.

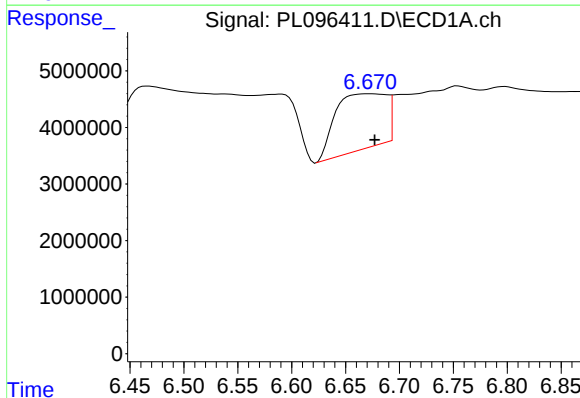


#16 4,4'-DDD

R.T.: 6.672 min
Delta R.T.: -0.006 min
Response: 32012298
Conc: 10.99 ng/ml

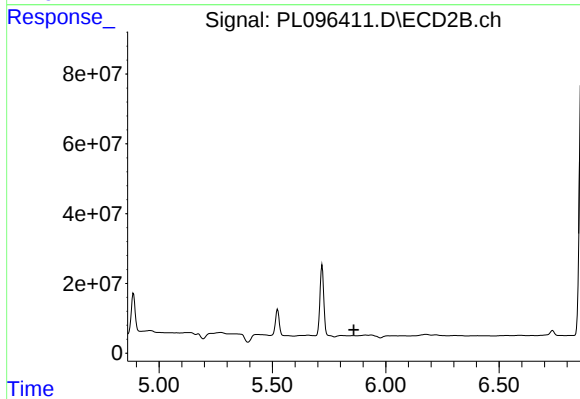

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.859 min
Response: 0
Conc: N.D.

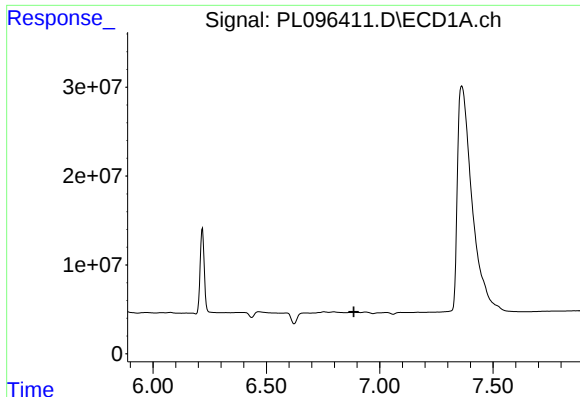

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

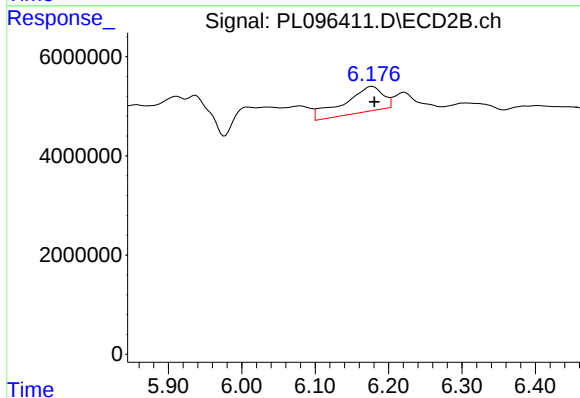


#18 Endrin aldehyde

R.T.: 6.178 min
Delta R.T.: -0.003 min
Response: 18590320
Conc: 4.17 ng/ml

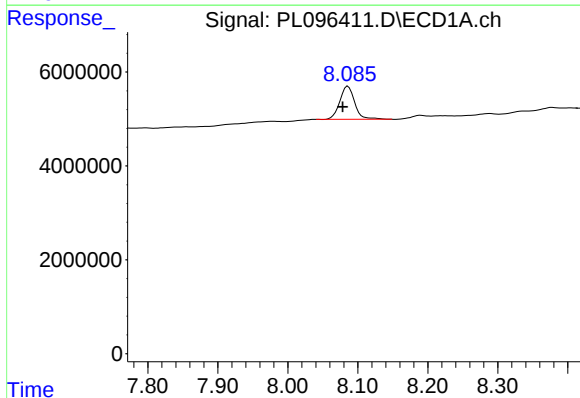


#22 Mirex

R.T.: 8.086 min
Delta R.T.: 0.007 min
Response: 10423296
Conc: 3.75 ng/ml

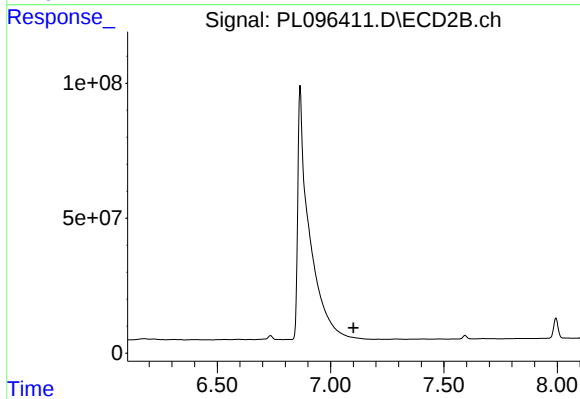

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.101 min
Response: 0
Conc: N.D.

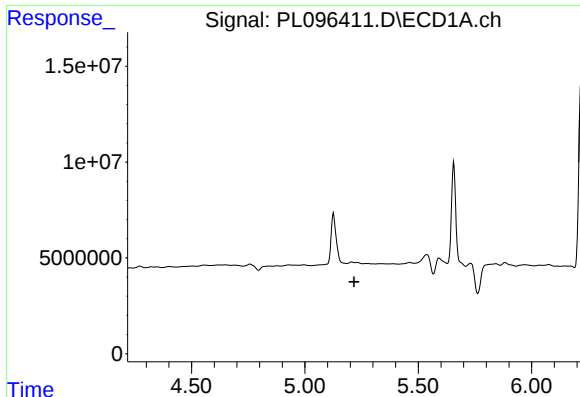

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.217 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

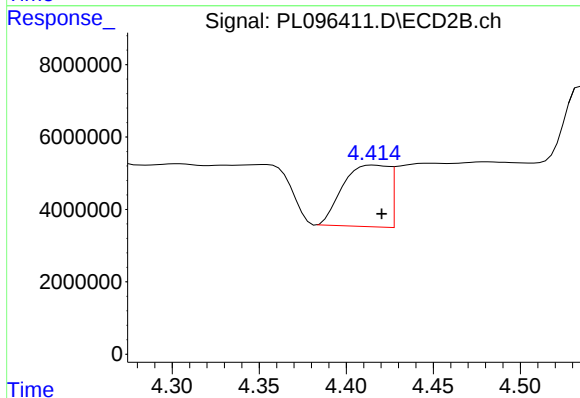


#24 Chlordane-2

R.T.: 4.416 min
Delta R.T.: -0.005 min
Response: 31087238
Conc: 113.11 ng/ml

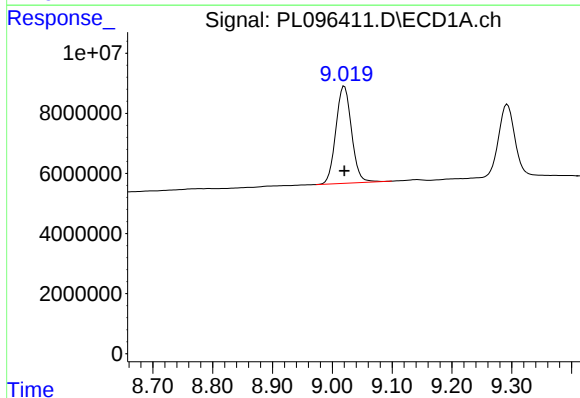

#28 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 59101088
Conc: 21.01 ng/ml

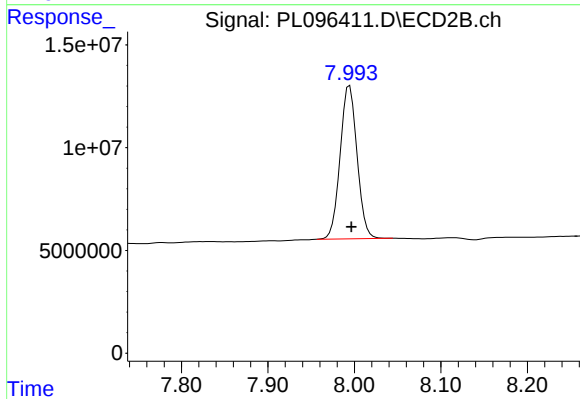

#28 Decachlorobiphenyl

R.T.: 7.994 min
Delta R.T.: -0.002 min
Response: 100583942
Conc: 20.17 ng/ml