

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071625\
 Data File : PL096421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jul 2025 20:42
 Operator : AR\AJ
 Sample : Q2579-03RE
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:47:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.829	71935268	114.8E6	19.714	19.890
28)	SA Decachlor...	9.019	7.993	56560091	100.4E6	20.106	20.127
Target Compounds							
3)	MA gamma-BHC...	0.000	3.669	0	17882556	N.D.	2.271 #
13)	MA Dieldrin	0.000	5.436	0	14000188	N.D.	2.053 #
14)	MA Endrin	6.562f	5.719	3906929	7313288	1.256	1.200
15)	B Endosulfa...	0.000	5.982f	0	12183394	N.D.	2.078 #
18)	B Endrin al...	0.000	6.175	0	13447096	N.D.	3.019 #
23)	Chlordane-1	0.000	3.835	0	17346716	N.D.	73.391 #
24)	Chlordane-2	0.000	4.451f	0	11393956	N.D.	41.455 #
27)	Chlordane-5	0.000	5.982f	0	12183394	N.D.	42.982 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071625\
Data File : PL096421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jul 2025 20:42
Operator : AR\AJ
Sample : Q2579-03RE
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:47:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

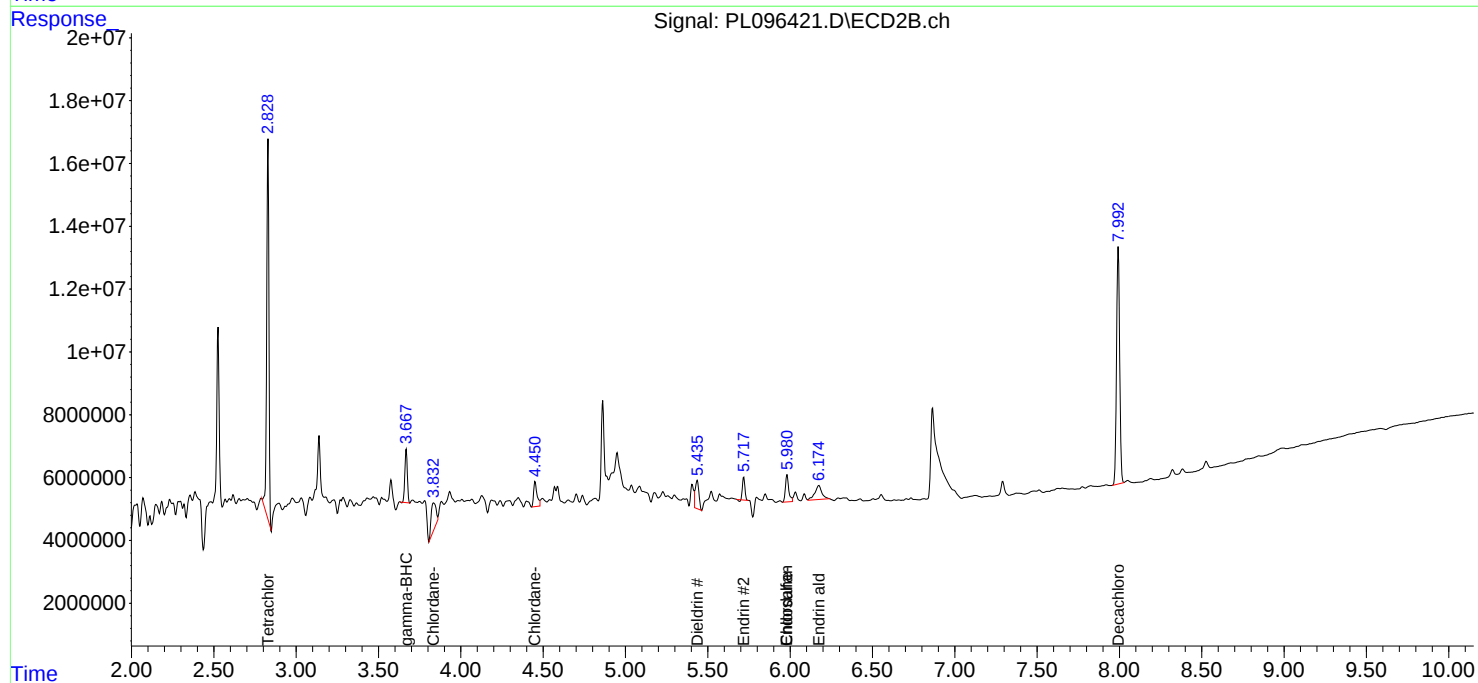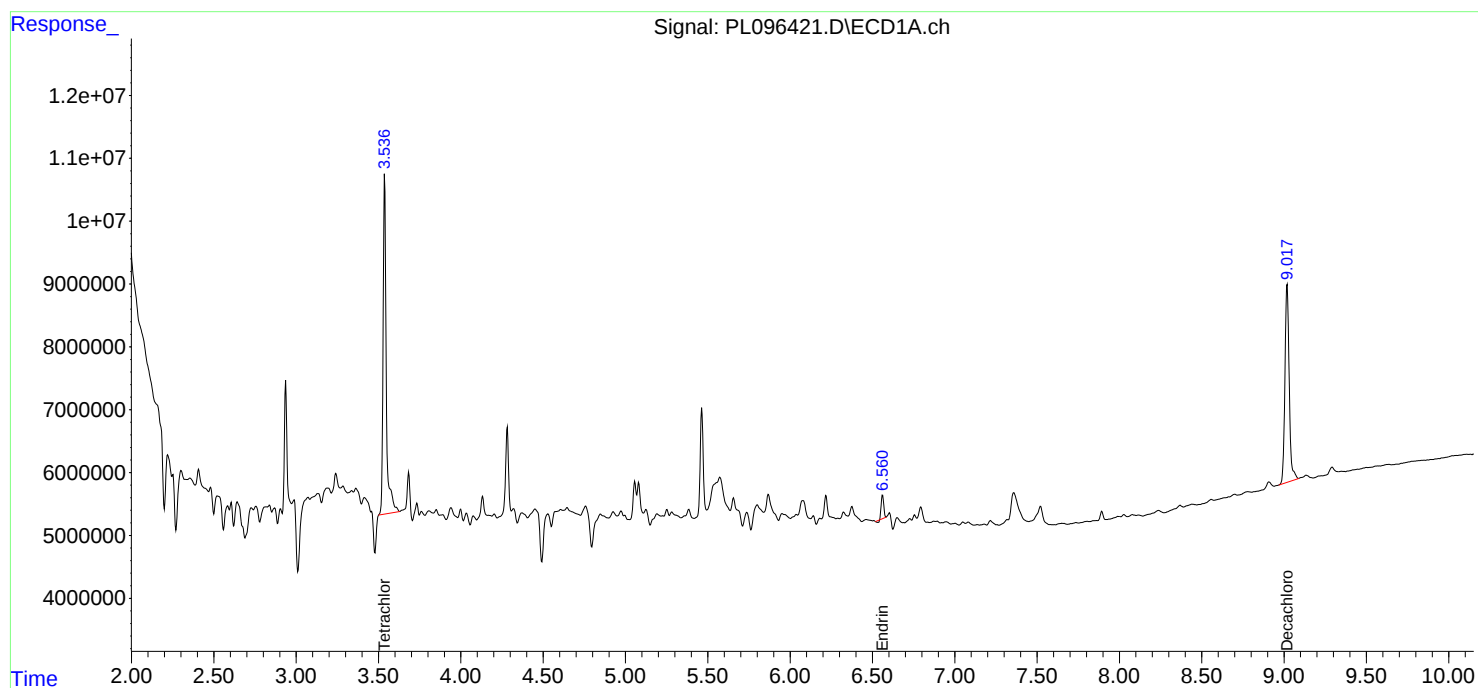


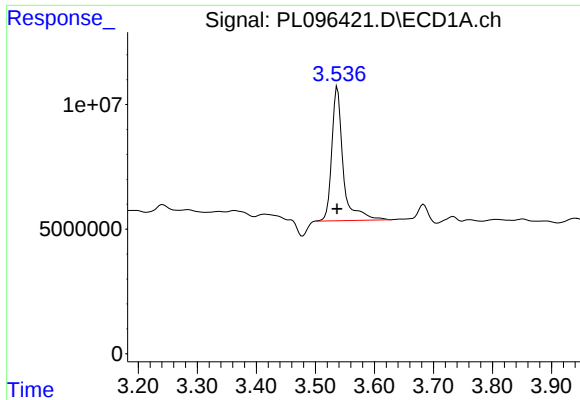

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 71935268
Conc: 19.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

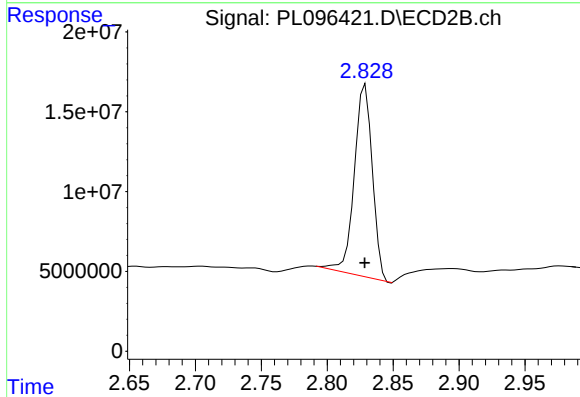


#1 Tetrachloro-m-xylene

R.T.: 2.829 min
Delta R.T.: 0.000 min
Response: 114790145
Conc: 19.89 ng/ml

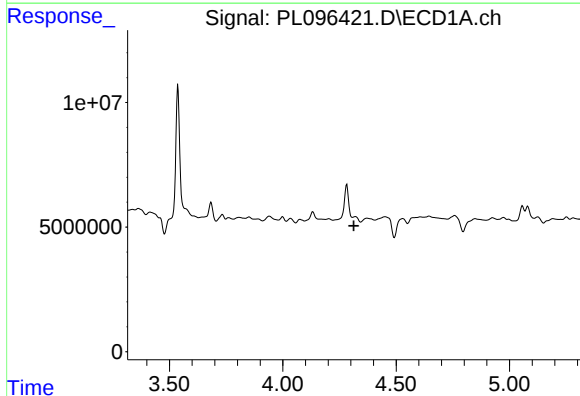


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.313 min
Response: 0
Conc: N.D.

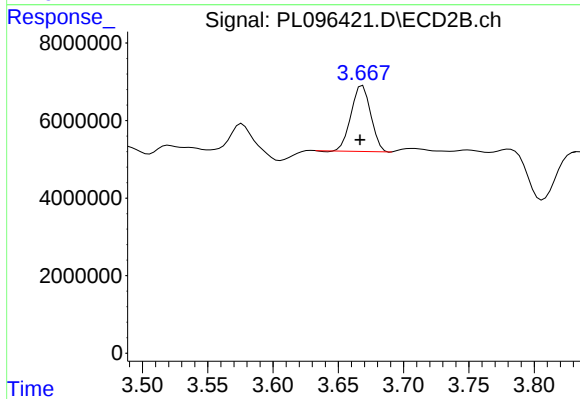

#3 gamma-BHC (Lindane)


R.T.: 3.669 min
Delta R.T.: 0.002 min
Response: 17882556
Conc: 2.27 ng/ml

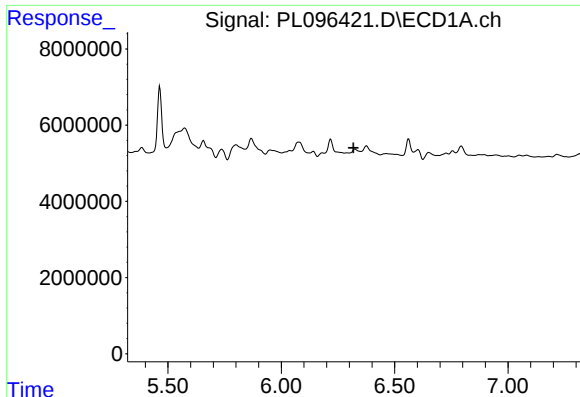

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

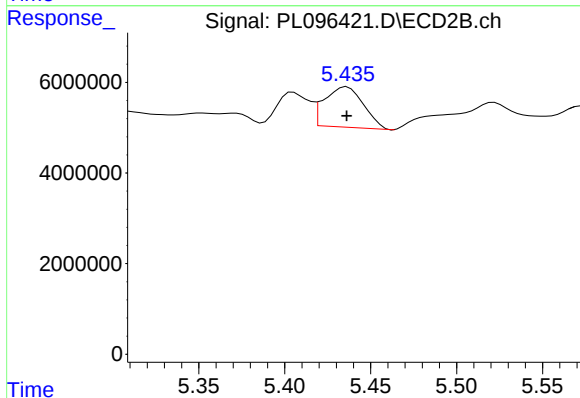


#13 Dieldrin

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 14000188
Conc: 2.05 ng/ml

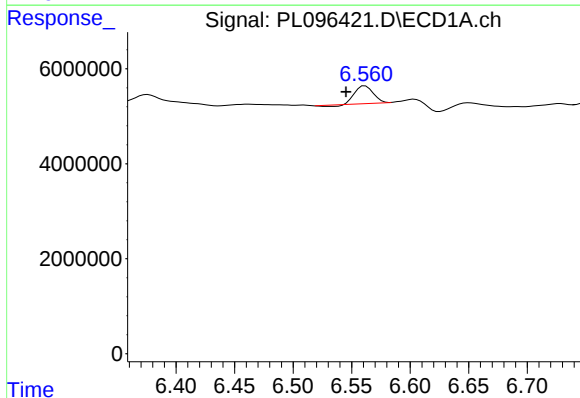


#14 Endrin

R.T.: 6.562 min
Delta R.T.: 0.016 min
Response: 3906929
Conc: 1.26 ng/ml

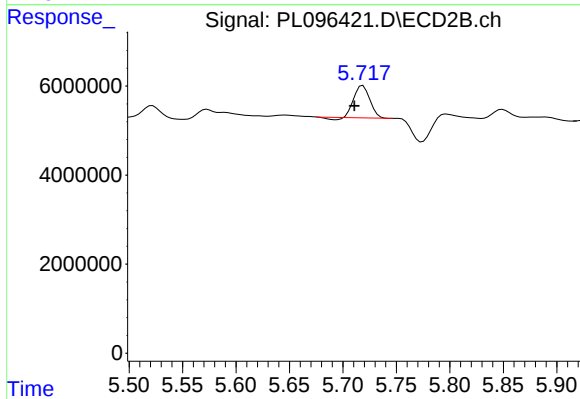

#14 Endrin


R.T.: 5.719 min
Delta R.T.: 0.008 min
Response: 7313288
Conc: 1.20 ng/ml

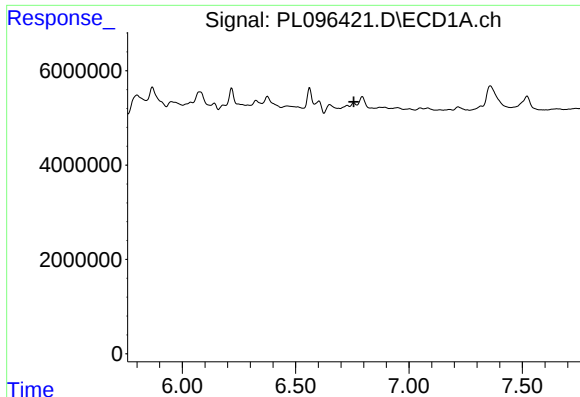

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.757 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

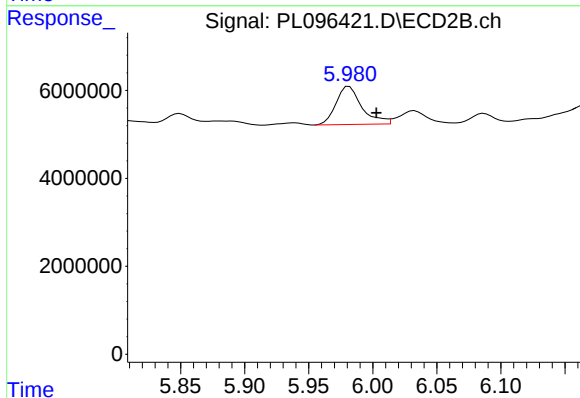


#15 Endosulfan II

R.T.: 5.982 min
Delta R.T.: -0.021 min
Response: 12183394
Conc: 2.08 ng/ml

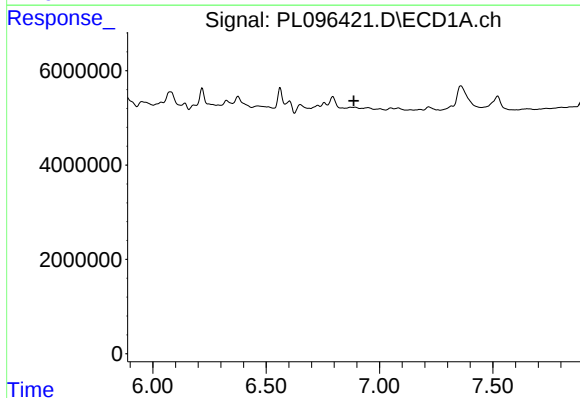


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.886 min
Response: 0
Conc: N.D.

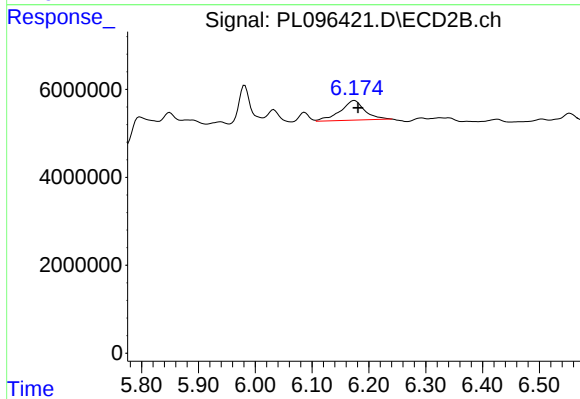

#18 Endrin aldehyde


R.T.: 6.175 min
Delta R.T.: -0.006 min
Response: 13447096
Conc: 3.02 ng/ml

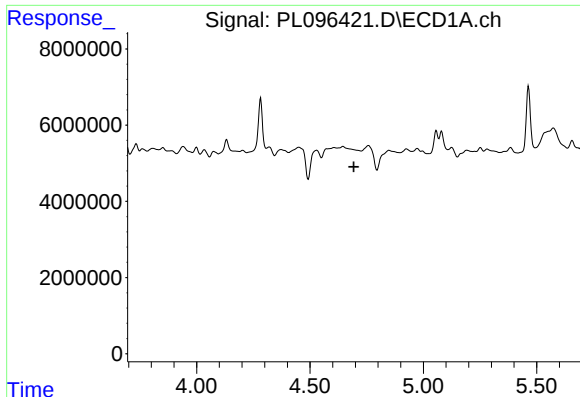

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

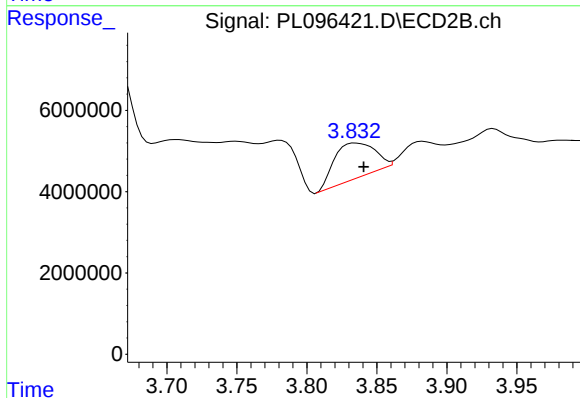


#23 Chlordane-1

R.T.: 3.835 min
Delta R.T.: -0.006 min
Response: 17346716
Conc: 73.39 ng/ml

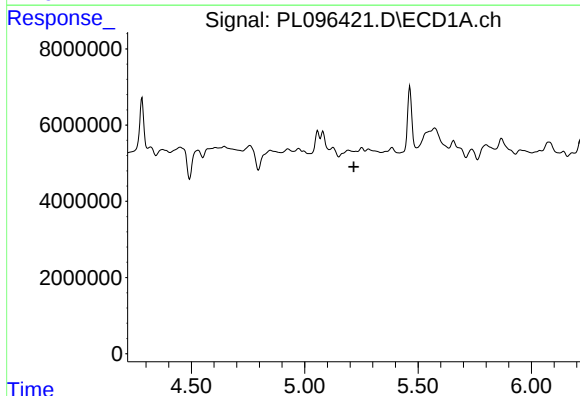


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.217 min
Response: 0
Conc: N.D.

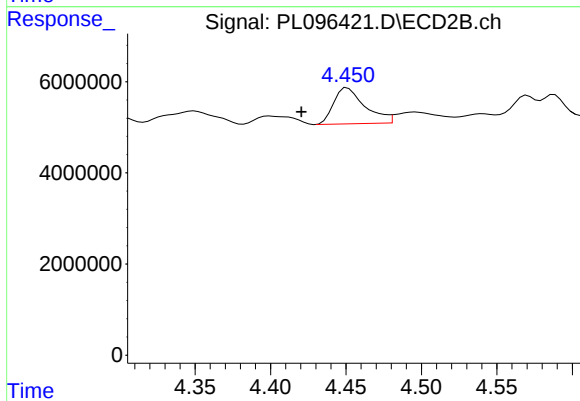

#24 Chlordane-2


R.T.: 4.451 min
Delta R.T.: 0.031 min
Response: 11393956
Conc: 41.45 ng/ml

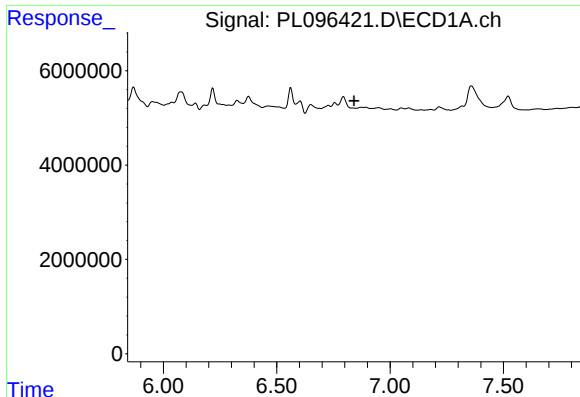

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.841 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

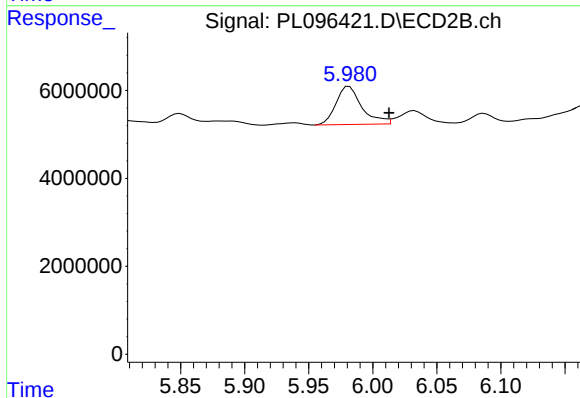


#27 Chlordane-5

R.T.: 5.982 min
Delta R.T.: -0.031 min
Response: 12183394
Conc: 42.98 ng/ml

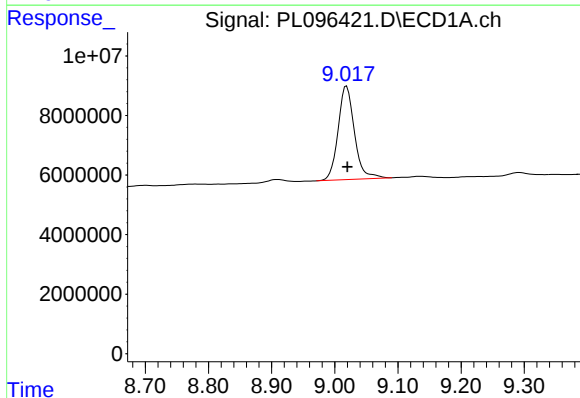

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: -0.001 min
Response: 56560091
Conc: 20.11 ng/ml

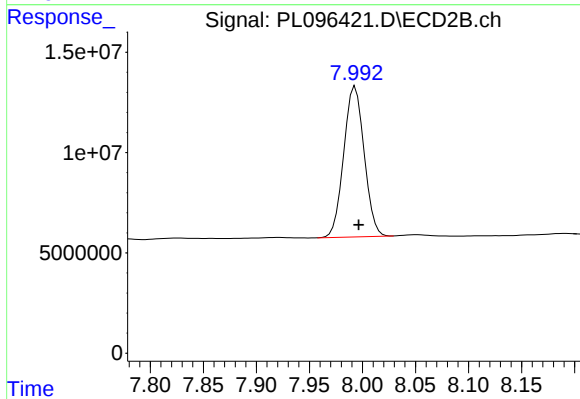

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 100365430
Conc: 20.13 ng/ml