

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL071625\  
 Data File : PL096423.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 16 Jul 2025 21:09  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 17 01:48:03 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL070725.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Jul 07 15:22:07 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

|                             | Compound        | RT#1  | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|-------|--------|----------|----------|--------|---------|
| -----                       |                 |       |        |          |          |        |         |
| System Monitoring Compounds |                 |       |        |          |          |        |         |
| 1)                          | SA Tetrachlo... | 3.537 | 2.829  | 81413381 | 145.6E6  | 22.311 | 25.233  |
| 28)                         | SA Decachlor... | 9.020 | 7.994  | 63085664 | 116.6E6  | 22.426 | 23.382  |
|                             |                 |       |        |          |          |        |         |
| Target Compounds            |                 |       |        |          |          |        |         |
| 13)                         | MA Dieldrin     | 0.000 | 5.419f | 0        | 1063198  | N.D.   | 0.156 # |
| 14)                         | MA Endrin       | 0.000 | 5.719  | 0        | 9991635  | N.D.   | 1.639 # |
| 15)                         | B Endosulfa...  | 6.746 | 0.000  | 7910585  | 0        | 2.280  | N.D. #  |
| 18)                         | B Endrin al...  | 0.000 | 6.175  | 0        | 18692723 | N.D.   | 4.196 # |
| -----                       |                 |       |        |          |          |        |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL071625\  
Data File : PL096423.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 16 Jul 2025 21:09  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 17 01:48:03 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL070725.M  
Quant Title : GC Extractables  
QLast Update : Mon Jul 07 15:22:07 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

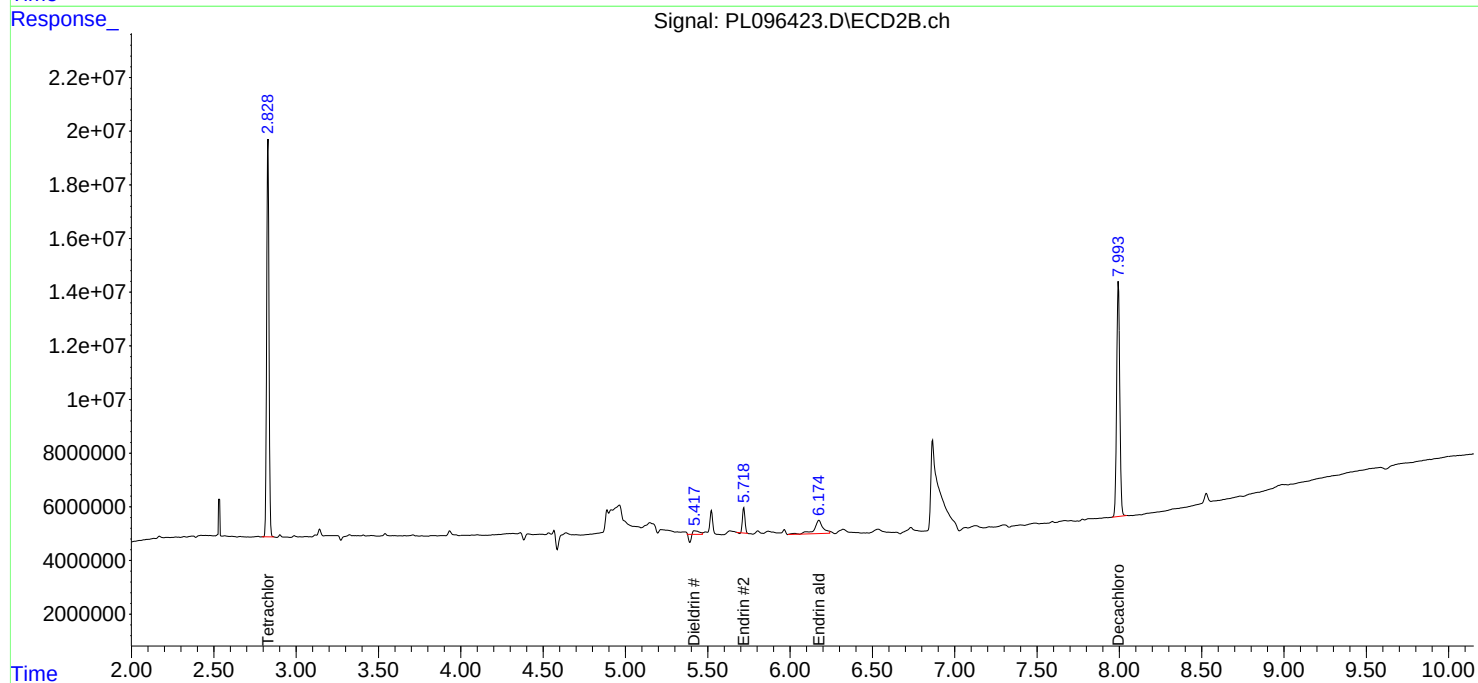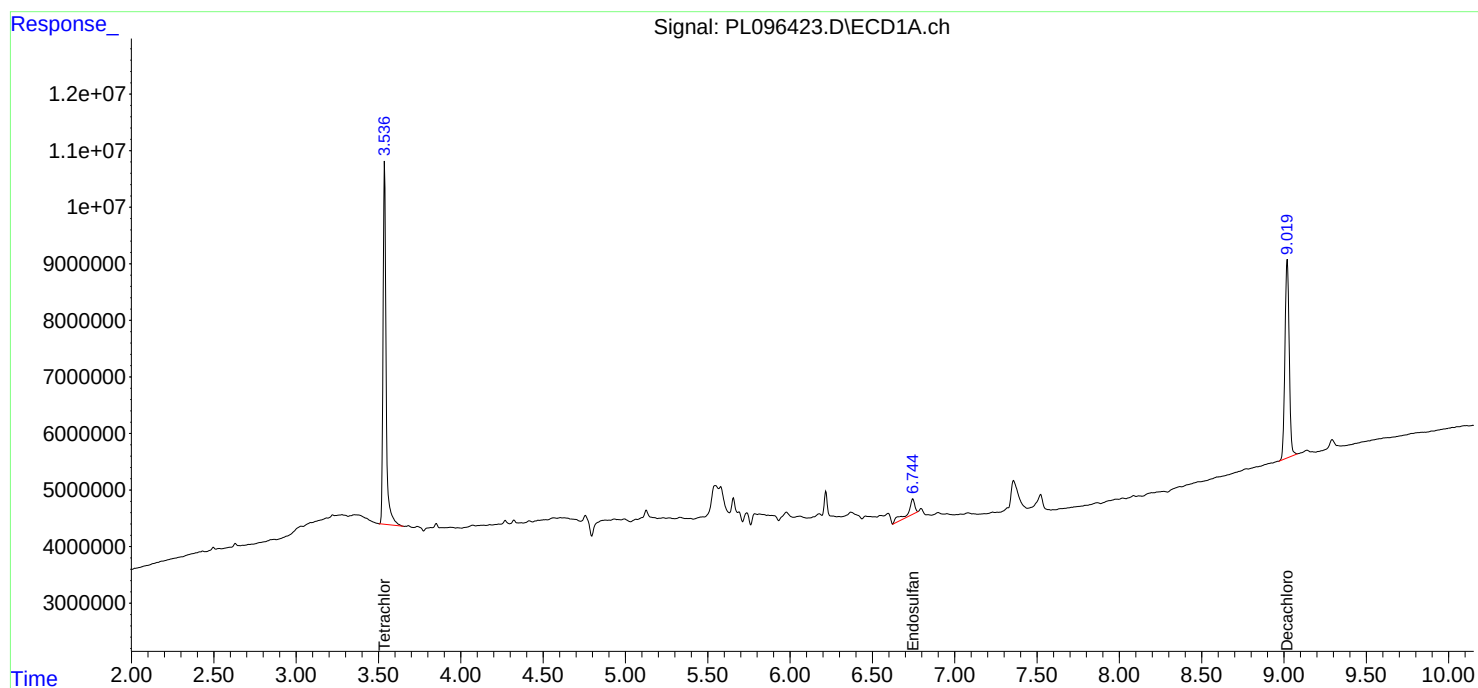


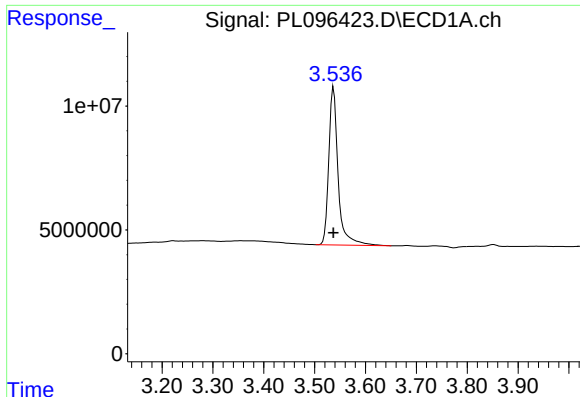

#1 Tetrachloro-m-xylene


R.T.: 3.537 min  
Delta R.T.: 0.000 min  
Response: 81413381  
Conc: 22.31 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

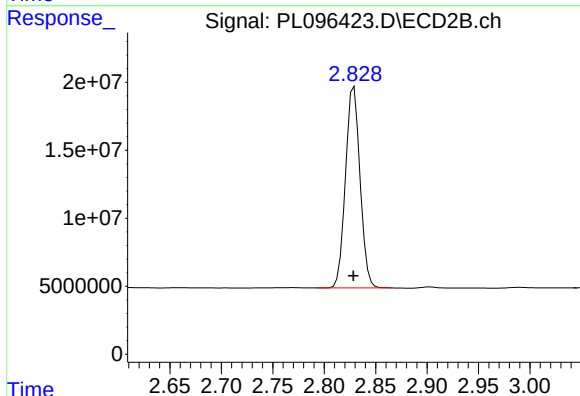


#1 Tetrachloro-m-xylene

R.T.: 2.829 min  
Delta R.T.: 0.000 min  
Response: 145623526  
Conc: 25.23 ng/ml

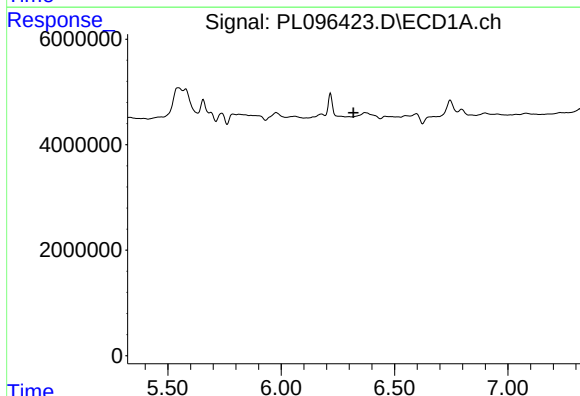


#13 Dieldrin

R.T.: 0.000 min  
Exp R.T. : 6.319 min  
Response: 0  
Conc: N.D.

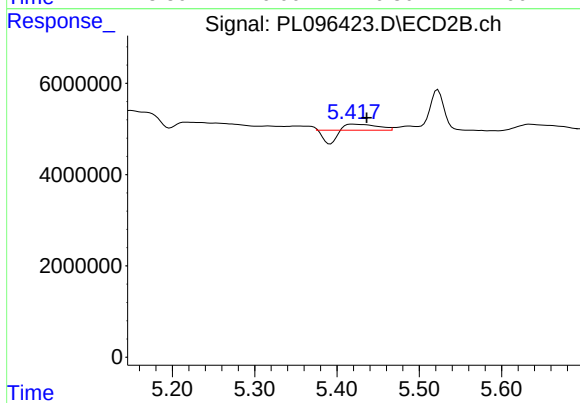

#13 Dieldrin


R.T.: 5.419 min  
Delta R.T.: -0.017 min  
Response: 1063198  
Conc: 0.16 ng/ml

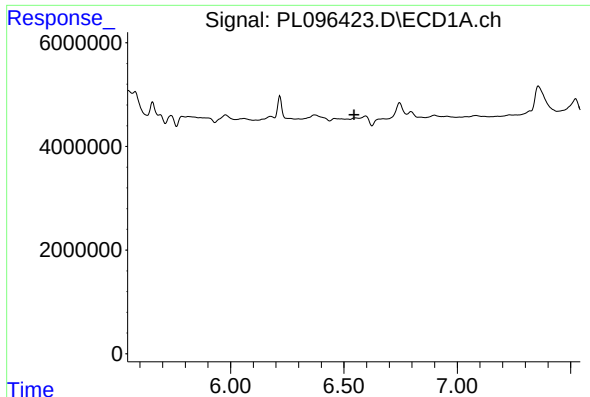

#14 Endrin


R.T.: 0.000 min  
Exp R.T.: 6.545 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

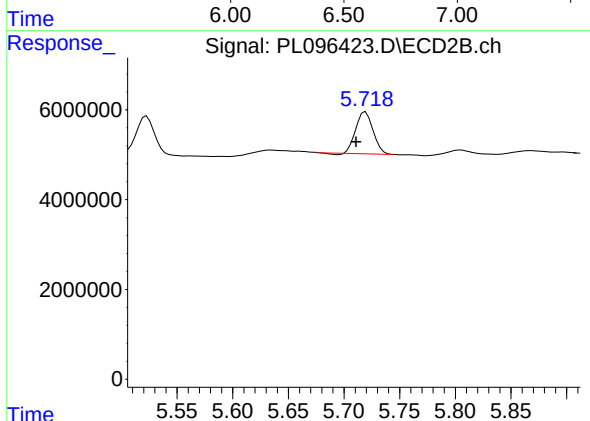


#14 Endrin

R.T.: 5.719 min  
Delta R.T.: 0.009 min  
Response: 9991635  
Conc: 1.64 ng/ml

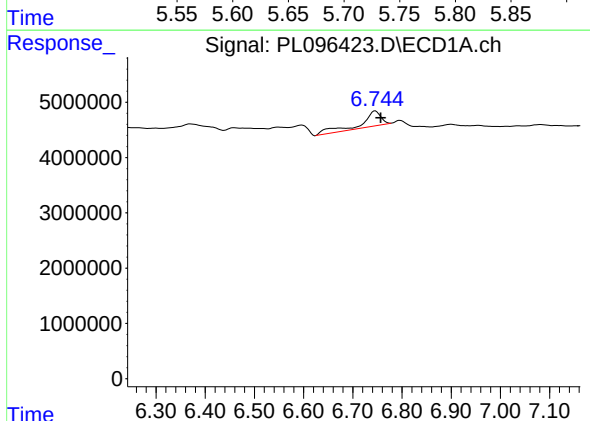


#15 Endosulfan II

R.T.: 6.746 min  
Delta R.T.: -0.011 min  
Response: 7910585  
Conc: 2.28 ng/ml

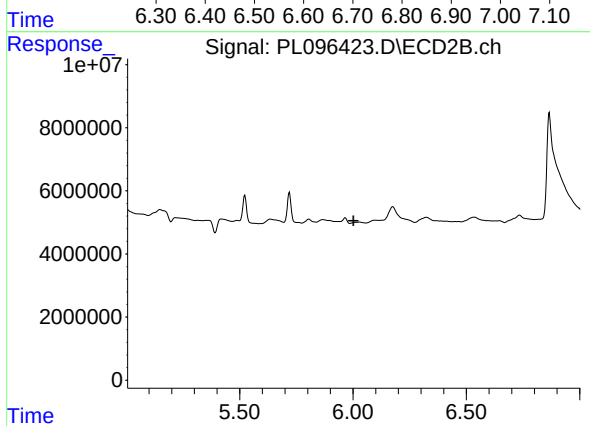

#15 Endosulfan II


R.T.: 0.000 min  
Exp R.T.: 6.003 min  
Response: 0  
Conc: N.D.

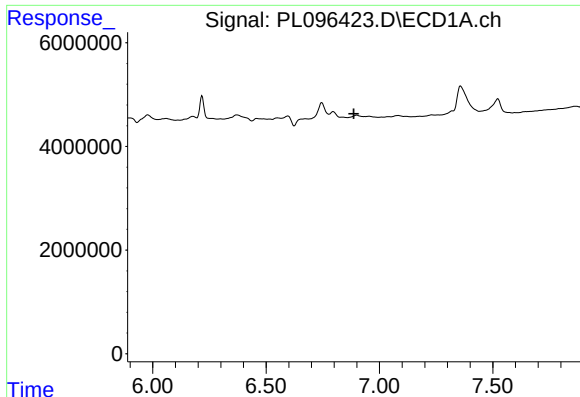

#18 Endrin aldehyde


R.T.: 0.000 min  
Exp R.T.: 6.886 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

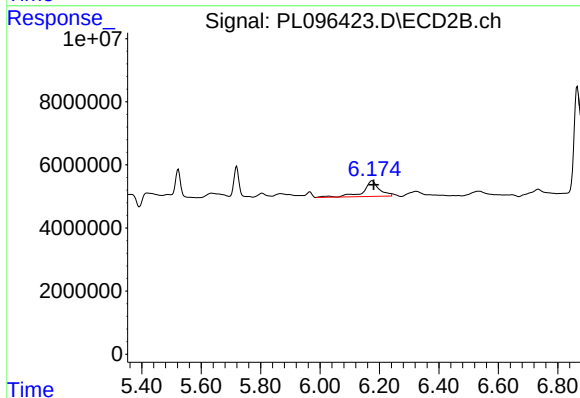


#18 Endrin aldehyde

R.T.: 6.175 min  
Delta R.T.: -0.005 min  
Response: 18692723  
Conc: 4.20 ng/ml

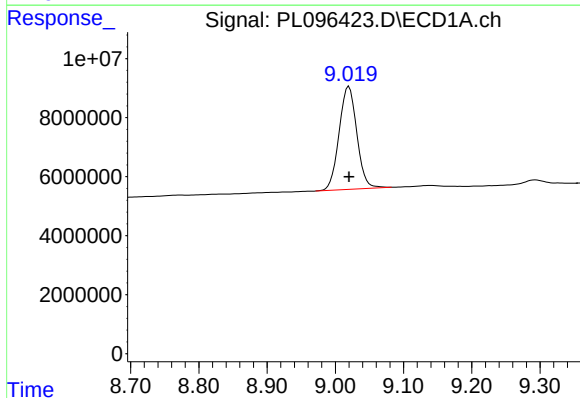

#28 Decachlorobiphenyl

R.T.: 9.020 min  
Delta R.T.: 0.000 min  
Response: 63085664  
Conc: 22.43 ng/ml

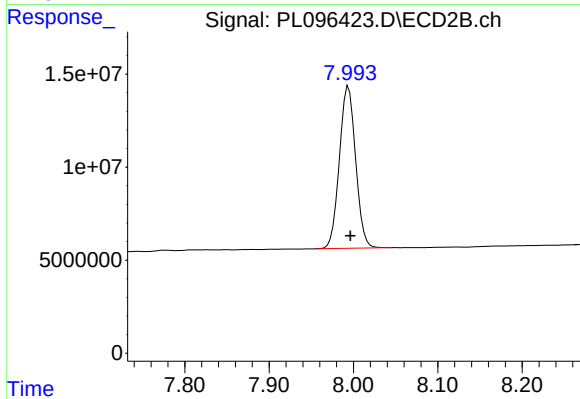

#28 Decachlorobiphenyl

R.T.: 7.994 min  
Delta R.T.: -0.002 min  
Response: 116592481  
Conc: 23.38 ng/ml