

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071718\
 Data File : PL038174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 16:02
 Operator : AJ\SJ
 Sample : PB111183BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 04:28:08 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.339	3.930	129.4E6	50089660	17.375	19.082
28)	SA Decachlor...	8.014	8.945	128.3E6	43938457	16.914	17.975
Target Compounds							
4)	MA Heptachlor	4.257f	0.000	6147632	0	0.578	N.D. #
6)	B beta-BHC	4.257f	0.000	6147632	0	1.302	N.D. #
7)	B delta-BHC	0.000	4.961	0	1949486	N.D.	0.588 #
14)	MA Endrin	0.000	6.647f	0	56143142	N.D.	23.509 #
15)	B Endosulfa...	0.000	6.827	0	788968	N.D.	0.329 #
16)	A 4,4'-DDD	6.012f	0.000	207.6E6	0	28.296	N.D. #
23)	Chlordane-1	4.114	4.961	9168935	1949486	26.481	16.823 #
27)	Chlordane-5	0.000	6.827	0	788968	N.D.	8.807 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071718\
Data File : PL038174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 16:02
Operator : AJ\SJ
Sample : PB111183BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 04:28:08 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

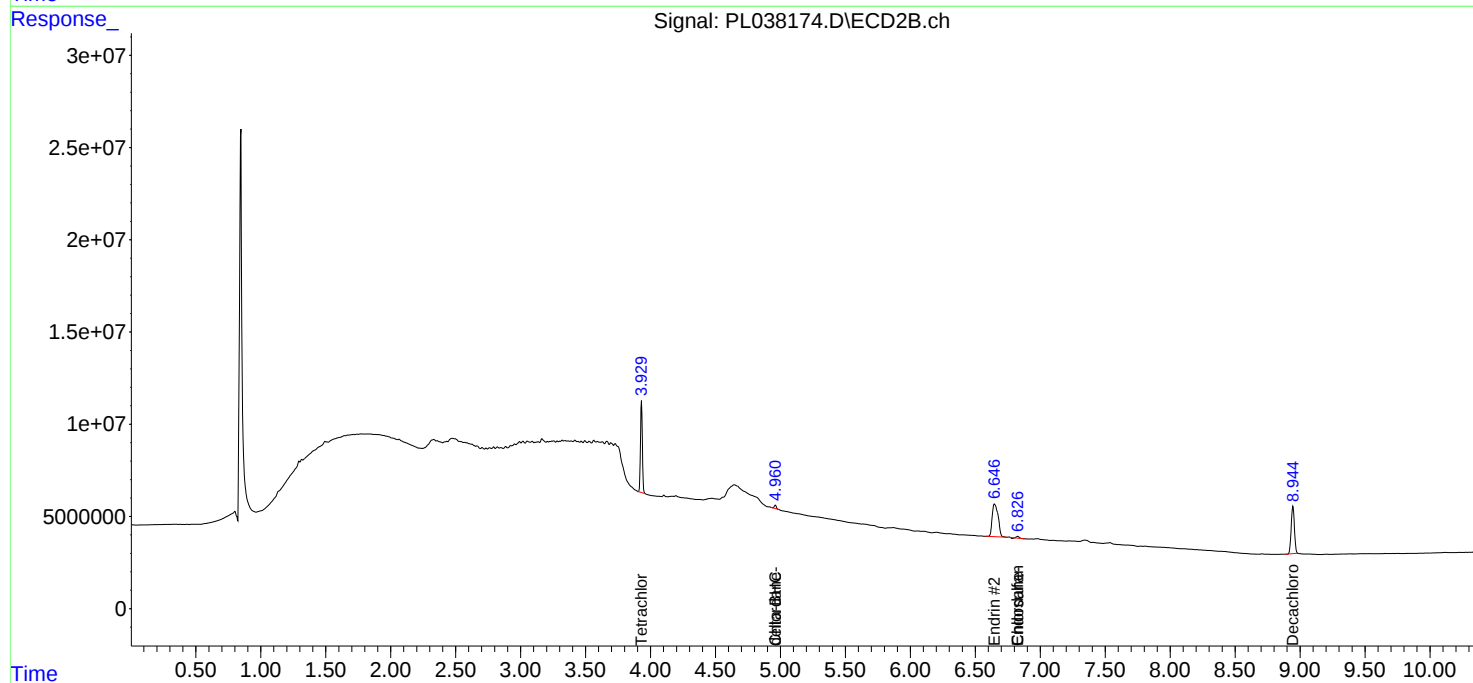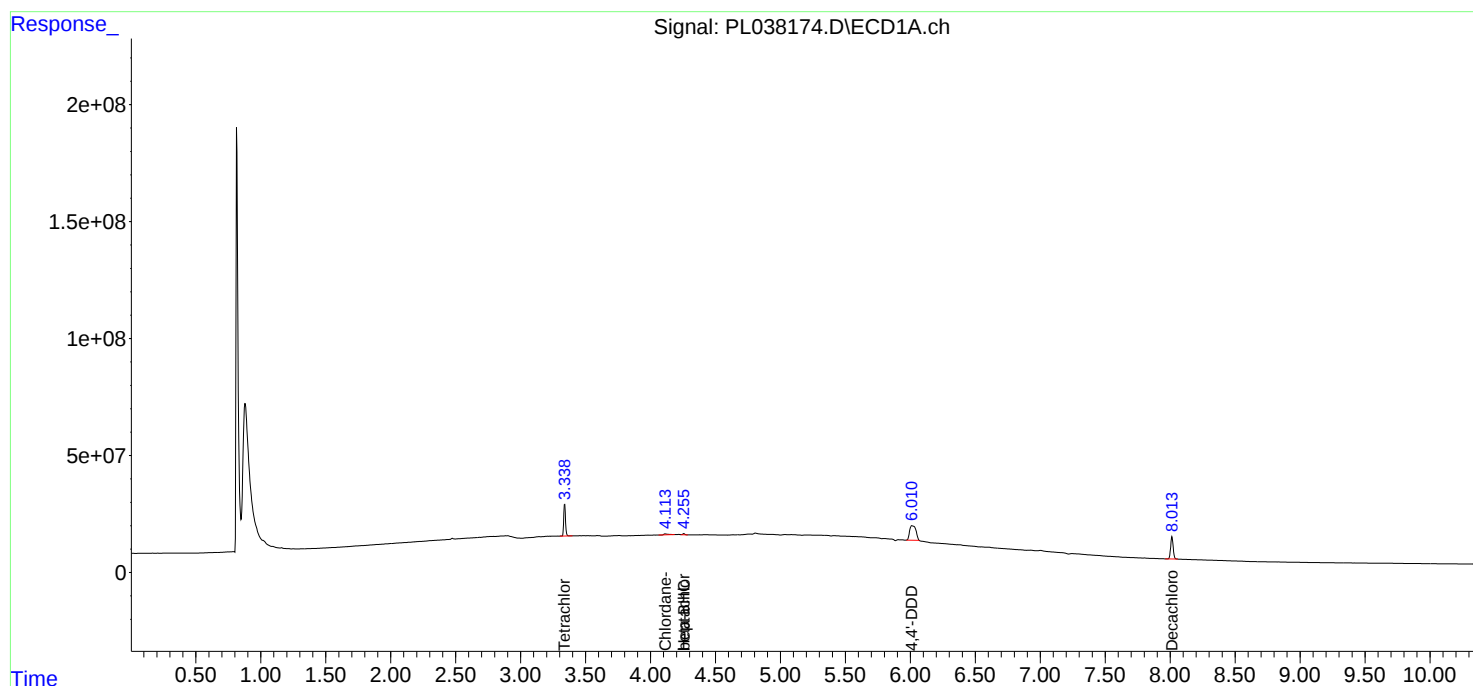


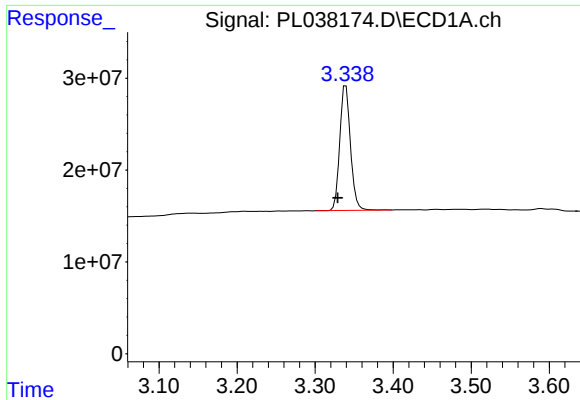

#1 Tetrachloro-m-xylene


R.T.: 3.339 min
Delta R.T.: 0.010 min
Response: 129378891
Conc: 17.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

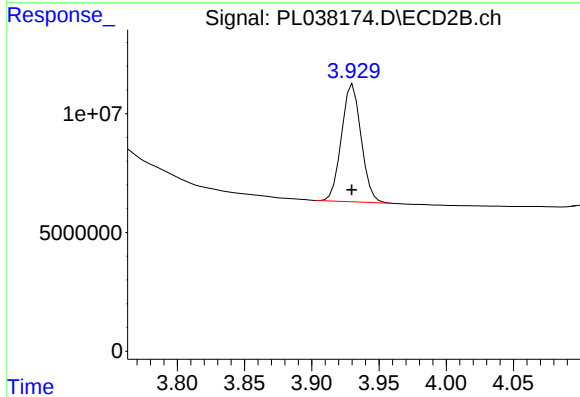


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 50089660
Conc: 19.08 ng/ml

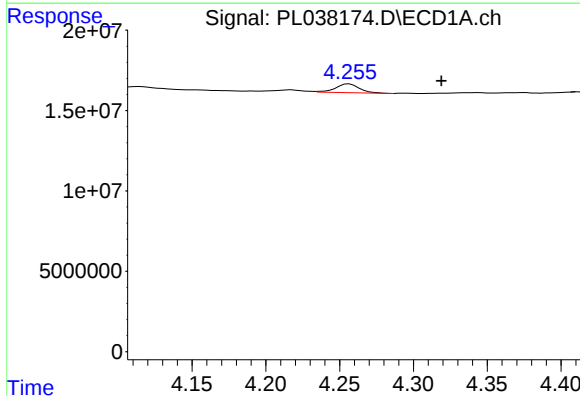


#4 Heptachlor

R.T.: 4.257 min
Delta R.T.: -0.062 min
Response: 6147632
Conc: 0.58 ng/ml

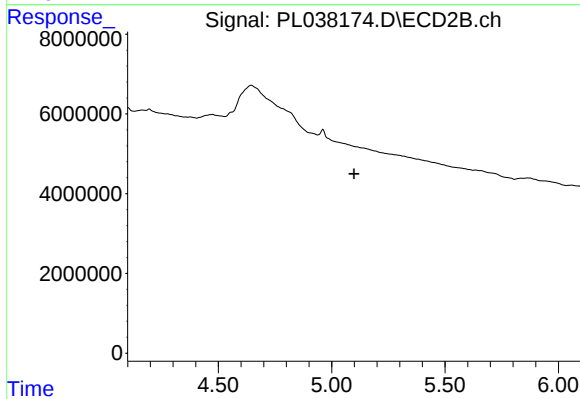

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.099 min
Response: 0
Conc: N.D.

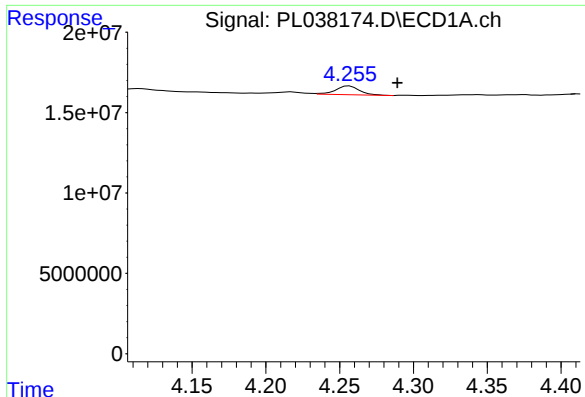

#6 beta-BHC


R.T.: 4.257 min
Delta R.T.: -0.033 min
Response: 6147632
Conc: 1.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

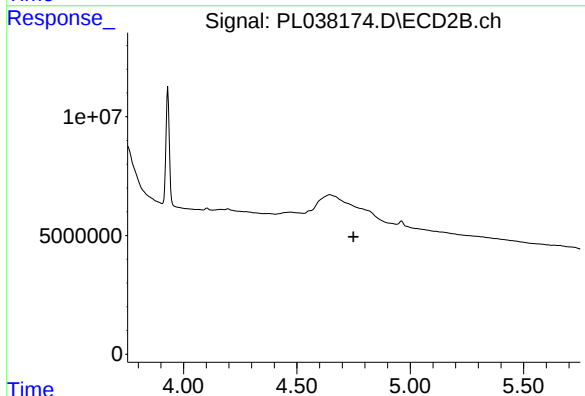


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

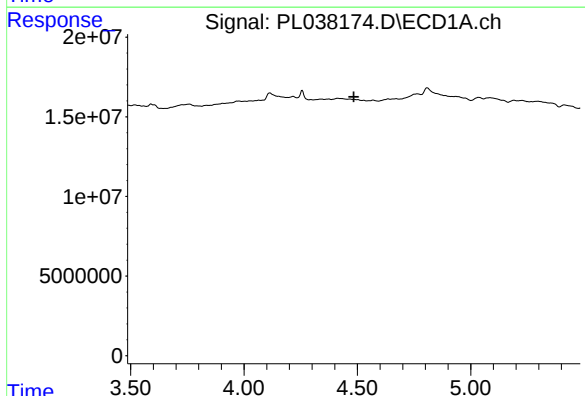


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

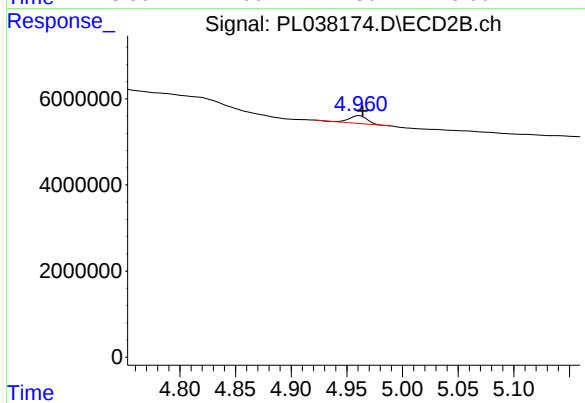

#7 delta-BHC


R.T.: 4.961 min
Delta R.T.: -0.003 min
Response: 1949486
Conc: 0.59 ng/ml

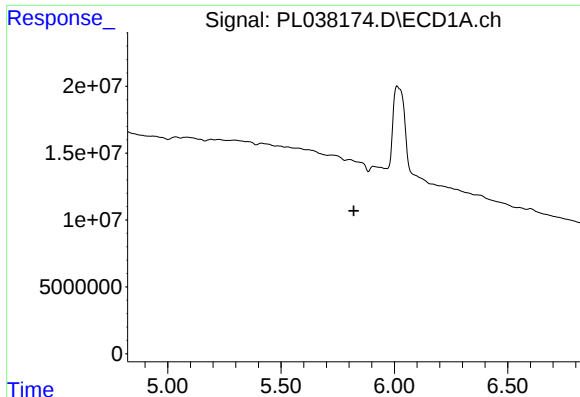

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

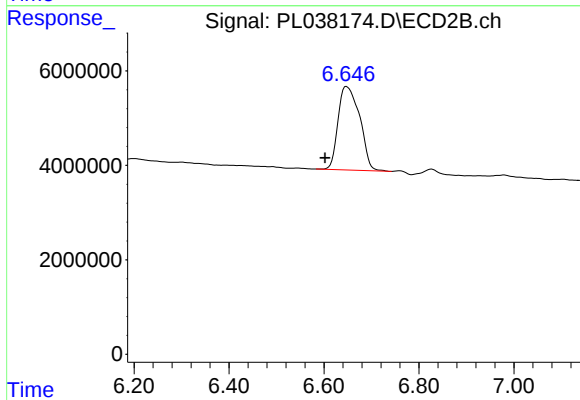


#14 Endrin

R.T.: 6.647 min
Delta R.T.: 0.045 min
Response: 56143142
Conc: 23.51 ng/ml

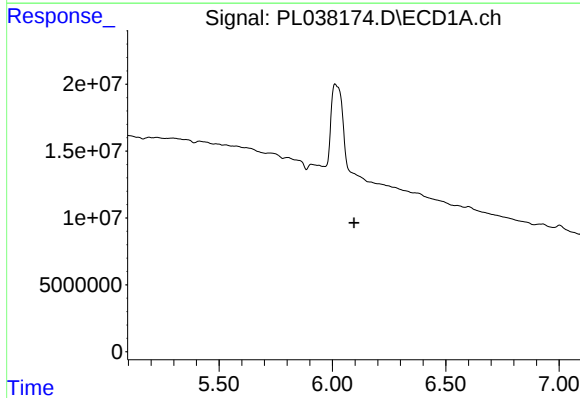


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

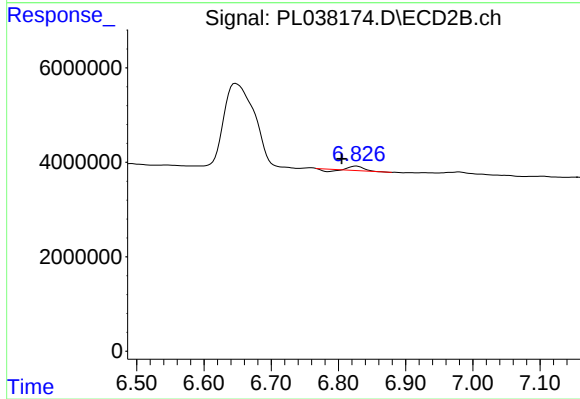

#15 Endosulfan II


R.T.: 6.827 min
Delta R.T.: 0.022 min
Response: 788968
Conc: 0.33 ng/ml

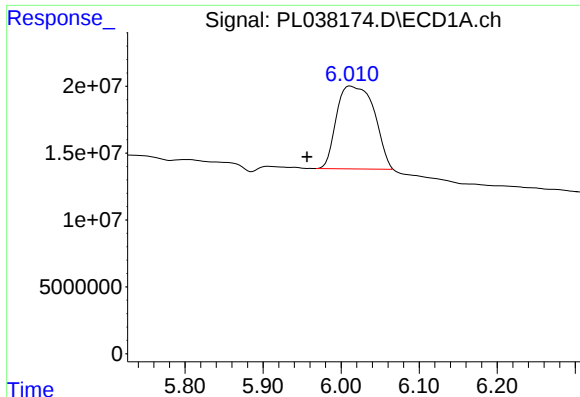

#16 4,4'-DDD


R.T.: 6.012 min
Delta R.T.: 0.056 min
Response: 207569637
Conc: 28.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

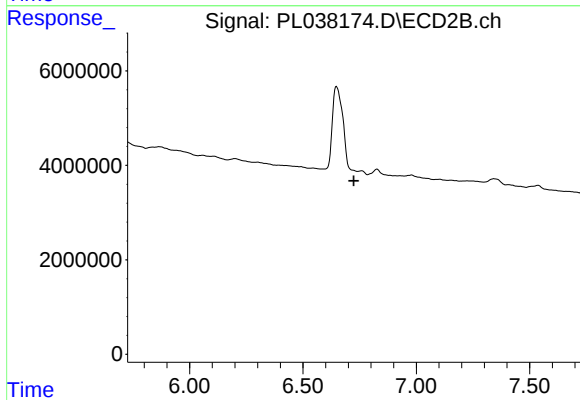


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.725 min
Response: 0
Conc: N.D.

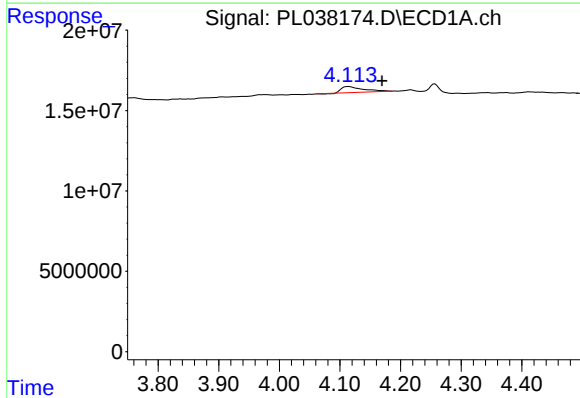


#23 Chlordane-1

R.T.: 4.114 min
Delta R.T.: -0.055 min
Response: 9168935
Conc: 26.48 ng/ml

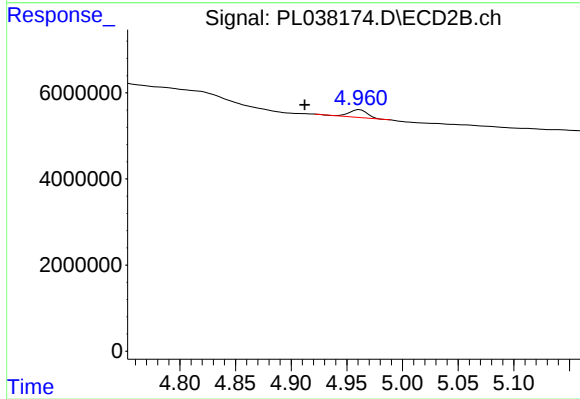

#23 Chlordane-1


R.T.: 4.961 min
Delta R.T.: 0.049 min
Response: 1949486
Conc: 16.82 ng/ml

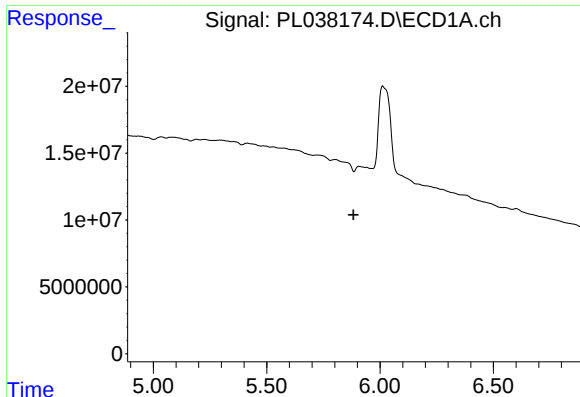

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

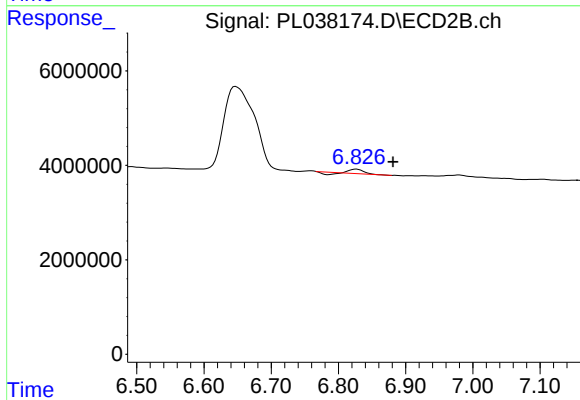


#27 Chlordane-5

R.T.: 6.827 min
Delta R.T.: -0.055 min
Response: 788968
Conc: 8.81 ng/ml

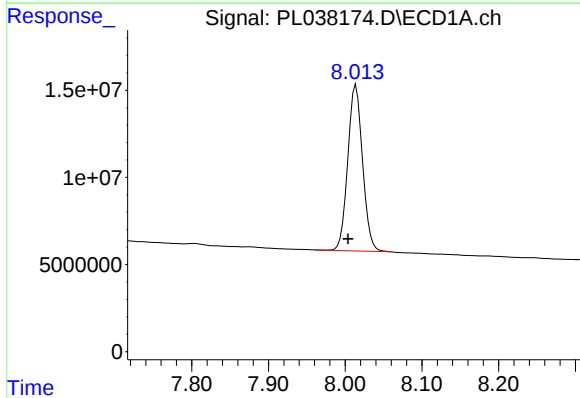

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: 0.010 min
Response: 128307142
Conc: 16.91 ng/ml

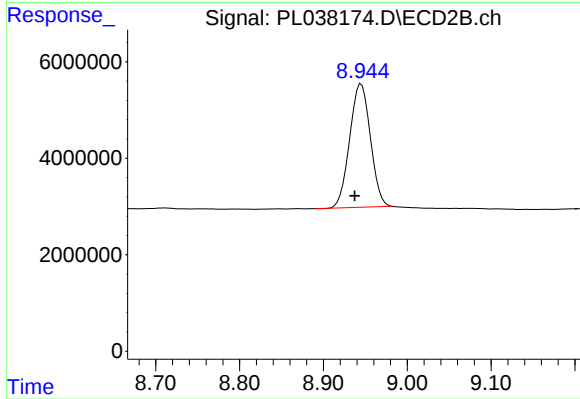

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: 0.008 min
Response: 43938457
Conc: 17.97 ng/ml