

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071718\
 Data File : PL038181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 17:41
 Operator : AJ\SJ
 Sample : J4013-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 04:29:08 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.931	65160136	26871017	8.751	10.237
28)	SA Decachlor...	8.002	8.940	72790985	26065008	9.596	10.663
Target Compounds							
2)	A alpha-BHC	3.721f	0.000	12214144	0	1.034	N.D. #
6)	B beta-BHC	4.244f	0.000	15485286	0	3.281	N.D. #
7)	B delta-BHC	0.000	4.962	0	4158124	N.D.	1.254 #
15)	B Endosulfa...	6.036f	0.000	28992925	0	3.656	N.D. #
16)	A 4,4'-DDD	0.000	6.679f	0	10187856	N.D.	4.760 #
23)	Chlordane-1	4.101	4.962	36809067	4158124	106.308	35.881 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071718\
Data File : PL038181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 17:41
Operator : AJ\SJ
Sample : J4013-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 04:29:08 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

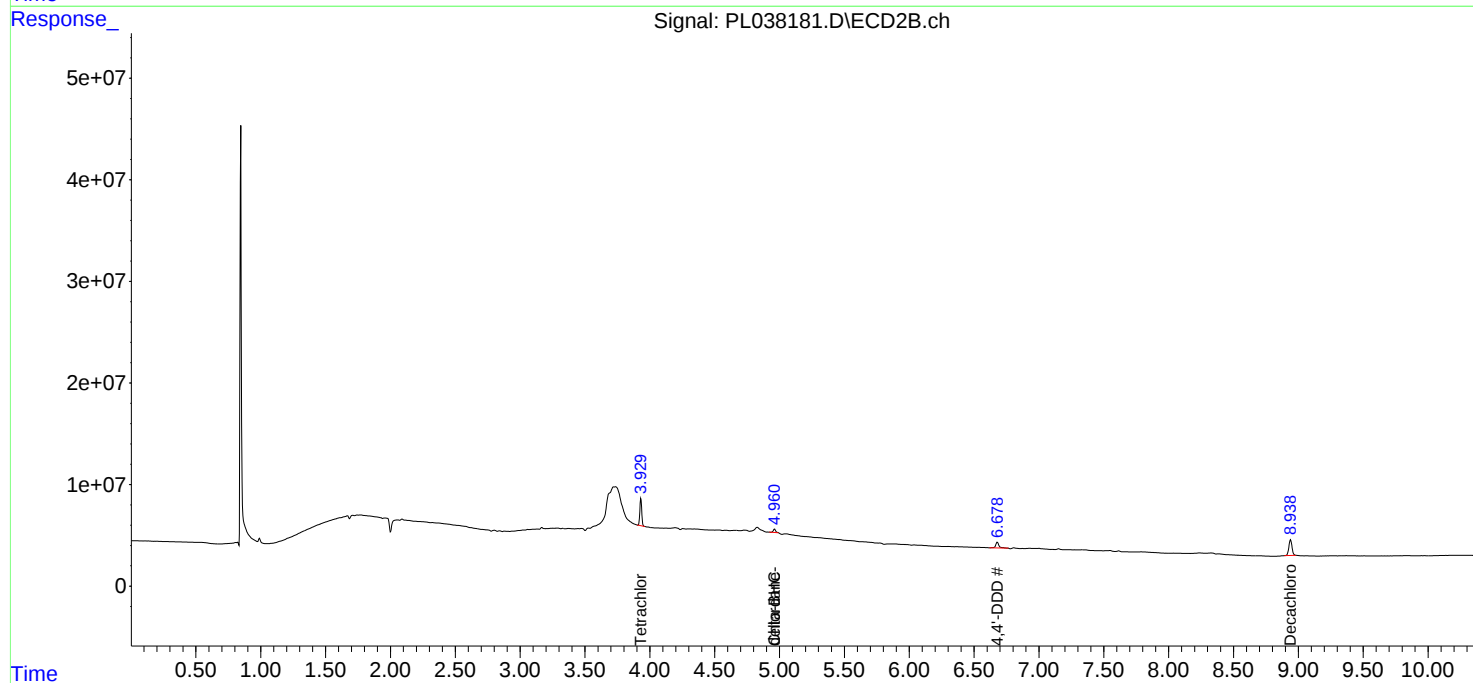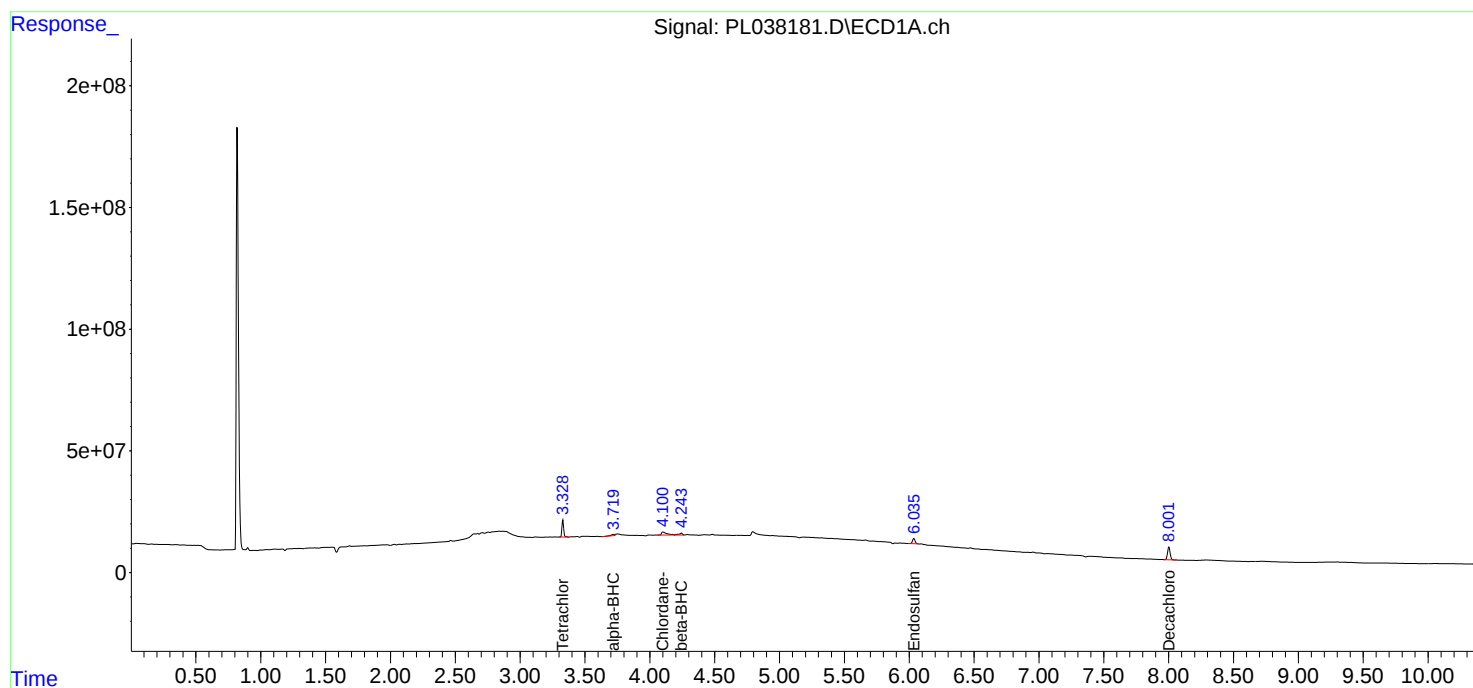


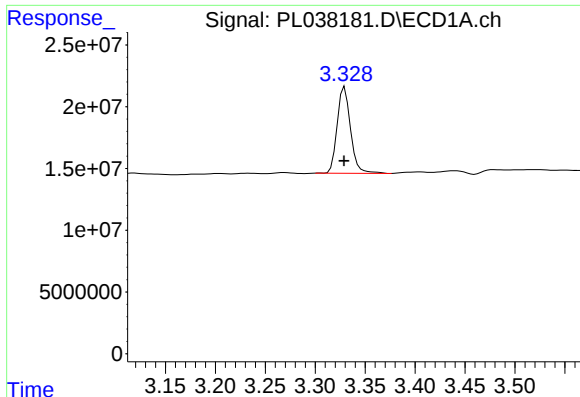

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 65160136
Conc: 8.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

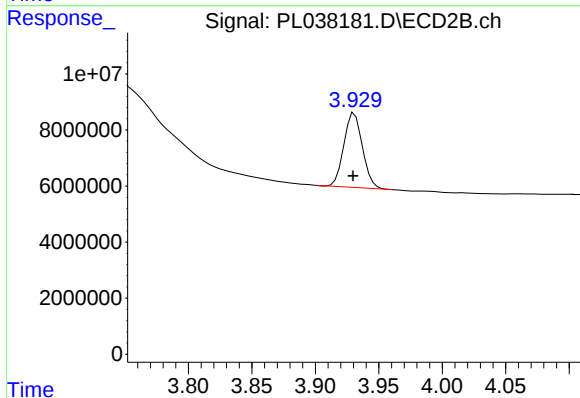


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.001 min
Response: 26871017
Conc: 10.24 ng/ml

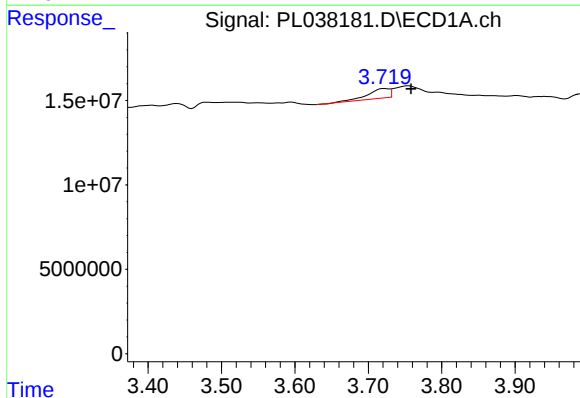


#2 alpha-BHC

R.T.: 3.721 min
Delta R.T.: -0.037 min
Response: 12214144
Conc: 1.03 ng/ml

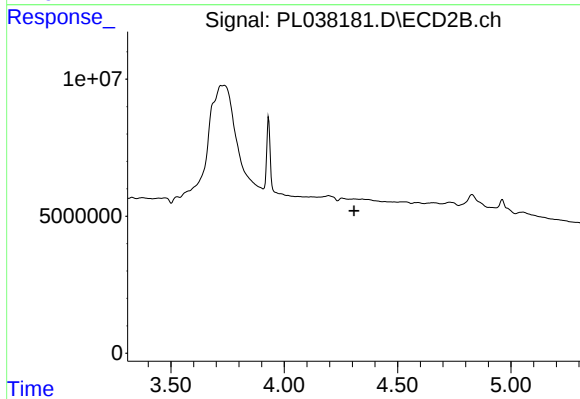

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.309 min
Response: 0
Conc: N.D.

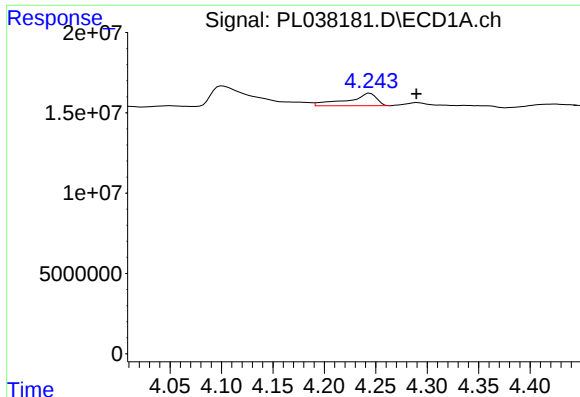

#6 beta-BHC


R.T.: 4.244 min
Delta R.T.: -0.045 min
Response: 15485286
Conc: 3.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

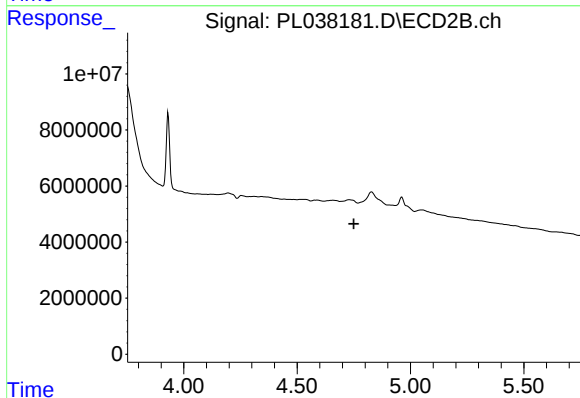


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

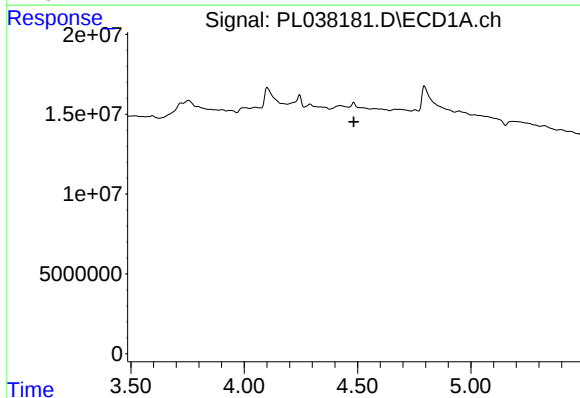


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

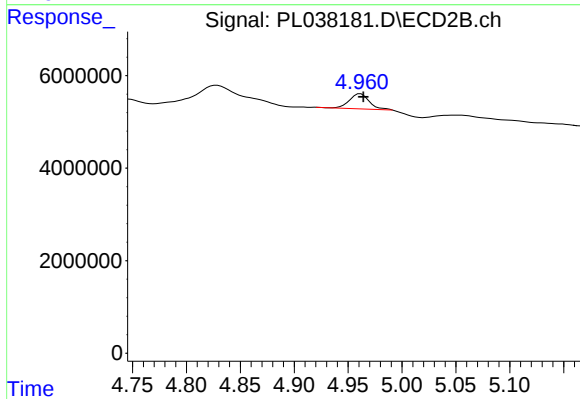

#7 delta-BHC


R.T.: 4.962 min
Delta R.T.: -0.003 min
Response: 4158124
Conc: 1.25 ng/ml

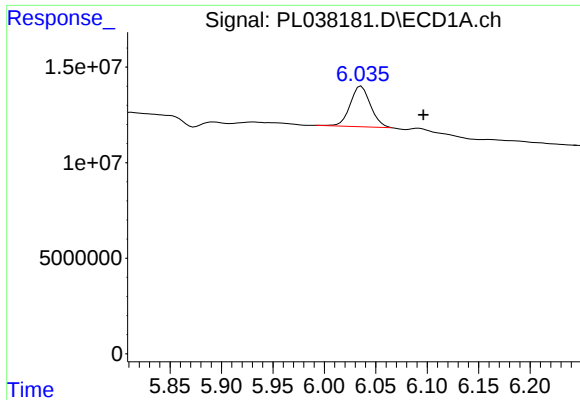

#15 Endosulfan II


R.T.: 6.036 min
Delta R.T.: -0.060 min
Response: 28992925
Conc: 3.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

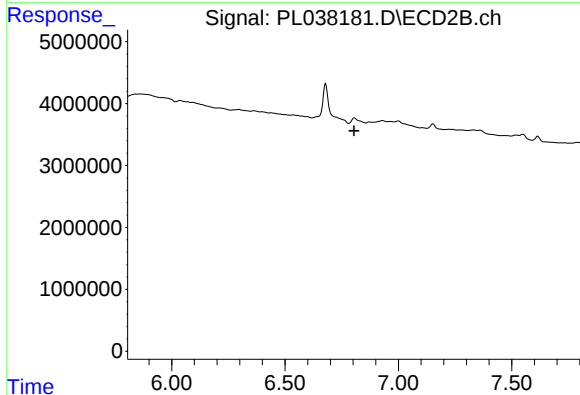


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

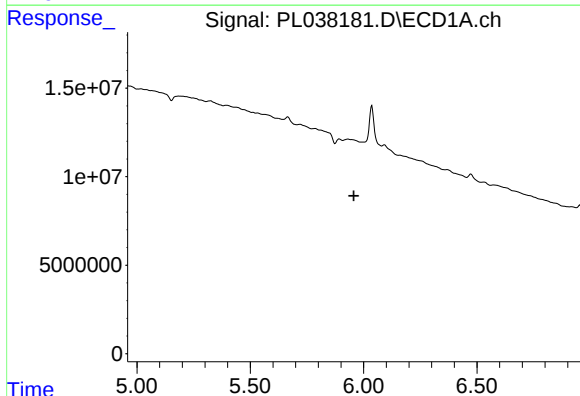


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

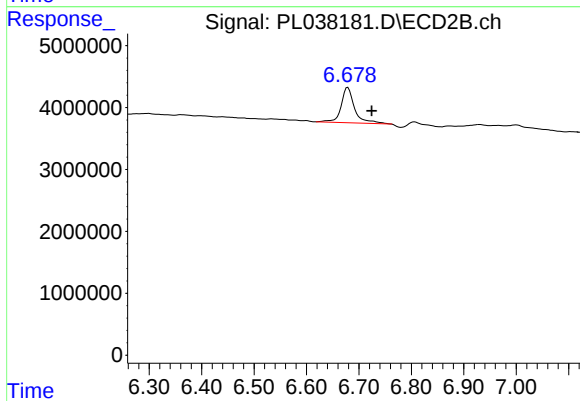

#16 4,4'-DDD


R.T.: 6.679 min
Delta R.T.: -0.046 min
Response: 10187856
Conc: 4.76 ng/ml

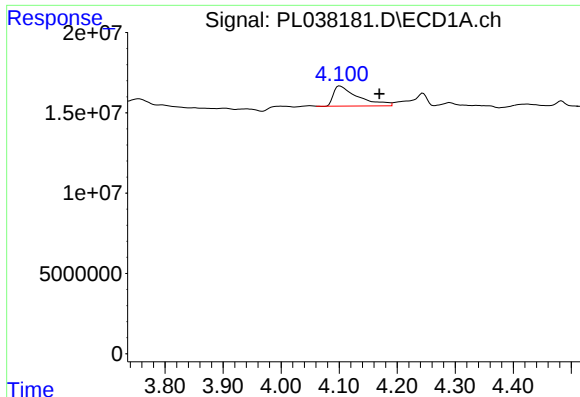

#23 Chlordane-1


R.T.: 4.101 min
Delta R.T.: -0.068 min
Response: 36809067
Conc: 106.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

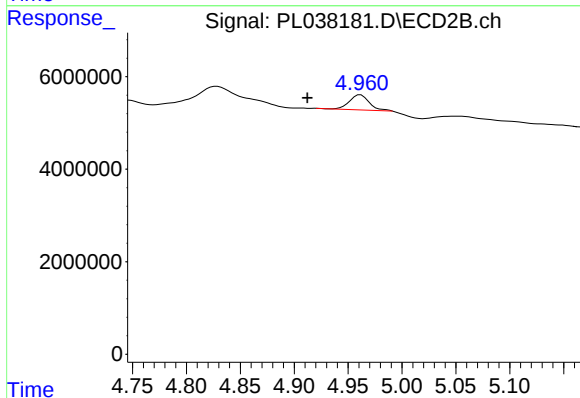


#23 Chlordane-1

R.T.: 4.962 min
Delta R.T.: 0.049 min
Response: 4158124
Conc: 35.88 ng/ml

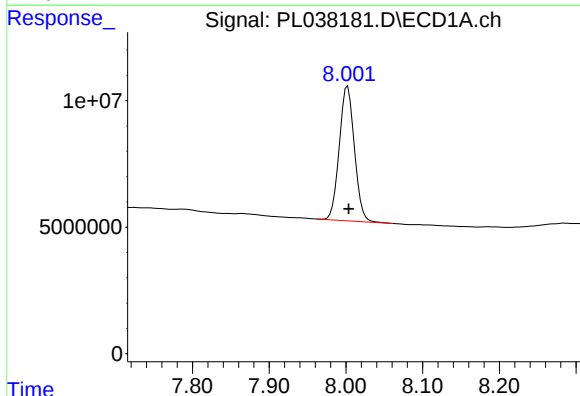

#28 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: -0.001 min
Response: 72790985
Conc: 9.60 ng/ml

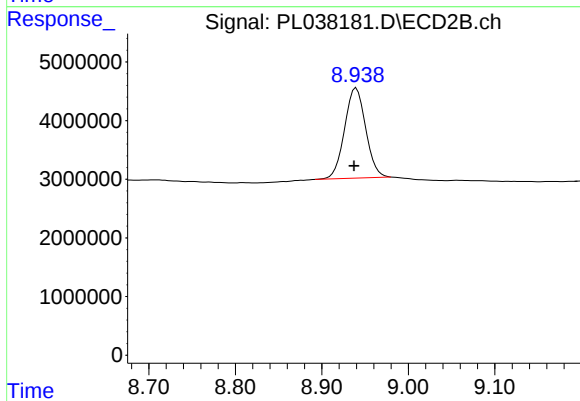

#28 Decachlorobiphenyl

R.T.: 8.940 min
Delta R.T.: 0.002 min
Response: 26065008
Conc: 10.66 ng/ml