

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071718\
 Data File : PL038185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2018 18:38
 Operator : AJ\SJ
 Sample : J4011-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 04:29:40 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.931	80586341	31746571	10.822	12.094
28)	SA Decachlor...	8.002	8.940	67692475	23928839	8.923	9.789
Target Compounds							
6)	B beta-BHC	4.245f	0.000	13528400	0	2.866	N.D. #
7)	B delta-BHC	0.000	4.961	0	3413091	N.D.	1.029 #
12)	B 4,4'-DDE	5.442	6.242	8916665	2002424	0.930	0.749
15)	B Endosulfa...	6.035f	0.000	28935884	0	3.649	N.D. #
16)	A 4,4'-DDD	0.000	6.679f	0	7530091	N.D.	3.518 #
23)	Chlordane-1	4.112	4.961	19200757	3413091	55.453	29.452 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071718\
Data File : PL038185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2018 18:38
Operator : AJ\SJ
Sample : J4011-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 04:29:40 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

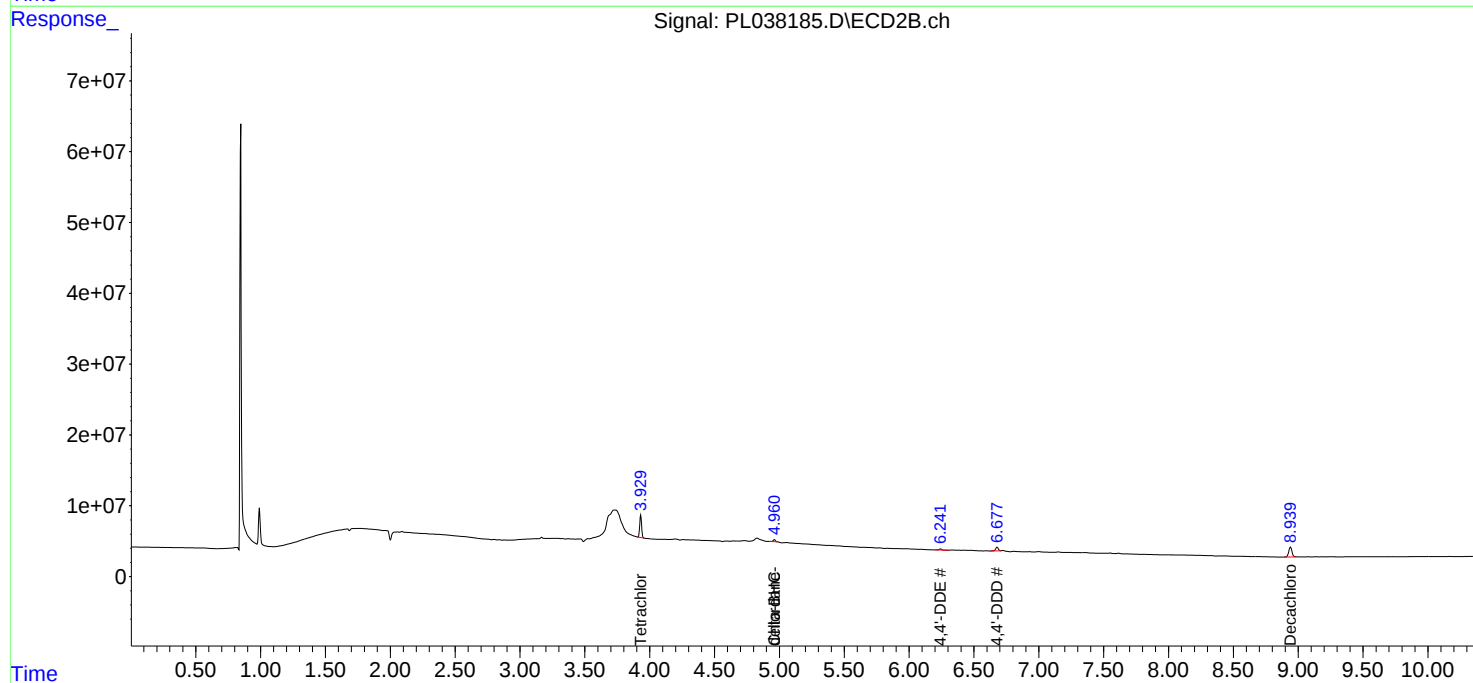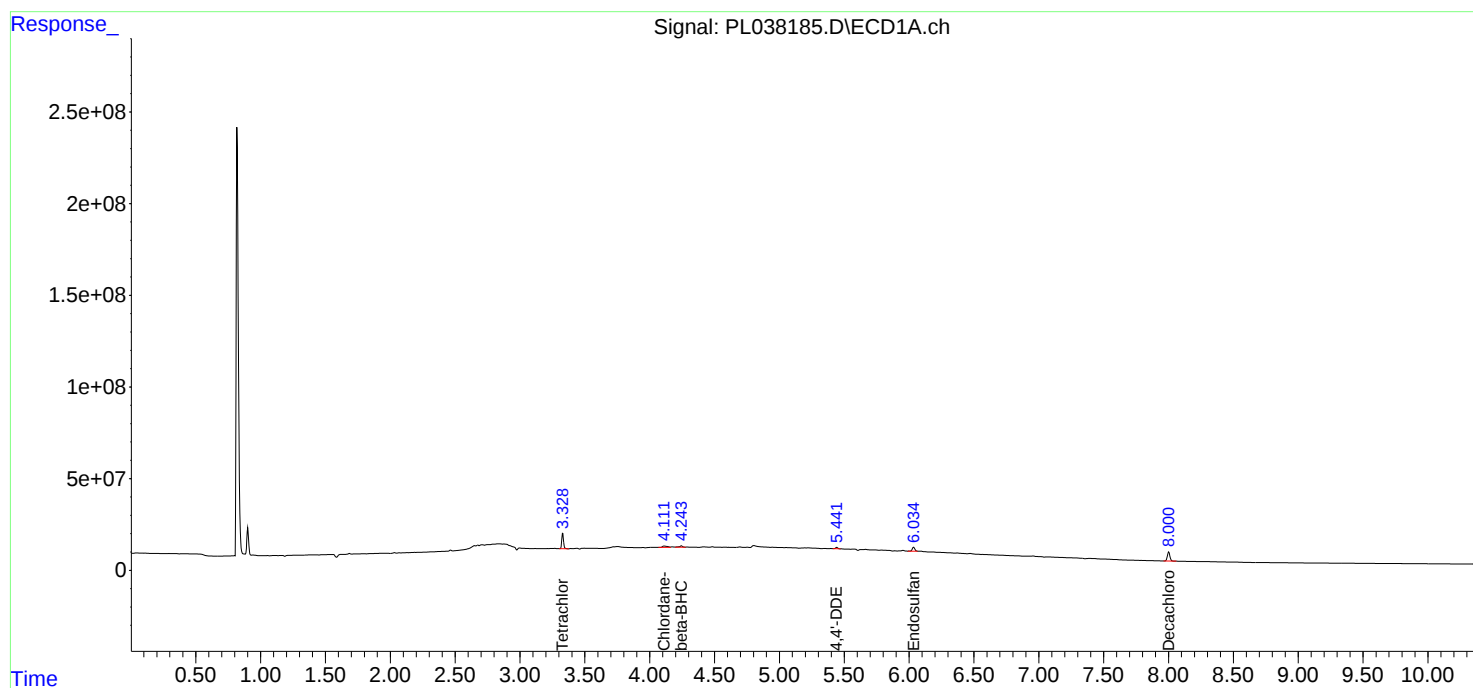


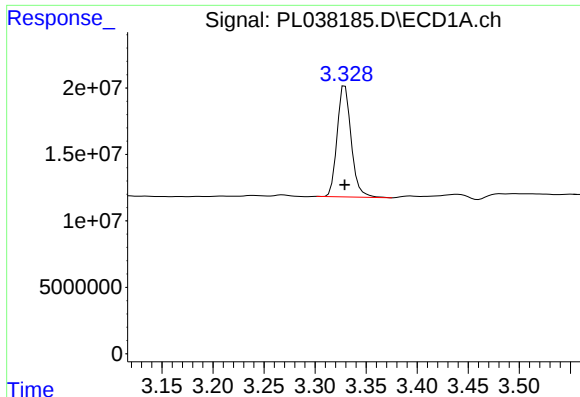

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 80586341
Conc: 10.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

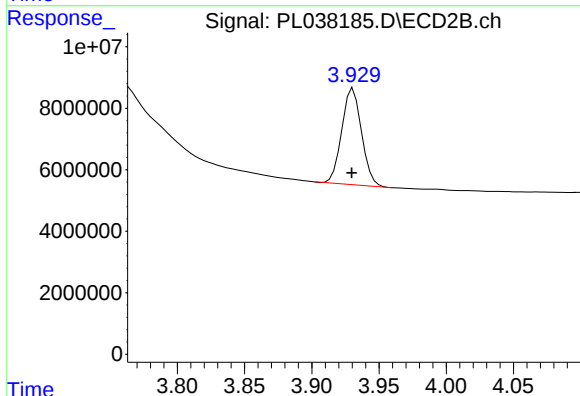


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.001 min
Response: 31746571
Conc: 12.09 ng/ml

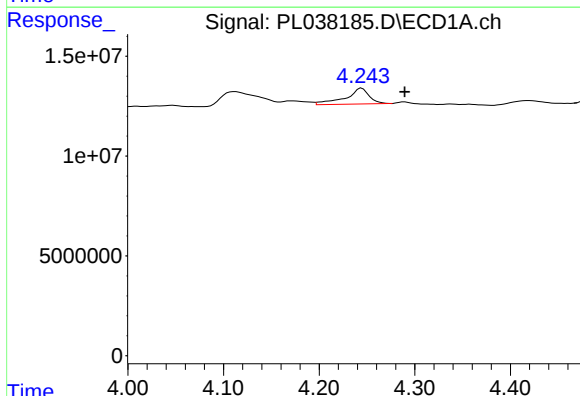


#6 beta-BHC

R.T.: 4.245 min
Delta R.T.: -0.045 min
Response: 13528400
Conc: 2.87 ng/ml

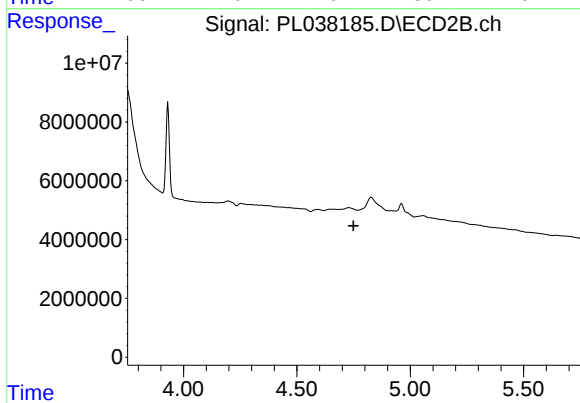

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

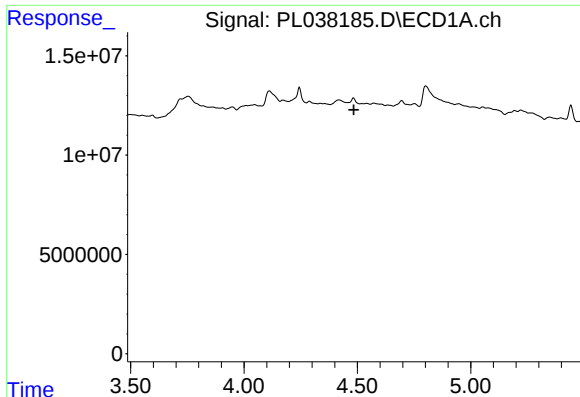

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

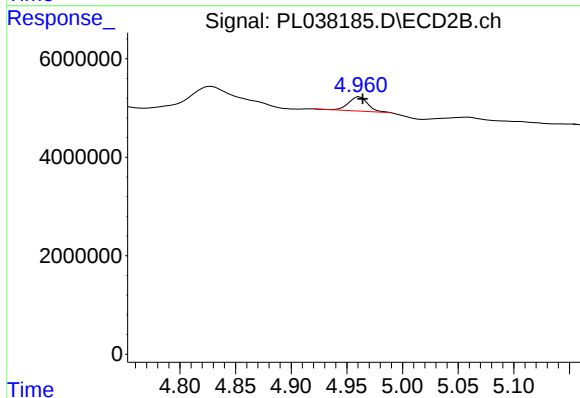


#7 delta-BHC

R.T.: 4.961 min
Delta R.T.: -0.003 min
Response: 3413091
Conc: 1.03 ng/ml

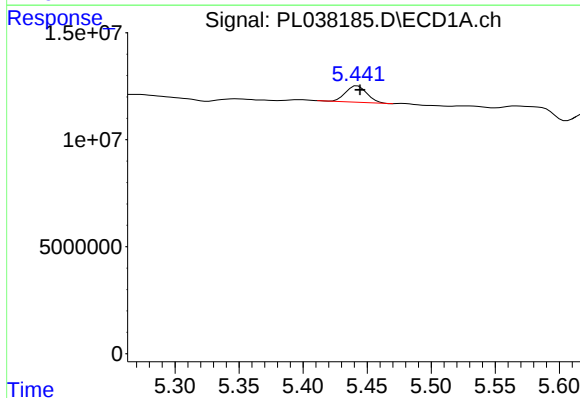


#12 4,4'-DDE

R.T.: 5.442 min
Delta R.T.: -0.002 min
Response: 8916665
Conc: 0.93 ng/ml

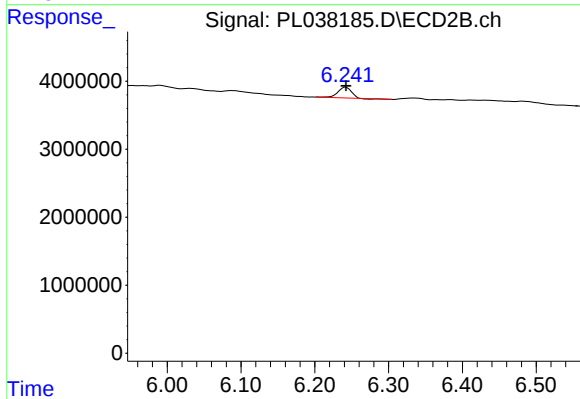

#12 4,4'-DDE


R.T.: 6.242 min
Delta R.T.: 0.000 min
Response: 2002424
Conc: 0.75 ng/ml

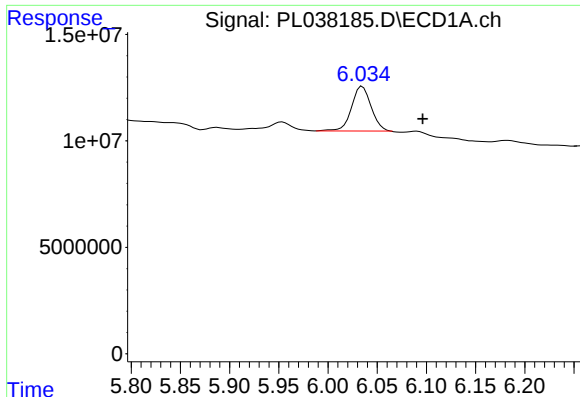

#15 Endosulfan II


R.T.: 6.035 min
Delta R.T.: -0.061 min
Response: 28935884
Conc: 3.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

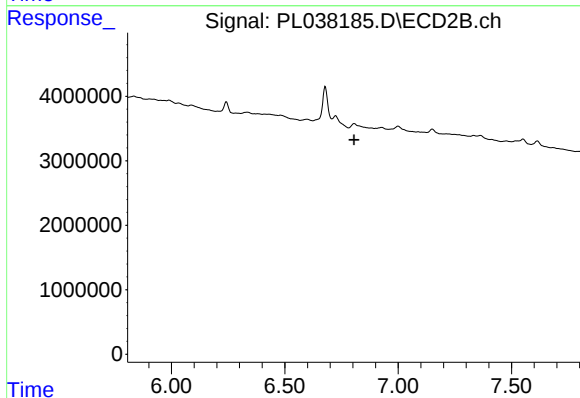


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.805 min
Response: 0
Conc: N.D.

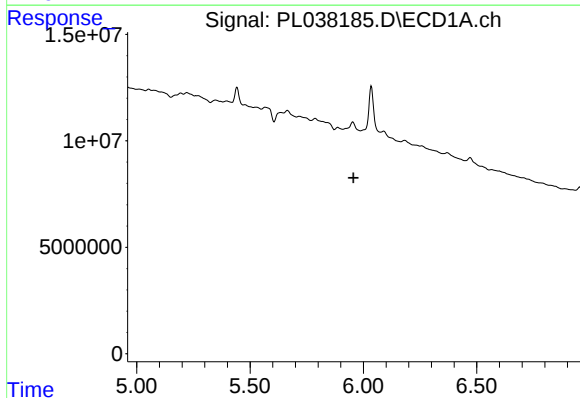


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

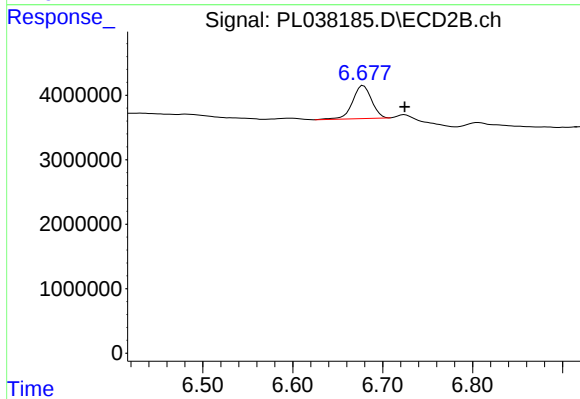

#16 4,4'-DDD


R.T.: 6.679 min
Delta R.T.: -0.046 min
Response: 7530091
Conc: 3.52 ng/ml

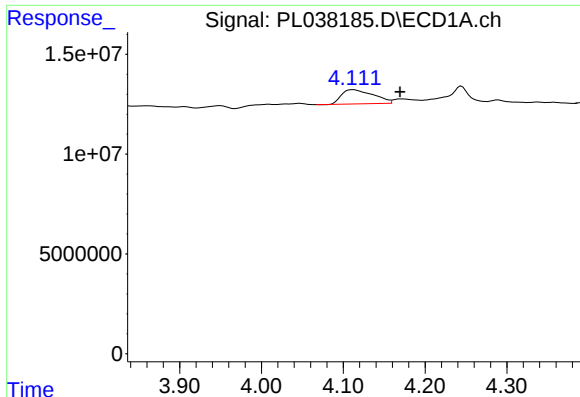

#23 Chlordane-1


R.T.: 4.112 min
Delta R.T.: -0.057 min
Response: 19200757
Conc: 55.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

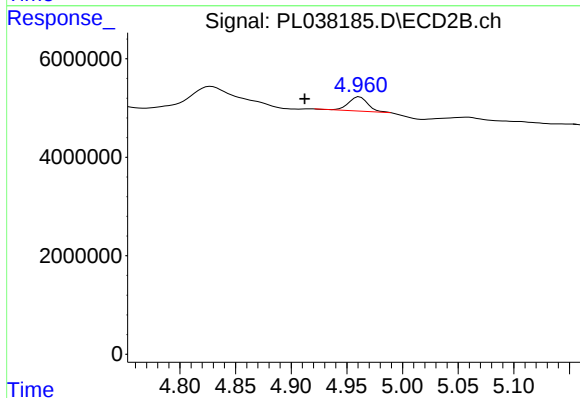


#23 Chlordane-1

R.T.: 4.961 min
Delta R.T.: 0.049 min
Response: 3413091
Conc: 29.45 ng/ml

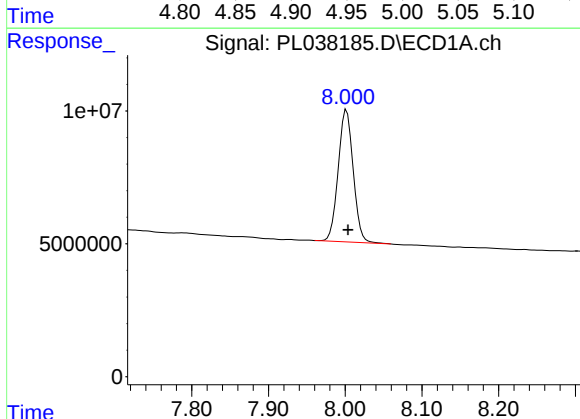

#28 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: -0.002 min
Response: 67692475
Conc: 8.92 ng/ml

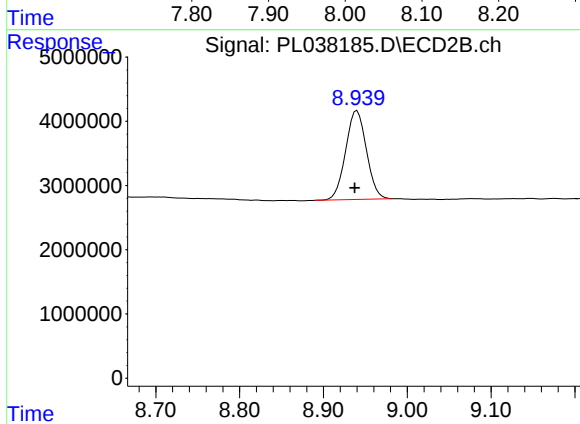

#28 Decachlorobiphenyl

R.T.: 8.940 min
Delta R.T.: 0.003 min
Response: 23928839
Conc: 9.79 ng/ml