

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
 Data File : PL050478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 18:41
 Operator : SM\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:19:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 03:18:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.931	884.7E6	215.7E6	76.752	75.626
28)	SA Decachlor...	7.981	8.963	768.1E6	202.7E6	73.865	72.421
Target Compounds							
23)	Chlordane-1	4.158	4.916	283.0E6	83882069	768.898	760.258
24)	Chlordane-2	4.648	5.383	330.4E6	86046765	751.390	737.990
25)	Chlordane-3	5.202	6.027	1066.8E6	367.4E6	763.538	760.085
26)	Chlordane-4	5.257	6.100	995.6E6	439.0E6	753.562	753.681
27)	Chlordane-5	6.079	6.903	379.3E6	72177863	738.519	755.561


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
Data File : PL050478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 18:41
Operator : SM\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:19:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 03:18:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

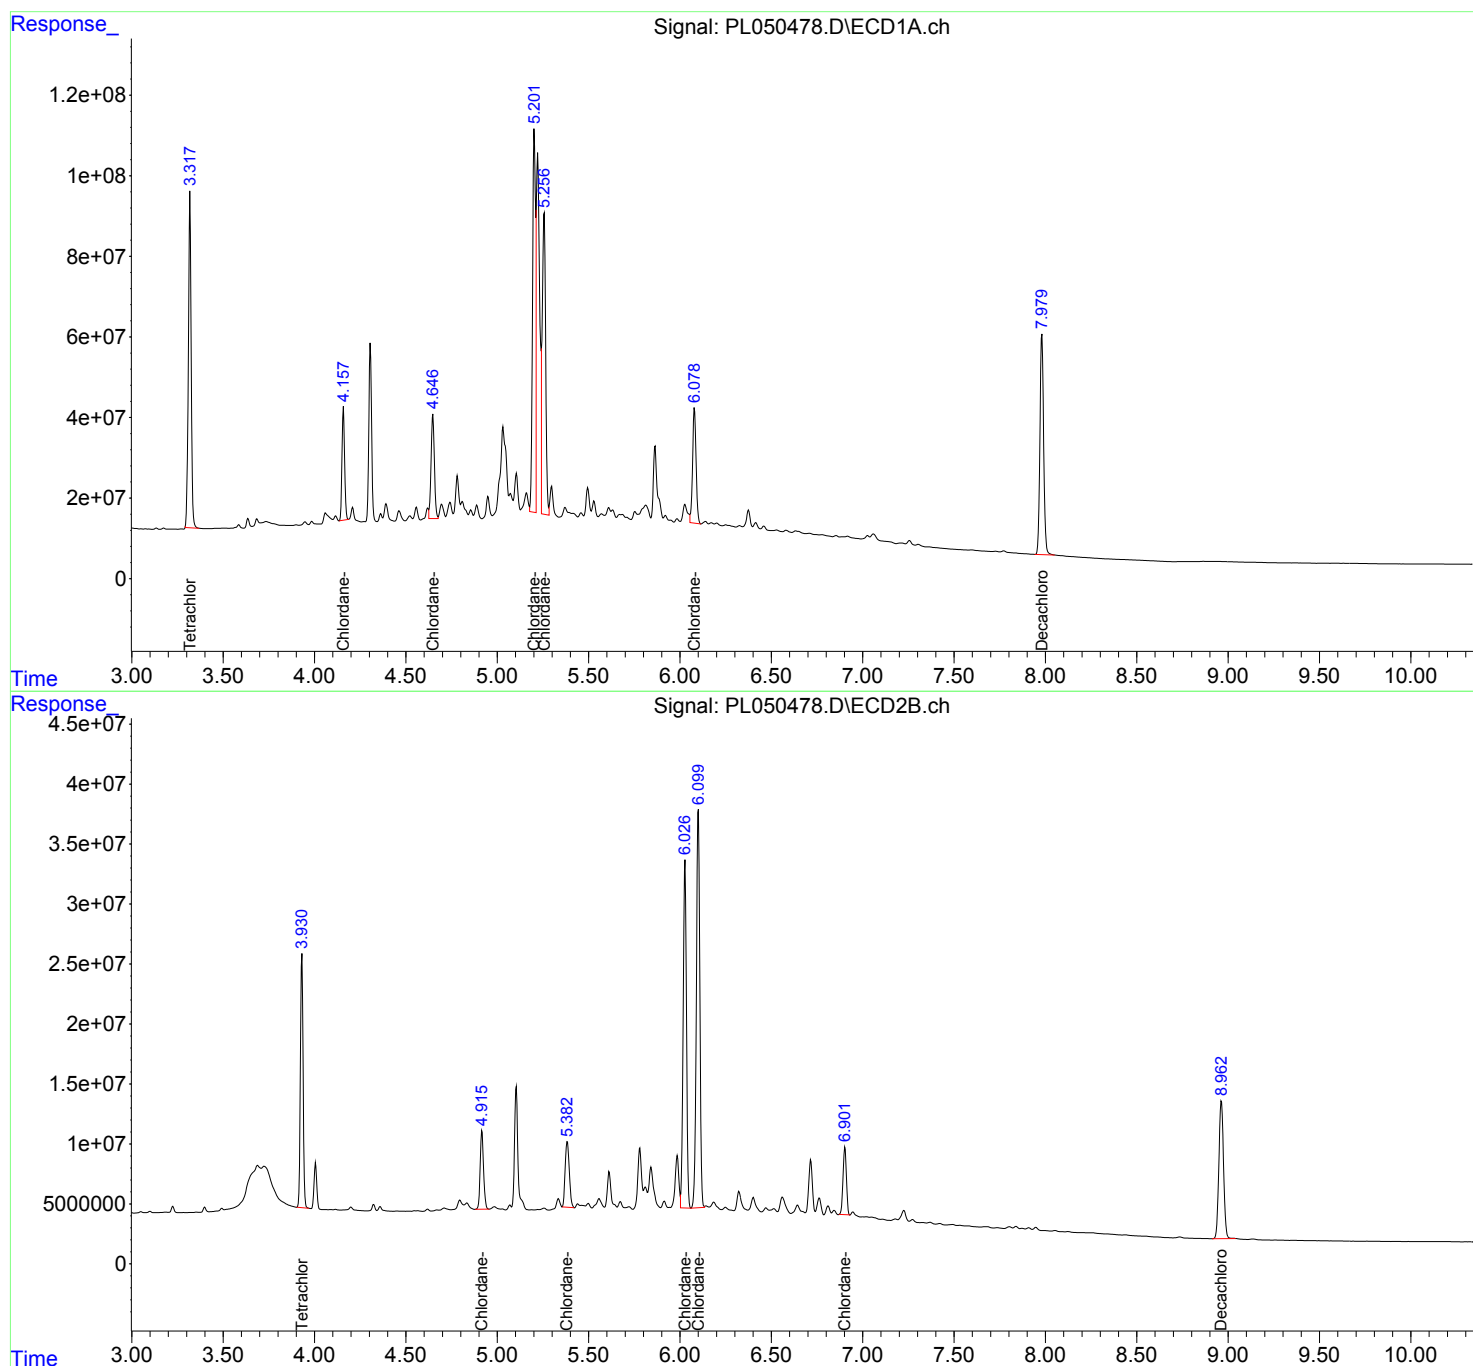


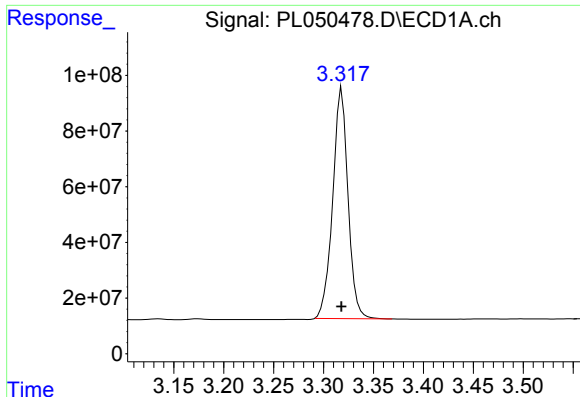

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 884660066
Conc: 76.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

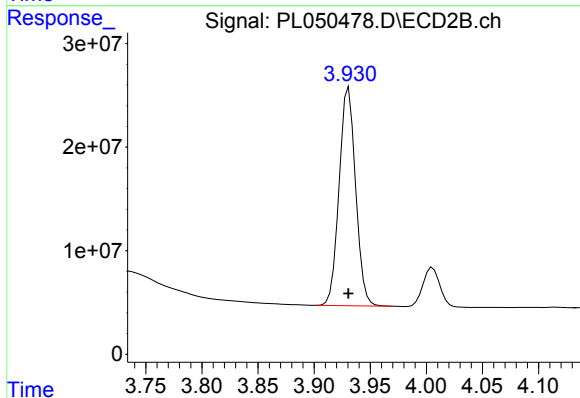


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 215655258
Conc: 75.63 ng/ml

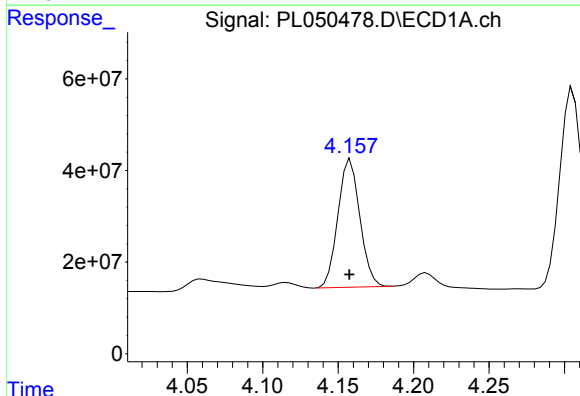


#23 Chlordane-1

R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 282972553
Conc: 768.90 ng/ml

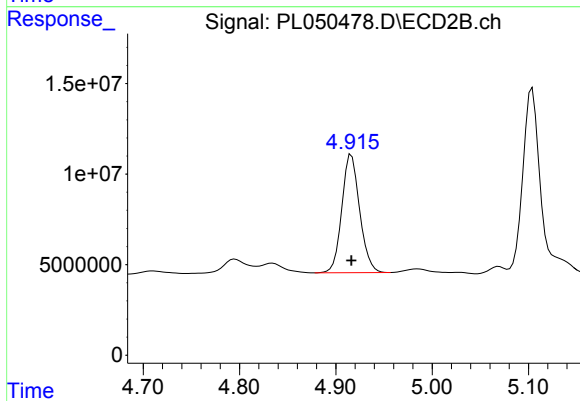

#23 Chlordane-1


R.T.: 4.916 min
Delta R.T.: 0.000 min
Response: 83882069
Conc: 760.26 ng/ml

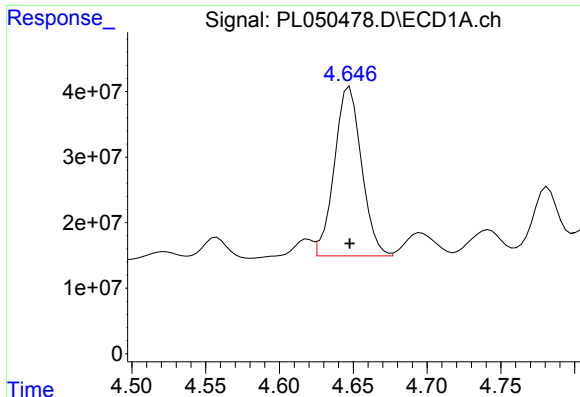

#24 Chlordane-2


R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 330368979
Conc: 751.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

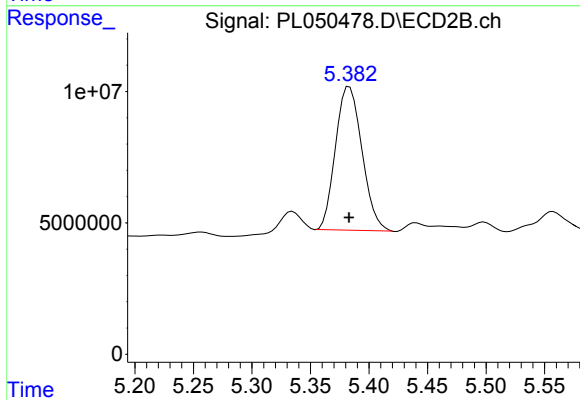


#24 Chlordane-2

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 86046765
Conc: 737.99 ng/ml

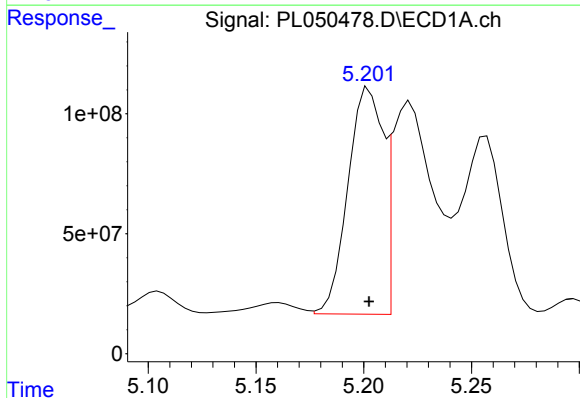


#25 Chlordane-3

R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 1066789776
Conc: 763.54 ng/ml

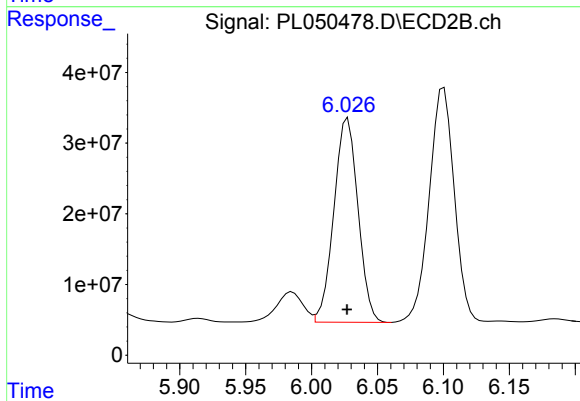

#25 Chlordane-3


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 367449030
Conc: 760.08 ng/ml

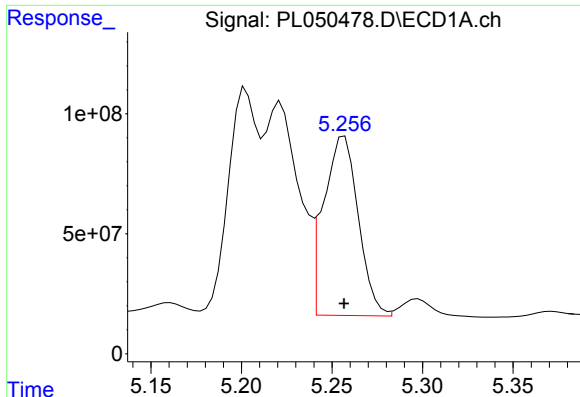

#26 Chlordane-4


R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 995636245
Conc: 753.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

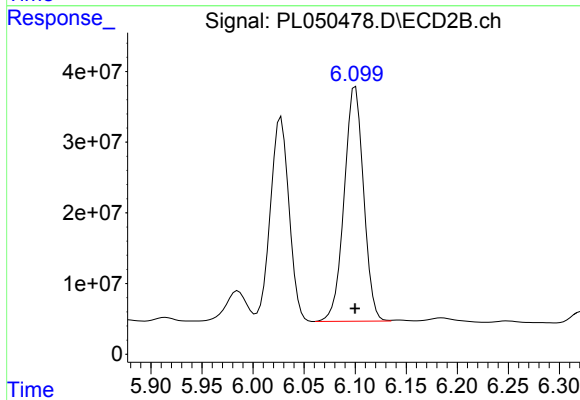


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 438960733
Conc: 753.68 ng/ml

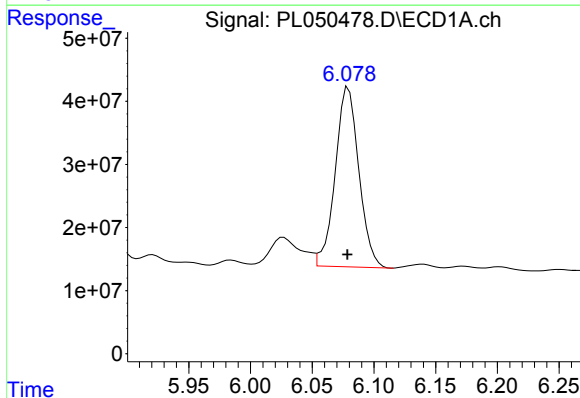


#27 Chlordane-5

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 379260861
Conc: 738.52 ng/ml

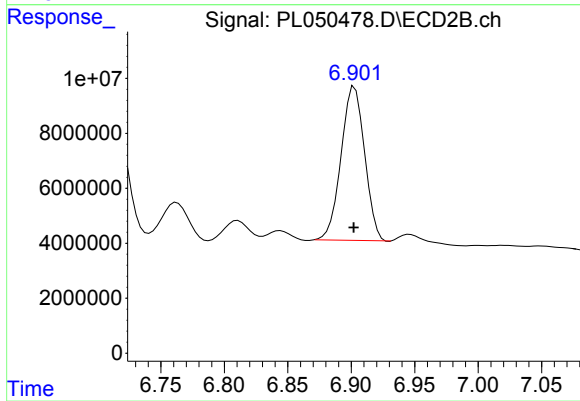

#27 Chlordane-5


R.T.: 6.903 min
Delta R.T.: 0.000 min
Response: 72177863
Conc: 755.56 ng/ml

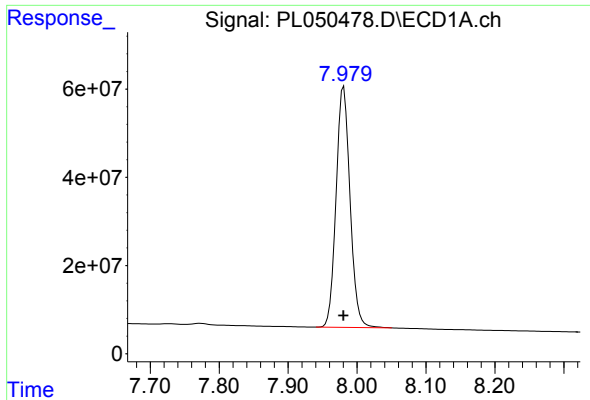

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 768096006
Conc: 73.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

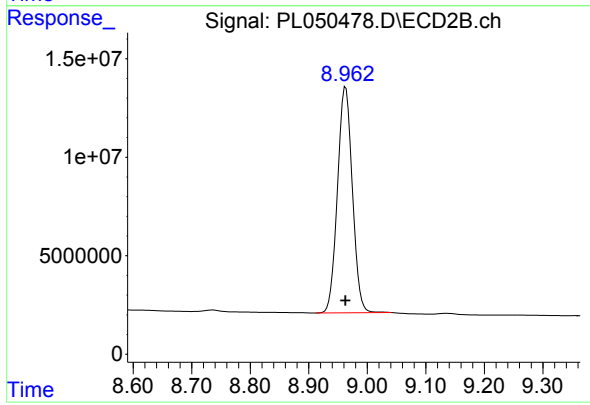

#28 Decachlorobiphenyl

R.T.: 8.963 min
Delta R.T.: 0.000 min
Response: 202714312
Conc: 72.42 ng/ml