

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
 Data File : PL050479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 18:56
 Operator : SM\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:19:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 03:18:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.931	576.3E6	142.6E6	50.000	50.000
28)	SA Decachlor...	7.980	8.963	519.9E6	140.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.157	4.916	184.0E6	55166860	500.000	500.000
24)	Chlordane-2	4.648	5.383	219.8E6	58298087	500.000	500.000
25)	Chlordane-3	5.202	6.027	698.6E6	241.7E6	500.000	500.000
26)	Chlordane-4	5.257	6.100	660.6E6	291.2E6	500.000	500.000
27)	Chlordane-5	6.079	6.902	256.8E6	47764396	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
Data File : PL050479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 18:56
Operator : SM\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:19:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 03:18:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

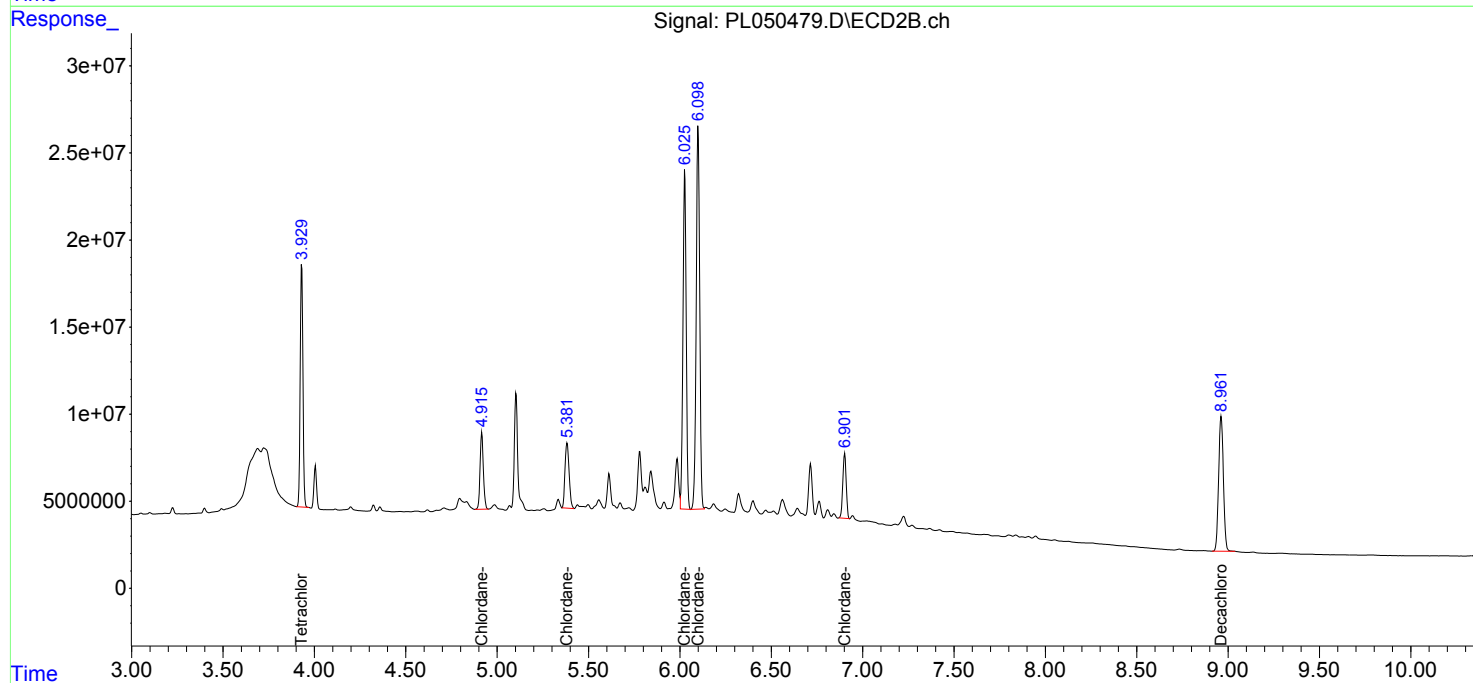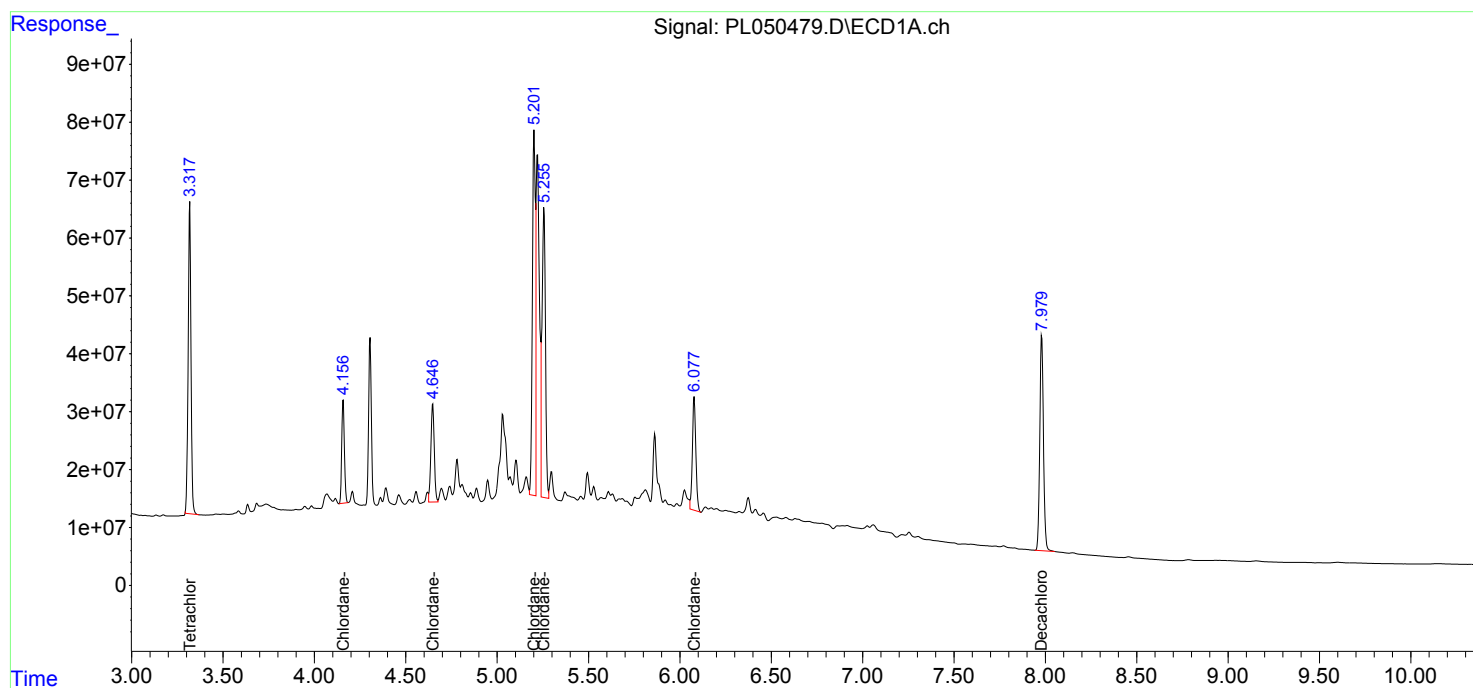


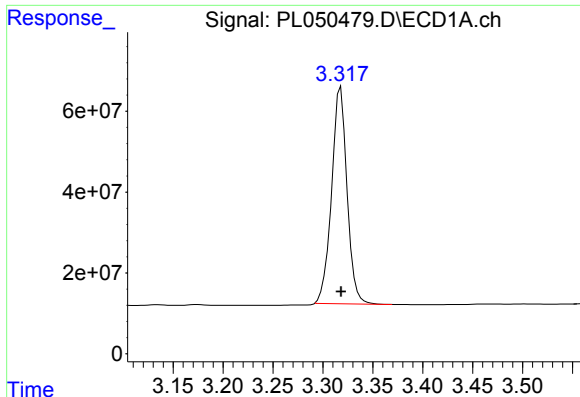

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 576308304
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

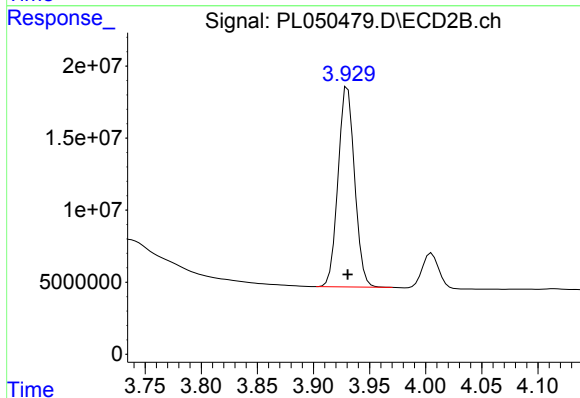


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 142579936
Conc: 50.00 ng/ml

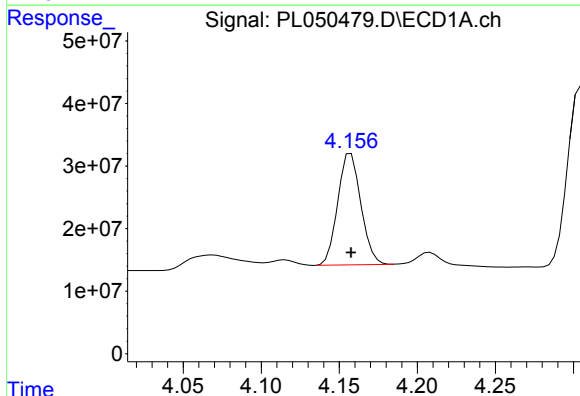


#23 Chlordane-1

R.T.: 4.157 min
Delta R.T.: 0.000 min
Response: 184011762
Conc: 500.00 ng/ml

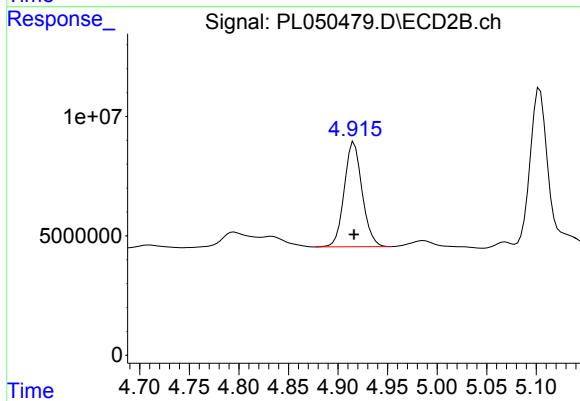

#23 Chlordane-1


R.T.: 4.916 min
Delta R.T.: 0.000 min
Response: 55166860
Conc: 500.00 ng/ml

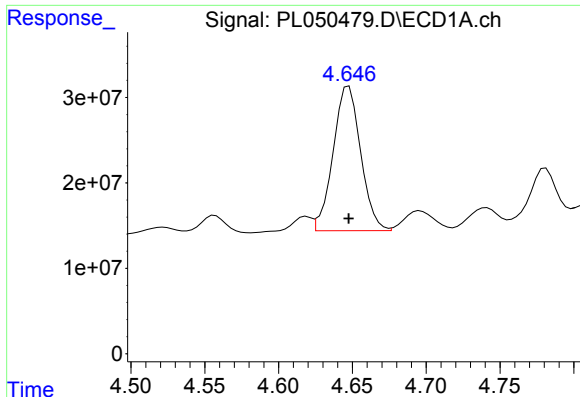

#24 Chlordane-2


R.T.: 4.648 min
Delta R.T.: 0.000 min
Response: 219838652
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

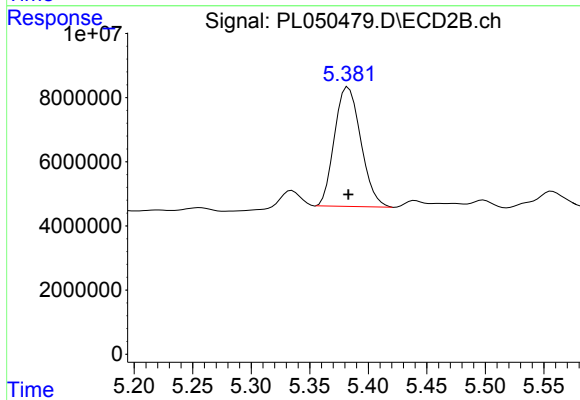


#24 Chlordane-2

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 58298087
Conc: 500.00 ng/ml

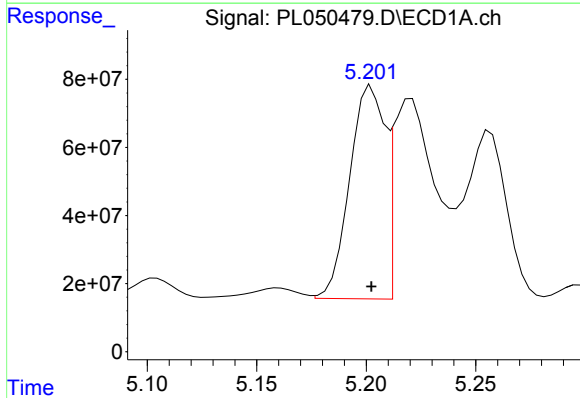


#25 Chlordane-3

R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 698583723
Conc: 500.00 ng/ml

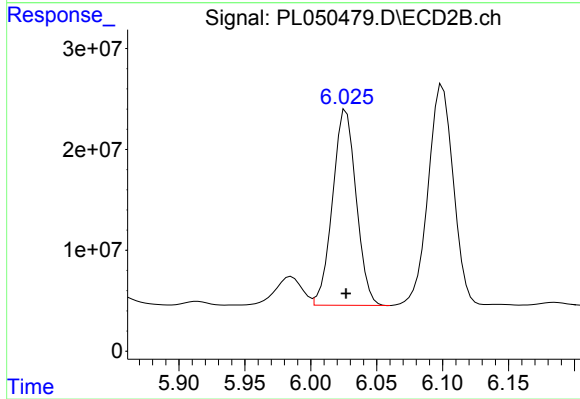

#25 Chlordane-3


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 241715779
Conc: 500.00 ng/ml

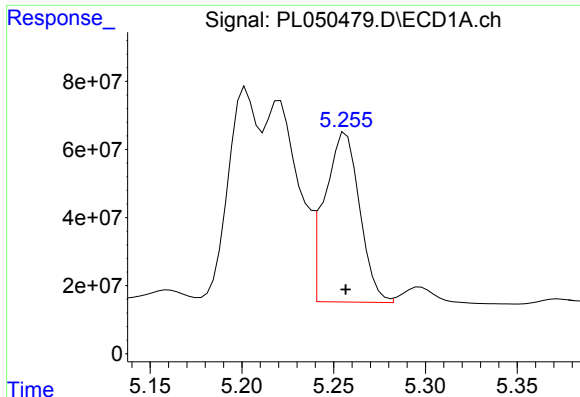

#26 Chlordane-4


R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 660619694
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

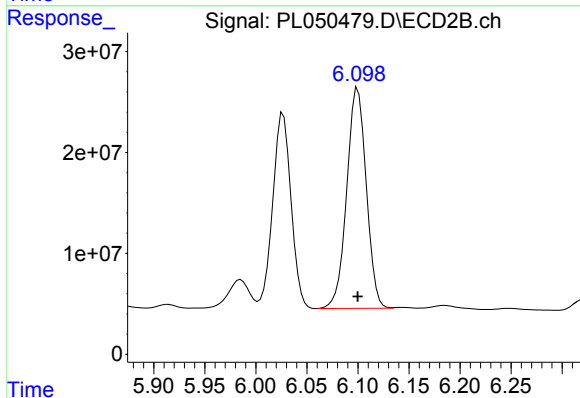


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 291211147
Conc: 500.00 ng/ml

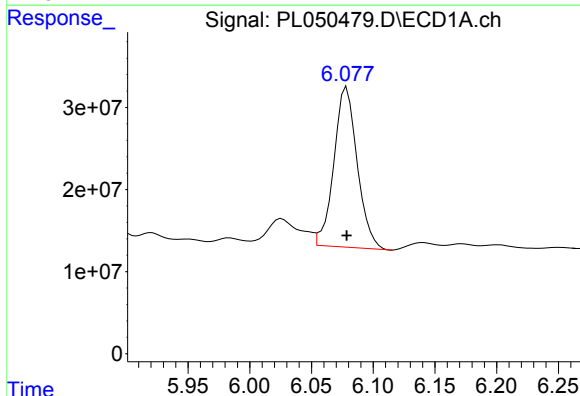


#27 Chlordane-5

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 256771348
Conc: 500.00 ng/ml

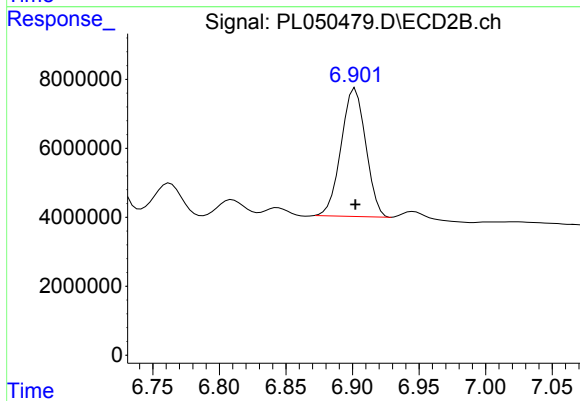

#27 Chlordane-5


R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 47764396
Conc: 500.00 ng/ml

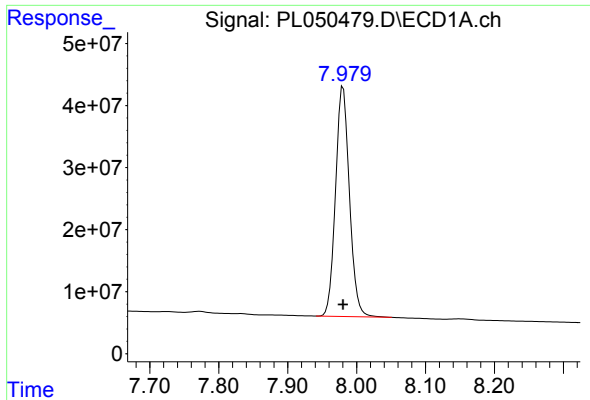

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 519931001
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

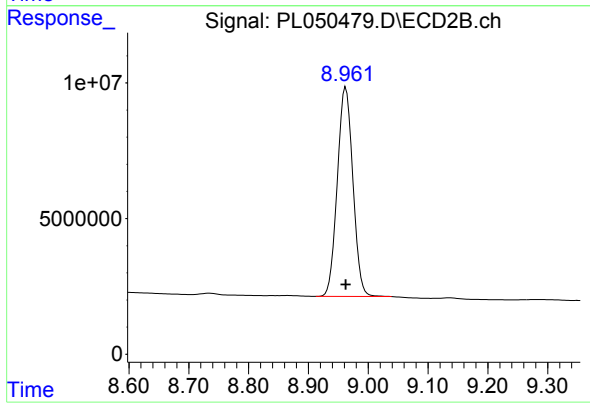

#28 Decachlorobiphenyl

R.T.: 8.963 min
Delta R.T.: 0.000 min
Response: 139955228
Conc: 50.00 ng/ml