

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
 Data File : PL050528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2019 06:50
 Operator : SM\AJ
 Sample : K3852-03
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3_071619

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 07:51:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 04:12:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.930	87725205	22882351	8.731	8.020
28)	SA Decachlor...	7.981	8.962	101.9E6	27577618	10.059	9.752
Target Compounds							
6)	B beta-BHC	0.000	4.799f	0	6566183	N.D.	3.798 #
23)	Chlordane-1	4.166	0.000	6407118	0	17.413	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
Data File : PL050528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2019 06:50
Operator : SM\AJ
Sample : K3852-03
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
COMP-3_071619

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 07:51:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 04:12:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

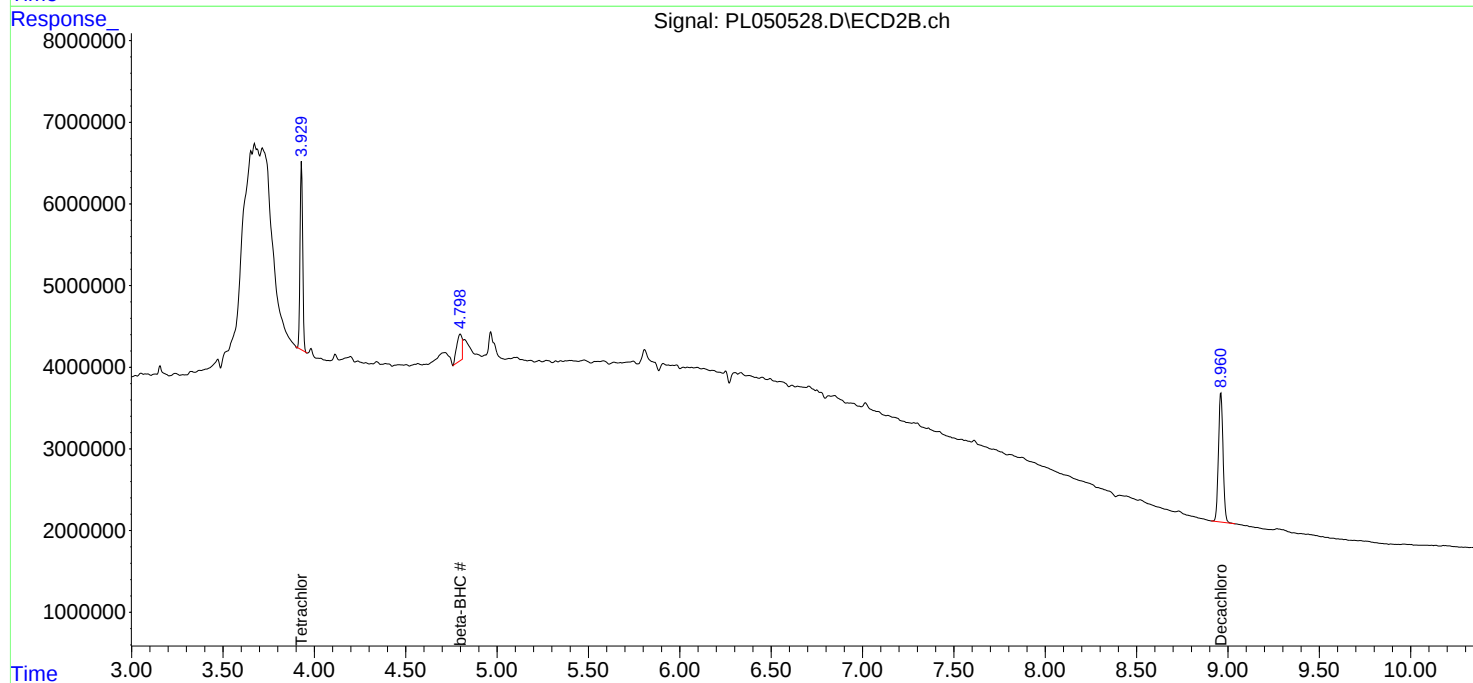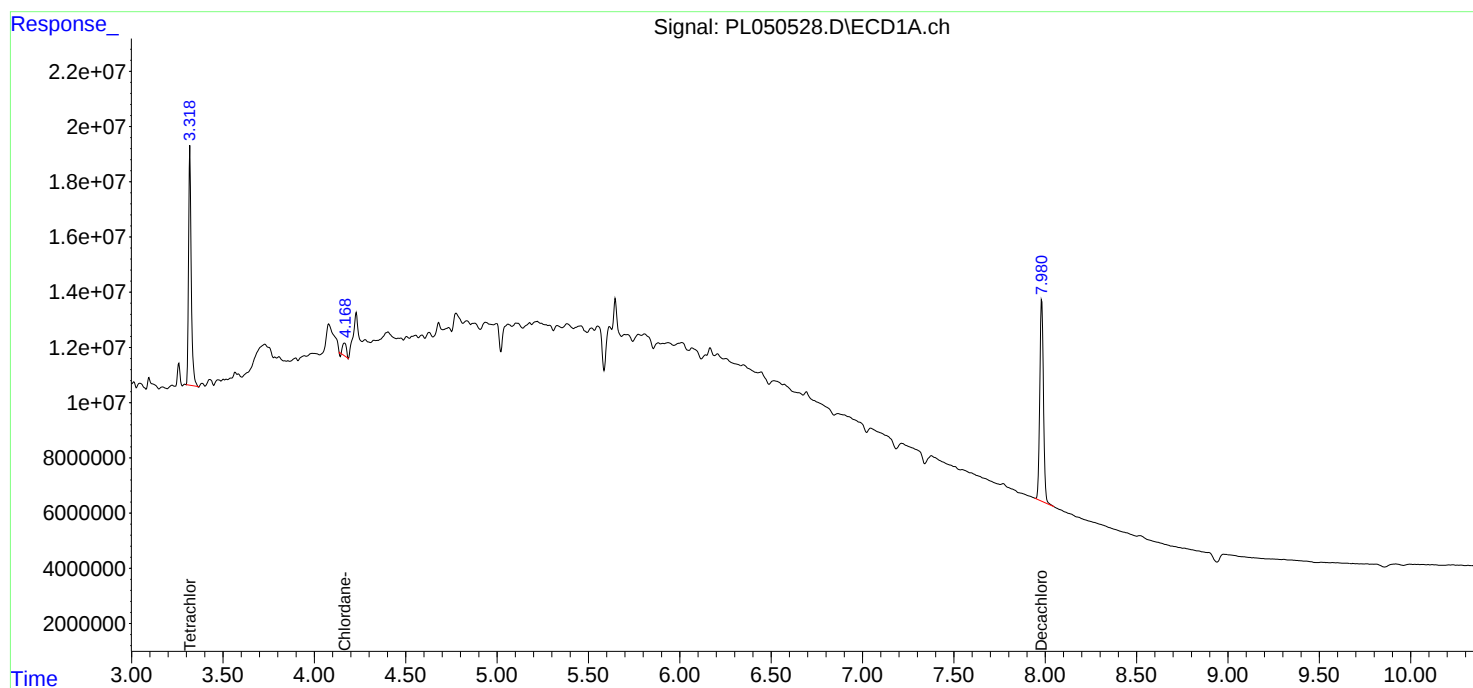


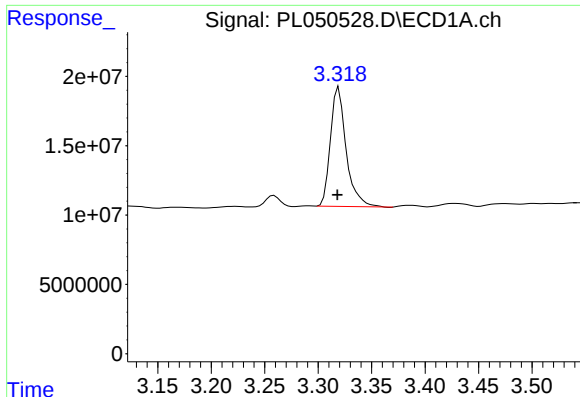

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.001 min
Response: 87725205
Conc: 8.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3_071619

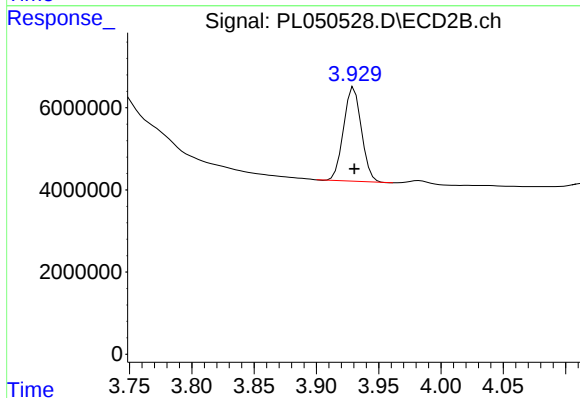


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 22882351
Conc: 8.02 ng/ml

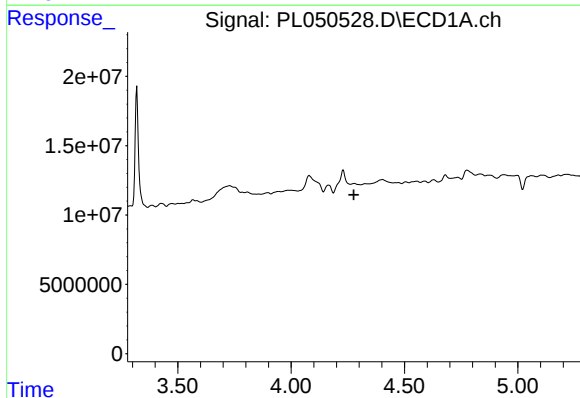


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

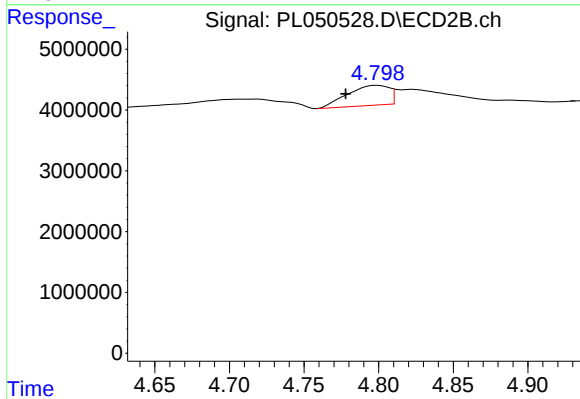

#6 beta-BHC


R.T.: 4.799 min
Delta R.T.: 0.021 min
Response: 6566183
Conc: 3.80 ng/ml

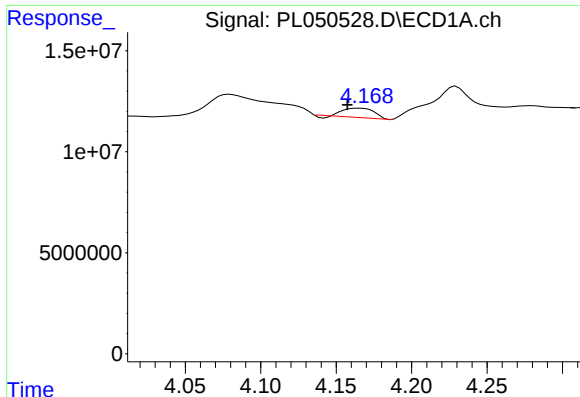

#23 Chlordane-1


R.T.: 4.166 min
Delta R.T.: 0.008 min
Response: 6407118
Conc: 17.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3_071619

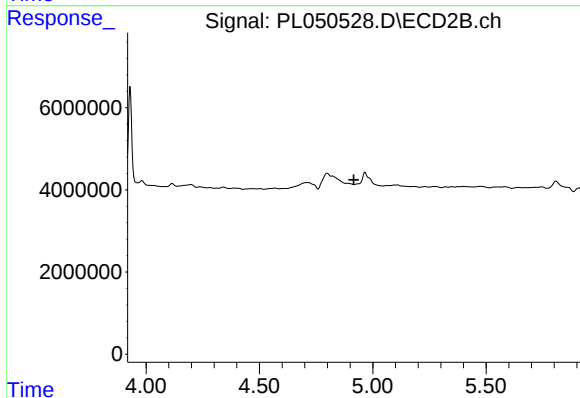


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.916 min
Response: 0
Conc: N.D.

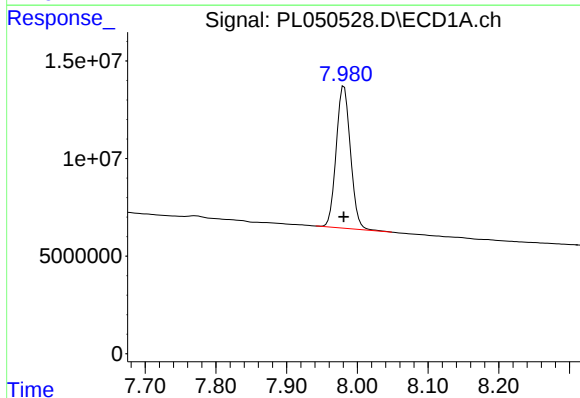

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 101854812
Conc: 10.06 ng/ml

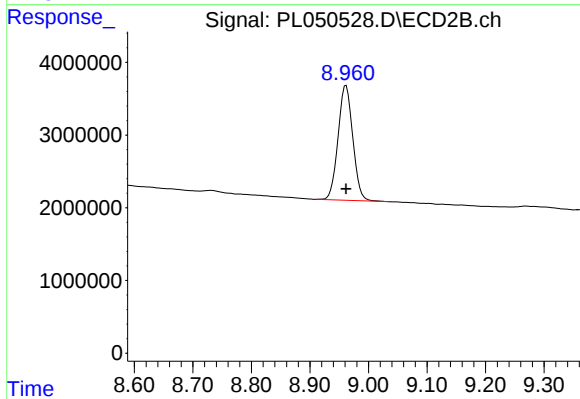

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: 0.000 min
Response: 27577618
Conc: 9.75 ng/ml