

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
 Data File : PL050471.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 17:01
 Operator : SM\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 06:35:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 04:12:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.931	198.3E6	56399411	19.733	19.767
28)	SA Decachlor...	7.981	8.963	202.6E6	57605597	20.008	20.370
Target Compounds							
9)	A Endosulfan I	5.309	6.148	138.8E6	32666400	9.541	9.499
10)	B gamma-Chl...	5.201	6.027	150.8E6	35147411	9.555	9.511
12)	B 4,4'-DDE	5.425	6.259	295.8E6	70084116	19.740	19.449
13)	MA Dieldrin	5.548	6.404	308.5E6	69104553	19.905	19.515
19)	B Endosulfa...	6.454	7.181	241.6E6	54760641	18.965	18.960
20)	A Methoxychlor	6.714	7.508	598.6E6	142.6E6	95.943	97.170
21)	B Endrin ke...	6.936	7.649	228.1E6	49069905	16.677	16.972



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
Data File : PL050471.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 17:01
Operator : SM\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 06:35:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 04:12:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

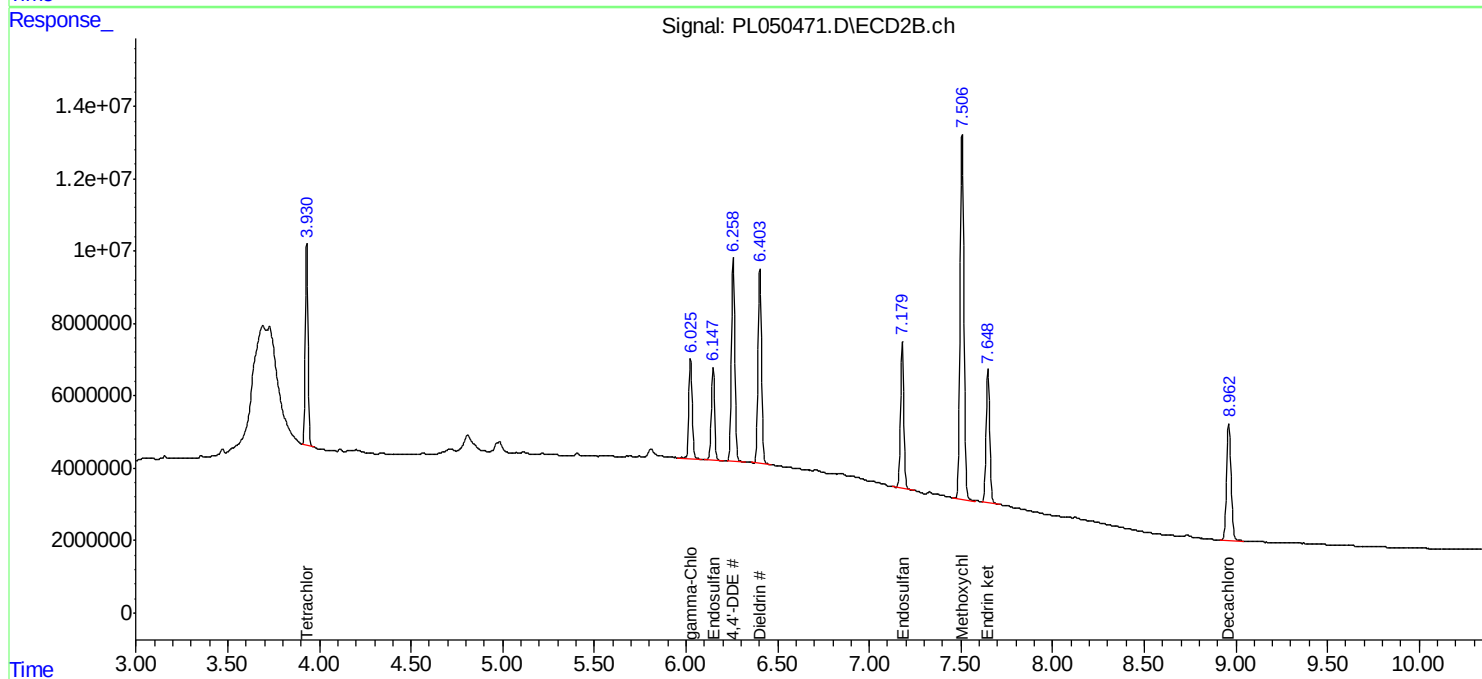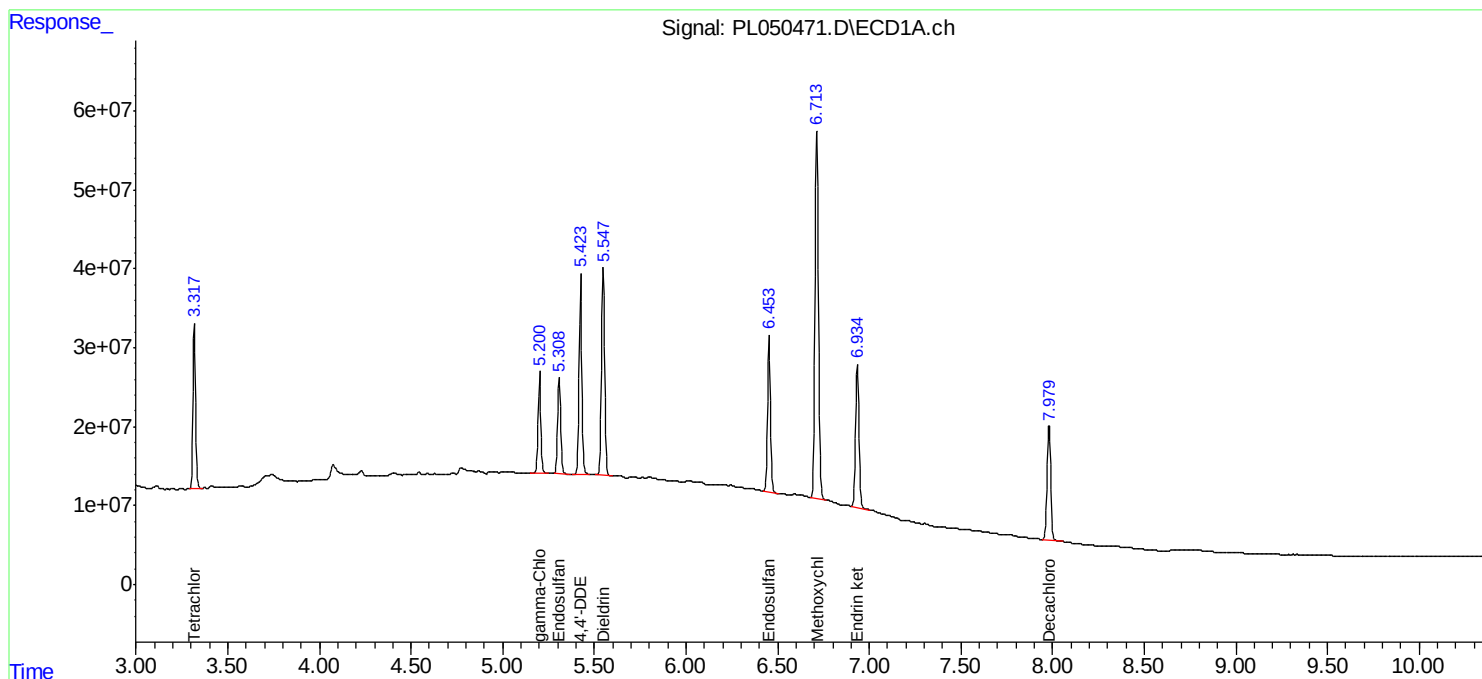


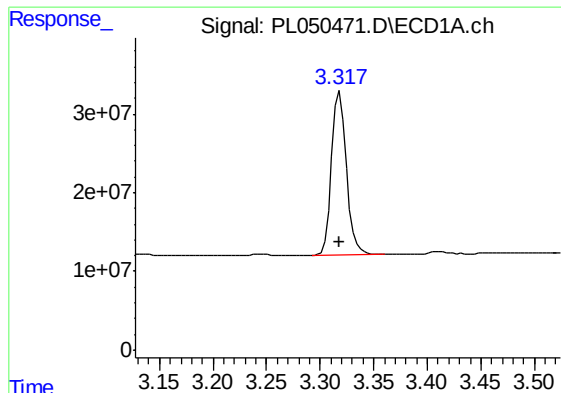

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 198276522
Conc: 19.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

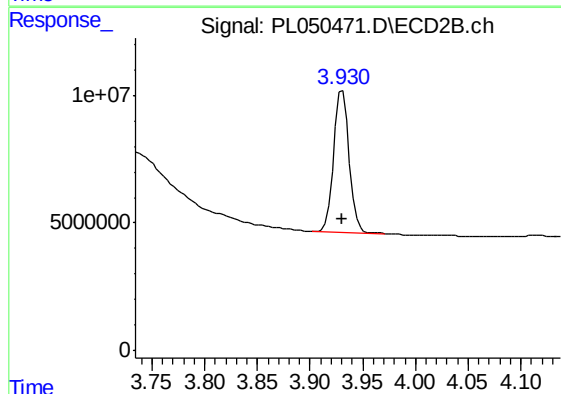


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 56399411
Conc: 19.77 ng/ml

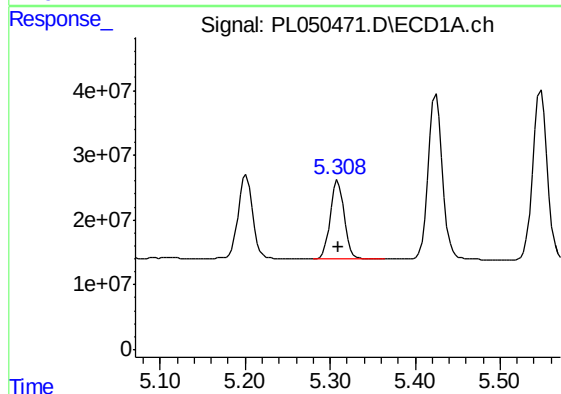


#9 Endosulfan I

R.T.: 5.309 min
Delta R.T.: 0.000 min
Response: 138766249
Conc: 9.54 ng/ml

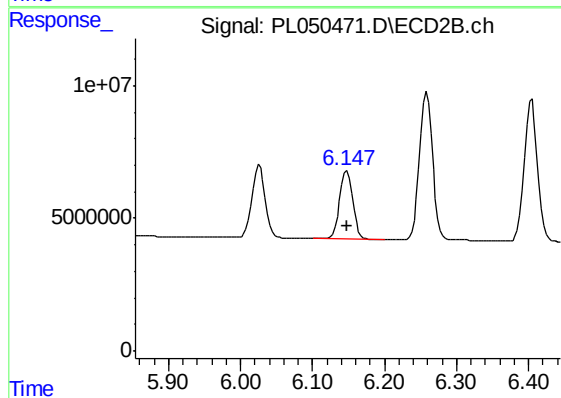

#9 Endosulfan I


R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 32666400
Conc: 9.50 ng/ml

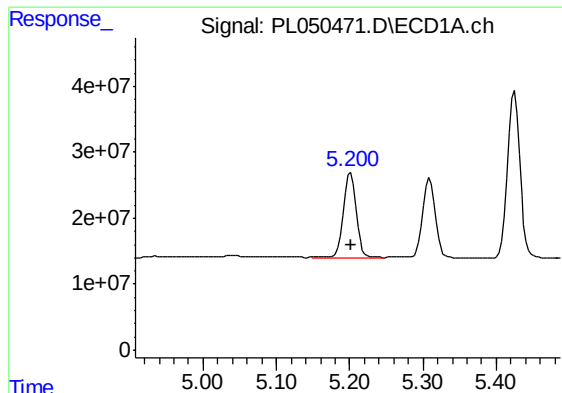

#10 gamma-Chlordane


R.T.: 5.201 min
Delta R.T.: 0.000 min
Response: 150811415
Conc: 9.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

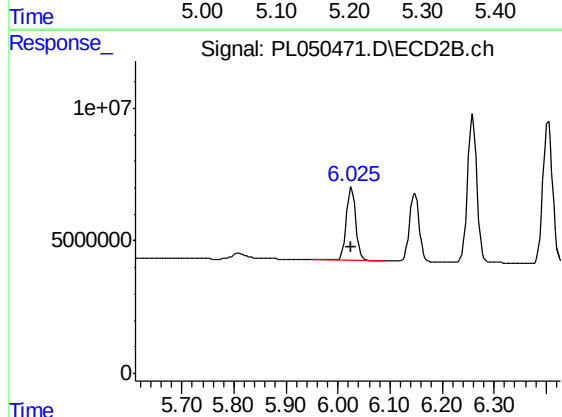


#10 gamma-Chlordane

R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 35147411
Conc: 9.51 ng/ml

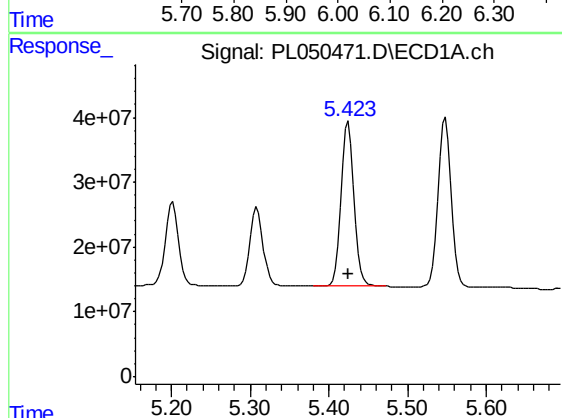


#12 4,4'-DDE

R.T.: 5.425 min
Delta R.T.: 0.000 min
Response: 295817856
Conc: 19.74 ng/ml

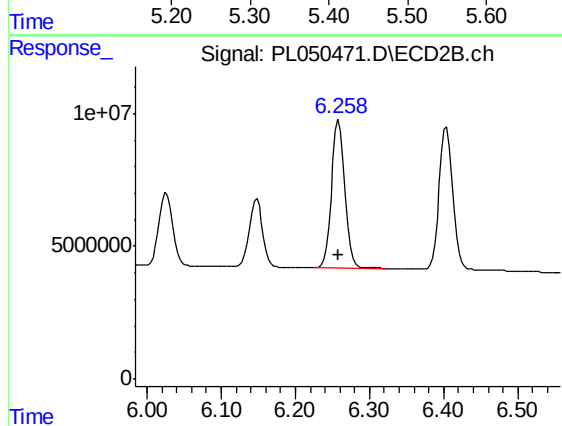

#12 4,4'-DDE


R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 70084116
Conc: 19.45 ng/ml

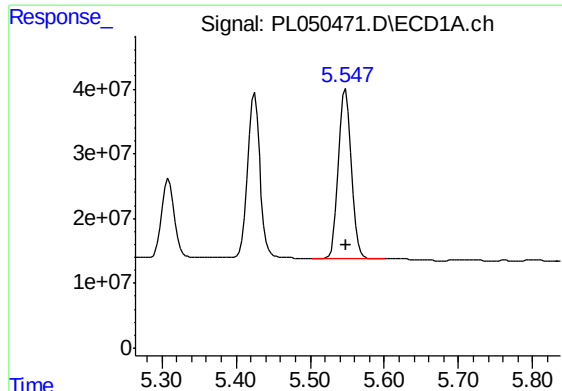

#13 Dielddrin


R.T.: 5.548 min
Delta R.T.: 0.000 min
Response: 308469546
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

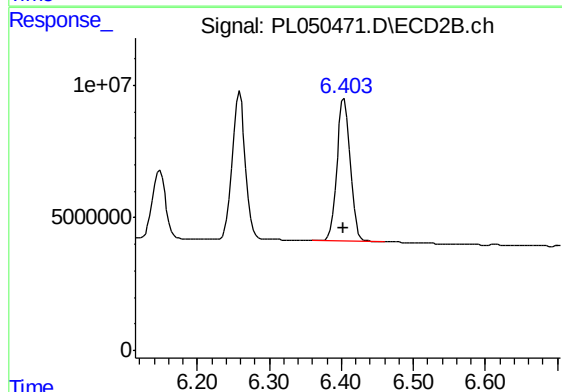


#13 Dielddrin

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 69104553
Conc: 19.51 ng/ml

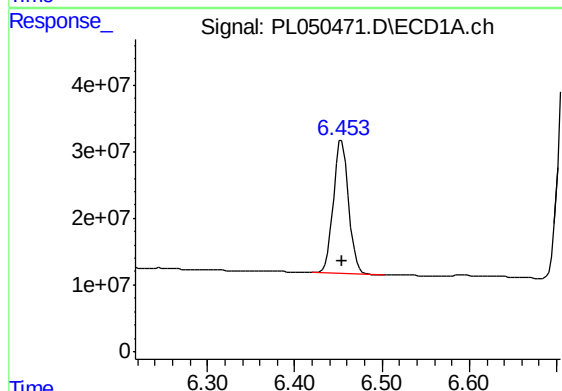


#19 Endosulfan Sulfate

R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 241606502
Conc: 18.97 ng/ml

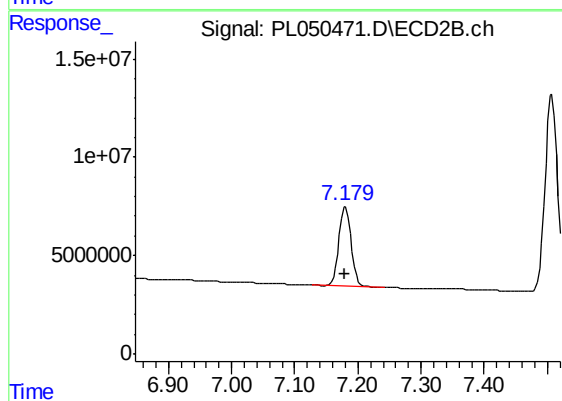

#19 Endosulfan Sulfate


R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 54760641
Conc: 18.96 ng/ml

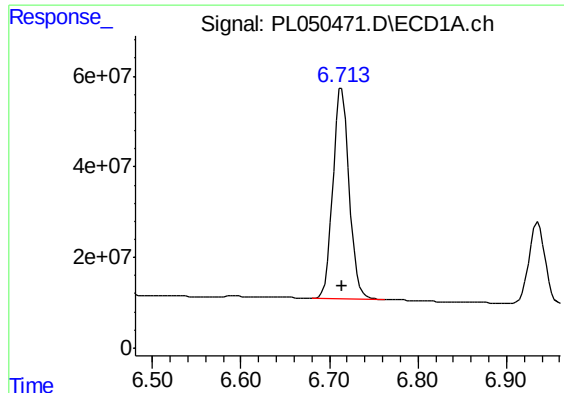

#20 Methoxychlor


R.T.: 6.714 min
Delta R.T.: 0.000 min
Response: 598583347
Conc: 95.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

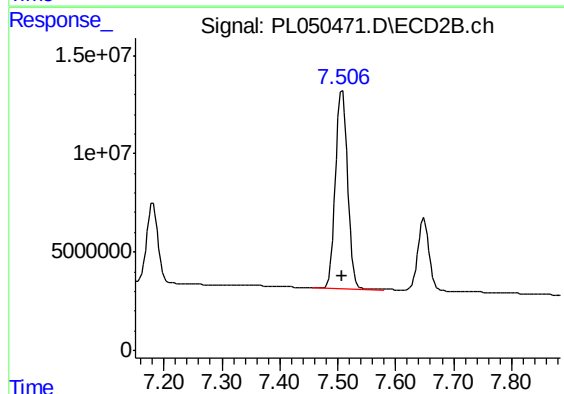


#20 Methoxychlor

R.T.: 7.508 min
Delta R.T.: 0.000 min
Response: 142573932
Conc: 97.17 ng/ml

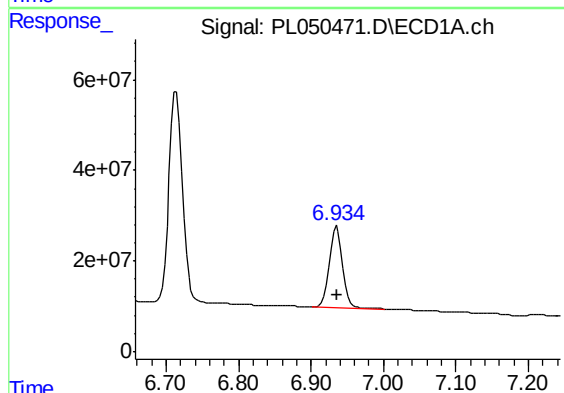


#21 Endrin ketone

R.T.: 6.936 min
Delta R.T.: 0.000 min
Response: 228093089
Conc: 16.68 ng/ml

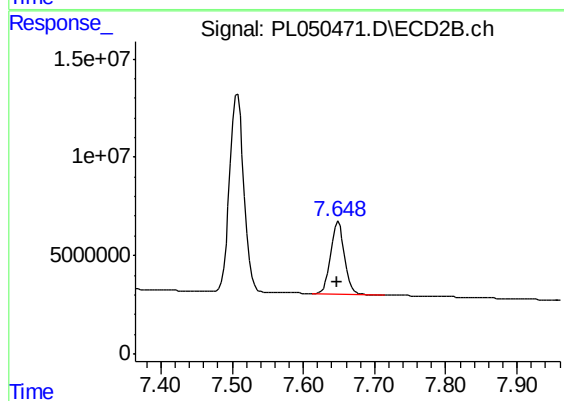

#21 Endrin ketone


R.T.: 7.649 min
Delta R.T.: 0.001 min
Response: 49069905
Conc: 16.97 ng/ml

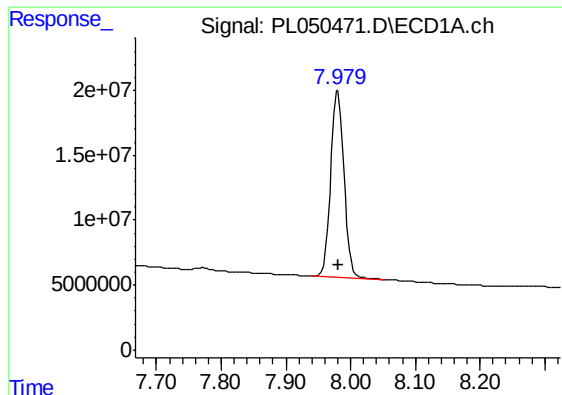

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 202589372
Conc: 20.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

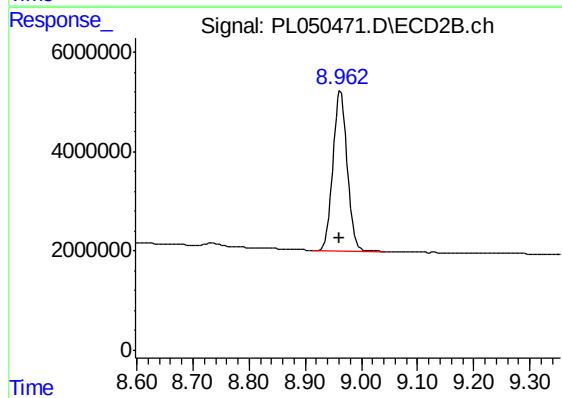

#28 Decachlorobiphenyl

R.T.: 8.963 min
Delta R.T.: 0.001 min
Response: 57605597
Conc: 20.37 ng/ml