

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
 Data File : PL050477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2019 18:27
 Operator : SM\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 03:19:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 18 03:18:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.931	1163.6E6	282.8E6	100.957	99.190
28)	SA Decachlor...	7.980	8.962	980.8E6	258.8E6	94.316	92.458
Target Compounds							
23)	Chlordane-1	4.157	4.916	371.7E6	110.6E6	1010.052	1002.754
24)	Chlordane-2	4.647	5.383	428.2E6	112.2E6	973.833	962.482
25)	Chlordane-3	5.202	6.027	1377.9E6	488.5E6	986.205	1010.388
26)	Chlordane-4	5.257	6.100	1314.0E6	581.3E6	994.548	998.157
27)	Chlordane-5	6.079	6.902	499.3E6	95772523	972.346	1002.551



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071719\
Data File : PL050477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2019 18:27
Operator : SM\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 03:19:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Thu Jul 18 03:18:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

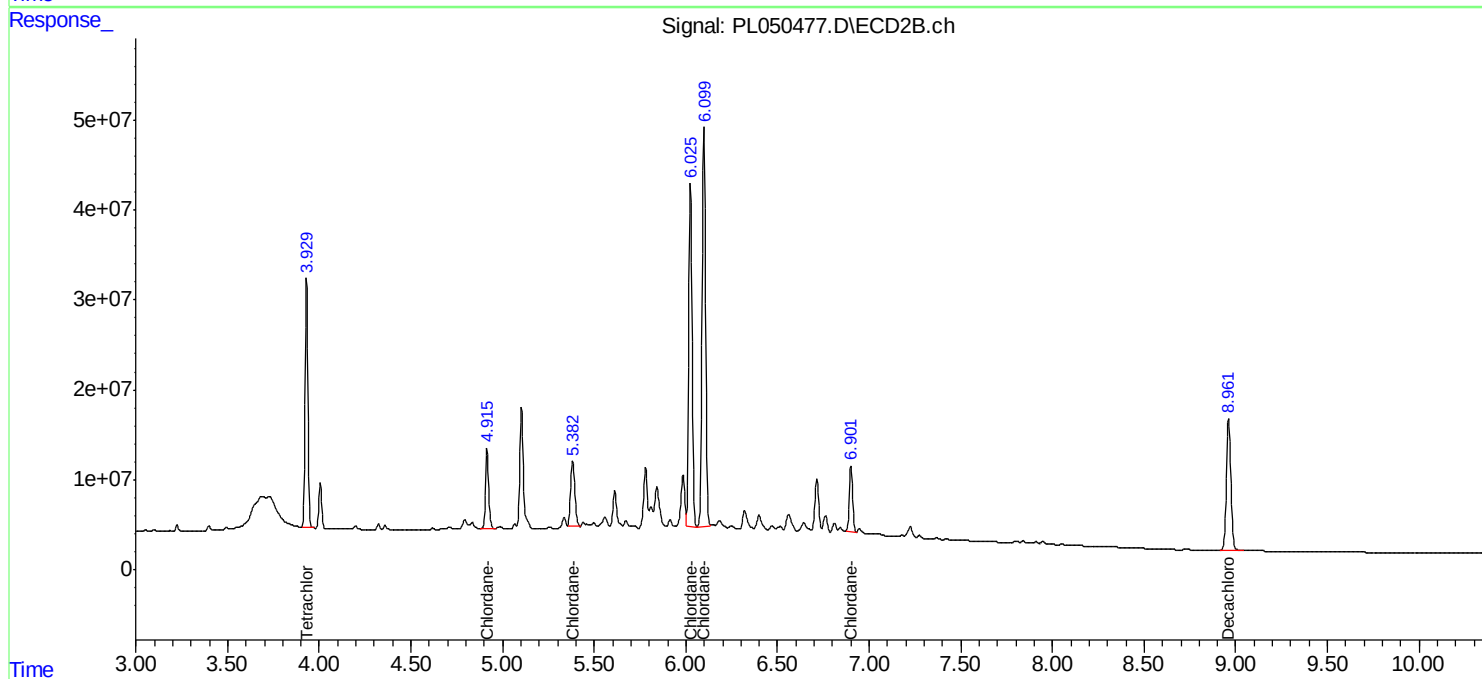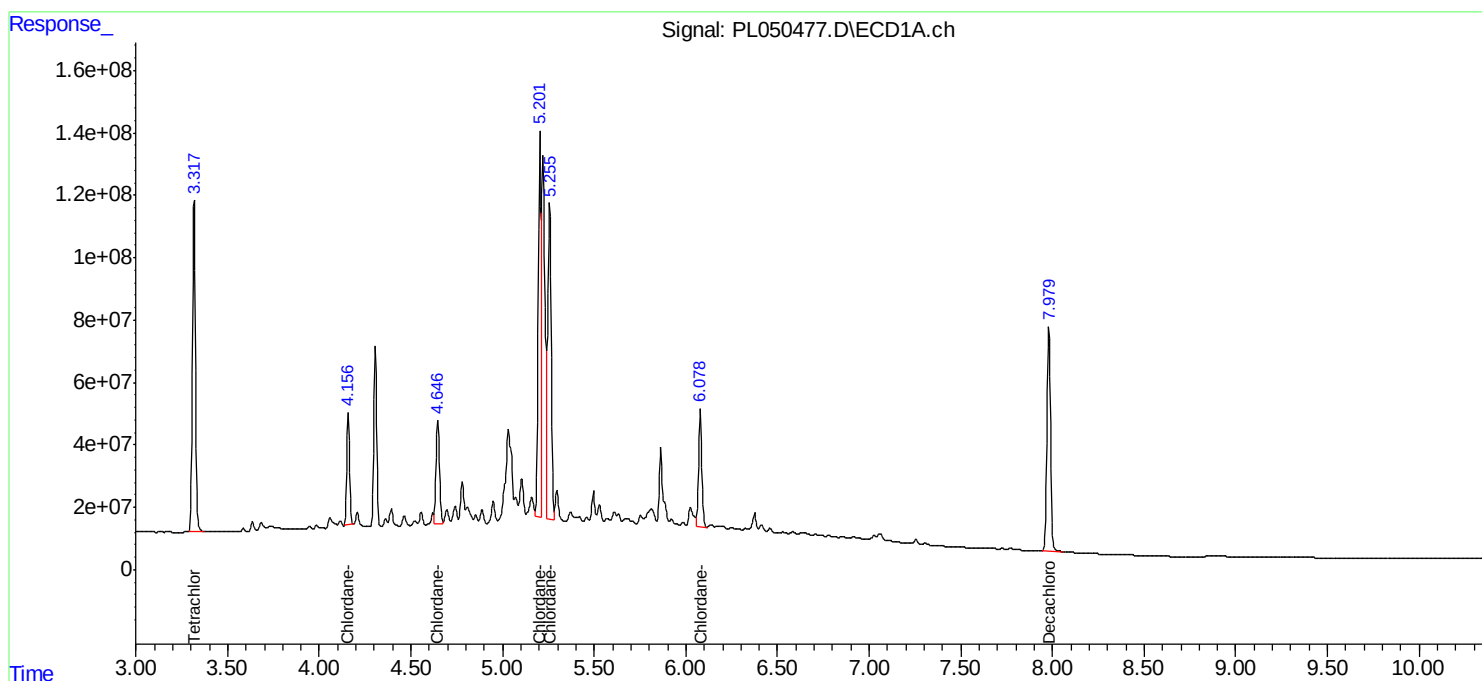


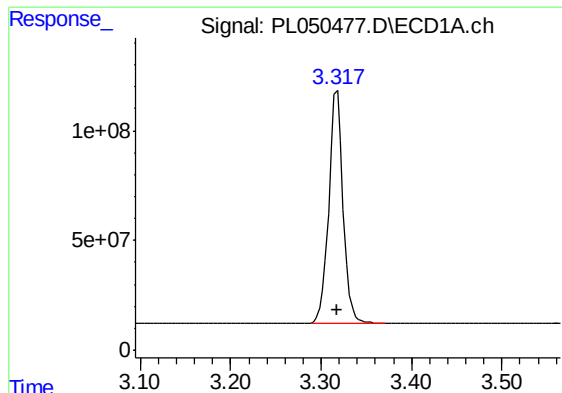

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 1163647660
Conc: 100.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

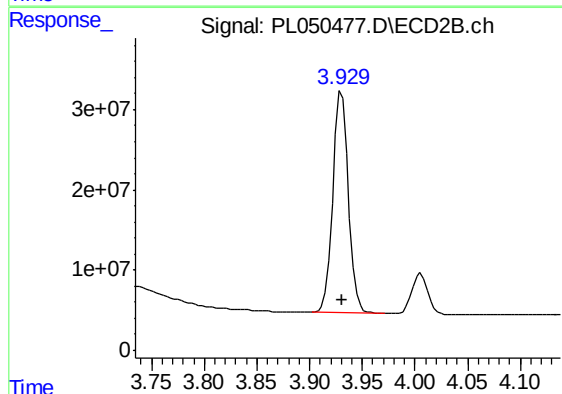


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: 0.000 min
Response: 282849929
Conc: 99.19 ng/ml

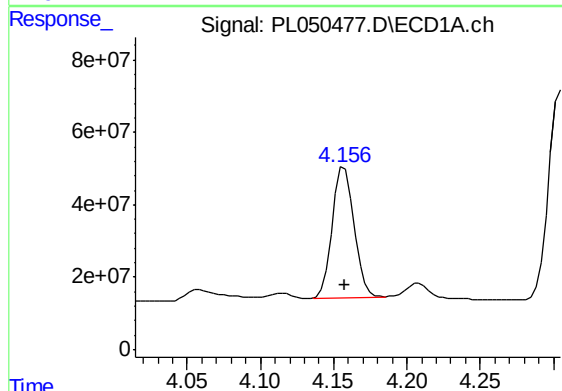


#23 Chlordane-1

R.T.: 4.157 min
Delta R.T.: 0.000 min
Response: 371722902
Conc: 1010.05 ng/ml

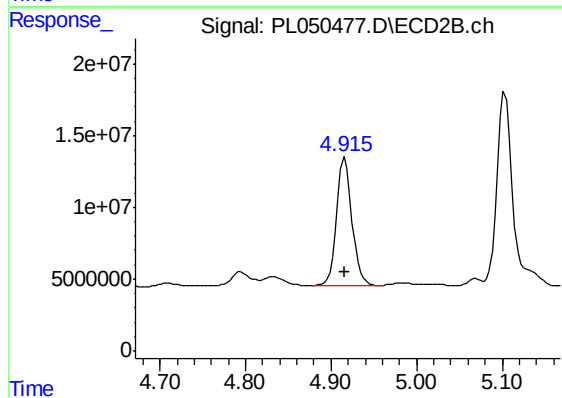

#23 Chlordane-1


R.T.: 4.916 min
Delta R.T.: 0.000 min
Response: 110637530
Conc: 1002.75 ng/ml

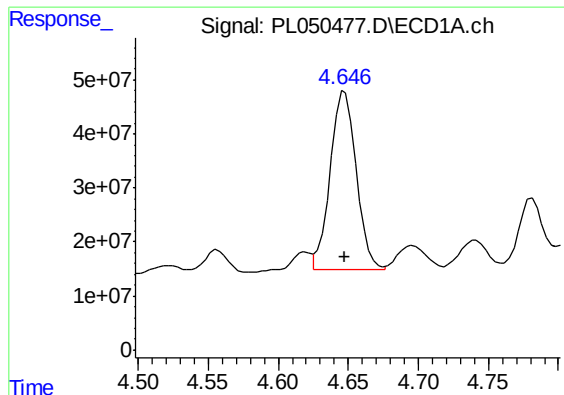

#24 Chlordane-2


R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 428172216
Conc: 973.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

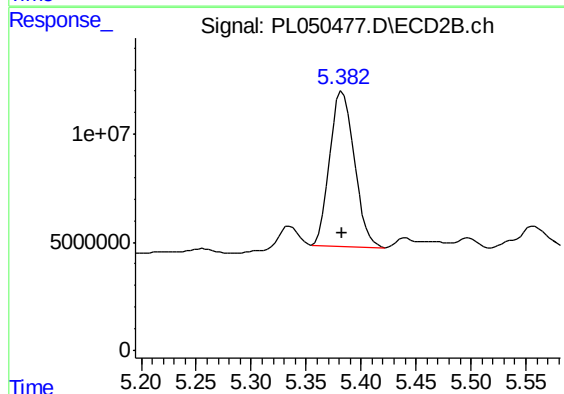


#24 Chlordane-2

R.T.: 5.383 min
Delta R.T.: 0.000 min
Response: 112221745
Conc: 962.48 ng/ml

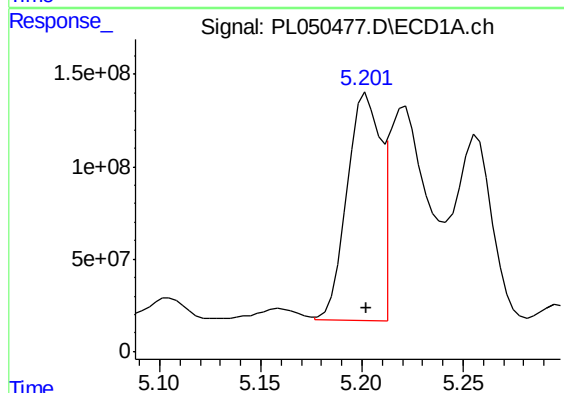


#25 Chlordane-3

R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 1377893922
Conc: 986.21 ng/ml

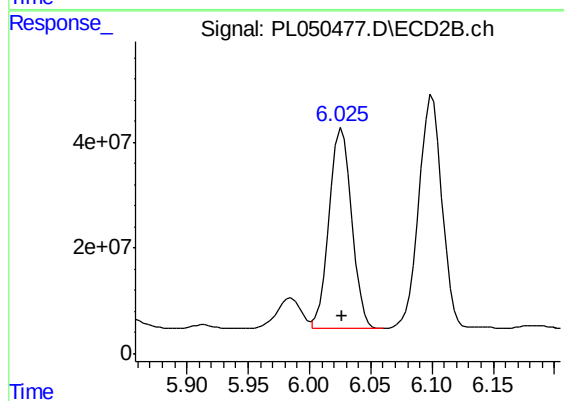

#25 Chlordane-3


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 488453230
Conc: 1010.39 ng/ml

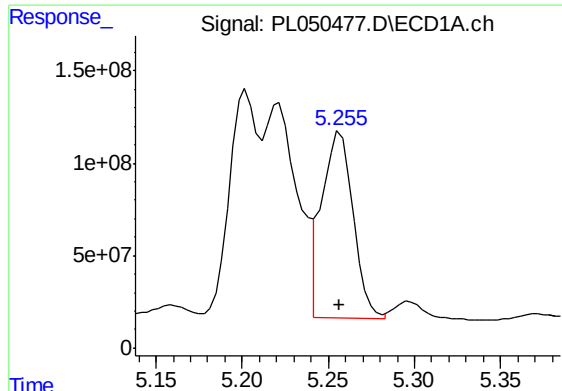

#26 Chlordane-4


R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 1314035970
Conc: 994.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

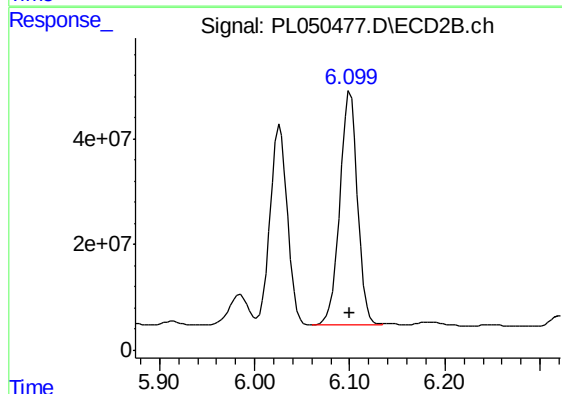


#26 Chlordane-4

R.T.: 6.100 min
Delta R.T.: 0.000 min
Response: 581348884
Conc: 998.16 ng/ml

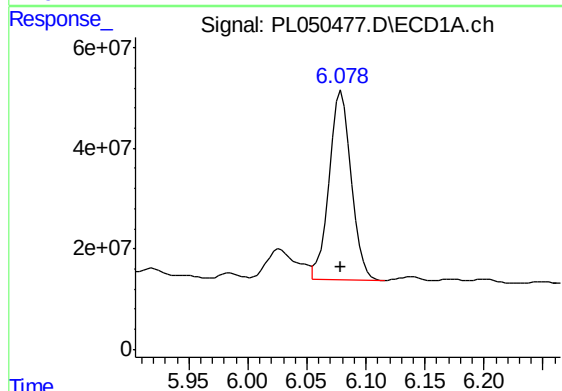


#27 Chlordane-5

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 499341360
Conc: 972.35 ng/ml

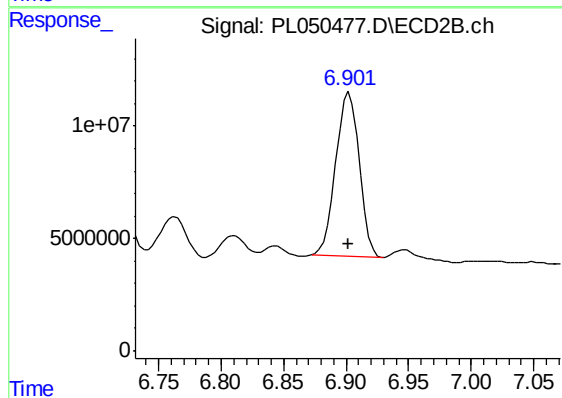

#27 Chlordane-5


R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 95772523
Conc: 1002.55 ng/ml

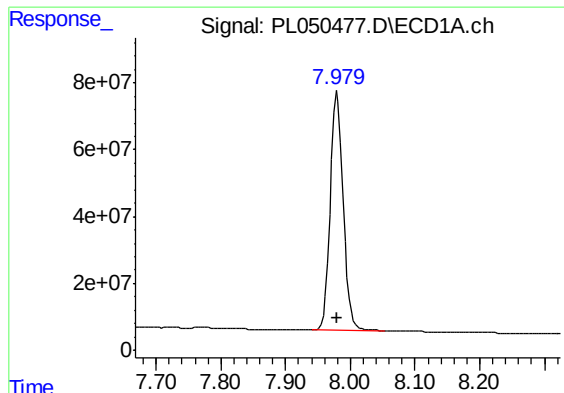

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 980751874
Conc: 94.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

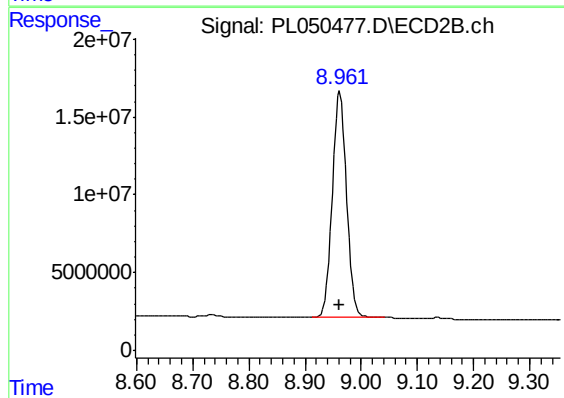

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: 0.000 min
Response: 258798315
Conc: 92.46 ng/ml